

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
 Data File : PL041330.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 00:36
 Operator : AJ\SJ
 Sample : J5639-04
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:15:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.104	110.8E6	58317874	20.219	20.915
28)	SA Decachlor...	8.220	9.234	84433317	35462171	16.239	13.714
Target Compounds							
6)	B beta-BHC	4.414f	4.994f	9849250	1923001	3.104	1.200 #
23)	Chlordane-1	4.389	5.151	4580209	-583719	17.946	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102418\
Data File : PL041330.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 00:36
Operator : AJ\SJ
Sample : J5639-04
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 01:15:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

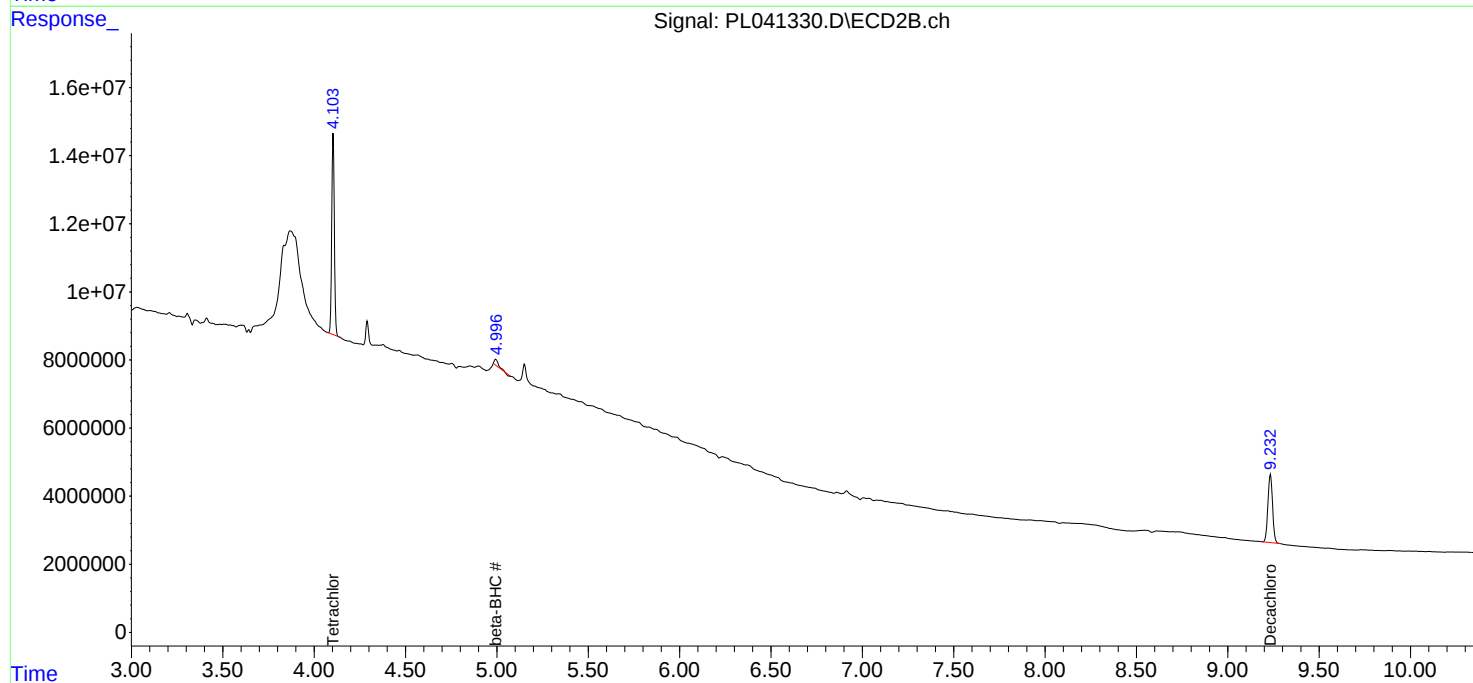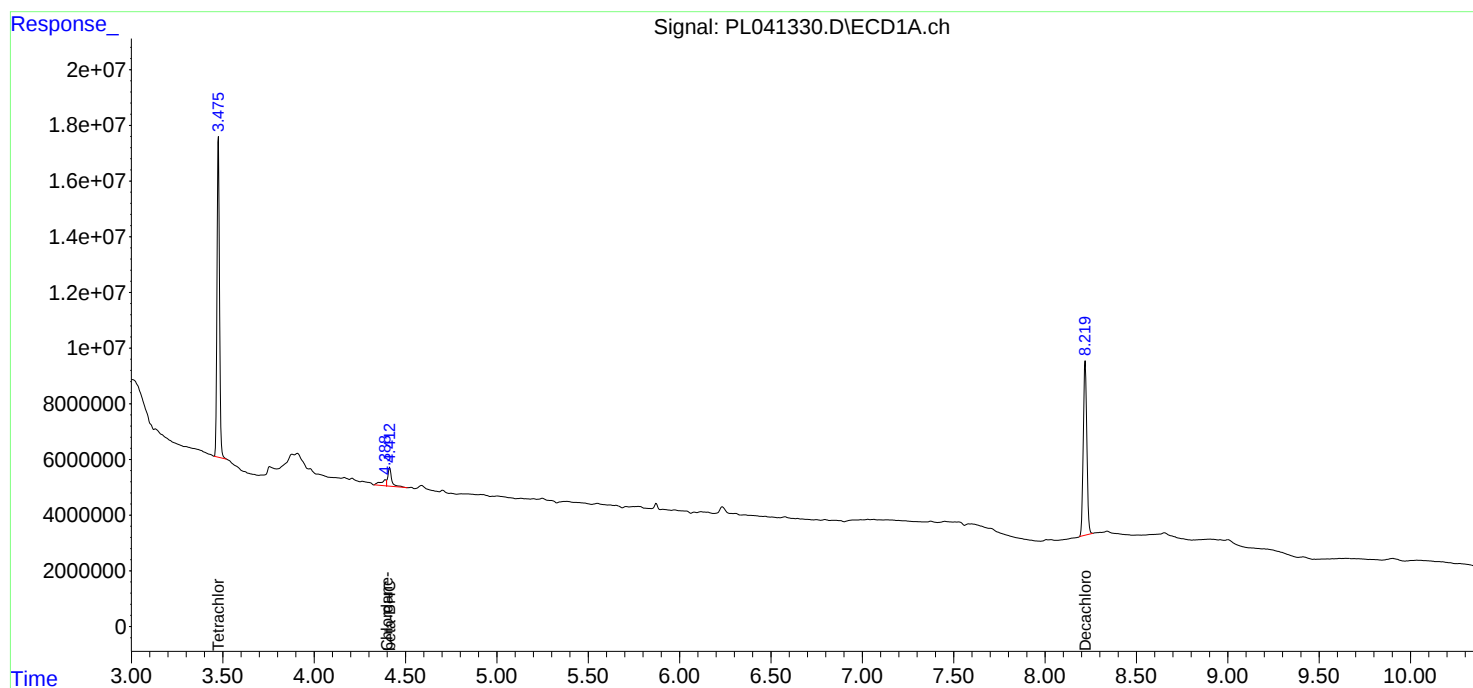


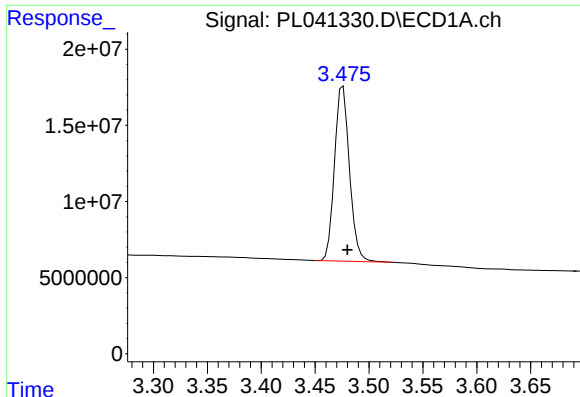

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 110813879
Conc: 20.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

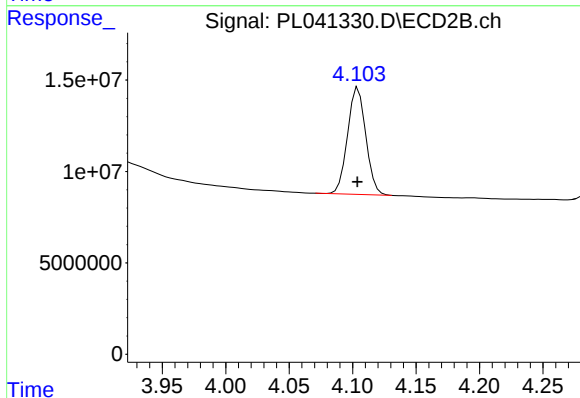


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 58317874
Conc: 20.92 ng/ml

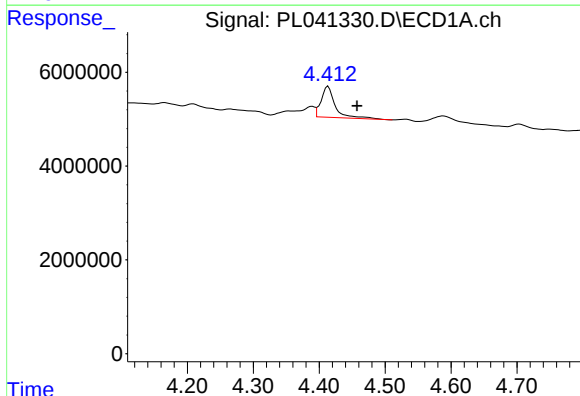


#6 beta-BHC

R.T.: 4.414 min
Delta R.T.: -0.044 min
Response: 9849250
Conc: 3.10 ng/ml

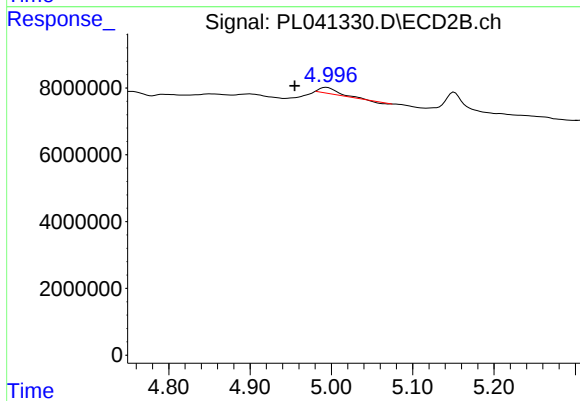

#6 beta-BHC


R.T.: 4.994 min
Delta R.T.: 0.039 min
Response: 1923001
Conc: 1.20 ng/ml

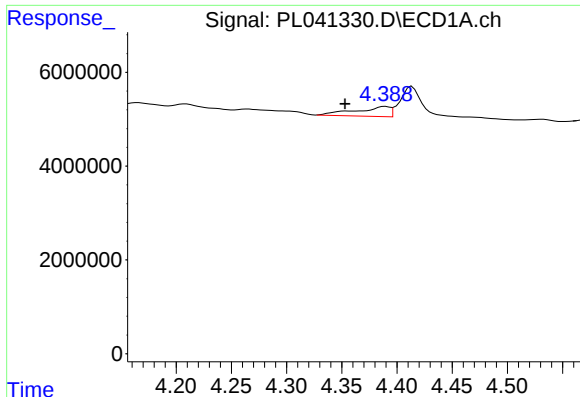

#23 Chlordane-1


R.T.: 4.389 min
Delta R.T.: 0.037 min
Response: 4580209
Conc: 17.95 ng/ml

Instrument :
ECD_L
ClientSampleId :

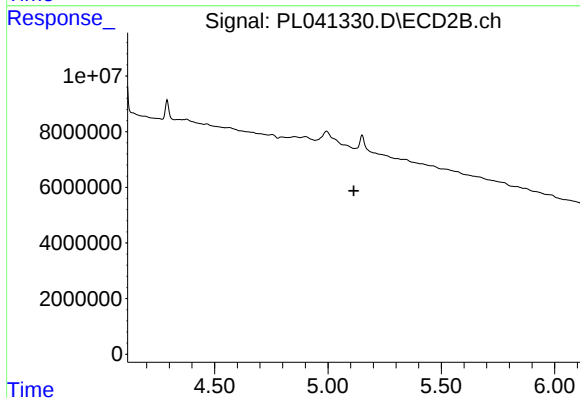


#23 Chlordane-1

R.T.: 5.151 min
Delta R.T.: 0.037 min
Response: -583719
Conc: N.D.

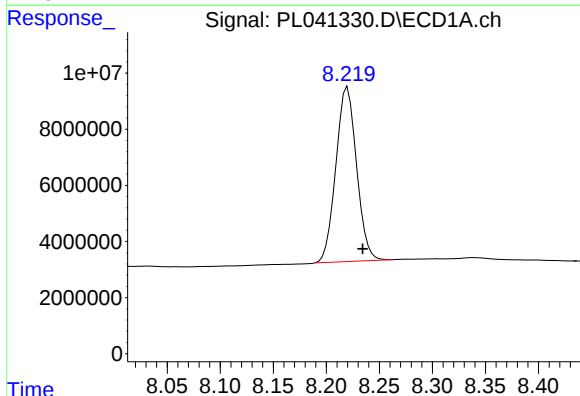

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 84433317
Conc: 16.24 ng/ml

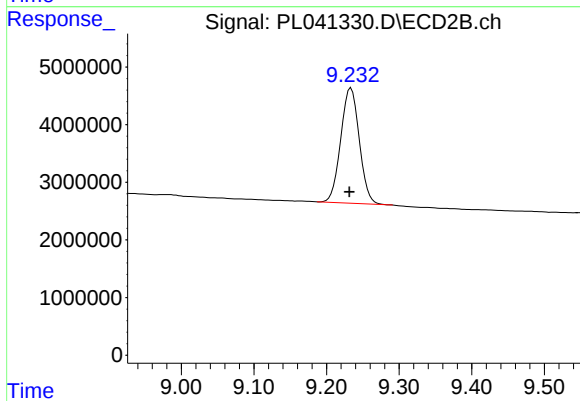

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.002 min
Response: 35462171
Conc: 13.71 ng/ml