

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041344.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 12:07
 Operator : AJ\SJ
 Sample : J5622-03RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 12:20:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.103	10435984	4460195	1.904	1.600
28)	SA Decachlor...	8.221	9.234	13508520	5263238	2.598	2.035
Target Compounds							
2)	A alpha-BHC	3.882f	0.000	10531240	0	1.329	N.D. #
6)	B beta-BHC	0.000	4.997f	0	1950494	N.D.	1.217 #
8)	B Heptachlo...	5.263f	5.992	31662742	43352832	4.828	15.115 #
14)	MA Endrin	6.035	0.000	3211330	0	0.559	N.D. #
16)	A 4,4'-DDD	0.000	6.914f	0	2177735	N.D.	1.040 #
17)	MA 4,4'-DDT	6.389	0.000	1604511	0	0.352	N.D. #
20)	A Methoxychlor	0.000	7.649f	0	12460366	N.D.	10.585 #
21)	B Endrin ke...	7.134f	0.000	2770180	0	0.529	N.D. #
23)	Chlordane-1	4.402	0.000	3680019	0	14.419	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041344.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 12:07
Operator : AJ\SJ
Sample : J5622-03RE
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 12:20:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

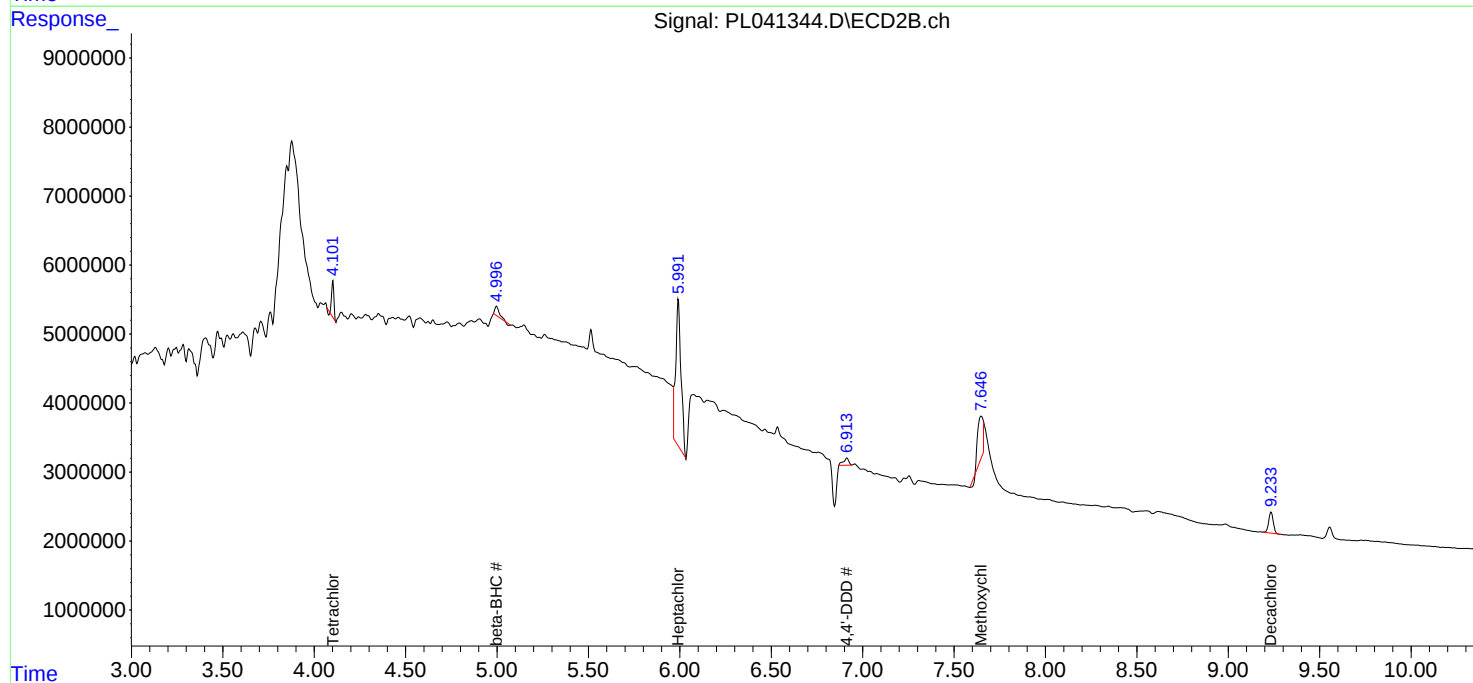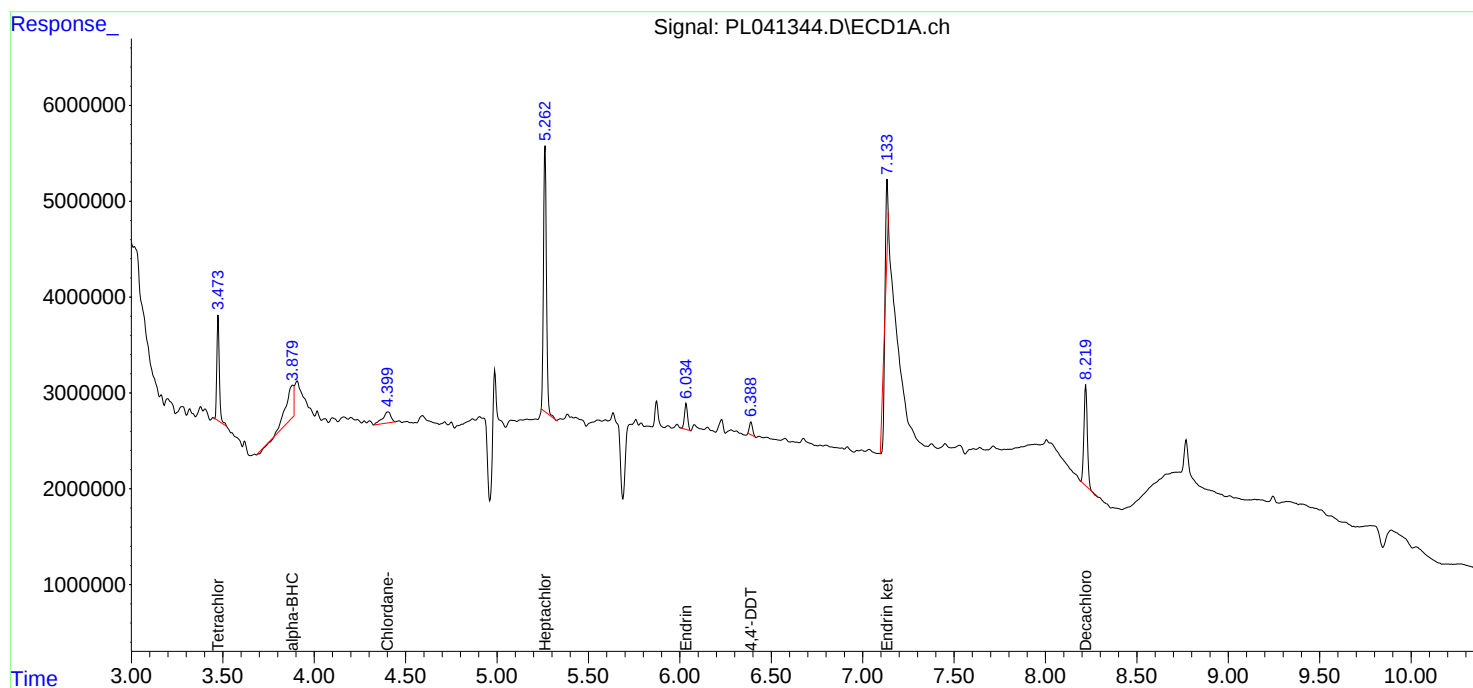


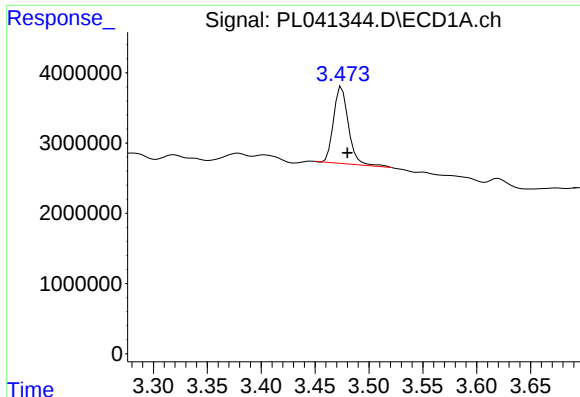

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 10435984
Conc: 1.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

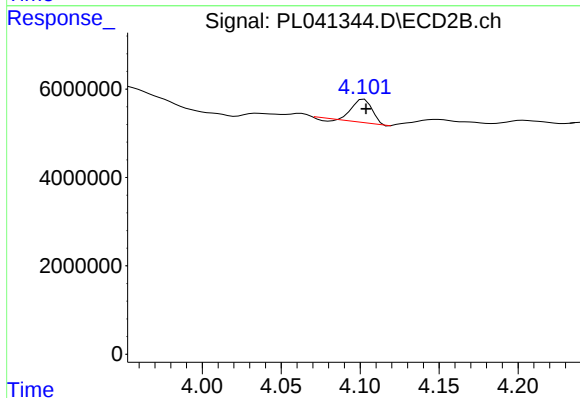


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.001 min
Response: 4460195
Conc: 1.60 ng/ml

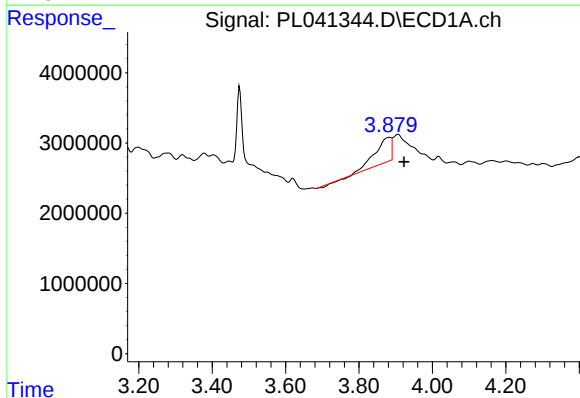


#2 alpha-BHC

R.T.: 3.882 min
Delta R.T.: -0.040 min
Response: 10531240
Conc: 1.33 ng/ml

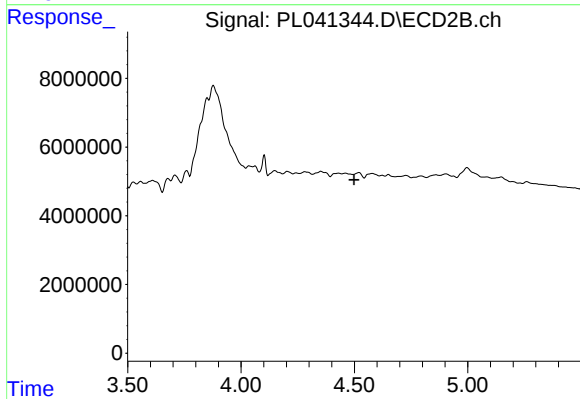

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.499 min
Response: 0
Conc: N.D.

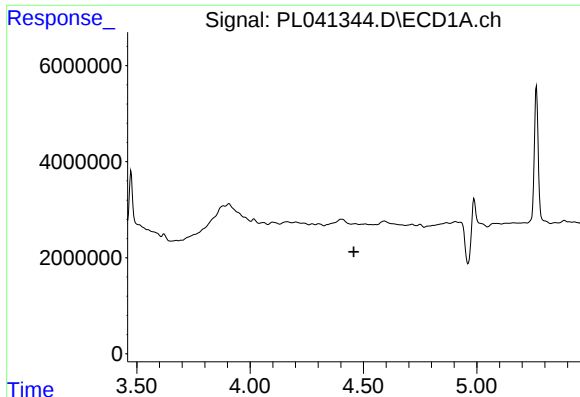

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

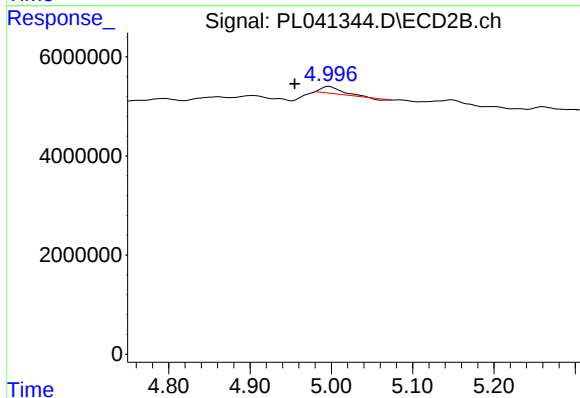


#6 beta-BHC

R.T.: 4.997 min
Delta R.T.: 0.042 min
Response: 1950494
Conc: 1.22 ng/ml

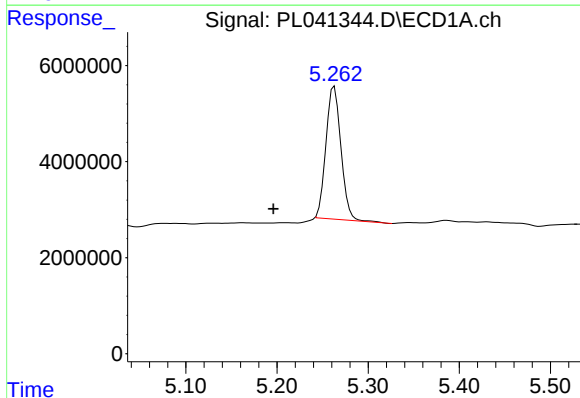


#8 Heptachlor epoxide

R.T.: 5.263 min
Delta R.T.: 0.067 min
Response: 31662742
Conc: 4.83 ng/ml

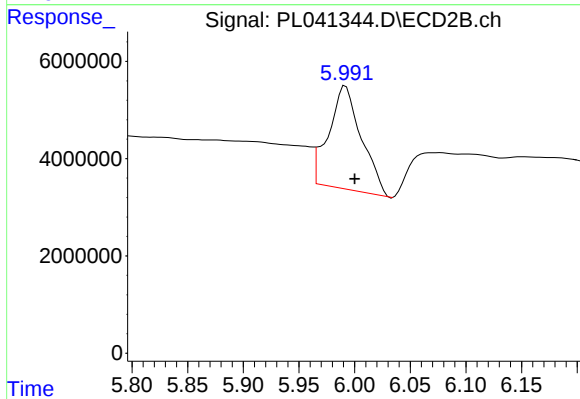

#8 Heptachlor epoxide


R.T.: 5.992 min
Delta R.T.: -0.008 min
Response: 43352832
Conc: 15.12 ng/ml

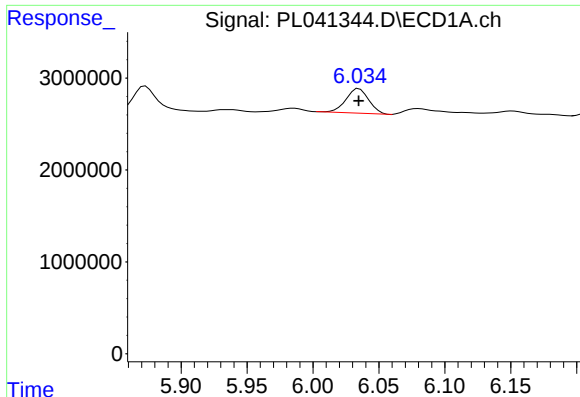

#14 Endrin


R.T.: 6.035 min
Delta R.T.: 0.000 min
Response: 3211330
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

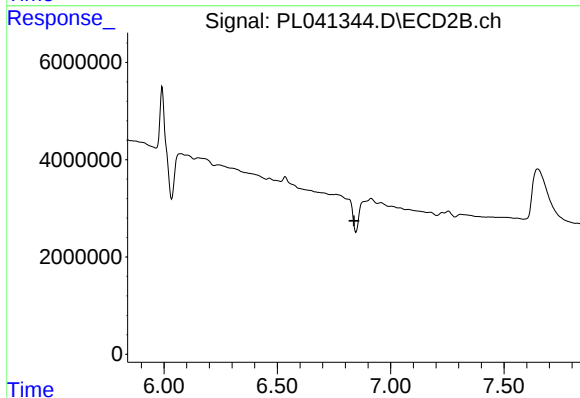


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.838 min
Response: 0
Conc: N.D.

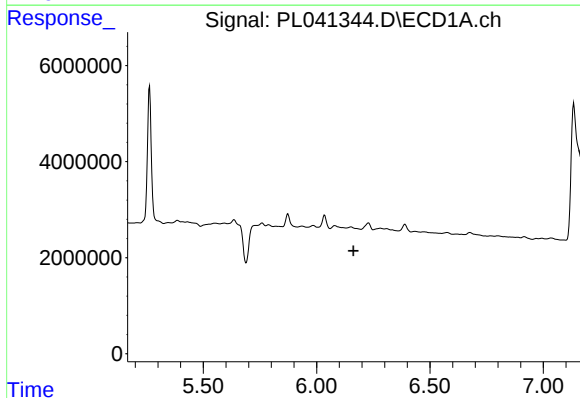


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.163 min
Response: 0
Conc: N.D.

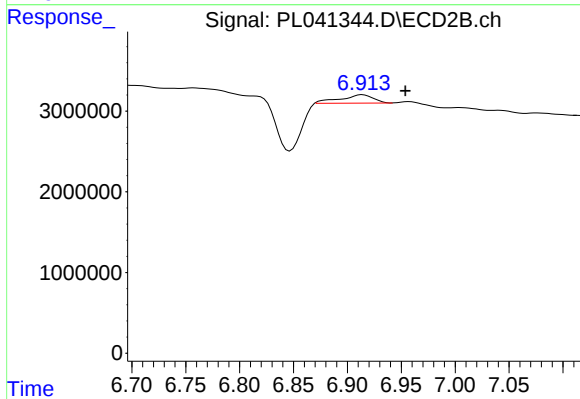

#16 4,4'-DDD


R.T.: 6.914 min
Delta R.T.: -0.040 min
Response: 2177735
Conc: 1.04 ng/ml

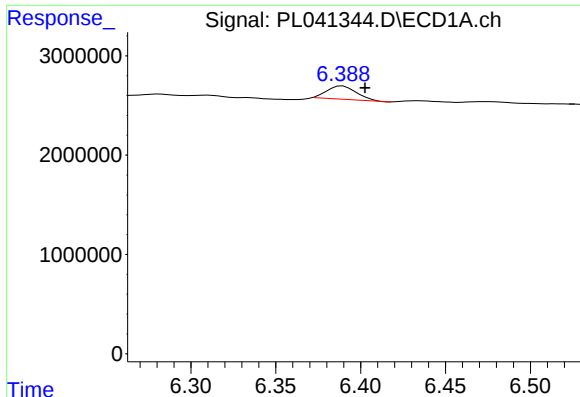

#17 4,4'-DDT


R.T.: 6.389 min
Delta R.T.: -0.013 min
Response: 1604511
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :

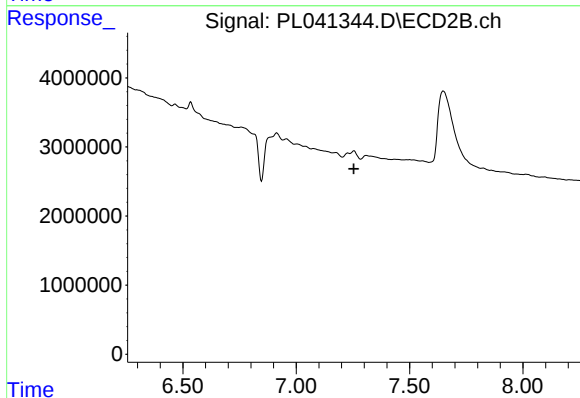


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

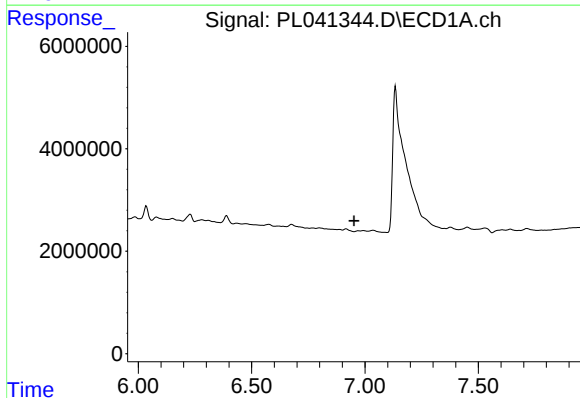


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

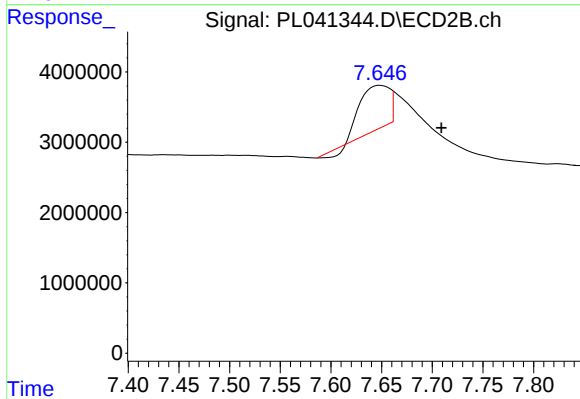

#20 Methoxychlor


R.T.: 7.649 min
Delta R.T.: -0.061 min
Response: 12460366
Conc: 10.59 ng/ml

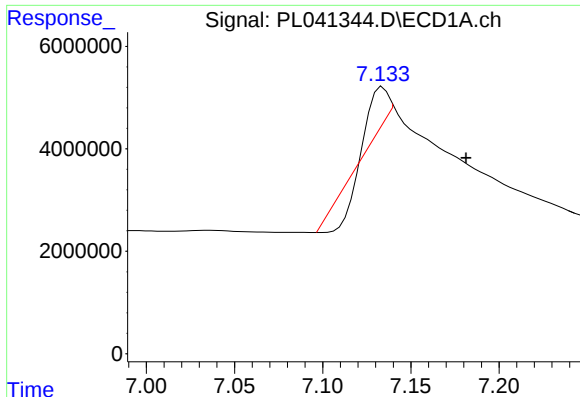

#21 Endrin ketone


R.T.: 7.134 min
Delta R.T.: -0.047 min
Response: 2770180
Conc: 0.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

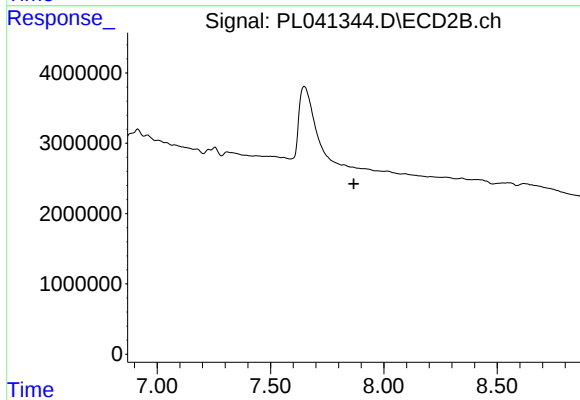


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.867 min
Response: 0
Conc: N.D.

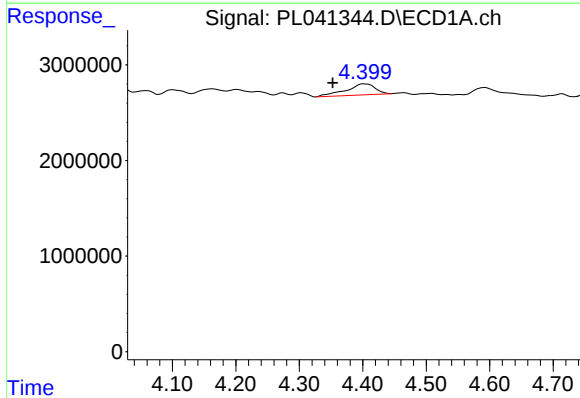


#23 Chlordane-1

R.T.: 4.402 min
Delta R.T.: 0.049 min
Response: 3680019
Conc: 14.42 ng/ml

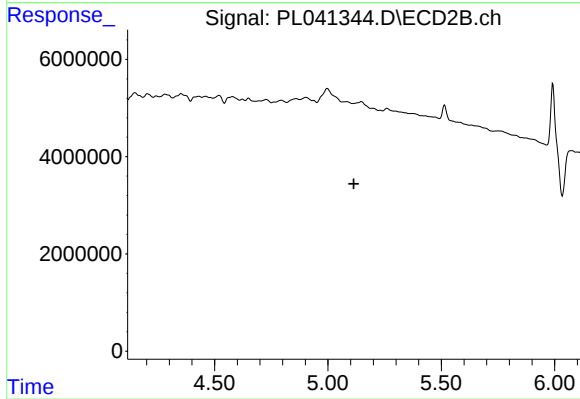

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

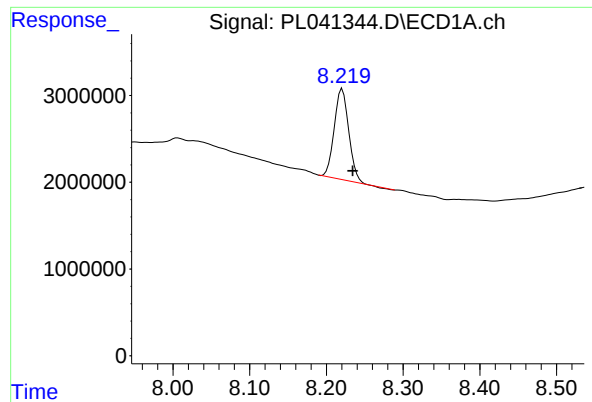

#28 Decachlorobiphenyl

R.T.: 8.221 min
Delta R.T.: -0.014 min
Response: 13508520
Conc: 2.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

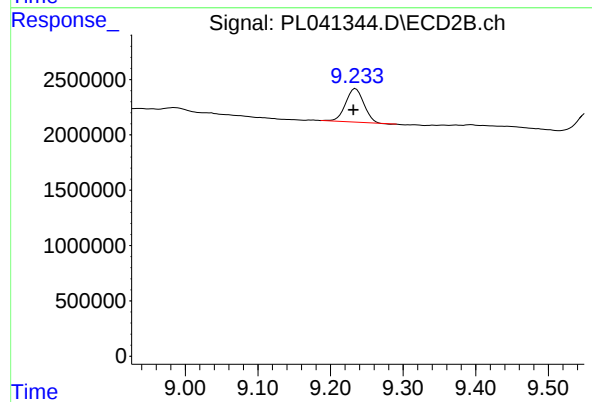

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.003 min
Response: 5263238
Conc: 2.04 ng/ml