

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102419\
 Data File : PL053675.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2019 13:11
 Operator : SG\AJ
 Sample : K5145-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HD-02-102319

Manual Integrations
 APPROVED

Ankita
 10/25/2019 12:12:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:29:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.542	4.044	107.2E6	25678447	9.893	10.262
28) SA Decachlor...	8.328	9.121	72319722	19980129	7.371	7.095
Target Compounds						
12) B 4,4'-DDE	5.726	6.383	6501621	3271830	0.547	1.162 #
17) MA 4,4'-DDT	6.486	7.171	5211760	1685901	0.526m	0.729m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102419\
Data File : PL053675.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2019 13:11
Operator : SG\AJ
Sample : K5145-04
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
HD-02-102319


Manual Integrations
APPROVED

Ankita
10/25/2019 12:12:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:29:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

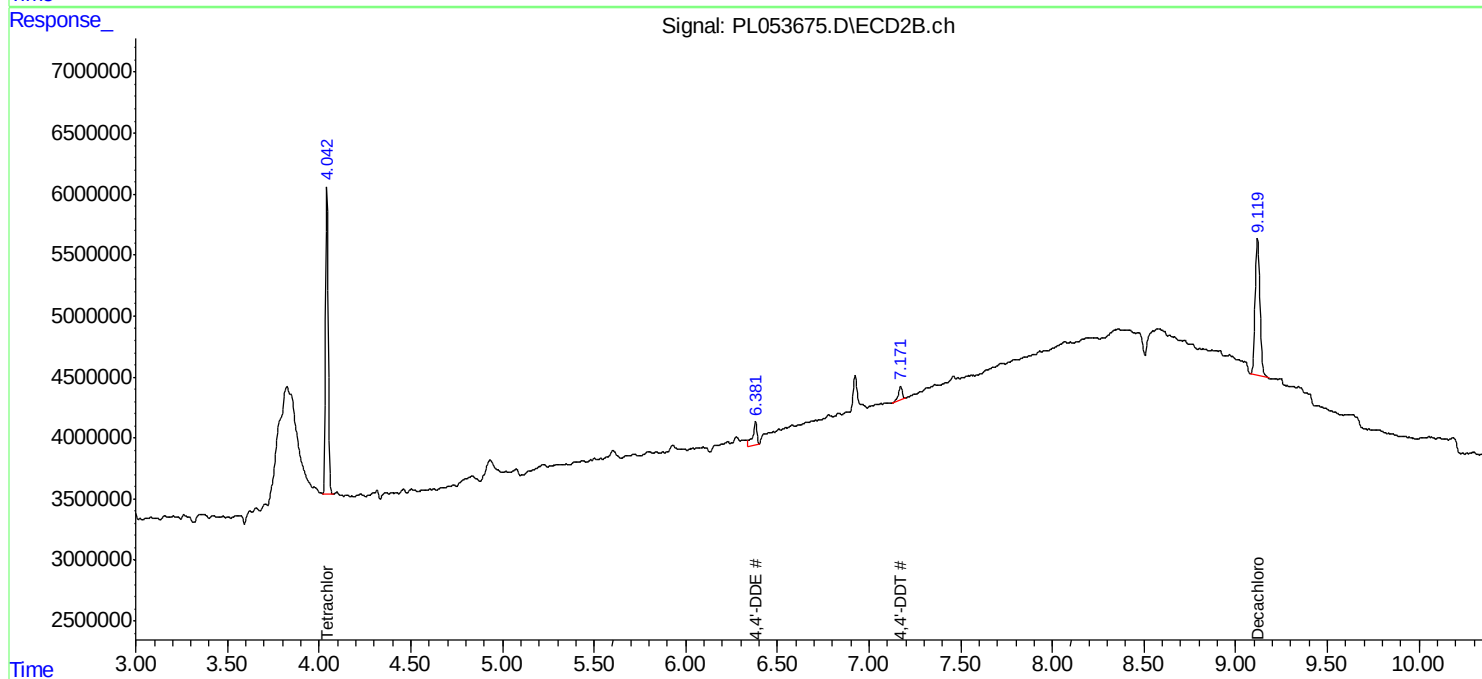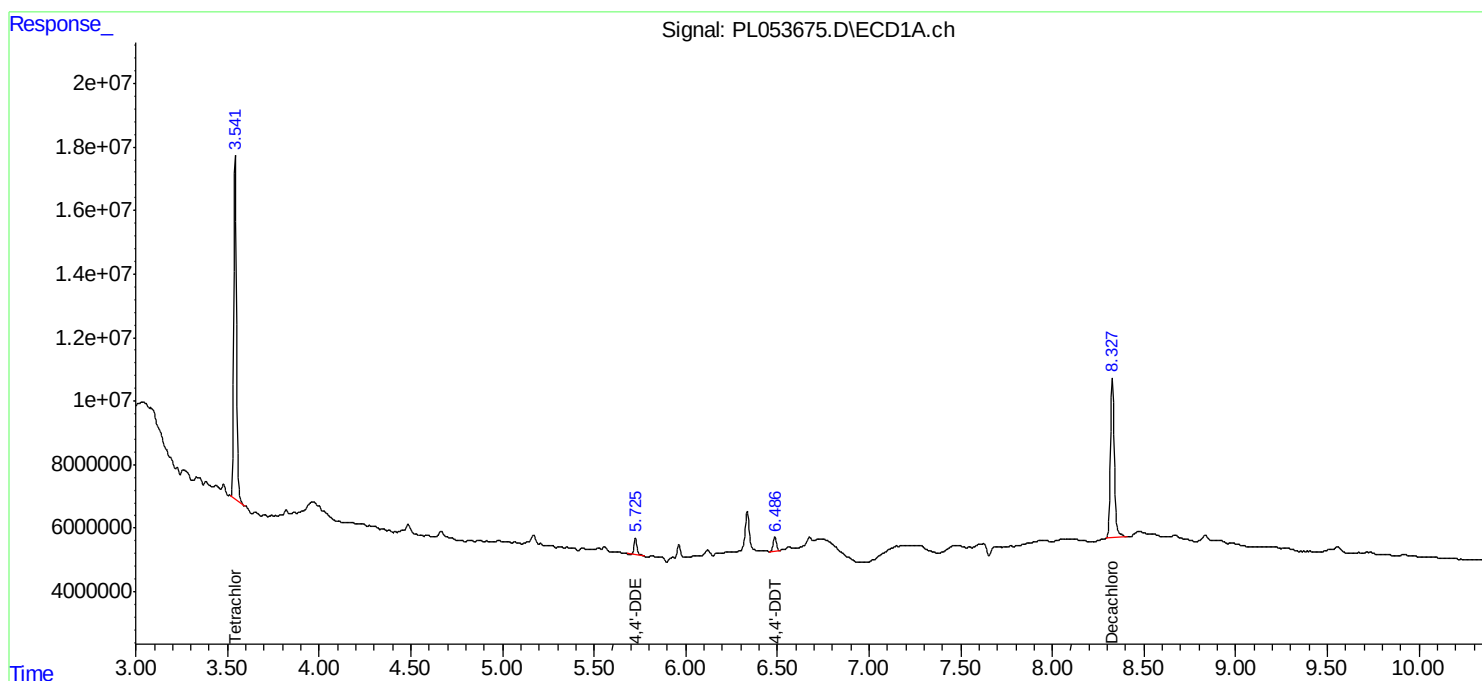

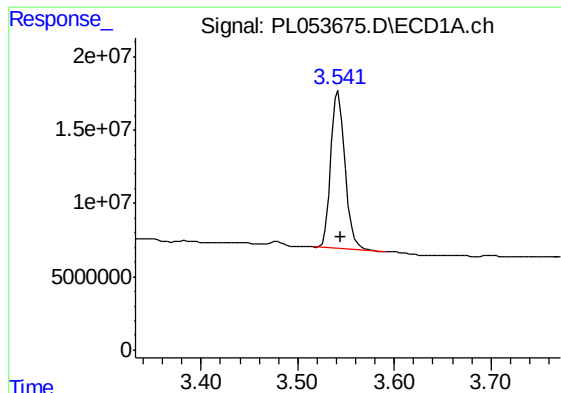


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 107230037
Conc: 9.89 ng/ml

Instrument :
ECD_L
ClientSampleId :
HD-02-102319


Manual Integrations
APPROVED

Ankita
10/25/2019 12:12:44 PM

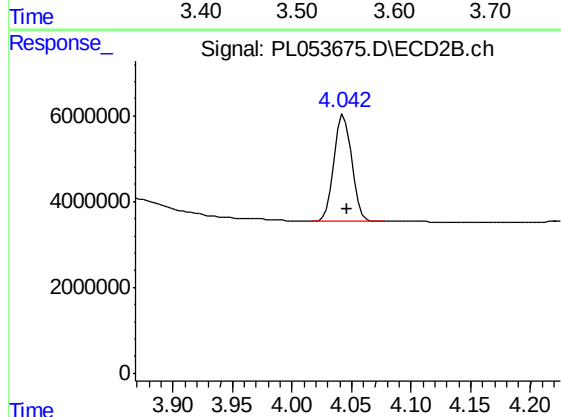


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 25678447
Conc: 10.26 ng/ml

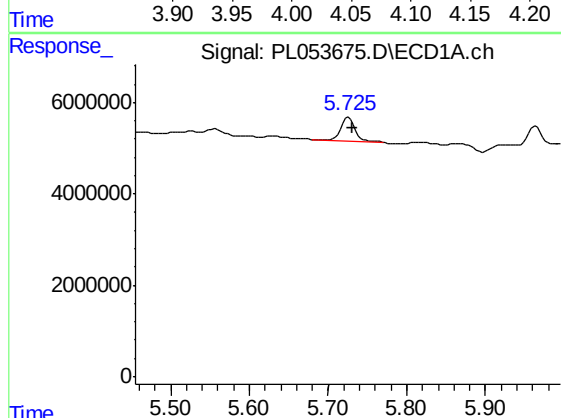


#12 4,4'-DDE

R.T.: 5.726 min
Delta R.T.: -0.004 min
Response: 6501621
Conc: 0.55 ng/ml

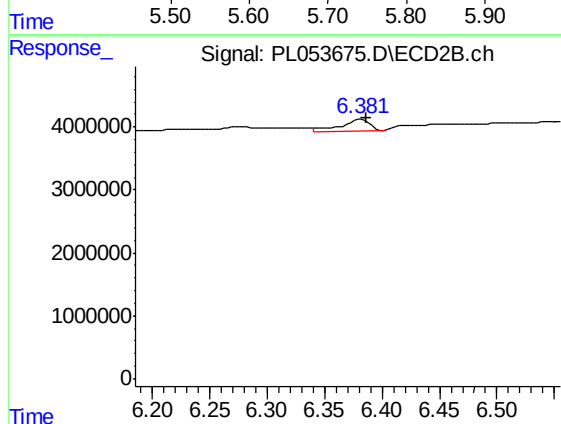

#12 4,4'-DDE

R.T.: 6.383 min
Delta R.T.: -0.004 min
Response: 3271830
Conc: 1.16 ng/ml

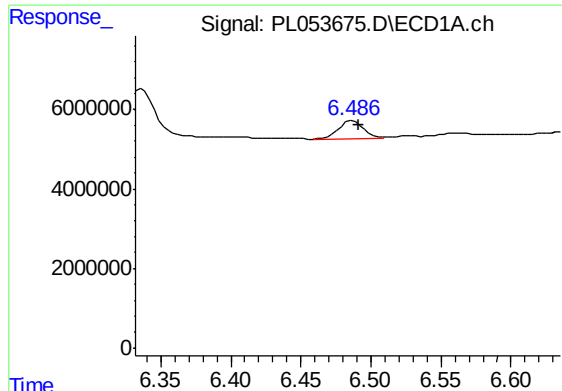


#17 4,4'-DDT

R.T.: 6.486 min
Delta R.T.: -0.006 min
Response: 5211760
Conc: 0.53 ng/ml m

Instrument :
ECD_L
ClientSampleId :
HD-02-102319


Manual Integrations
APPROVED

Ankita
10/25/2019 12:12:44 PM

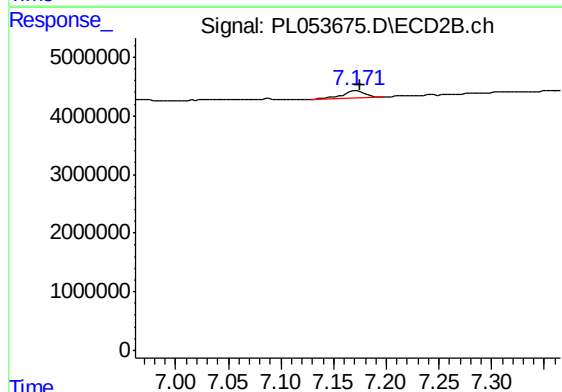


#17 4,4'-DDT

R.T.: 7.171 min
Delta R.T.: -0.005 min
Response: 1685901
Conc: 0.73 ng/ml m

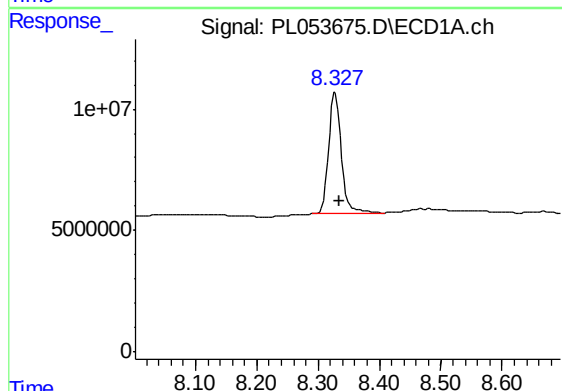

#28 Decachlorobiphenyl

R.T.: 8.328 min
Delta R.T.: -0.006 min
Response: 72319722
Conc: 7.37 ng/ml

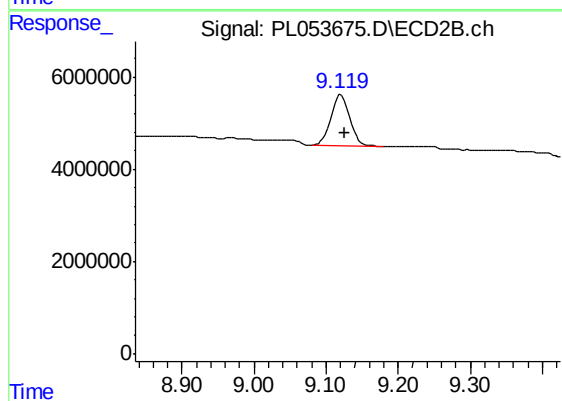

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 19980129
Conc: 7.10 ng/ml