

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102419\
 Data File : PL053718.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2019 23:14
 Operator : SG\AJ
 Sample : K5502-11
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 179-18-(0-2.1)

Manual Integrations
 APPROVED

Ankita
 10/25/2019 12:14:21 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 04:53:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.044	114.0E6	26920752	10.519	10.758
28)	SA Decachlor...	8.326	9.120	71692577	20678271	7.307	7.343
Target Compounds							
17)	MA 4,4'-DDT	6.484	7.171	7542345	1991058	0.761	0.861m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102419\
Data File : PL053718.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2019 23:14
Operator : SG\AJ
Sample : K5502-11
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
179-18-(0-2.1)


Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:21 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 04:53:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

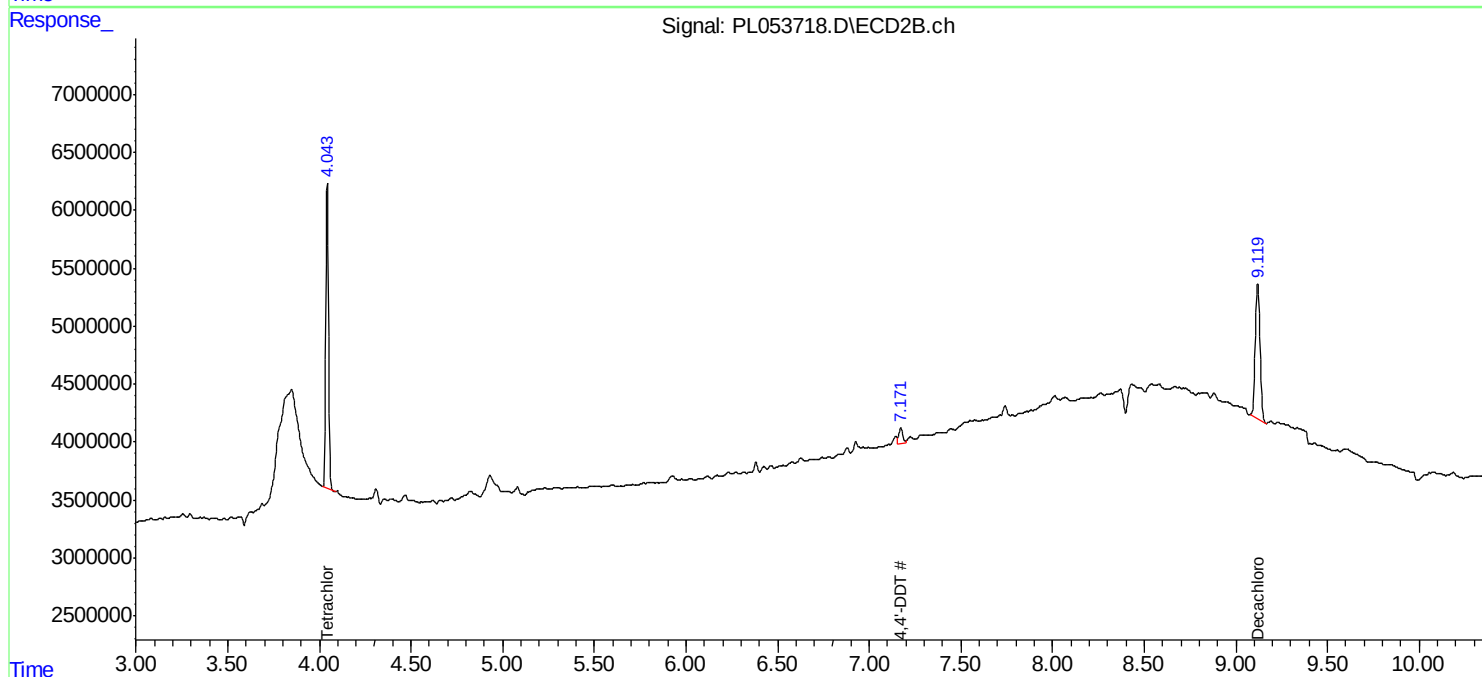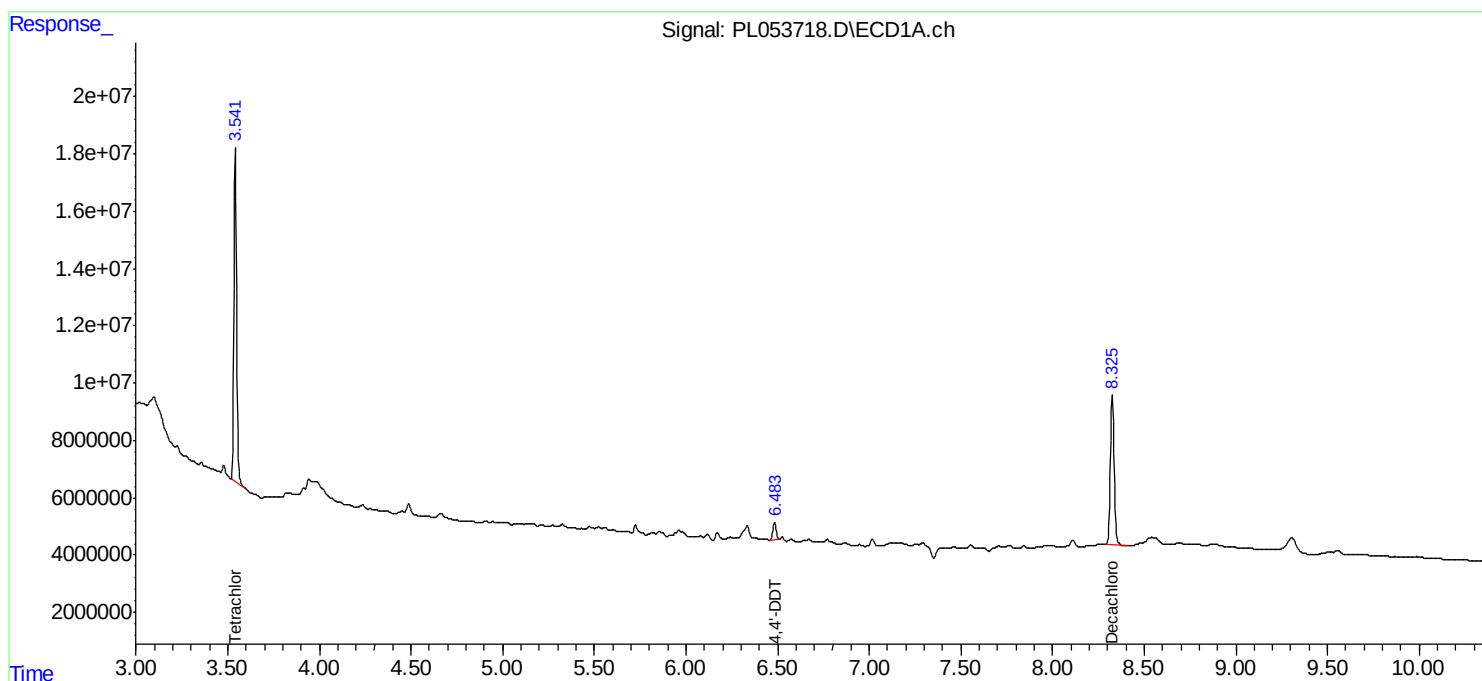

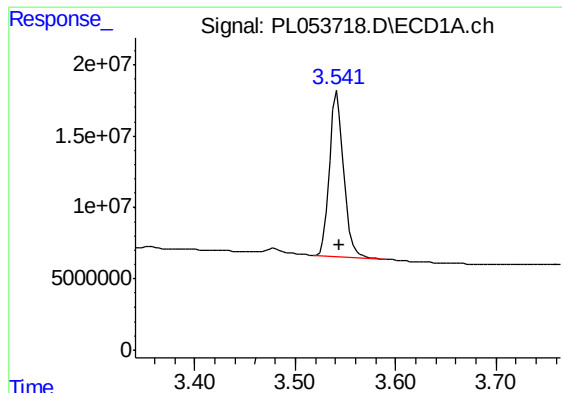


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 114017363
Conc: 10.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
179-18-(0-2.1)


Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:21 PM

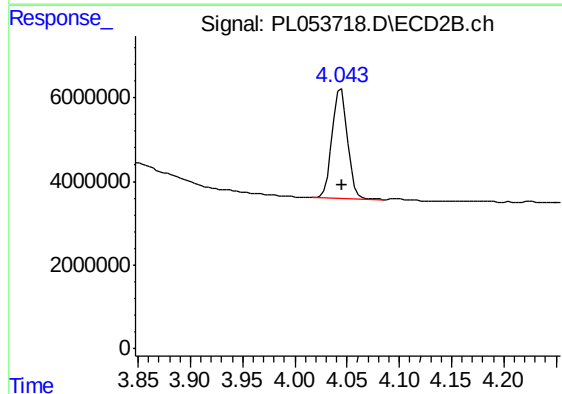


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 26920752
Conc: 10.76 ng/ml

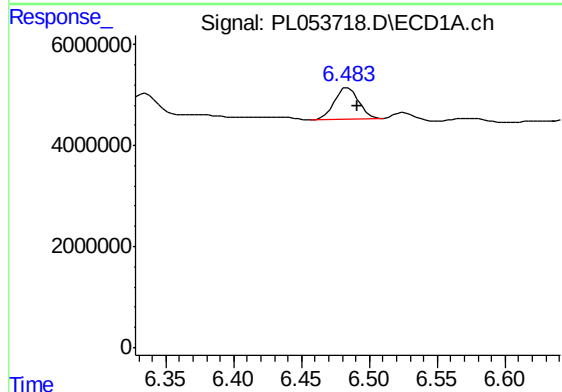


#17 4,4'-DDT

R.T.: 6.484 min
Delta R.T.: -0.007 min
Response: 7542345
Conc: 0.76 ng/ml

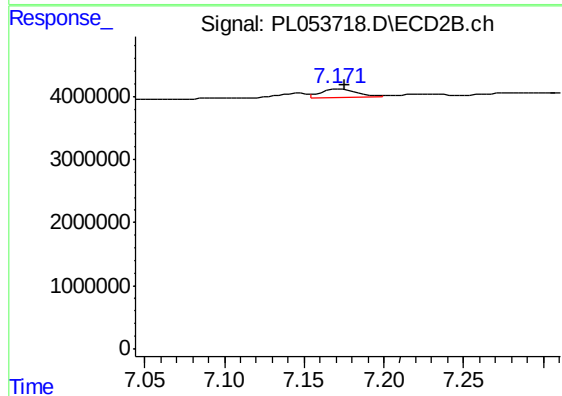

#17 4,4'-DDT

R.T.: 7.171 min
Delta R.T.: -0.005 min
Response: 1991058
Conc: 0.86 ng/ml m

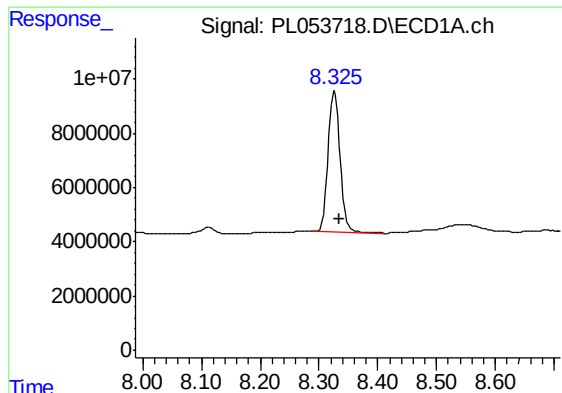


#28 Decachlorobiphenyl

R.T.: 8.326 min
Delta R.T.: -0.008 min
Response: 71692577
Conc: 7.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
179-18-(0-2.1)

Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:21 PM

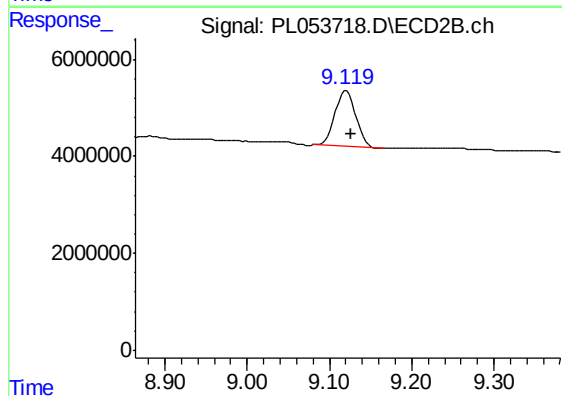

#28 Decachlorobiphenyl

R.T.: 9.120 min
Delta R.T.: -0.006 min
Response: 20678271
Conc: 7.34 ng/ml