

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102419\
 Data File : PL053726.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2019 01:06
 Operator : SG\AJ
 Sample : K5498-01RE 10X
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 189-62-(0-1)RE

Manual Integrations
 APPROVED

Ankita
 10/25/2019 12:14:34 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 05:15:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.044	24007056	6186002	2.215	2.472
28)	SA Decachlor...	8.327	9.118	19678577	5064094	2.006	1.798m
Target Compounds							
17)	MA 4,4'-DDT	6.487	7.172	34402525	10324836	3.473	4.465m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102419\
Data File : PL053726.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 01:06
Operator : SG\AJ
Sample : K5498-01RE 10X
Misc :
ALS Vial : 51 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
189-62-(0-1)RE


Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:34 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 05:15:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

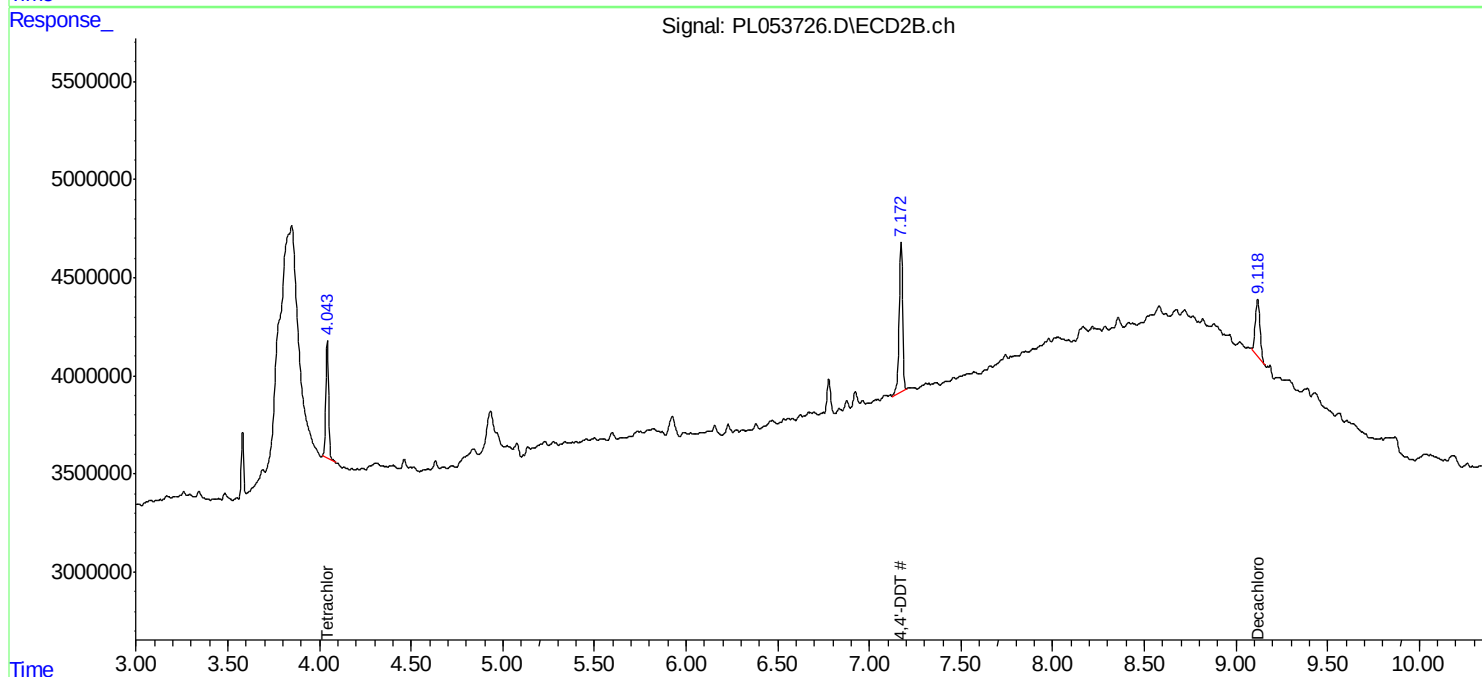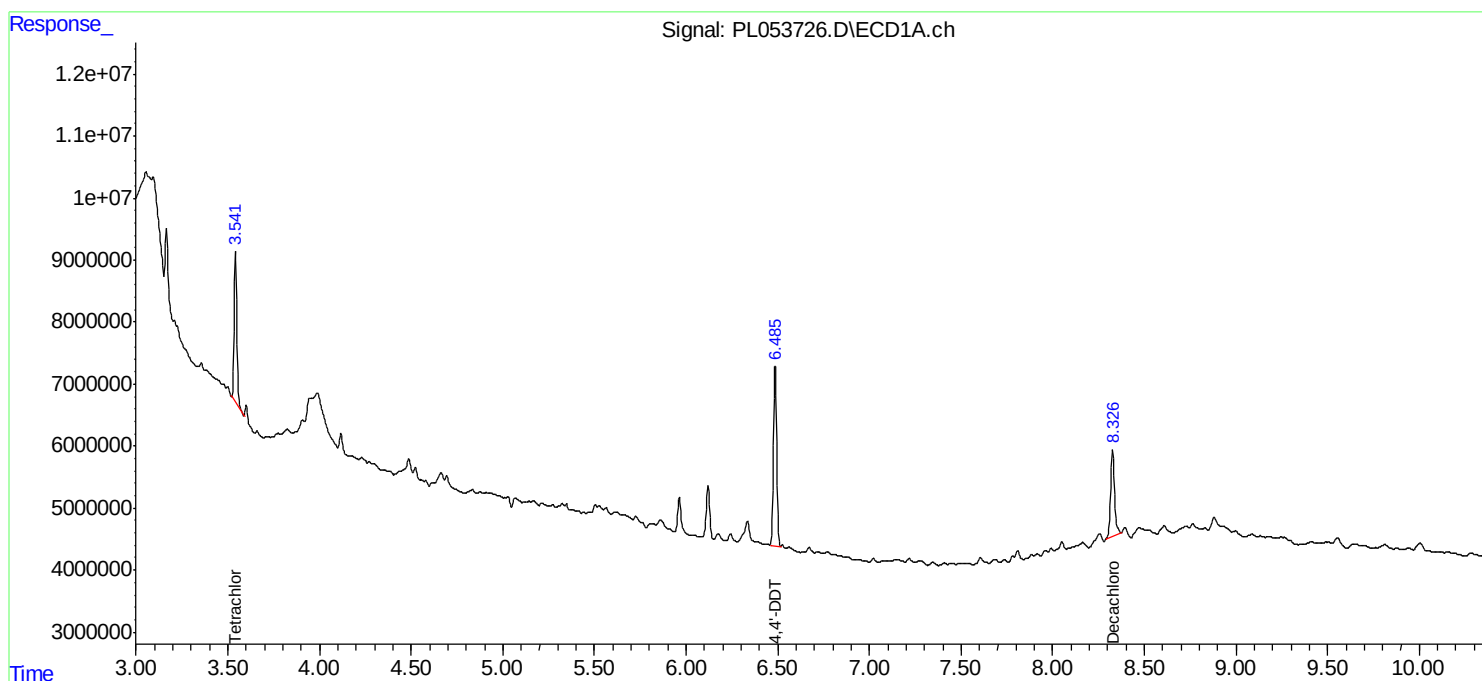

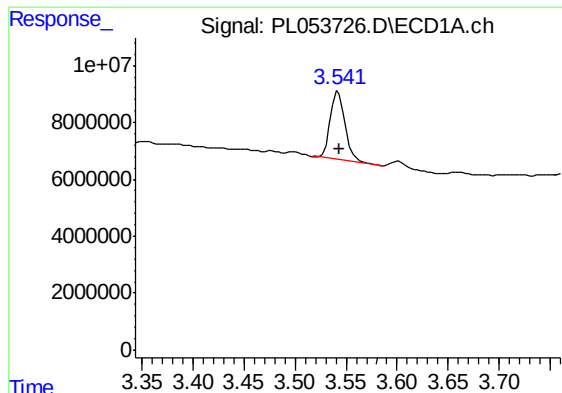


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 24007056
Conc: 2.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
189-62-(0-1)RE


Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:34 PM

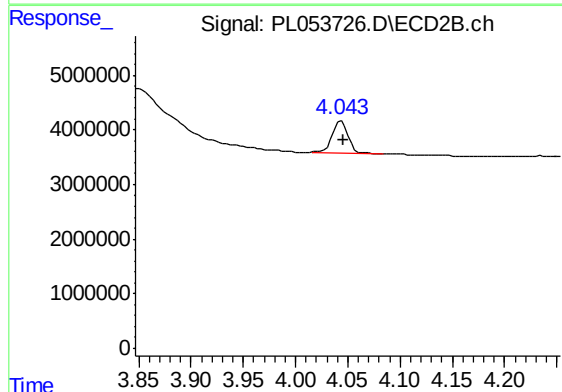


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 6186002
Conc: 2.47 ng/ml

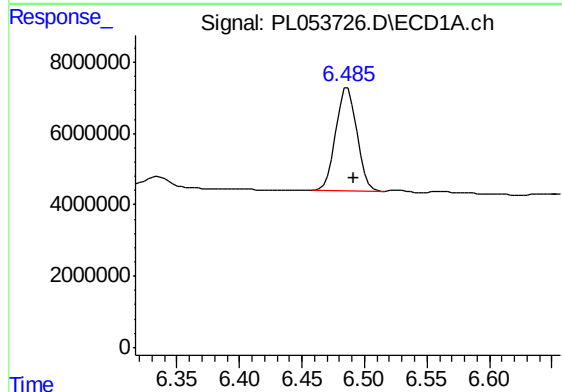


#17 4,4'-DDT

R.T.: 6.487 min
Delta R.T.: -0.005 min
Response: 34402525
Conc: 3.47 ng/ml

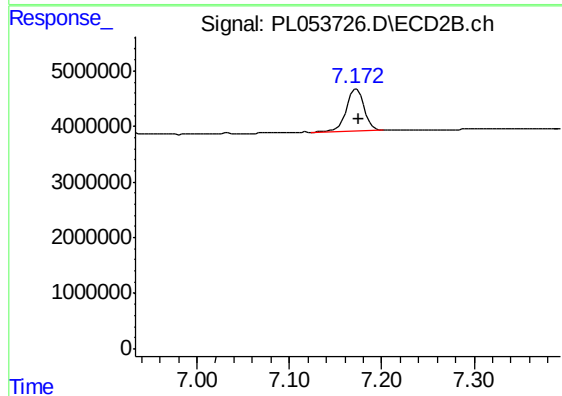

#17 4,4'-DDT

R.T.: 7.172 min
Delta R.T.: -0.004 min
Response: 10324836
Conc: 4.46 ng/ml m

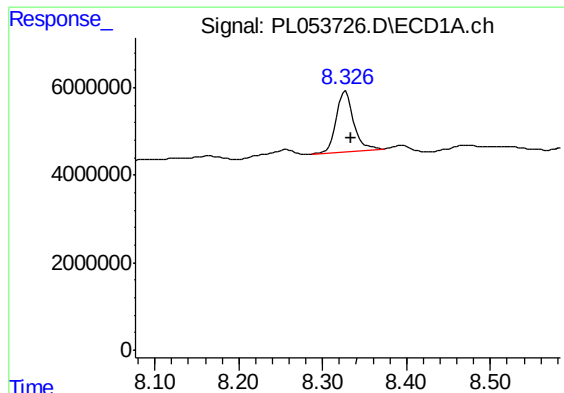


#28 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: -0.007 min
Response: 19678577
Conc: 2.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
189-62-(0-1)RE

Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:34 PM

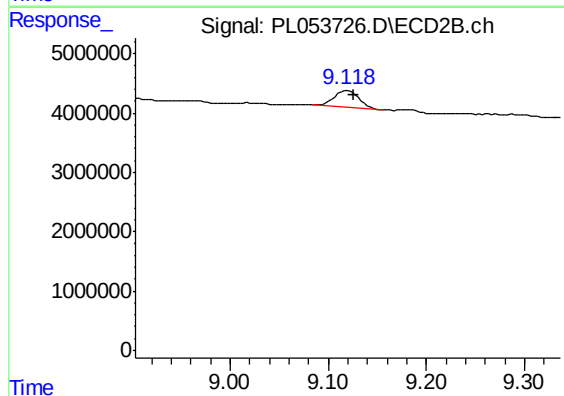

#28 Decachlorobiphenyl

R.T.: 9.118 min
Delta R.T.: -0.008 min
Response: 5064094
Conc: 1.80 ng/ml m