

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102419\
 Data File : PL053730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2019 02:02
 Operator : SG\AJ
 Sample : K5500-07 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 804-00-(0-1.8)

Manual Integrations
 APPROVED

Ankita
 10/25/2019 12:14:42 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 05:15:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	4.044	56645099	13690902	5.226	5.471
28) SA Decachlor...	8.327	9.121	30623626	9817922	3.121	3.486
Target Compounds						
17) MA 4,4'-DDT	6.486	7.171	15034040	4884868	1.518	2.112m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102419\
Data File : PL053730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 02:02
Operator : SG\AJ
Sample : K5500-07 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1


Instrument :
ECD_L
ClientSampleId :
804-00-(0-1.8)


Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:42 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 05:15:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

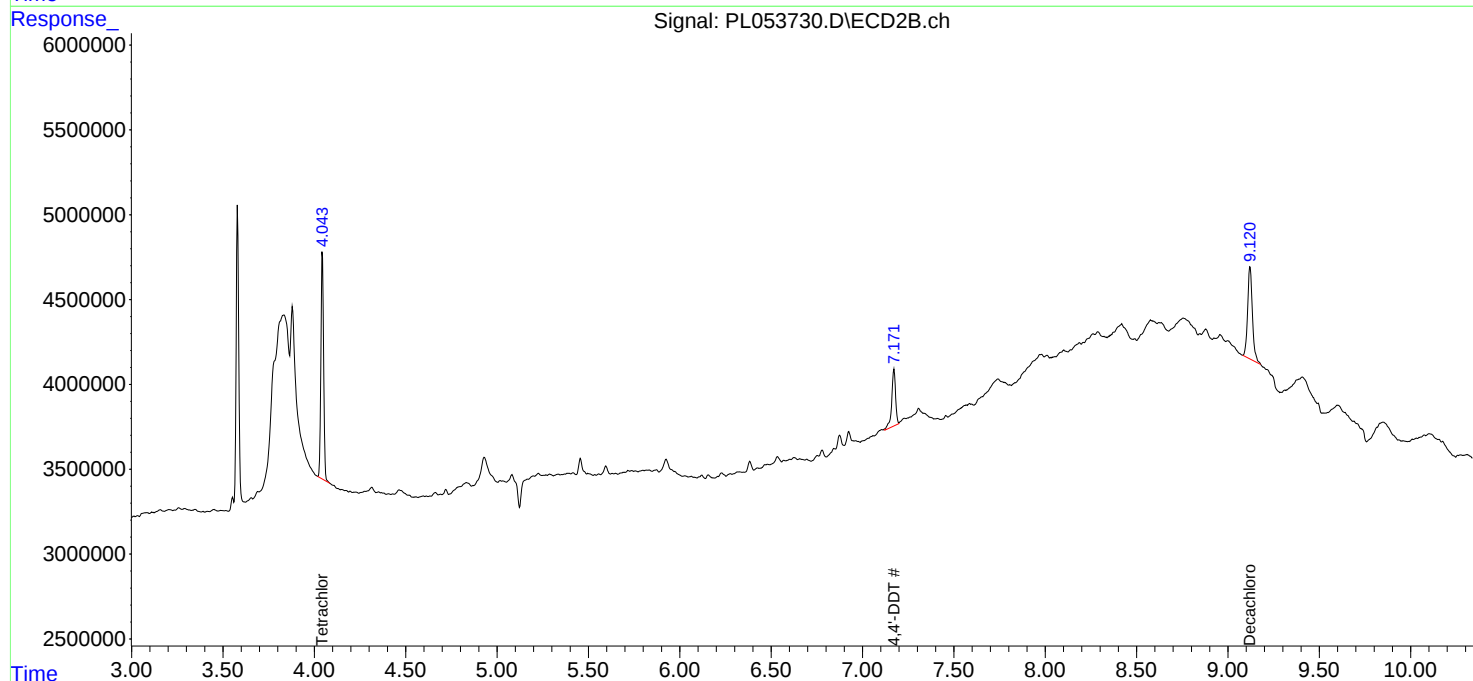

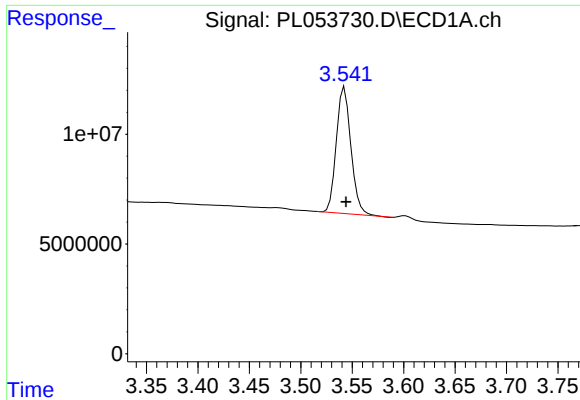


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 56645099
Conc: 5.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
804-00-(0-1.8)


Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:42 PM

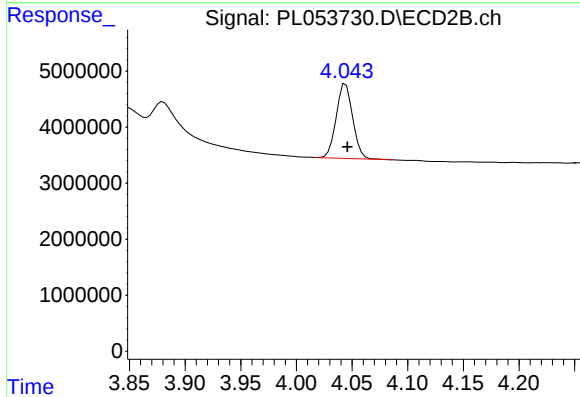


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.002 min
Response: 13690902
Conc: 5.47 ng/ml

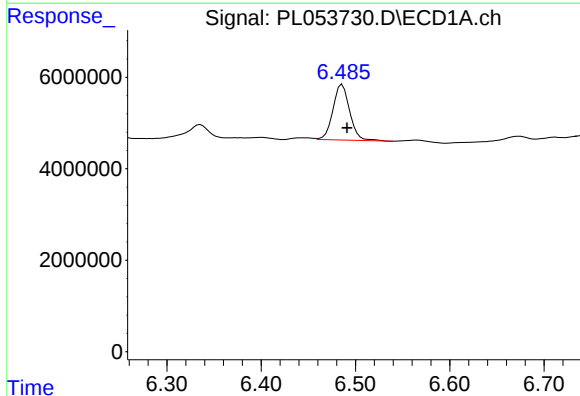


#17 4,4'-DDT

R.T.: 6.486 min
Delta R.T.: -0.005 min
Response: 15034040
Conc: 1.52 ng/ml

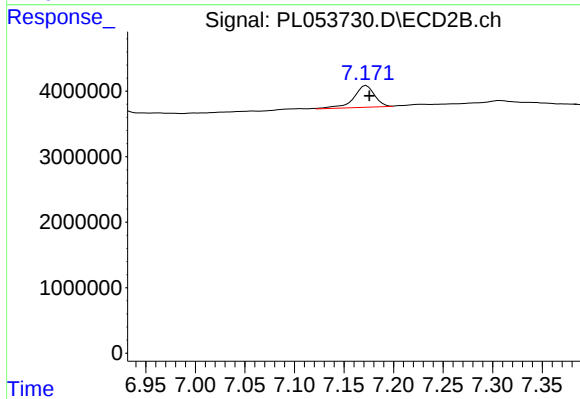

#17 4,4'-DDT

R.T.: 7.171 min
Delta R.T.: -0.004 min
Response: 4884868
Conc: 2.11 ng/ml m

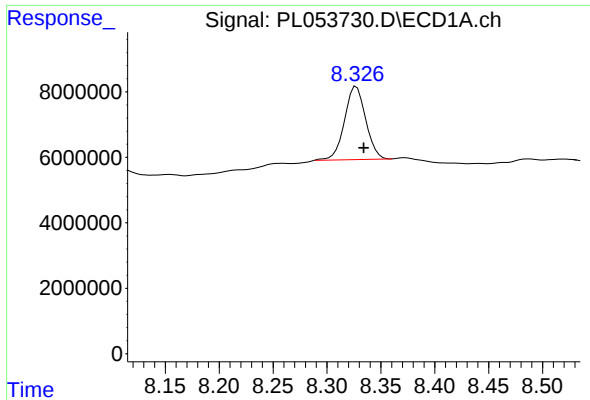


#28 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: -0.007 min
Response: 30623626
Conc: 3.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
804-00-(0-1.8)

Manual Integrations
APPROVED

Ankita
10/25/2019 12:14:42 PM

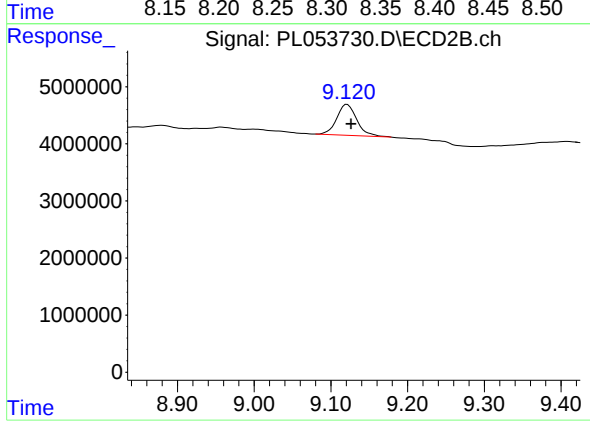

#28 Decachlorobiphenyl

R.T.: 9.121 min
Delta R.T.: -0.005 min
Response: 9817922
Conc: 3.49 ng/ml