

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102422\
 Data File : PL078492.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2022 18:55
 Operator : AR\AJ
 Sample : PB148508BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 22:39:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 21 07:08:41 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.323	2.572	31668612	44220240	16.606	17.320
28)	SA Decachlor...	8.773	7.641	26501869	35713070	17.617	18.855
Target Compounds							
8)	B Heptachlo...	5.469	0.000	297258	0	0.140	N.D. #
9)	A Endosulfan I	5.860f	4.860f	1212268	87828	0.568	0.031 #
10)	B gamma-Chl...	5.723	0.000	171567	0	0.076	N.D. #
11)	B alpha-Chl...	5.791	0.000	269995	0	0.117	N.D. #
13)	MA Dieldrin	6.150f	0.000	108392	0	0.050	N.D. #
14)	MA Endrin	6.339	5.398f	375336	353944	0.198	0.136 #
15)	B Endosulfa...	6.559f	5.643f	1340470	770066	0.714	0.338 #
17)	MA 4,4'-DDT	6.830f	0.000	345363	0	0.193	N.D. #
25)	Chlordane-3	5.723	0.000	171567	0	0.514	N.D. #
26)	Chlordane-4	5.791	0.000	269995	0	0.658	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102422\
Data File : PL078492.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2022 18:55
Operator : AR\AJ
Sample : PB148508BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 22:39:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102122.M
Quant Title : GC Extractables
QLast Update : Fri Oct 21 07:08:41 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

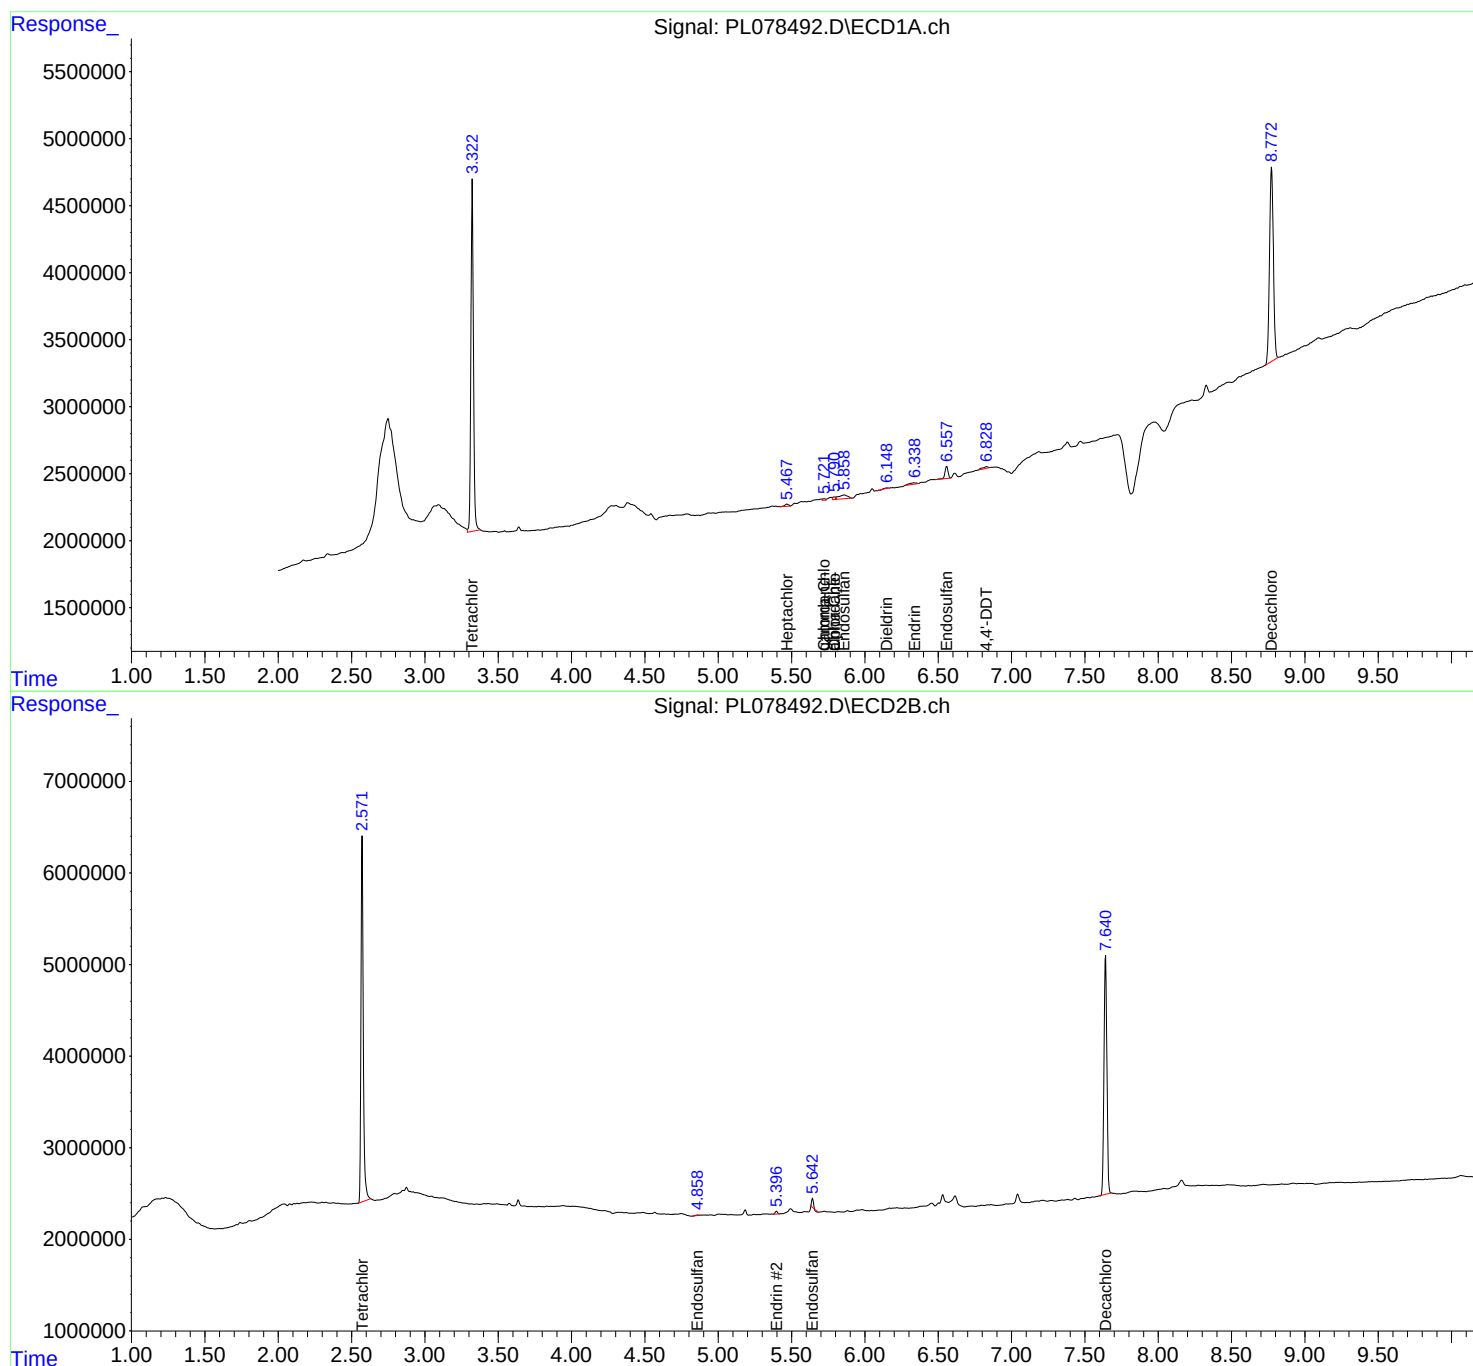


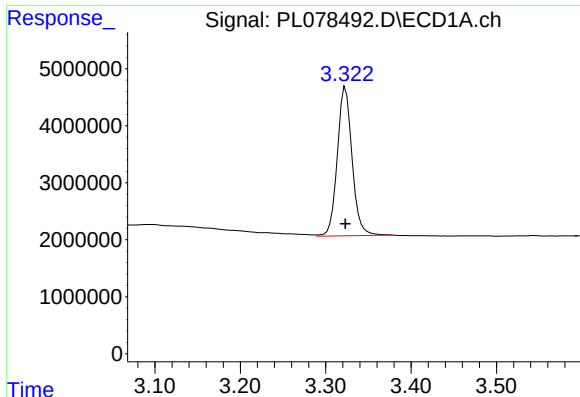

#1 Tetrachloro-m-xylene


R.T.: 3.323 min
Delta R.T.: 0.000 min
Response: 31668612
Conc: 16.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

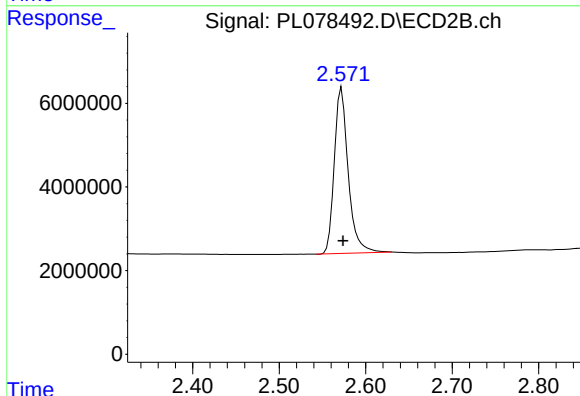


#1 Tetrachloro-m-xylene

R.T.: 2.572 min
Delta R.T.: -0.001 min
Response: 44220240
Conc: 17.32 ng/ml

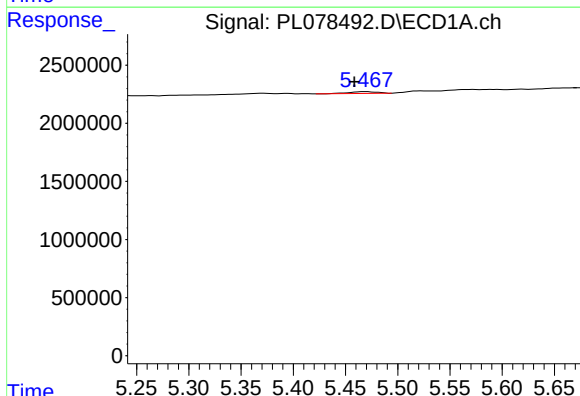


#8 Heptachlor epoxide

R.T.: 5.469 min
Delta R.T.: 0.010 min
Response: 297258
Conc: 0.14 ng/ml

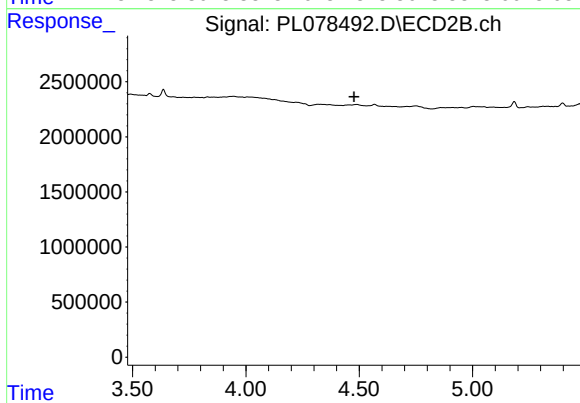

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 4.477 min
Response: 0
Conc: N.D.

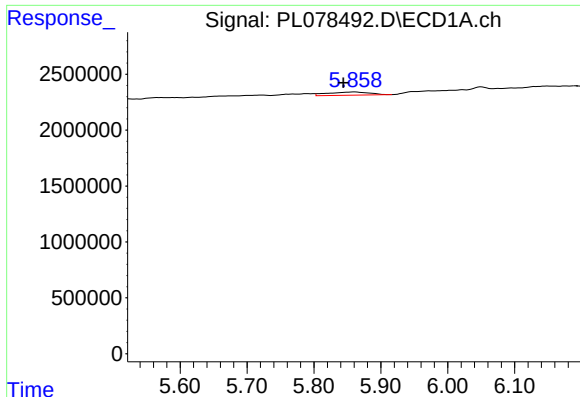

#9 Endosulfan I


R.T.: 5.860 min
Delta R.T.: 0.016 min
Response: 1212268
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :

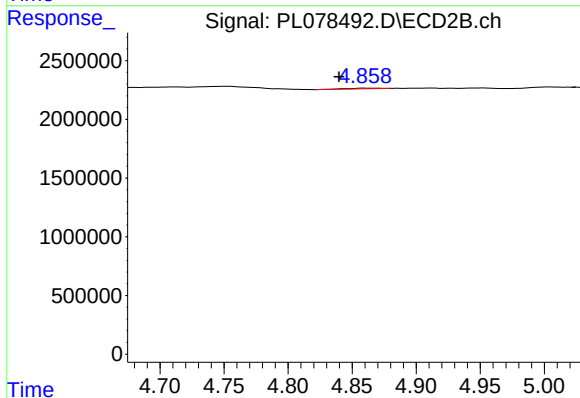


#9 Endosulfan I

R.T.: 4.860 min
Delta R.T.: 0.020 min
Response: 87828
Conc: 0.03 ng/ml

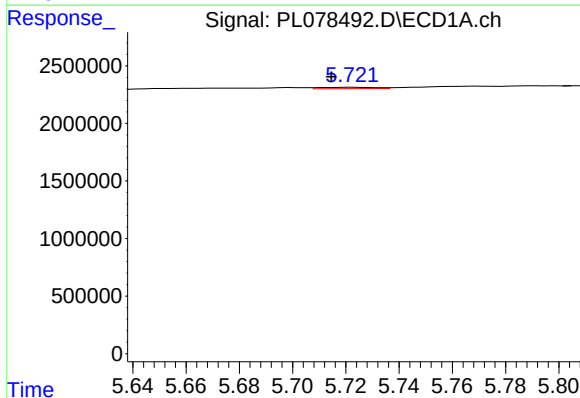


#10 gamma-Chlordane

R.T.: 5.723 min
Delta R.T.: 0.008 min
Response: 171567
Conc: 0.08 ng/ml

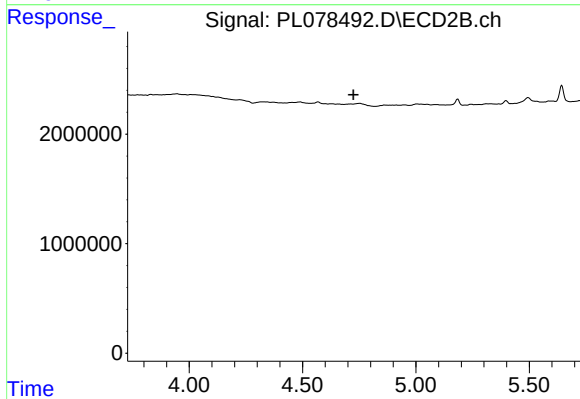

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 4.725 min
Response: 0
Conc: N.D.

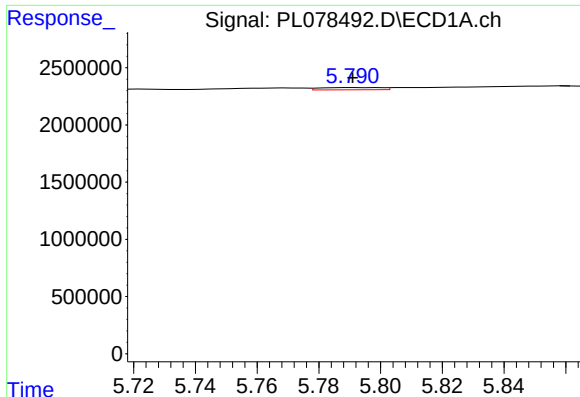

#11 alpha-Chlordane


R.T.: 5.791 min
Delta R.T.: 0.000 min
Response: 269995
Conc: 0.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

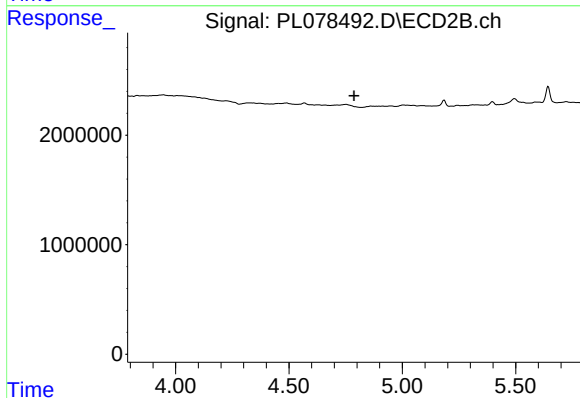


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T. : 4.787 min
Response: 0
Conc: N.D.

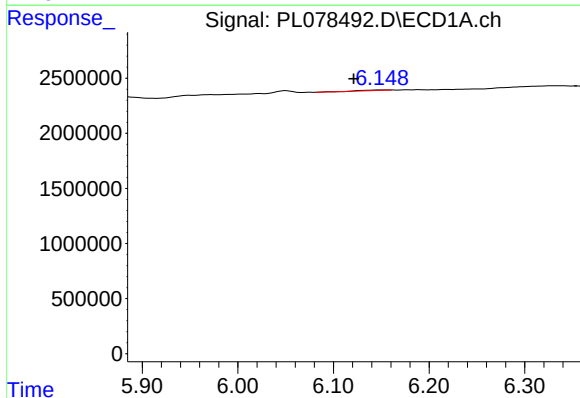


#13 Dieldrin

R.T.: 6.150 min
Delta R.T.: 0.029 min
Response: 108392
Conc: 0.05 ng/ml

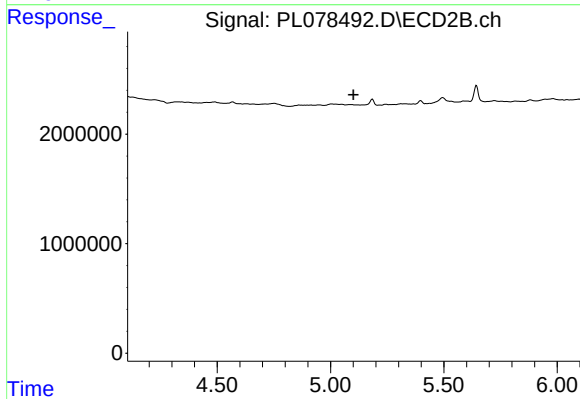

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 5.102 min
Response: 0
Conc: N.D.

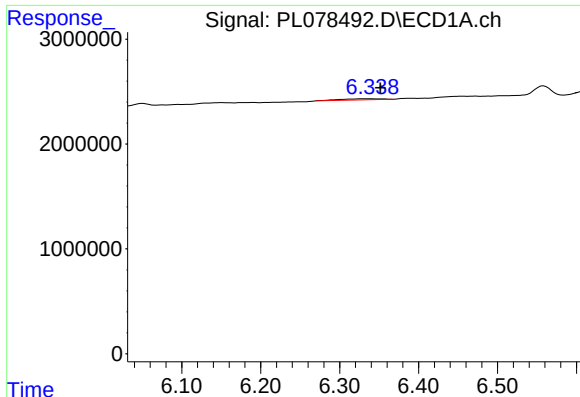

#14 Endrin


R.T.: 6.339 min
Delta R.T.: -0.012 min
Response: 375336
Conc: 0.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

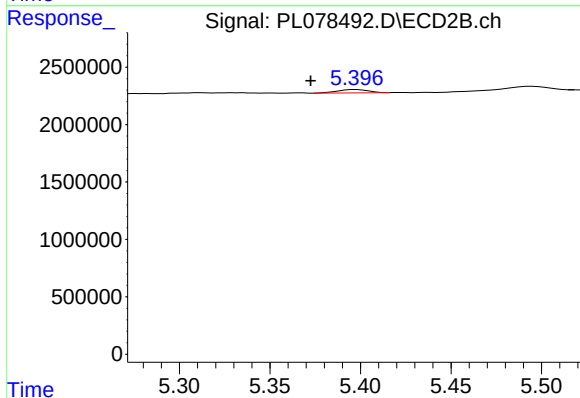


#14 Endrin

R.T.: 5.398 min
Delta R.T.: 0.025 min
Response: 353944
Conc: 0.14 ng/ml

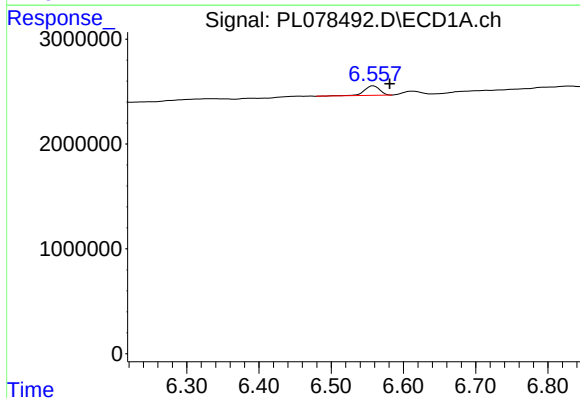


#15 Endosulfan II

R.T.: 6.559 min
Delta R.T.: -0.023 min
Response: 1340470
Conc: 0.71 ng/ml

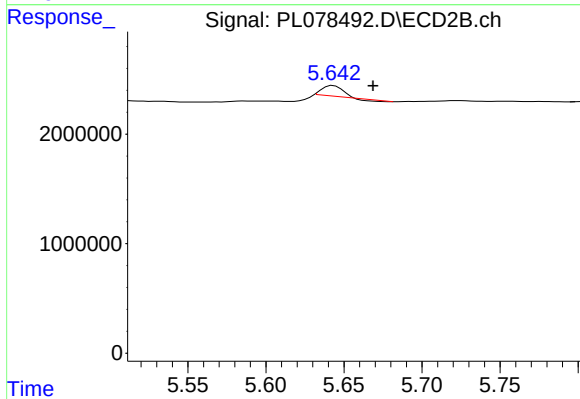

#15 Endosulfan II


R.T.: 5.643 min
Delta R.T.: -0.025 min
Response: 770066
Conc: 0.34 ng/ml

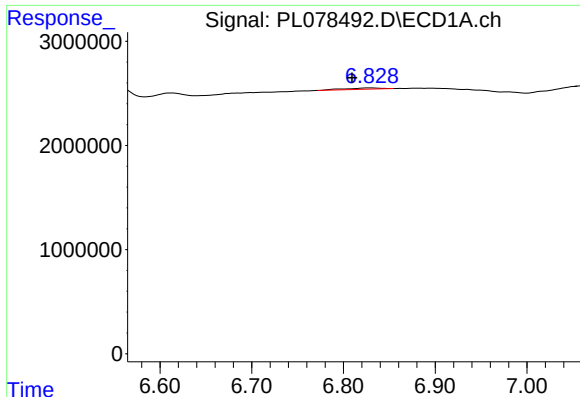

#17 4,4'-DDT


R.T.: 6.830 min
Delta R.T.: 0.021 min
Response: 345363
Conc: 0.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

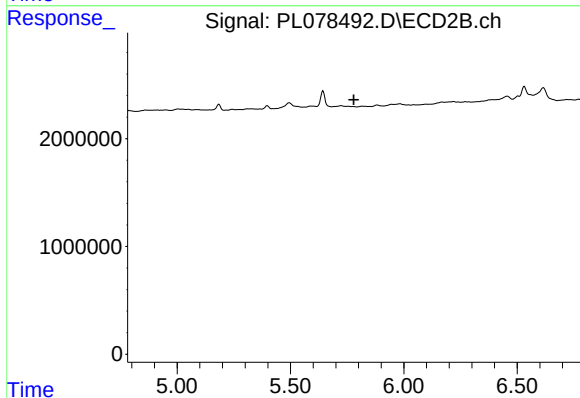


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 5.779 min
Response: 0
Conc: N.D.

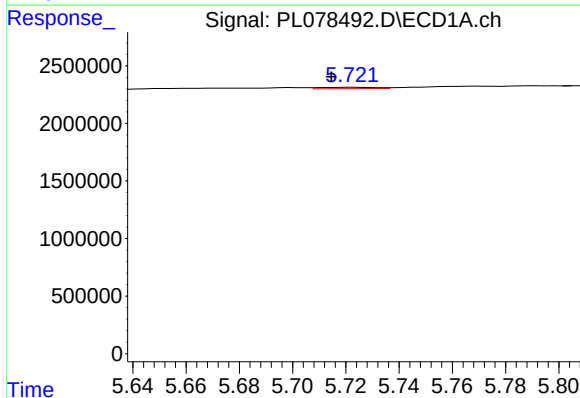


#25 Chlordane-3

R.T.: 5.723 min
Delta R.T.: 0.008 min
Response: 171567
Conc: 0.51 ng/ml

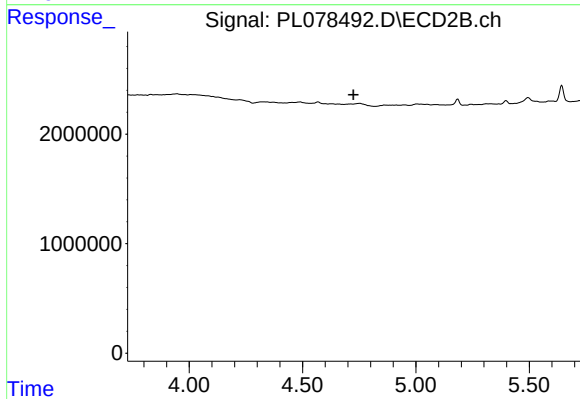

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 4.725 min
Response: 0
Conc: N.D.

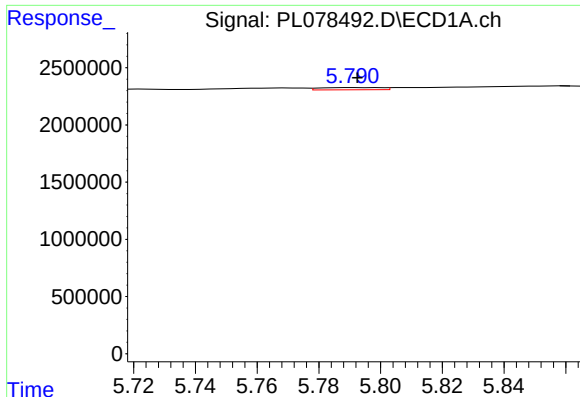

#26 Chlordane-4


R.T.: 5.791 min
Delta R.T.: -0.001 min
Response: 269995
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

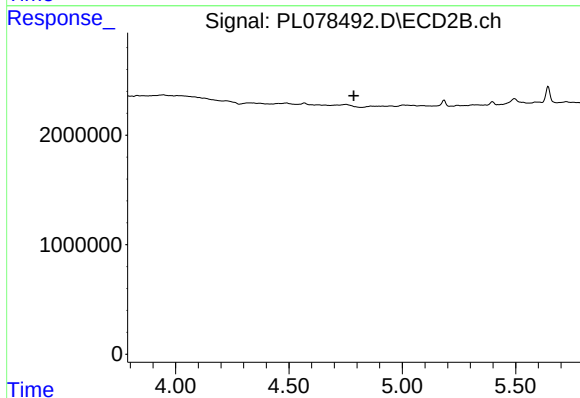


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 4.785 min
Response: 0
Conc: N.D.

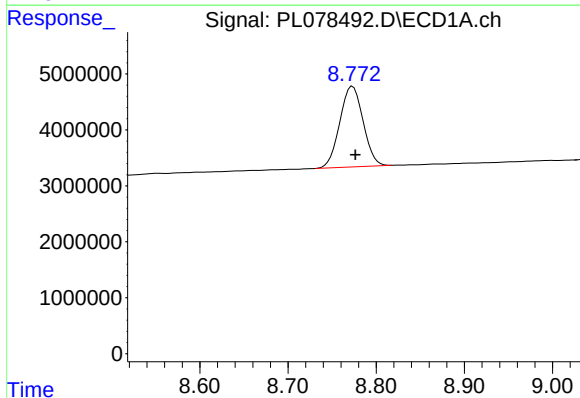

#28 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: -0.003 min
Response: 26501869
Conc: 17.62 ng/ml

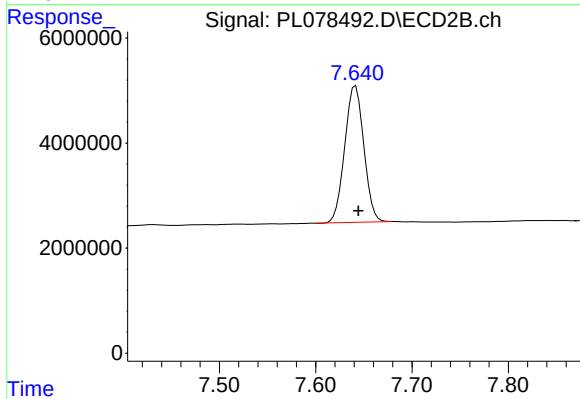

#28 Decachlorobiphenyl

R.T.: 7.641 min
Delta R.T.: -0.003 min
Response: 35713070
Conc: 18.85 ng/ml