

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102423\
 Data File : PL086101.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 09:43
 Operator : AR\AJ
 Sample : 04976-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-426-COMP-01

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/25/2023
 Supervised By : Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 11:59:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.355	2.622	61369062	18792441	20.634m	20.118
28)	SA Decachlor...	8.854	7.771	57928185	24564671	26.596	26.614
Target Compounds							
20)	A Methoxychlor	7.337	6.470	4386858	1084691	3.141	2.062 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102423\
Data File : PL086101.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 09:43
Operator : AR\AJ
Sample : 04976-03
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-426-COMP-01


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/25/2023
Supervised By : Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 11:59:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

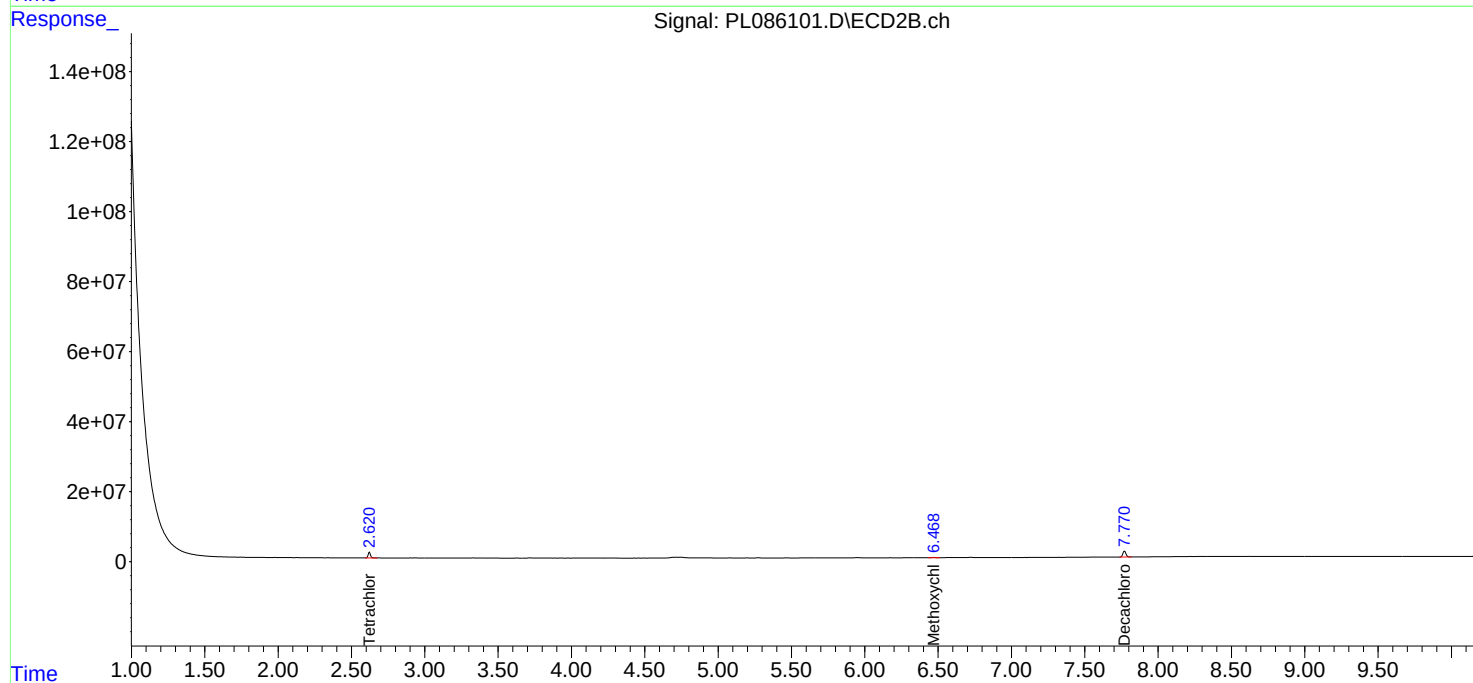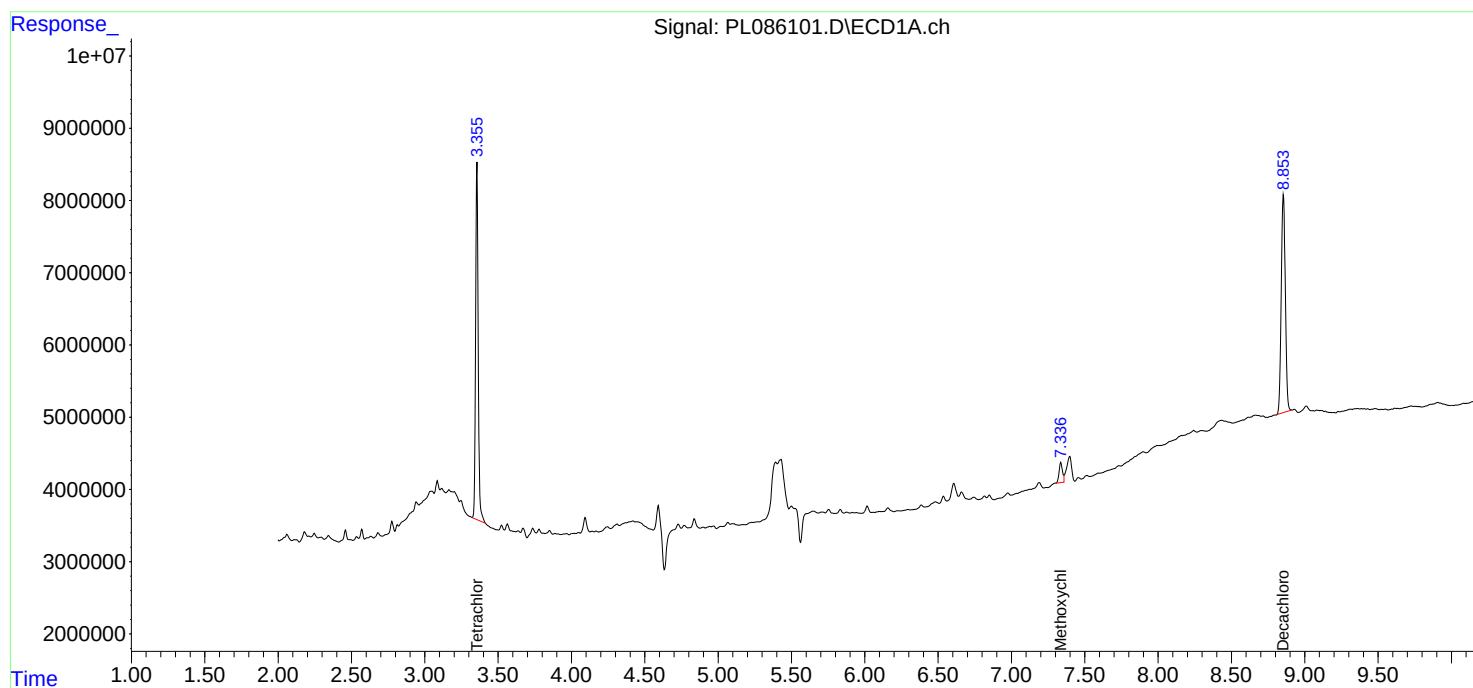

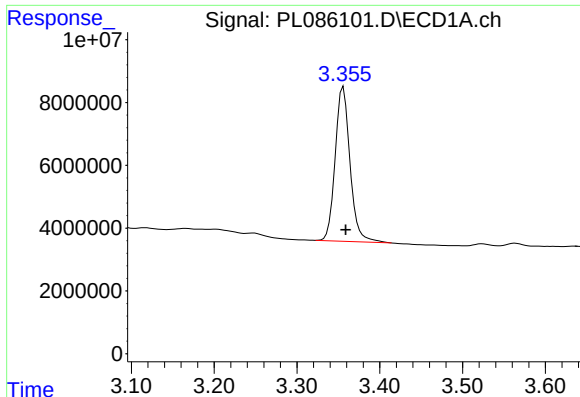


#1 Tetrachloro-m-xylene

R.T.: 3.355 min
Delta R.T.: -0.004 min
Response: 61369062
Conc: 20.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-426-COMP-01


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

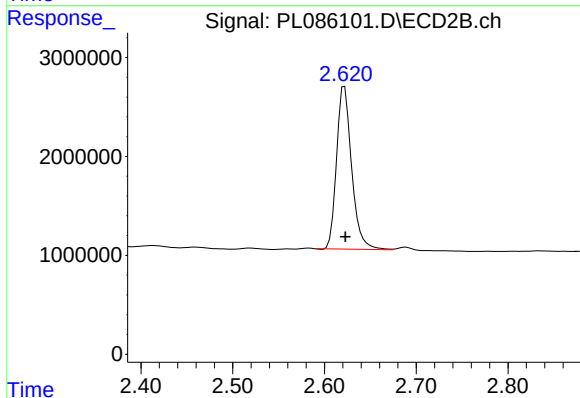


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: 0.000 min
Response: 18792441
Conc: 20.12 ng/ml

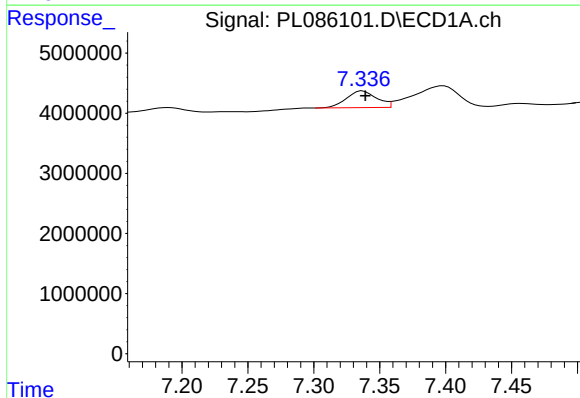


#20 Methoxychlor

R.T.: 7.337 min
Delta R.T.: -0.002 min
Response: 4386858
Conc: 3.14 ng/ml

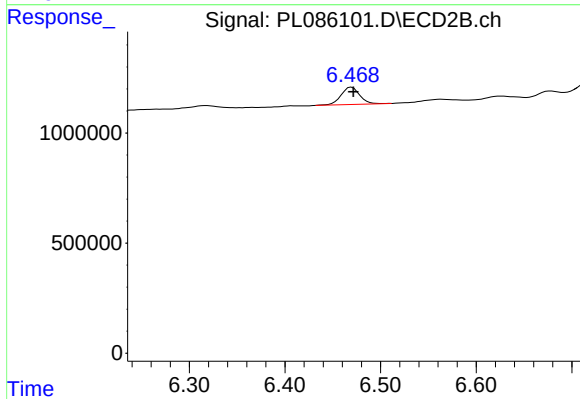

#20 Methoxychlor

R.T.: 6.470 min
Delta R.T.: -0.002 min
Response: 1084691
Conc: 2.06 ng/ml

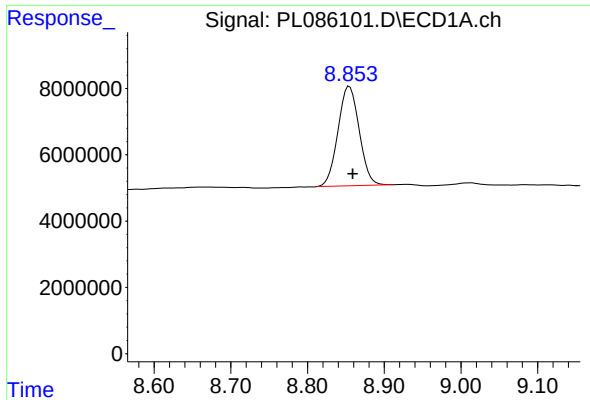


#28 Decachlorobiphenyl

R.T.: 8.854 min
Delta R.T.: -0.004 min
Response: 57928185
Conc: 26.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-426-COMP-01

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

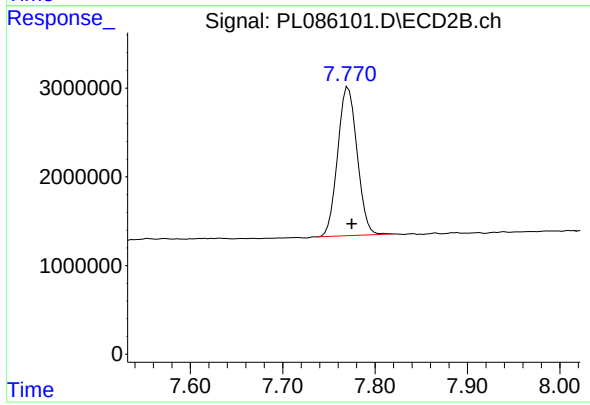

#28 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: -0.004 min
Response: 24564671
Conc: 26.61 ng/ml