

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102423\
 Data File : PL086104.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 10:25
 Operator : AR\AJ
 Sample : 04977-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-406-COMP-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 11:05:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.355	2.621	60676670	18159905	20.401	19.441
28)	SA Decachlor...	8.852	7.771	51764667	22250516	23.766	24.107

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102423\
Data File : PL086104.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 10:25
Operator : AR\AJ
Sample : 04977-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
NB-406-COMP-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 11:05:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

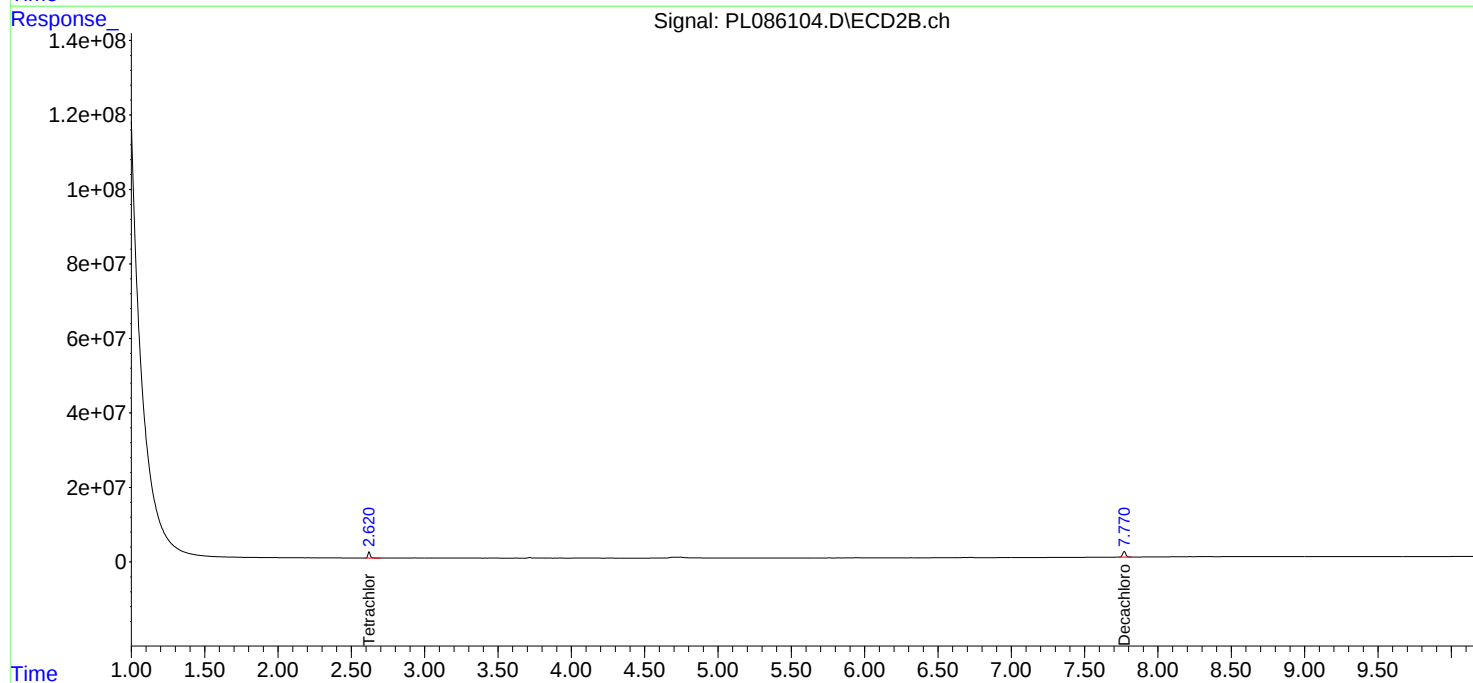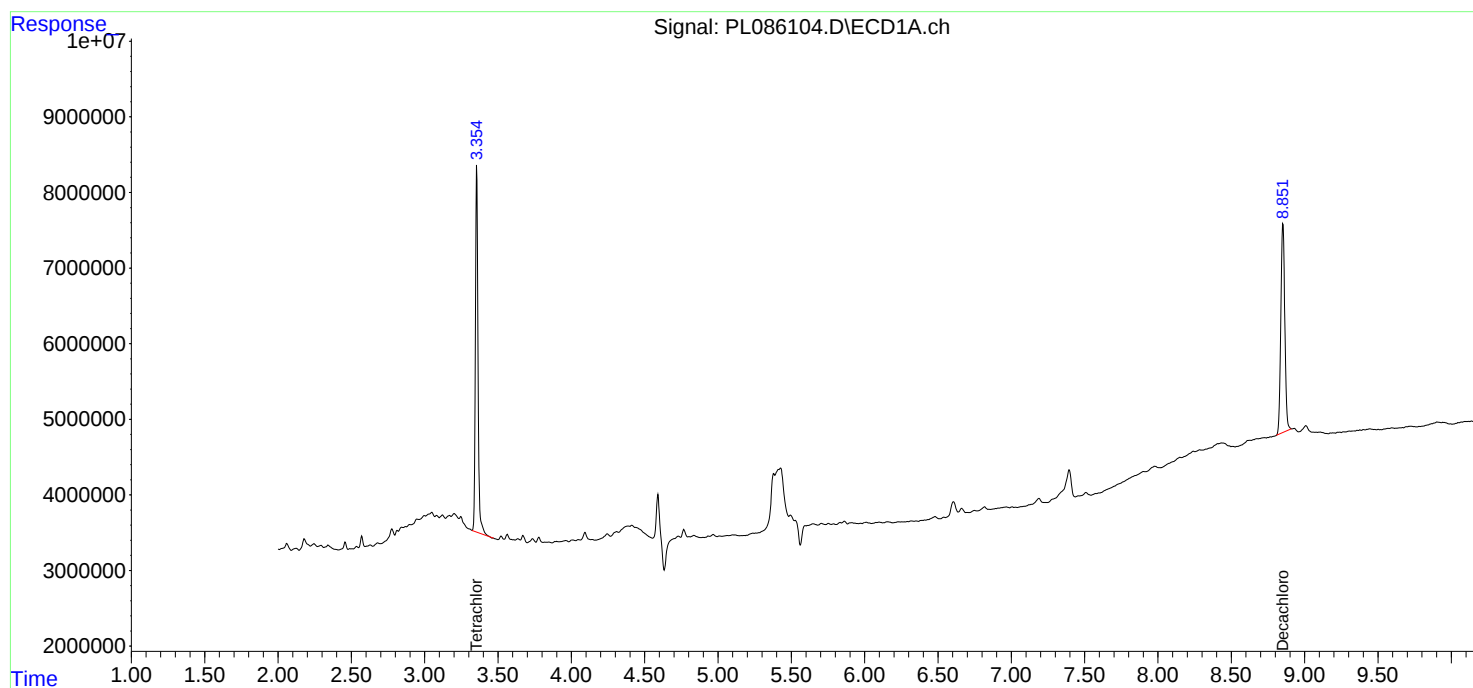


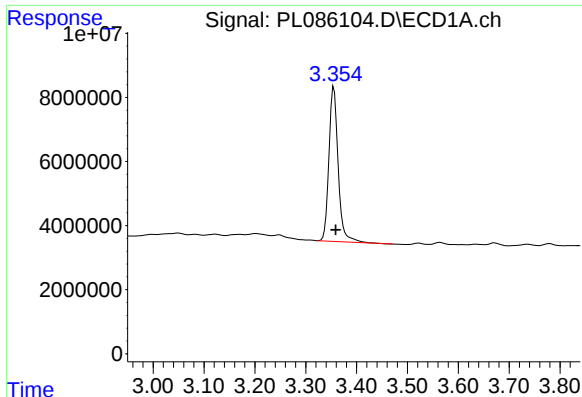

#1 Tetrachloro-m-xylene


R.T.: 3.355 min
Delta R.T.: -0.004 min
Response: 60676670
Conc: 20.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-406-COMP-01

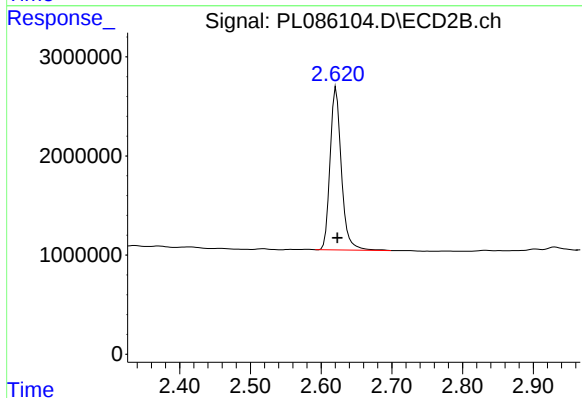


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.001 min
Response: 18159905
Conc: 19.44 ng/ml

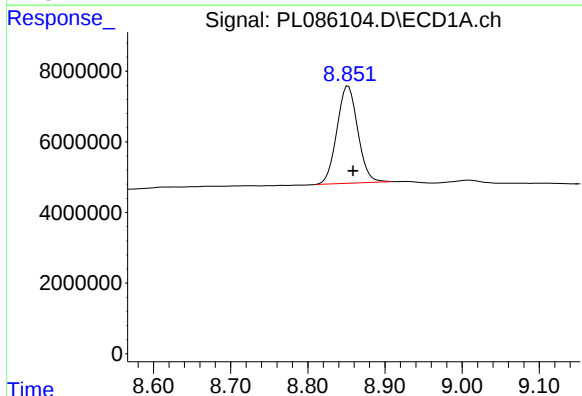

#28 Decachlorobiphenyl

R.T.: 8.852 min
Delta R.T.: -0.006 min
Response: 51764667
Conc: 23.77 ng/ml

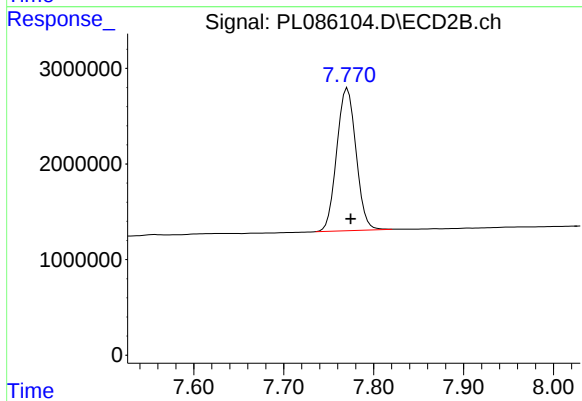

#28 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: -0.004 min
Response: 22250516
Conc: 24.11 ng/ml