

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102423\
 Data File : PL086118.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 13:38
 Operator : AR\AJ
 Sample : 05005-03
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N-2(5-10)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/25/2023
 Supervised By : Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 21:19:18 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.355	2.622	48712060	16159085	16.378	17.299
28)	SA Decachlor...	8.851	7.769	11391576	12453363	5.230m	13.492m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102423\
Data File : PL086118.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 13:38
Operator : AR\AJ
Sample : 05005-03
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
N-2(5-10)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 21:19:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

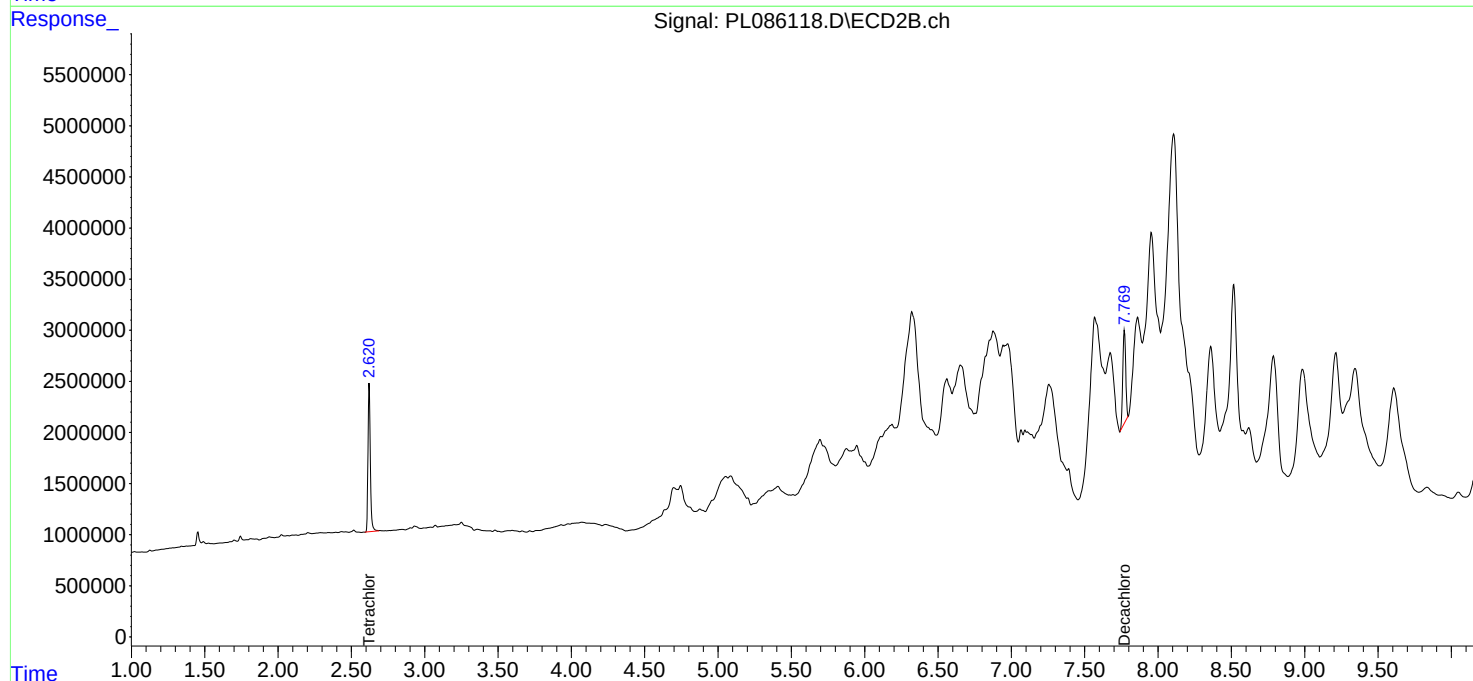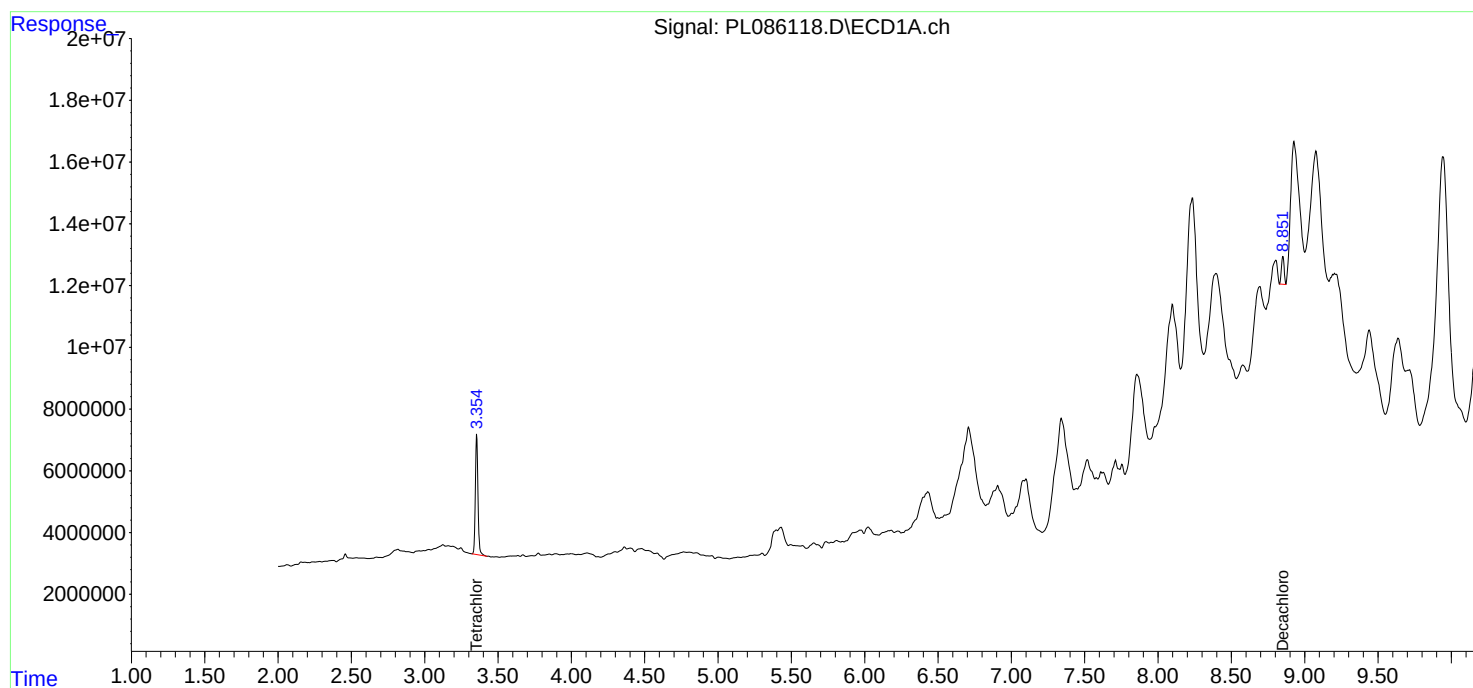

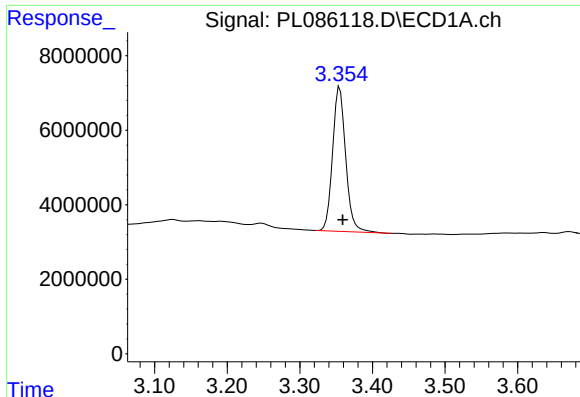


#1 Tetrachloro-m-xylene

R.T.: 3.355 min
Delta R.T.: -0.004 min
Response: 48712060
Conc: 16.38 ng/ml

Instrument :
ECD_L
ClientSampleId :
N-2(5-10)


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

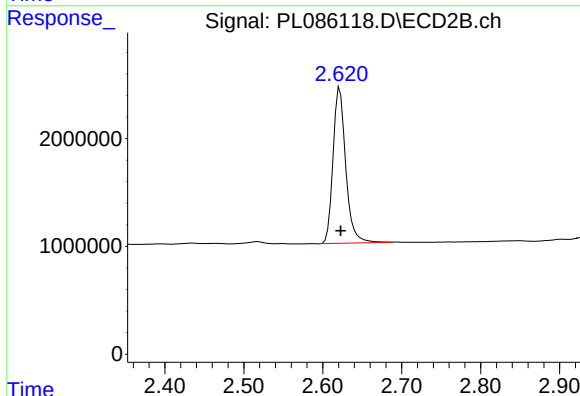


#1 Tetrachloro-m-xylene

R.T.: 2.622 min
Delta R.T.: -0.001 min
Response: 16159085
Conc: 17.30 ng/ml

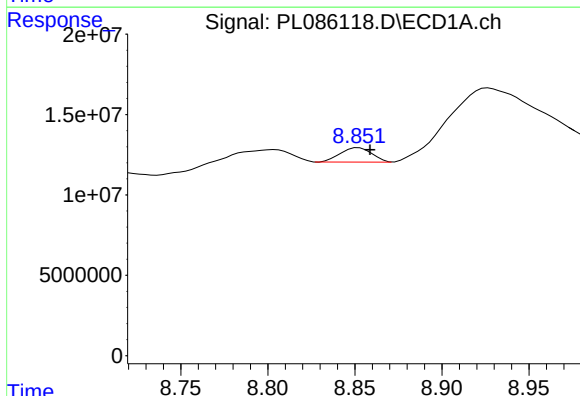

#28 Decachlorobiphenyl

R.T.: 8.851 min
Delta R.T.: -0.008 min
Response: 11391576
Conc: 5.23 ng/ml m

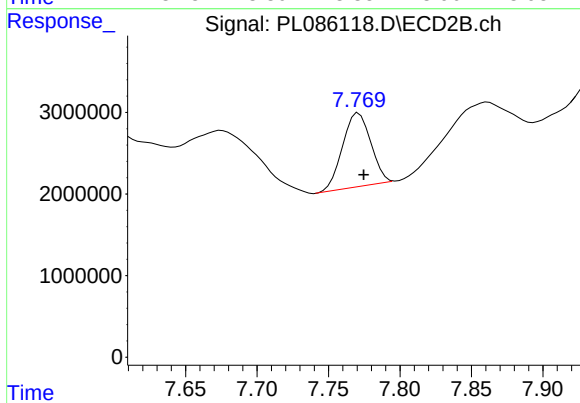

#28 Decachlorobiphenyl

R.T.: 7.769 min
Delta R.T.: -0.005 min
Response: 12453363
Conc: 13.49 ng/ml m