

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102423\
 Data File : PL086128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2023 18:43
 Operator : AR\AJ
 Sample : 05010-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 343

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/25/2023
 Supervised By :Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 24 21:22:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.355	2.621	45788154	15373511	15.395	16.458
28) SA Decachlor...	8.854	7.771	29773625	13355829	13.670	14.470
Target Compounds						
11) B alpha-Chl...	5.837	4.876	4089425	563843	1.197m	0.517m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102423\
Data File : PL086128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2023 18:43
Operator : AR\AJ
Sample : 05010-01
Misc :
ALS Vial : 28 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
343


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/25/2023
Supervised By : Ankita Jodhani 10/25/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 24 21:22:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

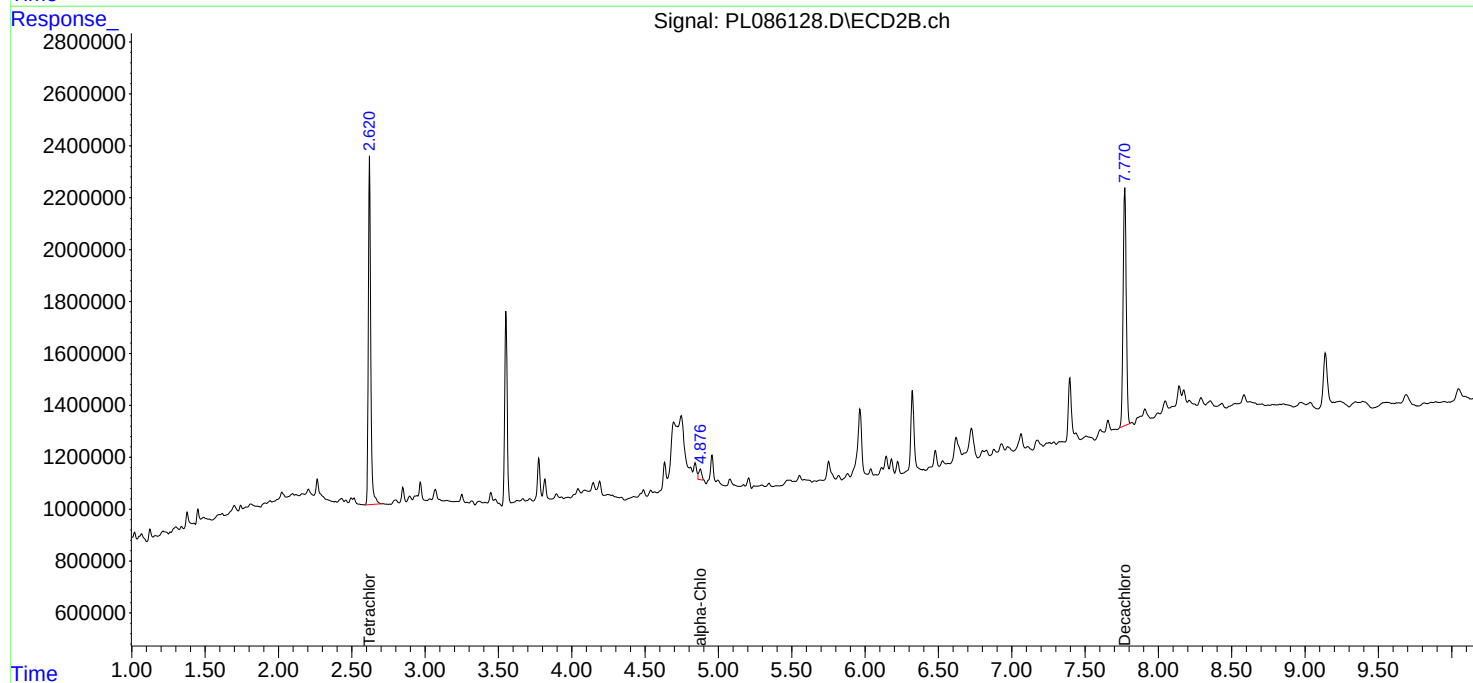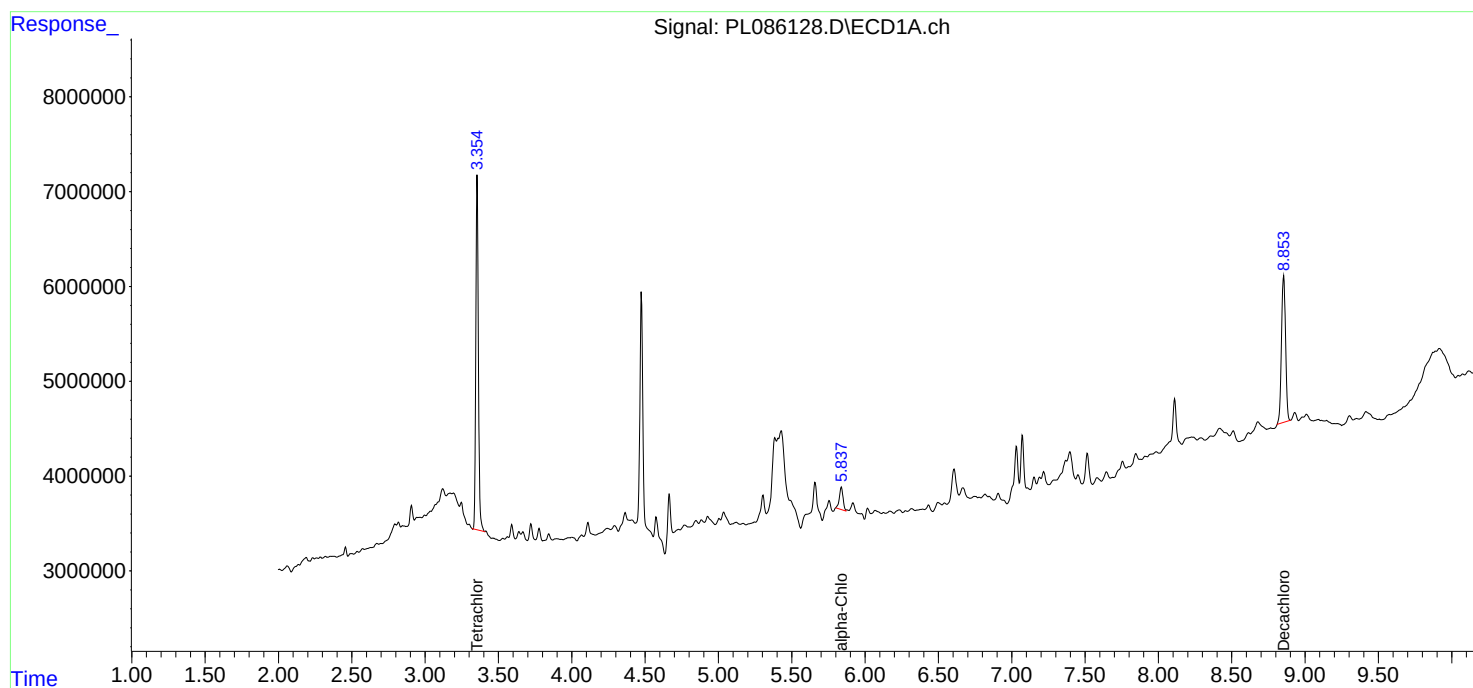

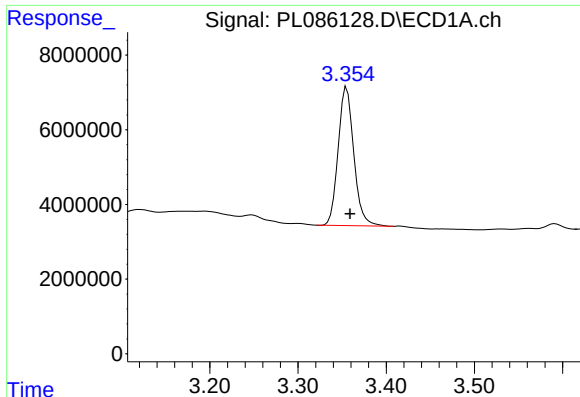


#1 Tetrachloro-m-xylene

R.T.: 3.355 min
Delta R.T.: -0.004 min
Response: 45788154
Conc: 15.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
343


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

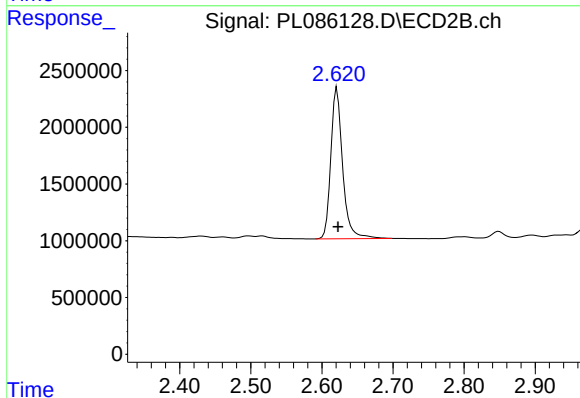


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.001 min
Response: 15373511
Conc: 16.46 ng/ml

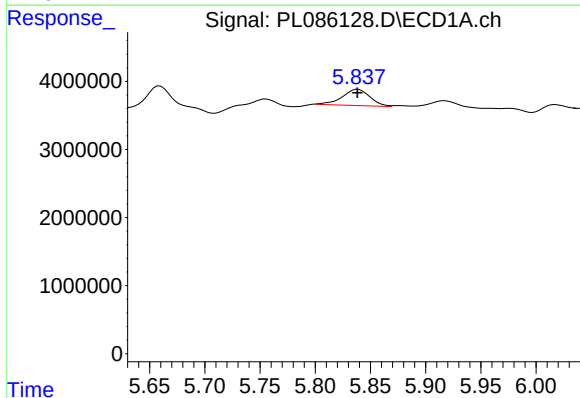


#11 alpha-Chlordane

R.T.: 5.837 min
Delta R.T.: -0.001 min
Response: 4089425
Conc: 1.20 ng/ml m

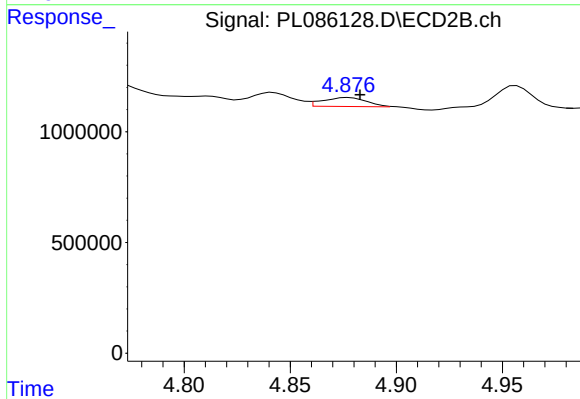

#11 alpha-Chlordane

R.T.: 4.876 min
Delta R.T.: -0.007 min
Response: 563843
Conc: 0.52 ng/ml m

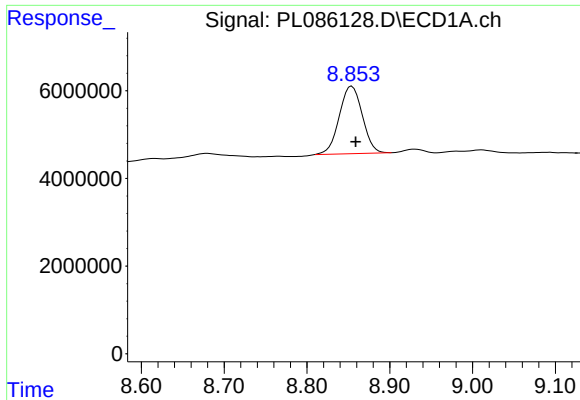


#28 Decachlorobiphenyl

R.T.: 8.854 min
Delta R.T.: -0.004 min
Response: 29773625
Conc: 13.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
343

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2023
Supervised By :Ankita Jodhani 10/25/2023

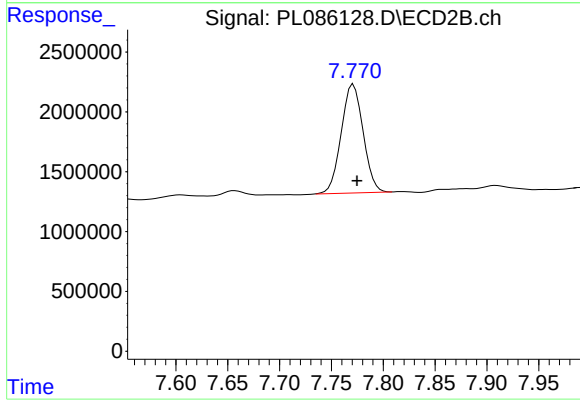

#28 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: -0.003 min
Response: 13355829
Conc: 14.47 ng/ml