

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
 Data File : PL092623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 19:39
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050


Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 01:50:53 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 17:09:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.779	130.2E6	150.5E6	48.328	54.185
28)	SA Decachlor...	9.056	7.918	98141716	140.3E6	48.318	53.241
Target Compounds							
2)	A alpha-BHC	3.997	3.282	184.1E6	228.1E6	44.664	52.851
3)	MA gamma-BHC...	4.329	3.612	176.0E6	219.2E6	45.757	53.225
4)	MA Heptachlor	4.918	3.951	158.1E6	211.0E6	44.598	52.535
5)	MB Aldrin	5.260	4.231	157.1E6	205.6E6	42.695	51.715
6)	B beta-BHC	4.527	3.911	76667454	90855908	49.389	52.038
7)	B delta-BHC	4.774	4.141	168.7E6	218.5E6	44.844	51.943
8)	B Heptachlo...	5.686	4.734	142.5E6	186.4E6	42.907	52.901
9)	A Endosulfan I	6.071	5.104	129.5E6	168.1E6	42.884	52.819
10)	B gamma-Chl...	5.942	4.984	139.2E6	187.8E6	42.226	51.038
11)	B alpha-Chl...	6.021	5.047	137.5E6	183.4E6	42.211	51.612
12)	B 4,4'-DDE	6.194	5.236	124.4E6	181.2E6	41.930	52.101
13)	MA Dieldrin	6.346	5.368	136.5E6	185.4E6	41.971	50.739
14)	MA Endrin	6.576	5.643	116.5E6	167.7E6	41.265	51.219
15)	B Endosulfa...	6.796	5.938	119.1E6	155.8E6	42.080	49.832
16)	A 4,4'-DDD	6.711	5.791	103.6E6	142.6E6	42.870	51.313
17)	MA 4,4'-DDT	7.025	6.041	105.8E6	146.2E6	42.915	49.768
18)	B Endrin al...	6.926	6.117	96721601	123.6E6	45.280	50.300
19)	B Endosulfa...	7.160	6.340	110.6E6	145.3E6	43.755	49.147
20)	A Methoxychlor	7.501	6.616	58880145	76307961	49.995	53.819
21)	B Endrin ke...	7.645	6.845	123.7E6	163.9E6	44.981	51.014
22)	Mirex	8.118	7.026	97913365	133.4E6	46.924	51.032
23)	Chlordane-1	0.000	3.772	0	56726	N.D.	0.477 #
24)	Chlordane-2	5.260f	4.368	157.1E6	6002042	1185.427	42.965 #
25)	Chlordane-3	5.942	4.984	139.2E6	187.8E6	288.470	468.449 #
26)	Chlordane-4	6.021	5.047	137.5E6	183.4E6	235.071	472.915 #
27)	Chlordane-5	0.000	5.938	0	155.8E6	N.D.	1113.348 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

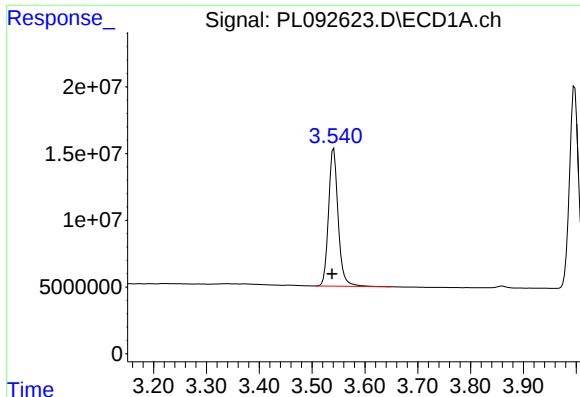

#1 Tetrachloro-m-xylene


R.T.: 3.541 min
Delta R.T.: 0.003 min
Response: 130186722
Conc: 48.33 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

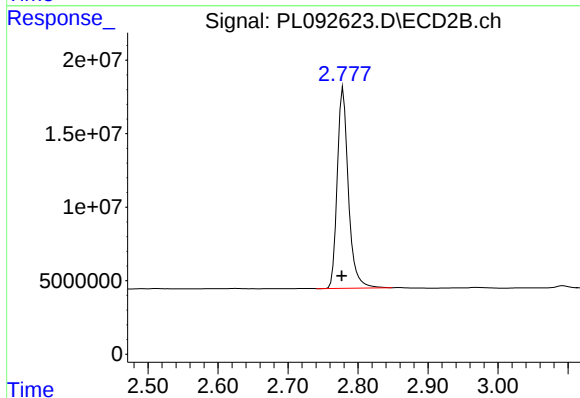


#1 Tetrachloro-m-xylene

R.T.: 2.779 min
Delta R.T.: 0.002 min
Response: 150494395
Conc: 54.18 ng/ml

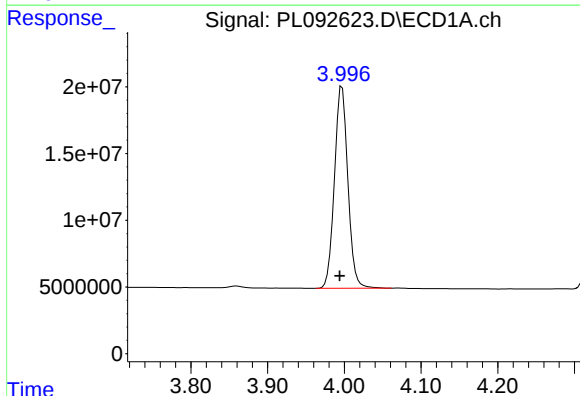


#2 alpha-BHC

R.T.: 3.997 min
Delta R.T.: 0.003 min
Response: 184069304
Conc: 44.66 ng/ml

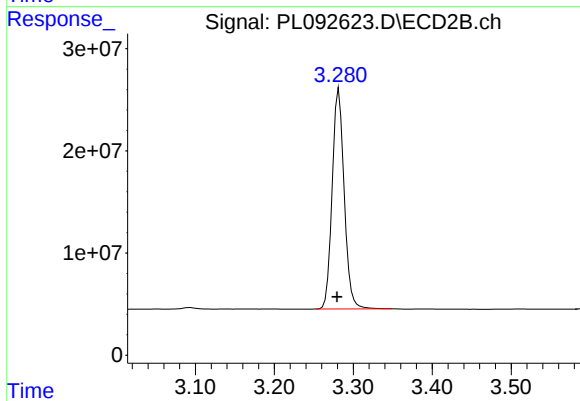

#2 alpha-BHC


R.T.: 3.282 min
Delta R.T.: 0.002 min
Response: 228056097
Conc: 52.85 ng/ml

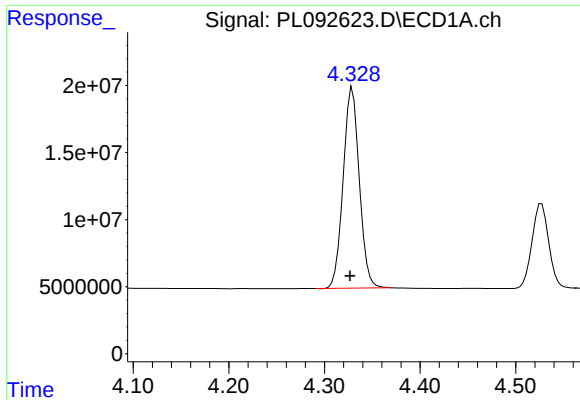

#3 gamma-BHC (Lindane)


R.T.: 4.329 min
Delta R.T.: 0.003 min
Response: 176016501
Conc: 45.76 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

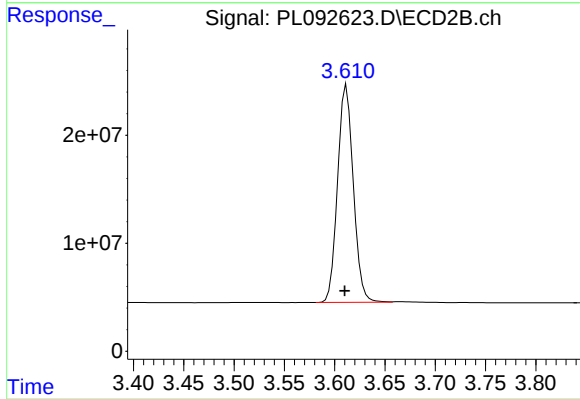


#3 gamma-BHC (Lindane)

R.T.: 3.612 min
Delta R.T.: 0.002 min
Response: 219183545
Conc: 53.23 ng/ml

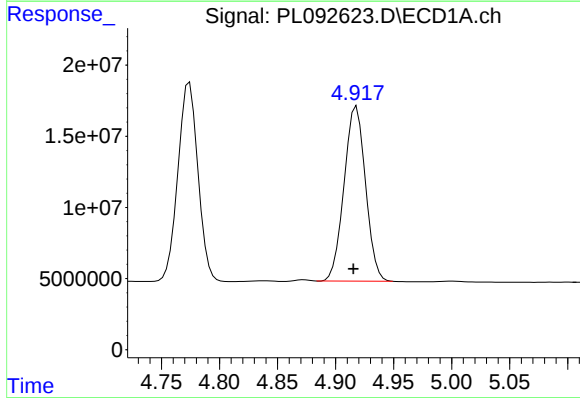


#4 Heptachlor

R.T.: 4.918 min
Delta R.T.: 0.003 min
Response: 158132245
Conc: 44.60 ng/ml

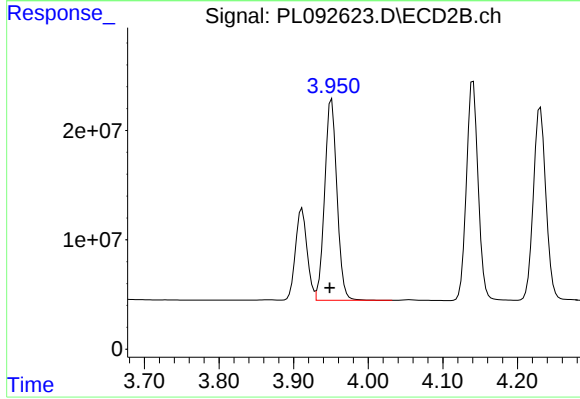

#4 Heptachlor


R.T.: 3.951 min
Delta R.T.: 0.002 min
Response: 210968240
Conc: 52.54 ng/ml

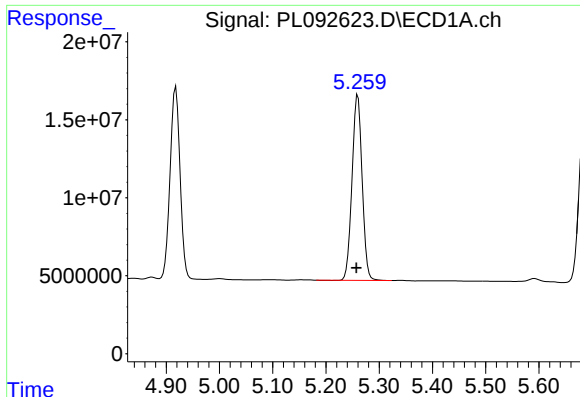

#5 Aldrin


R.T.: 5.260 min
Delta R.T.: 0.003 min
Response: 157060162
Conc: 42.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

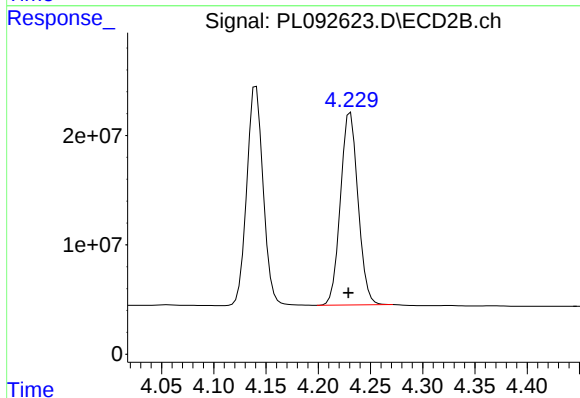


#5 Aldrin

R.T.: 4.231 min
Delta R.T.: 0.002 min
Response: 205591482
Conc: 51.71 ng/ml

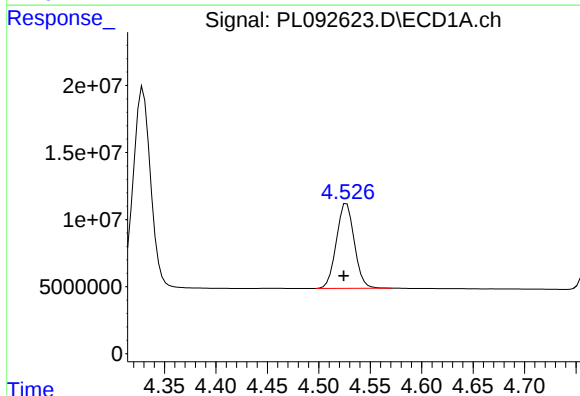


#6 beta-BHC

R.T.: 4.527 min
Delta R.T.: 0.003 min
Response: 76667454
Conc: 49.39 ng/ml

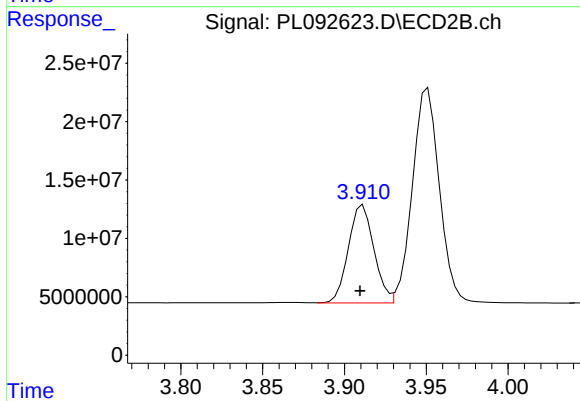

#6 beta-BHC


R.T.: 3.911 min
Delta R.T.: 0.002 min
Response: 90855908
Conc: 52.04 ng/ml

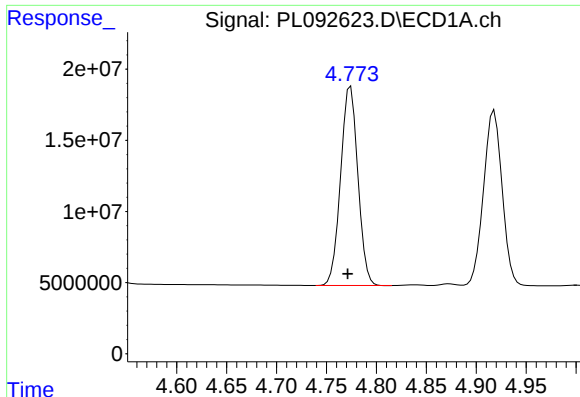

#7 delta-BHC


R.T.: 4.774 min
Delta R.T.: 0.003 min
Response: 168705154
Conc: 44.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

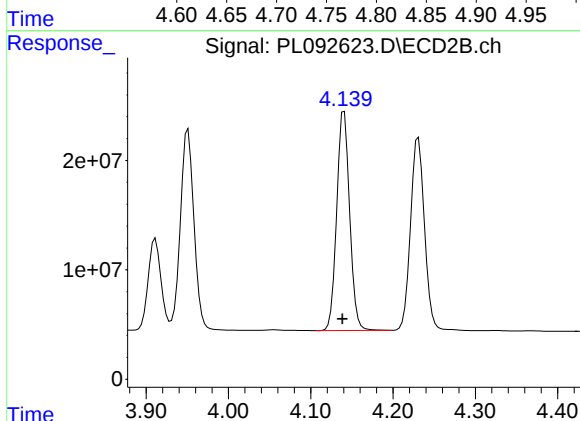


#7 delta-BHC

R.T.: 4.141 min
Delta R.T.: 0.002 min
Response: 218485094
Conc: 51.94 ng/ml

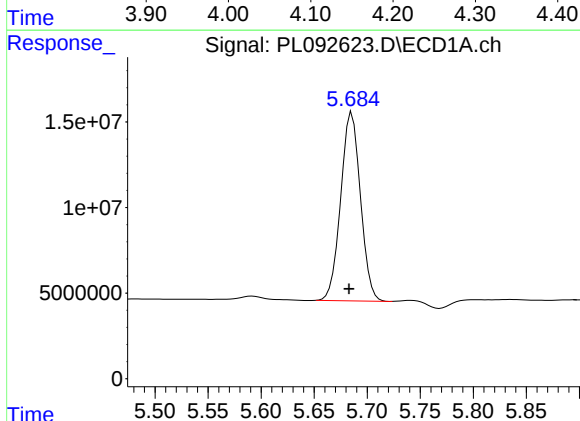


#8 Heptachlor epoxide

R.T.: 5.686 min
Delta R.T.: 0.003 min
Response: 142483120
Conc: 42.91 ng/ml

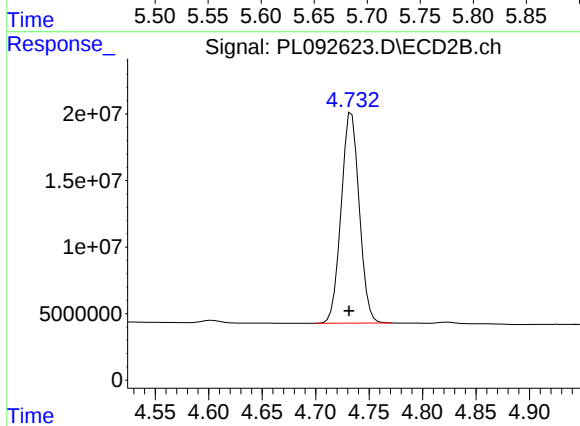

#8 Heptachlor epoxide


R.T.: 4.734 min
Delta R.T.: 0.002 min
Response: 186399765
Conc: 52.90 ng/ml

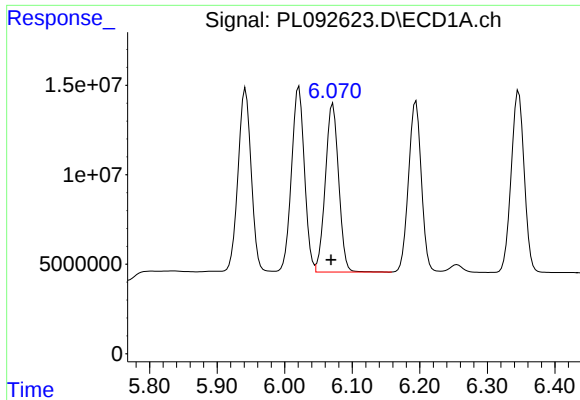

#9 Endosulfan I


R.T.: 6.071 min
Delta R.T.: 0.002 min
Response: 129482849
Conc: 42.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

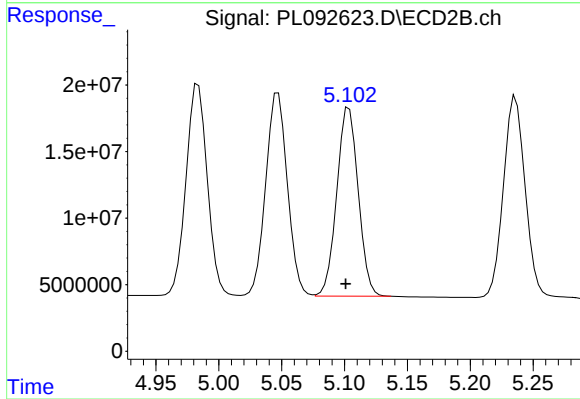


#9 Endosulfan I

R.T.: 5.104 min
Delta R.T.: 0.003 min
Response: 168124382
Conc: 52.82 ng/ml

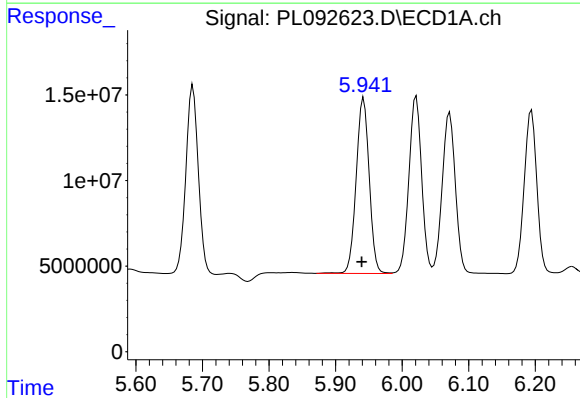


#10 gamma-Chlordane

R.T.: 5.942 min
Delta R.T.: 0.003 min
Response: 139216907
Conc: 42.23 ng/ml

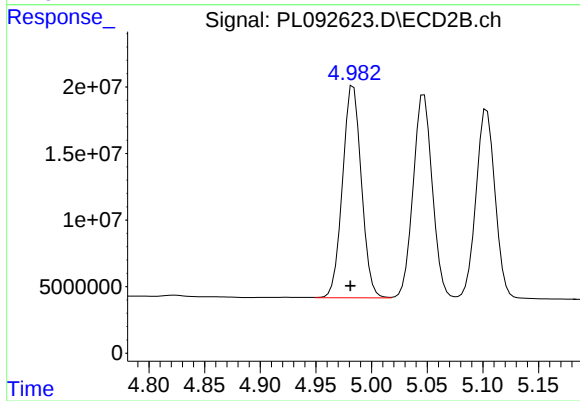

#10 gamma-Chlordane


R.T.: 4.984 min
Delta R.T.: 0.003 min
Response: 187780115
Conc: 51.04 ng/ml

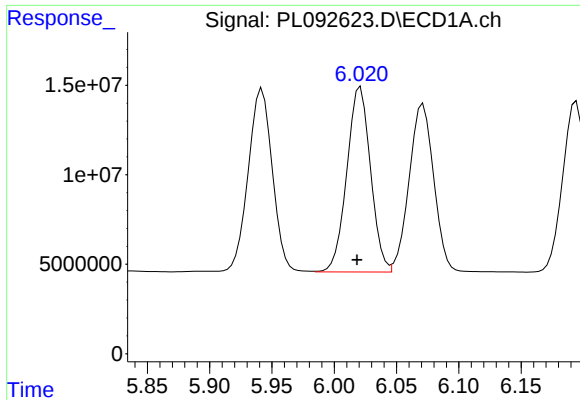

#11 alpha-Chlordane


R.T.: 6.021 min
Delta R.T.: 0.003 min
Response: 137454939
Conc: 42.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

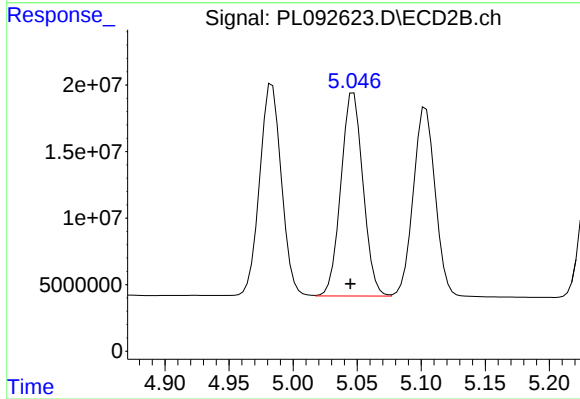


#11 alpha-Chlordane

R.T.: 5.047 min
Delta R.T.: 0.002 min
Response: 183430363
Conc: 51.61 ng/ml

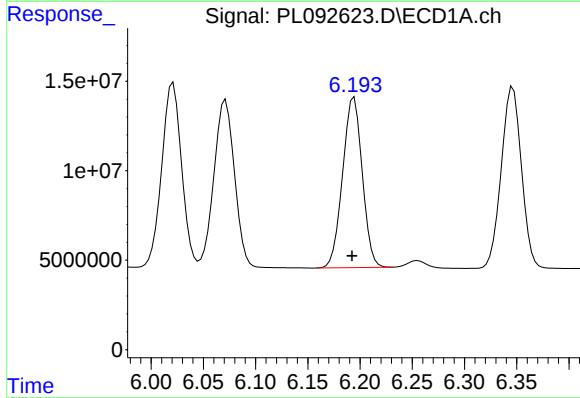


#12 4,4'-DDE

R.T.: 6.194 min
Delta R.T.: 0.002 min
Response: 124360293
Conc: 41.93 ng/ml

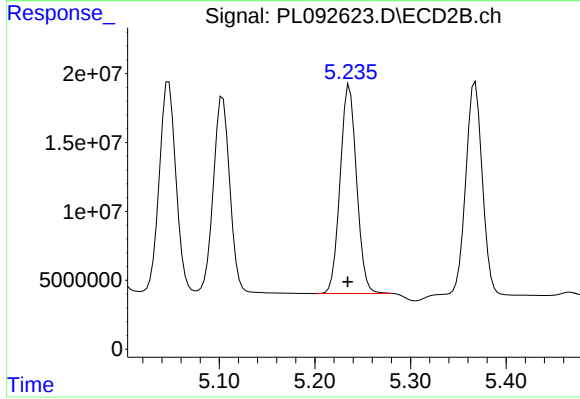

#12 4,4'-DDE


R.T.: 5.236 min
Delta R.T.: 0.002 min
Response: 181172583
Conc: 52.10 ng/ml

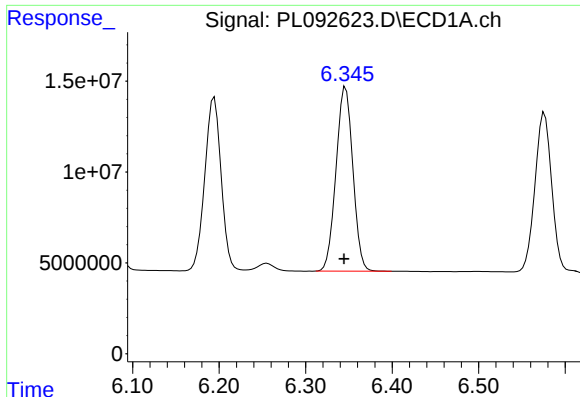

#13 Dieldrin


R.T.: 6.346 min
Delta R.T.: 0.002 min
Response: 136485807
Conc: 41.97 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

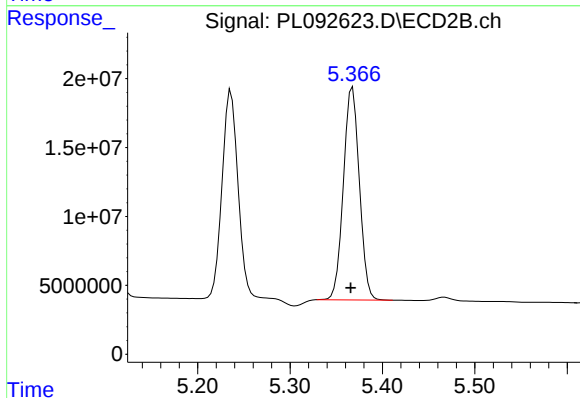


#13 Dieldrin

R.T.: 5.368 min
Delta R.T.: 0.002 min
Response: 185417371
Conc: 50.74 ng/ml

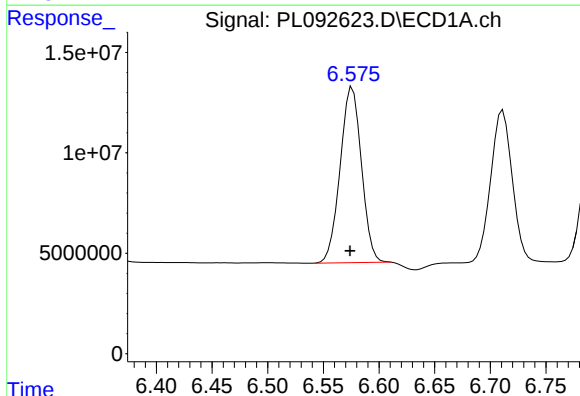


#14 Endrin

R.T.: 6.576 min
Delta R.T.: 0.002 min
Response: 116522017
Conc: 41.27 ng/ml

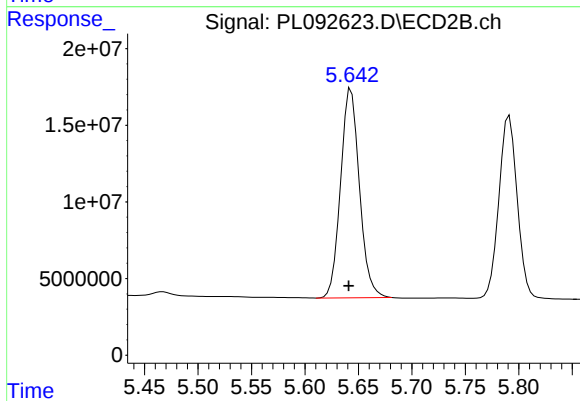

#14 Endrin


R.T.: 5.643 min
Delta R.T.: 0.002 min
Response: 167738183
Conc: 51.22 ng/ml

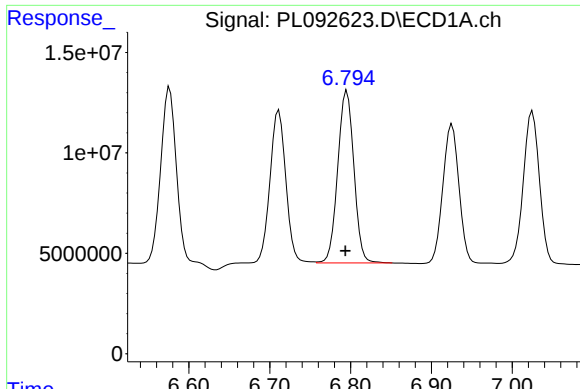

#15 Endosulfan II


R.T.: 6.796 min
Delta R.T.: 0.002 min
Response: 119077562
Conc: 42.08 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

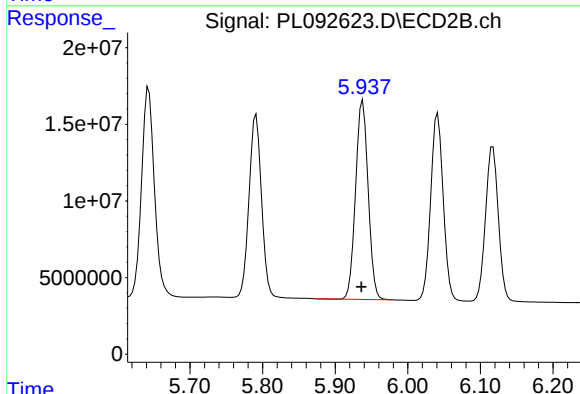


#15 Endosulfan II

R.T.: 5.938 min
Delta R.T.: 0.002 min
Response: 155784691
Conc: 49.83 ng/ml

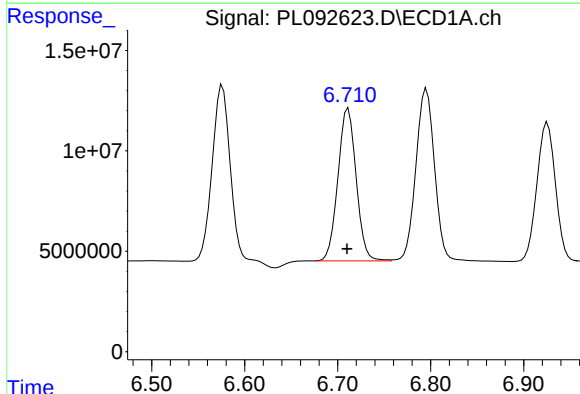


#16 4,4'-DDD

R.T.: 6.711 min
Delta R.T.: 0.001 min
Response: 103572873
Conc: 42.87 ng/ml

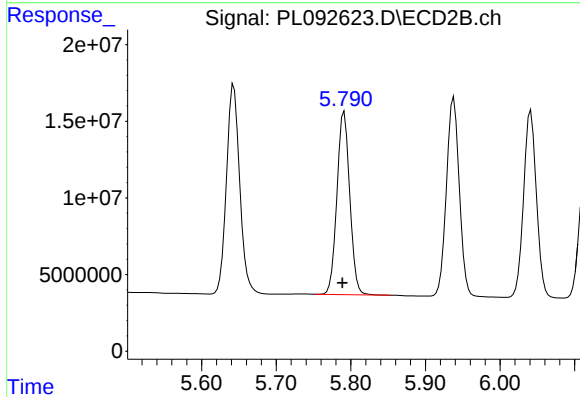

#16 4,4'-DDD


R.T.: 5.791 min
Delta R.T.: 0.002 min
Response: 142558517
Conc: 51.31 ng/ml

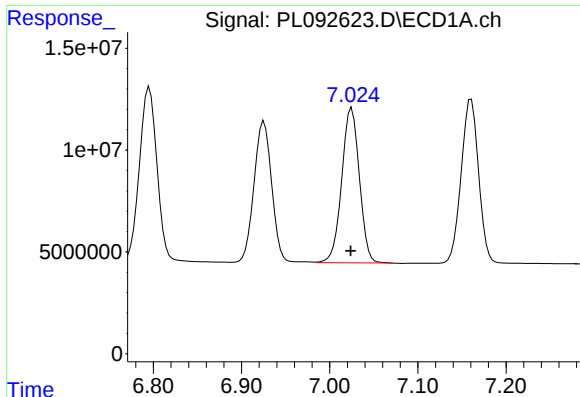

#17 4,4'-DDT


R.T.: 7.025 min
Delta R.T.: 0.000 min
Response: 105831060
Conc: 42.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

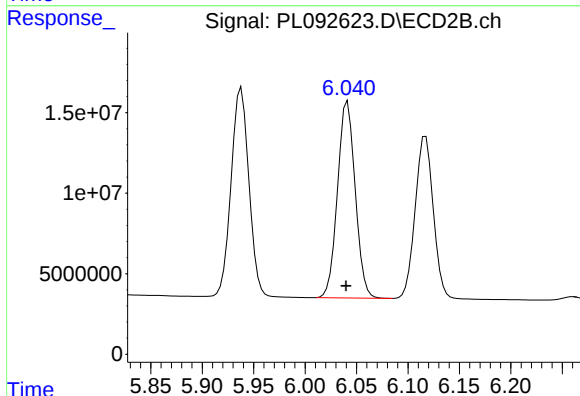


#17 4,4'-DDT

R.T.: 6.041 min
Delta R.T.: 0.002 min
Response: 146165905
Conc: 49.77 ng/ml

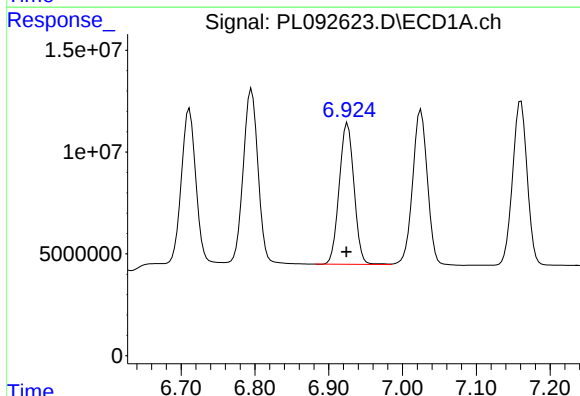


#18 Endrin aldehyde

R.T.: 6.926 min
Delta R.T.: 0.002 min
Response: 96721601
Conc: 45.28 ng/ml

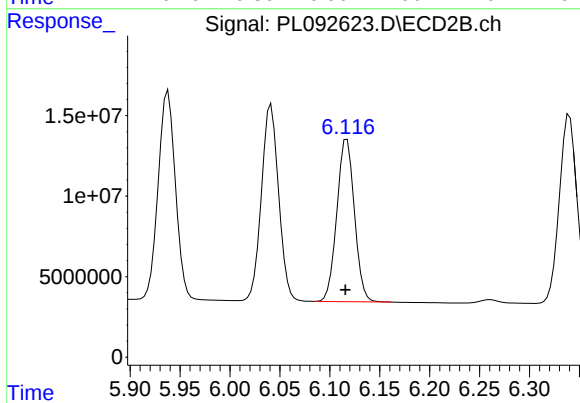

#18 Endrin aldehyde


R.T.: 6.117 min
Delta R.T.: 0.002 min
Response: 123565087
Conc: 50.30 ng/ml

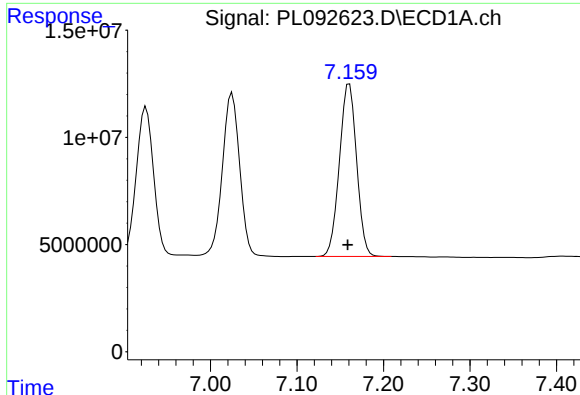

#19 Endosulfan Sulfate


R.T.: 7.160 min
Delta R.T.: 0.002 min
Response: 110552555
Conc: 43.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

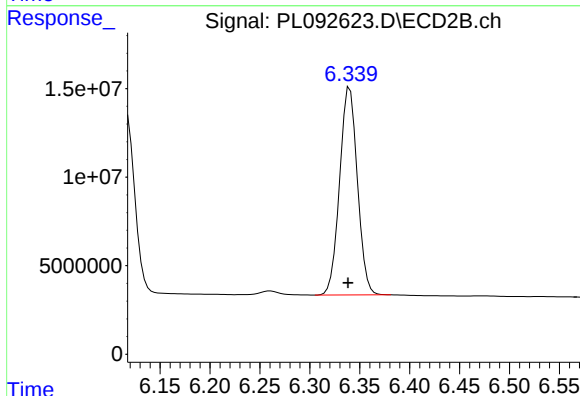


#19 Endosulfan Sulfate

R.T.: 6.340 min
Delta R.T.: 0.002 min
Response: 145291765
Conc: 49.15 ng/ml

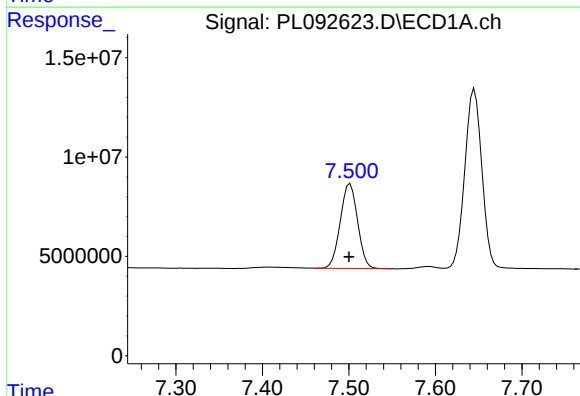


#20 Methoxychlor

R.T.: 7.501 min
Delta R.T.: 0.001 min
Response: 58880145
Conc: 50.00 ng/ml

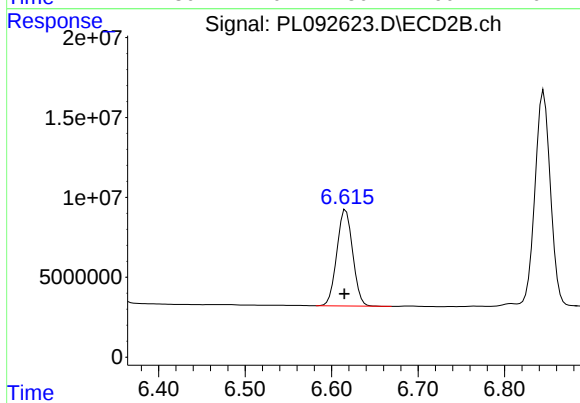

#20 Methoxychlor


R.T.: 6.616 min
Delta R.T.: 0.002 min
Response: 76307961
Conc: 53.82 ng/ml

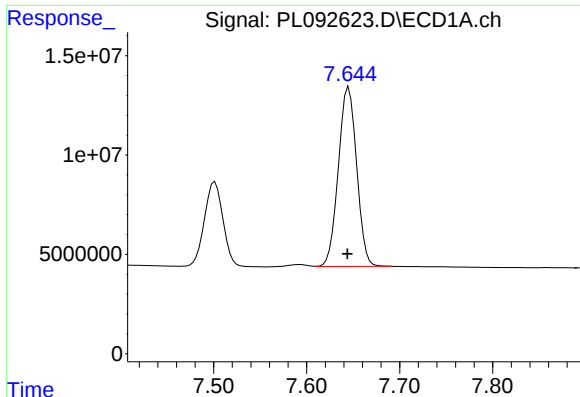

#21 Endrin ketone


R.T.: 7.645 min
Delta R.T.: 0.001 min
Response: 123688510
Conc: 44.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

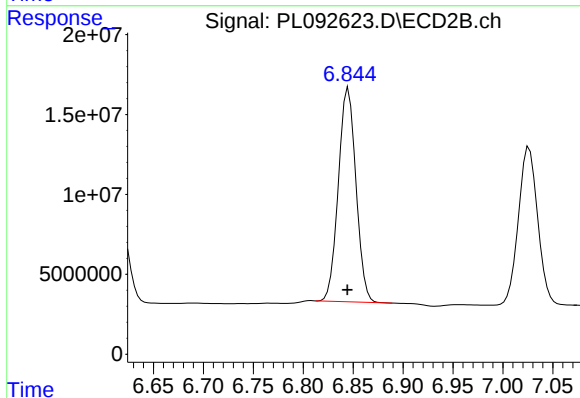


#21 Endrin ketone

R.T.: 6.845 min
Delta R.T.: 0.001 min
Response: 163864219
Conc: 51.01 ng/ml

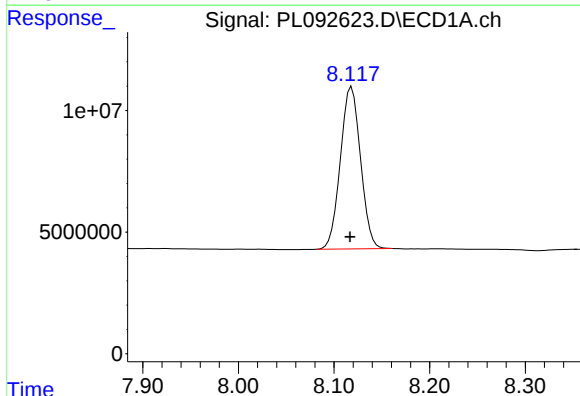


#22 Mirex

R.T.: 8.118 min
Delta R.T.: 0.002 min
Response: 97913365
Conc: 46.92 ng/ml

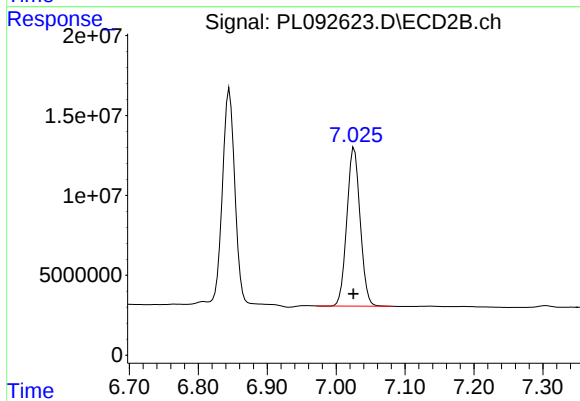

#22 Mirex


R.T.: 7.026 min
Delta R.T.: 0.002 min
Response: 133372152
Conc: 51.03 ng/ml

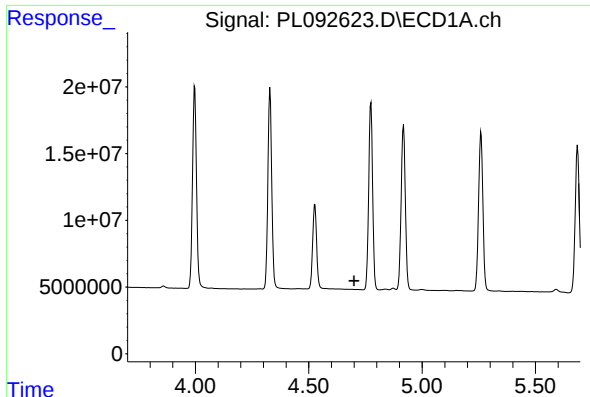

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 4.700 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

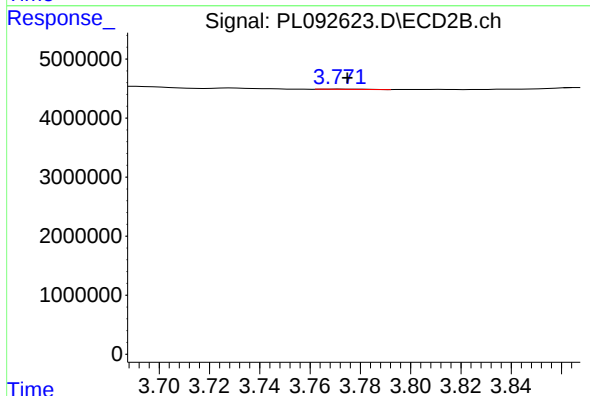


#23 Chlordane-1

R.T.: 3.772 min
Delta R.T.: -0.003 min
Response: 56726
Conc: 0.48 ng/ml

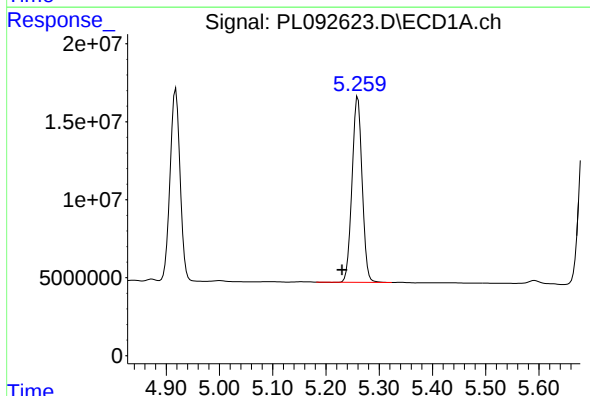


#24 Chlordane-2

R.T.: 5.260 min
Delta R.T.: 0.029 min
Response: 157060162
Conc: 1185.43 ng/ml

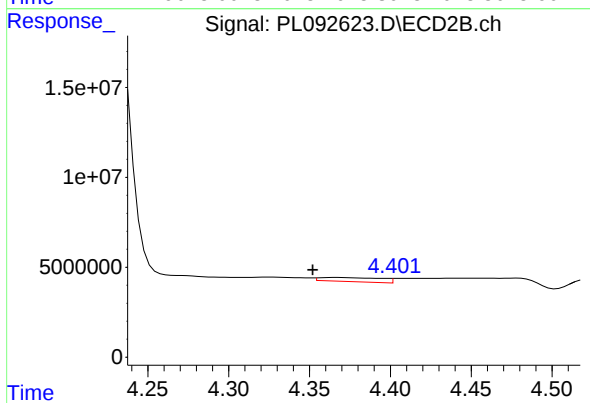

#24 Chlordane-2


R.T.: 4.368 min
Delta R.T.: 0.016 min
Response: 6002042
Conc: 42.97 ng/ml

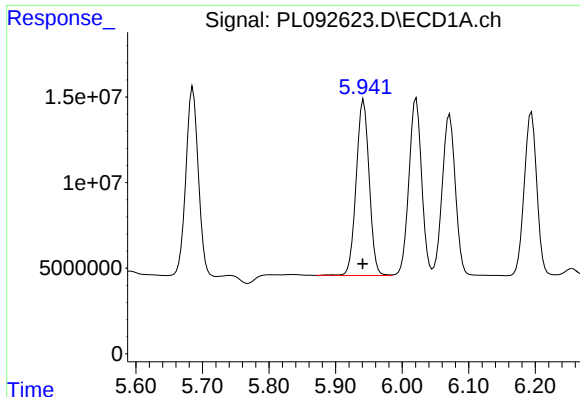

#25 Chlordane-3


R.T.: 5.942 min
Delta R.T.: 0.001 min
Response: 139216907
Conc: 288.47 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

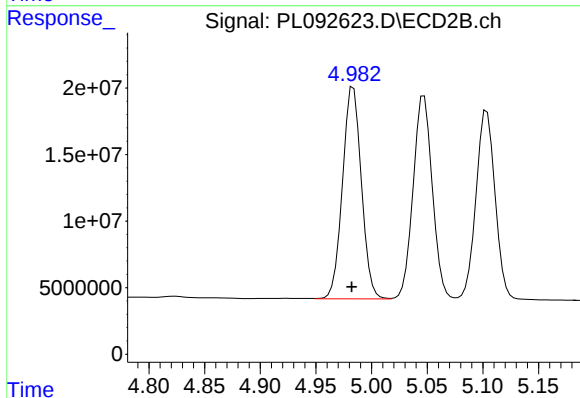


#25 Chlordane-3

R.T.: 4.984 min
Delta R.T.: 0.002 min
Response: 187780115
Conc: 468.45 ng/ml

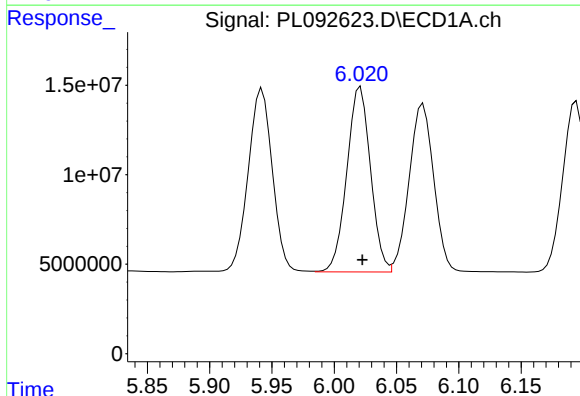


#26 Chlordane-4

R.T.: 6.021 min
Delta R.T.: -0.002 min
Response: 137454939
Conc: 235.07 ng/ml

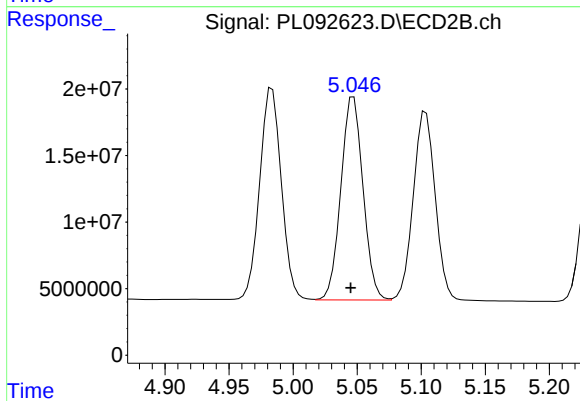

#26 Chlordane-4


R.T.: 5.047 min
Delta R.T.: 0.002 min
Response: 183430363
Conc: 472.92 ng/ml

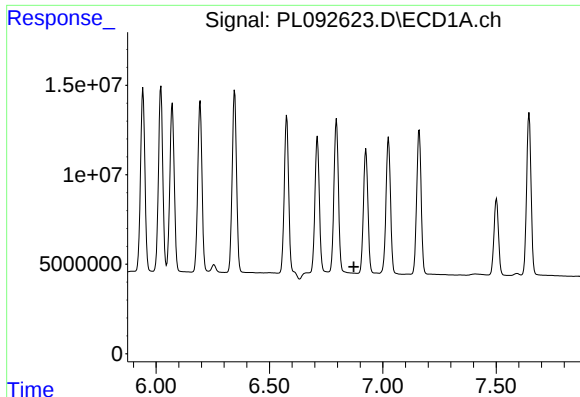

#27 Chlordane-5


R.T.: 0.000 min
Exp R.T.: 6.872 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050

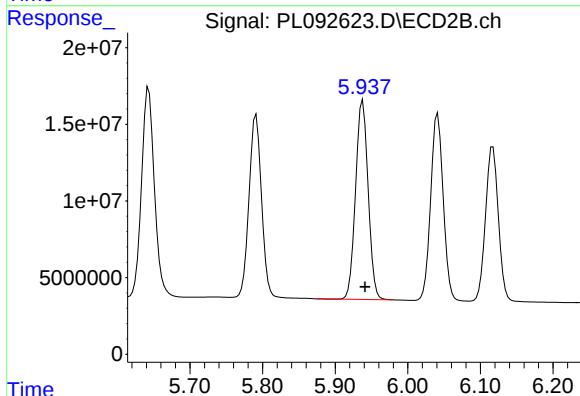


#27 Chlordane-5

R.T.: 5.938 min
Delta R.T.: -0.003 min
Response: 155784691
Conc: 1113.35 ng/ml

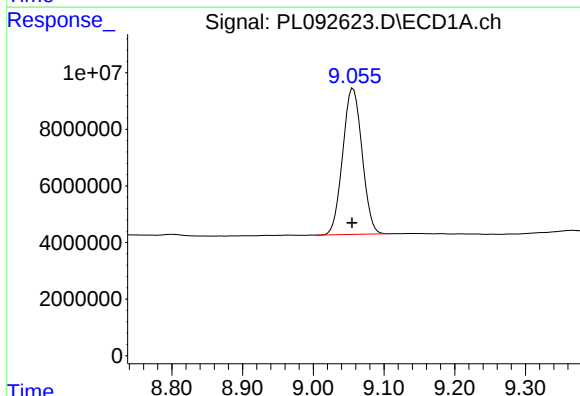

#28 Decachlorobiphenyl

R.T.: 9.056 min
Delta R.T.: 0.001 min
Response: 98141716
Conc: 48.32 ng/ml

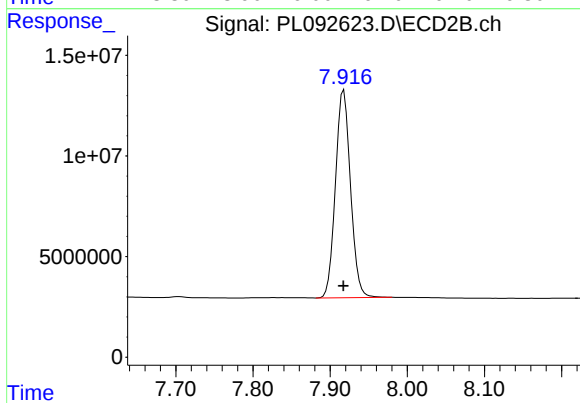

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.000 min
Response: 140288584
Conc: 53.24 ng/ml