

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
 Data File : PL092594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 11:22
 Operator : AR\AJ
 Sample : P4472-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BP-F-28

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/25/2024
 Supervised By :Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:05:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 17:09:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.539	2.777	38473272	52758770	14.282m	18.995m#
28) SA Decachlor...	9.057	7.918	36291943	45789554	17.868	17.378

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
Data File : PL092594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 11:22
Operator : AR\AJ
Sample : P4472-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BP-F-28


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/25/2024
Supervised By : Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:05:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 17:09:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

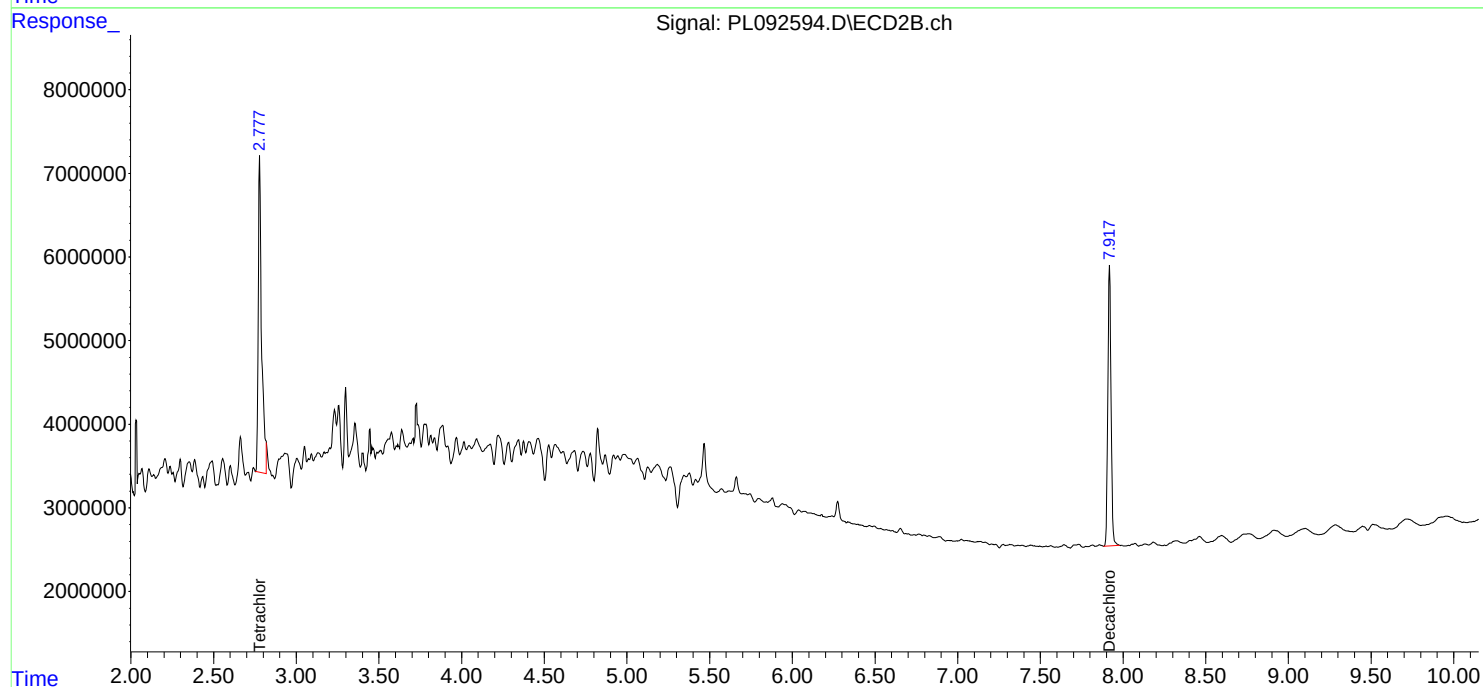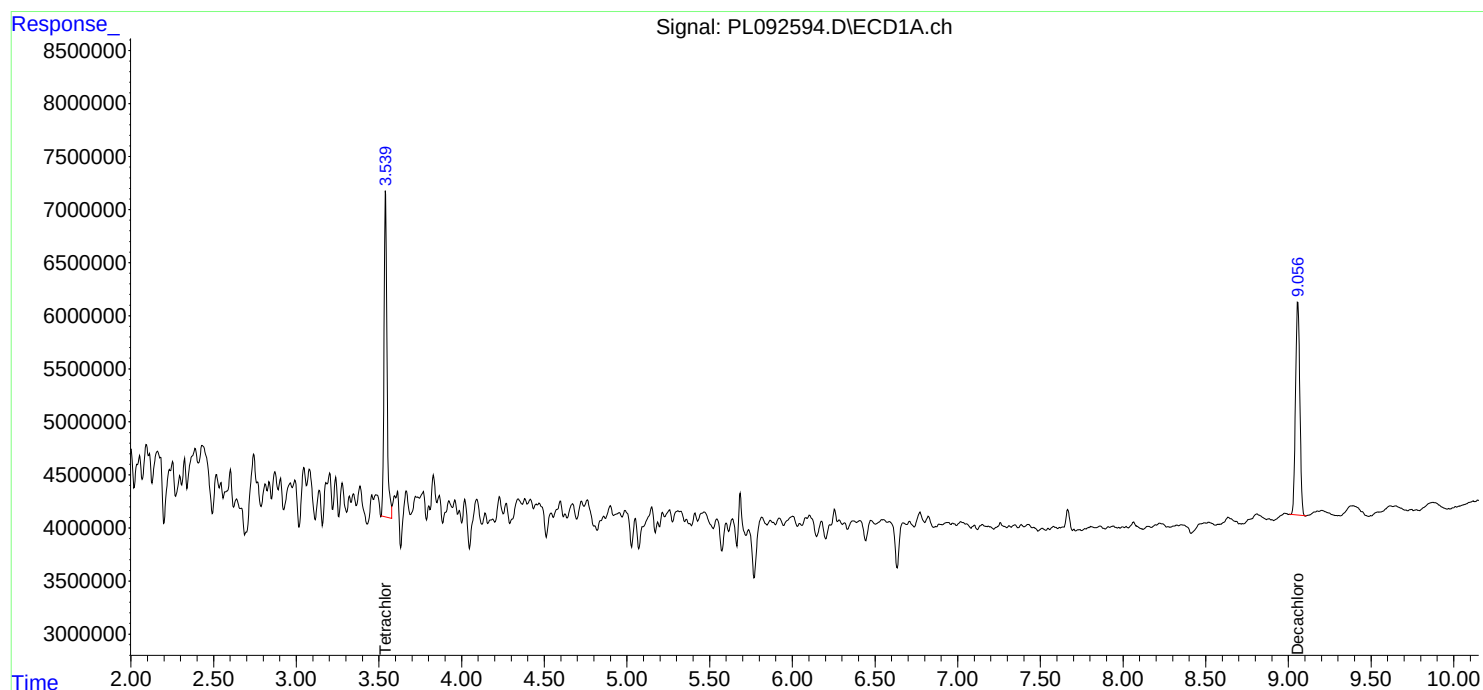

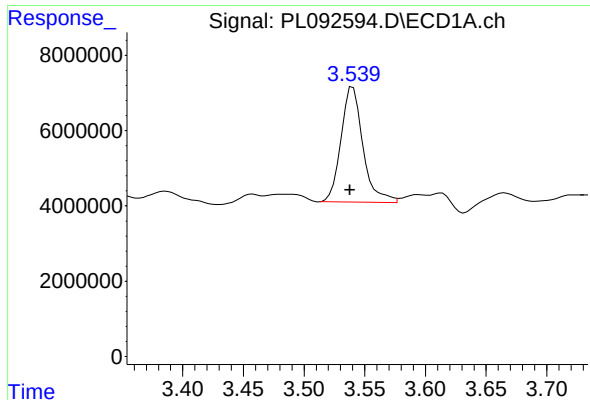


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: 0.000 min
Response: 38473272
Conc: 14.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
BP-F-28


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2024
Supervised By :Ankita Jodhani 10/28/2024

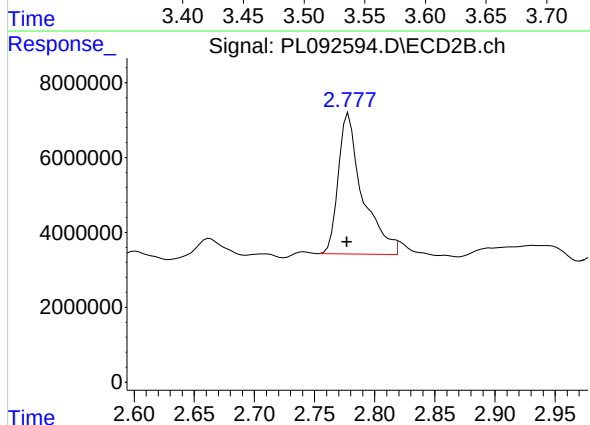


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 52758770
Conc: 19.00 ng/ml

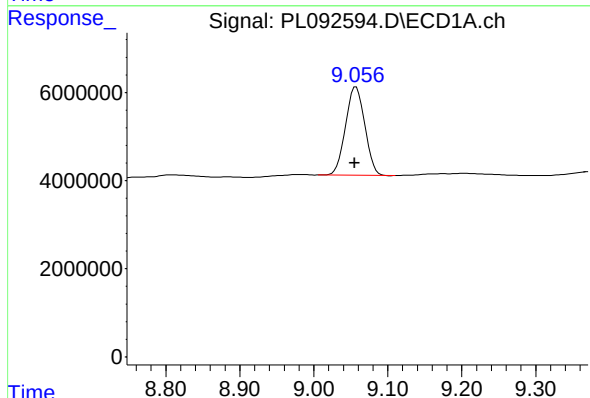

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: 0.002 min
Response: 36291943
Conc: 17.87 ng/ml

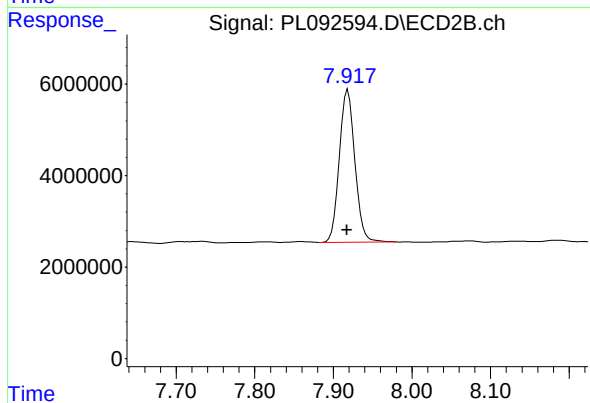

#28 Decachlorobiphenyl

R.T.: 7.918 min
Delta R.T.: 0.001 min
Response: 45789554
Conc: 17.38 ng/ml