

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
 Data File : PL092597.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 12:02
 Operator : AR\AJ
 Sample : P4472-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BP-F-6

Manual Integrations APPROVED

Reviewed By :Abdul
 Mirza

10/25/2024
 Supervised By :Ankita
 Jodhani

10/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:08:58 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 17:09:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.778	35761850	77740571	13.275m	27.990 #
28) SA Decachlor...	9.057	7.917	25912998	32458886	12.758	12.318m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
Data File : PL092597.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 12:02
Operator : AR\AJ
Sample : P4472-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
BP-F-6

Manual Integrations
APPROVED



Reviewed By :Abdul
Mirza


10/25/2024
Supervised By :Ankita
Jodhani

10/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:08:58 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 17:09:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

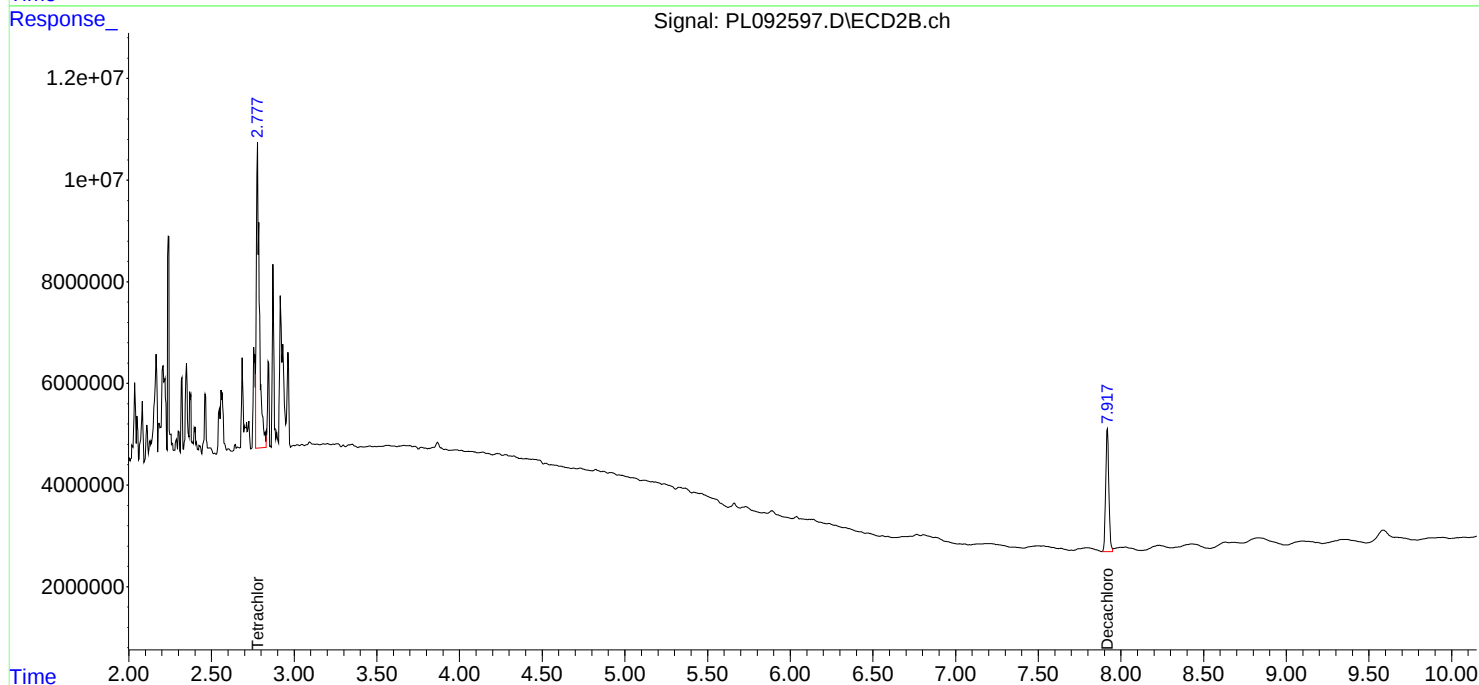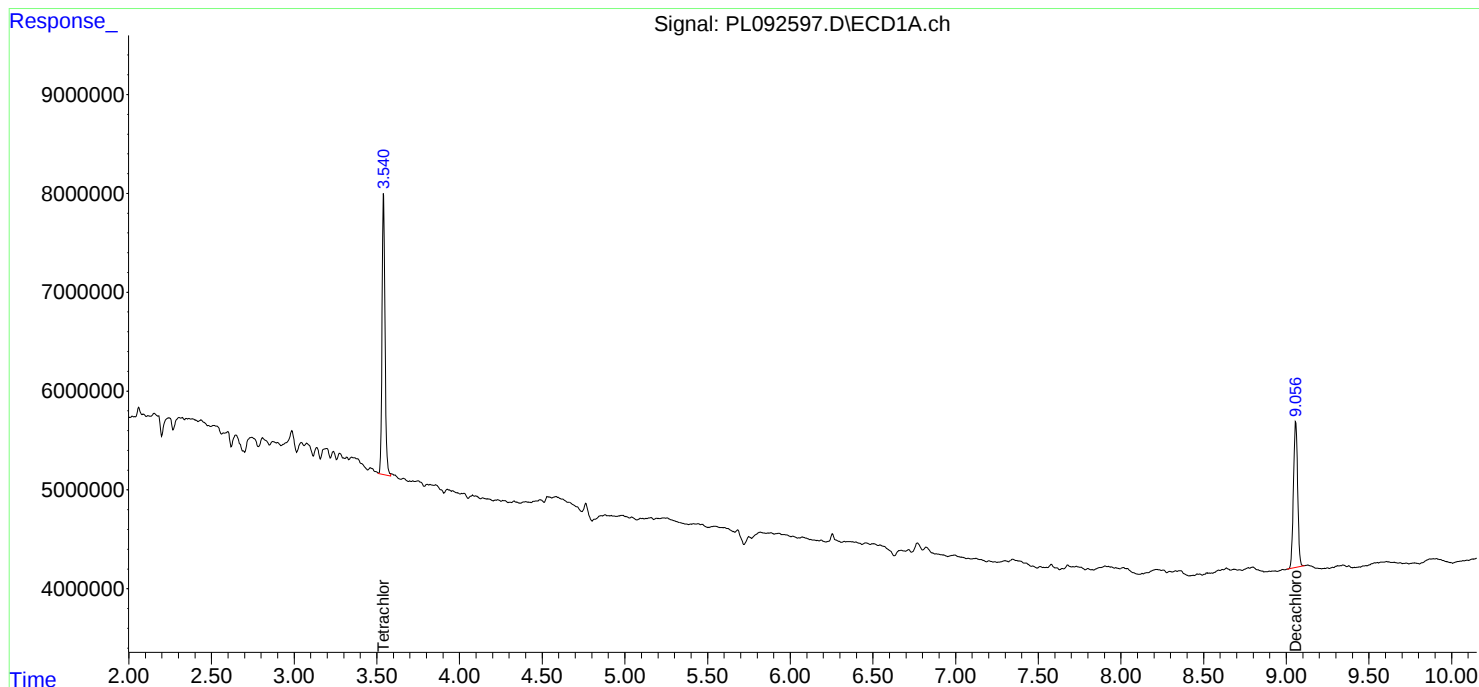

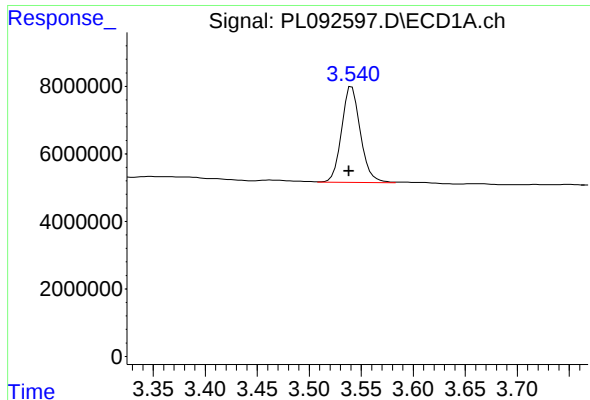

#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.002 min
Response: 35761850
Conc: 13.28 ng/ml


Instrument :
ECD_L
ClientSampleId :
BP-F-6

Manual Integrations
APPROVED

Reviewed By :Abdul
Mirza


10/25/2024
Supervised By :Ankita
Jodhani

10/28/2024

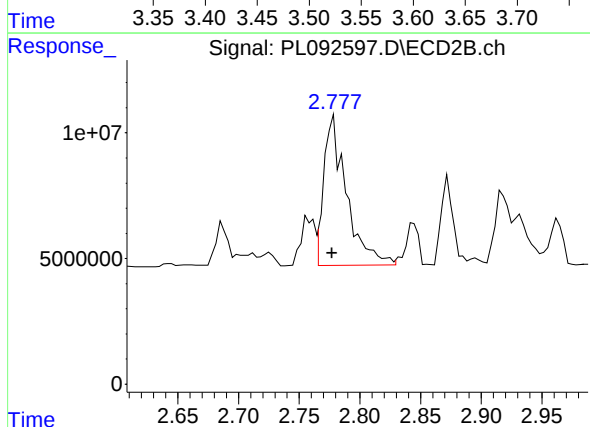


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.001 min
Response: 77740571
Conc: 27.99 ng/ml

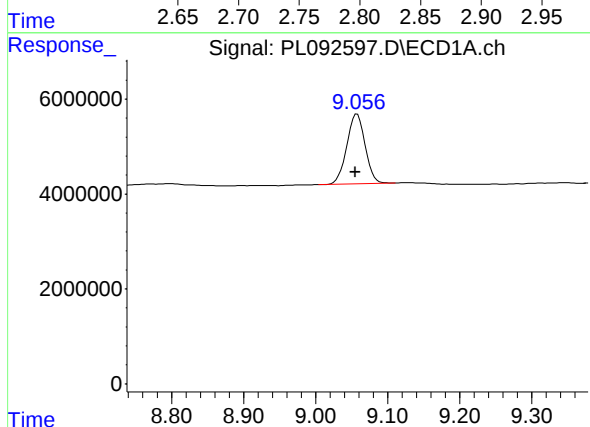

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: 0.002 min
Response: 25912998
Conc: 12.76 ng/ml

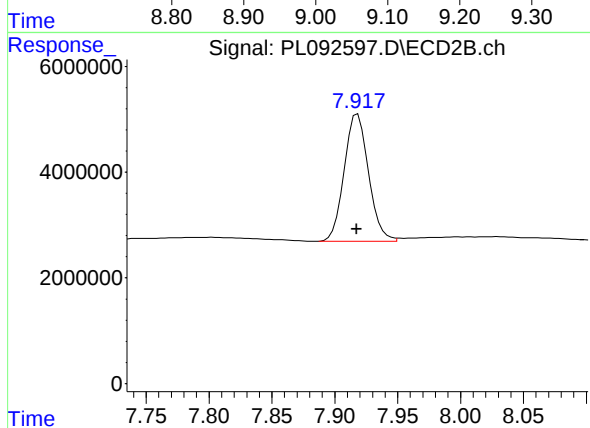

#28 Decachlorobiphenyl

R.T.: 7.917 min
Delta R.T.: 0.000 min
Response: 32458886
Conc: 12.32 ng/ml m