

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
 Data File : PL092611.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 16:35
 Operator : AR\AJ
 Sample : PB164365BL
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB164365BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/25/2024
 Supervised By : Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:20:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 17:09:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.546	2.778	46024411	49643329	17.085	17.874m
28) SA Decachlor...	9.062	7.921	39184875	50381807	19.292m	19.120

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
Data File : PL092611.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 16:35
Operator : AR\AJ
Sample : PB164365BL
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PB164365BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/25/2024
Supervised By : Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:20:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 17:09:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

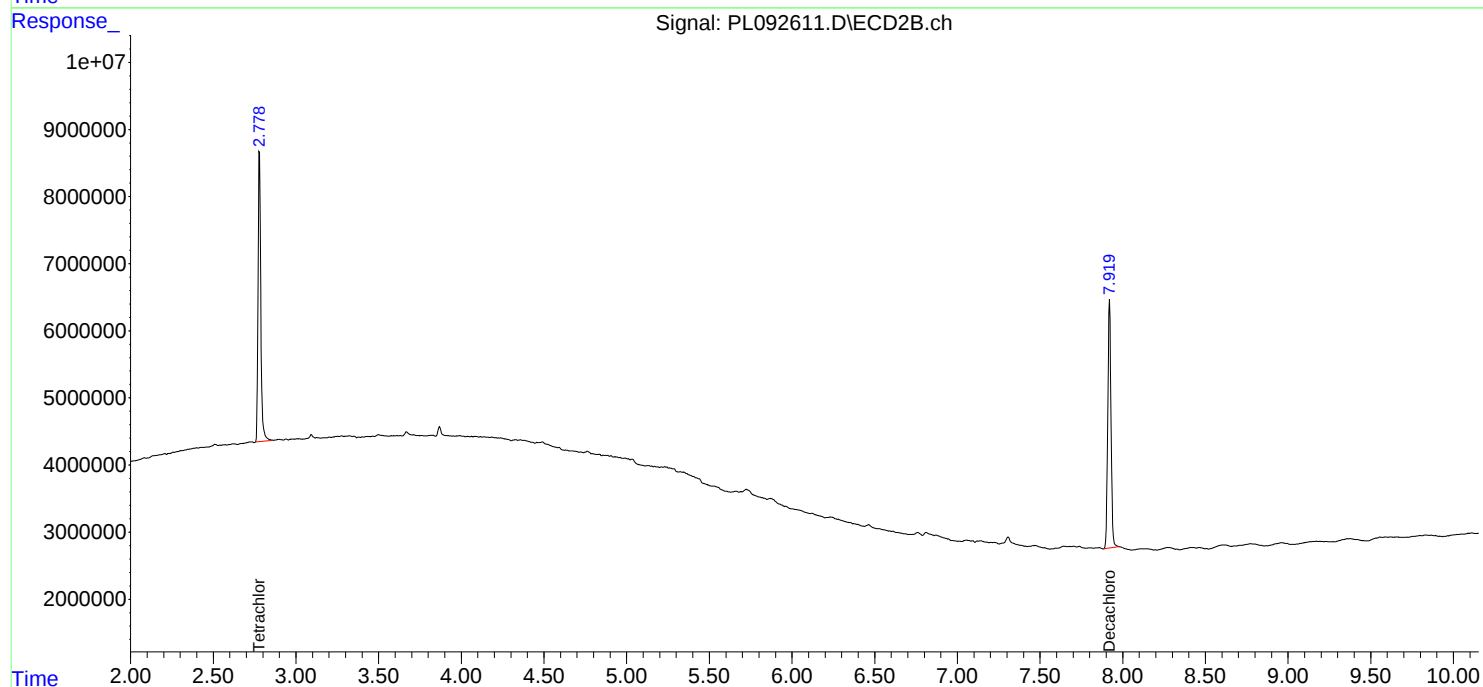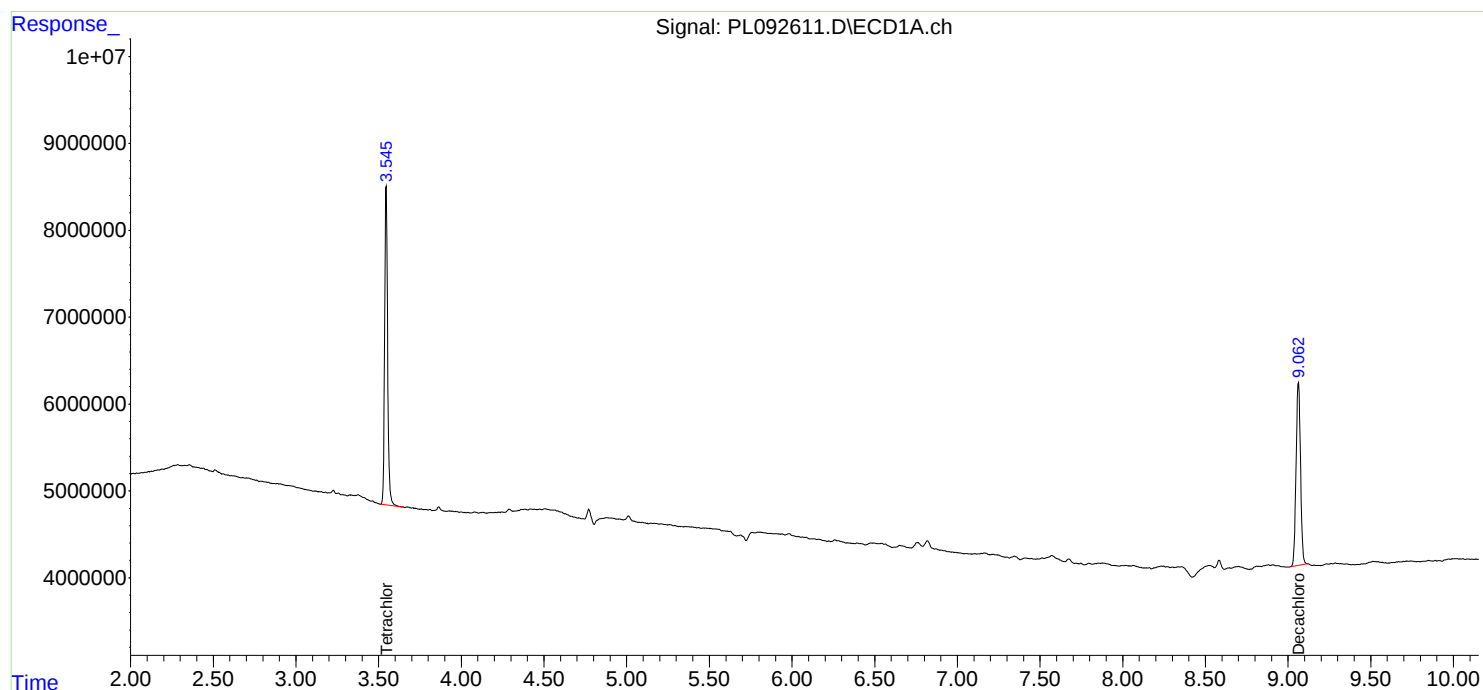

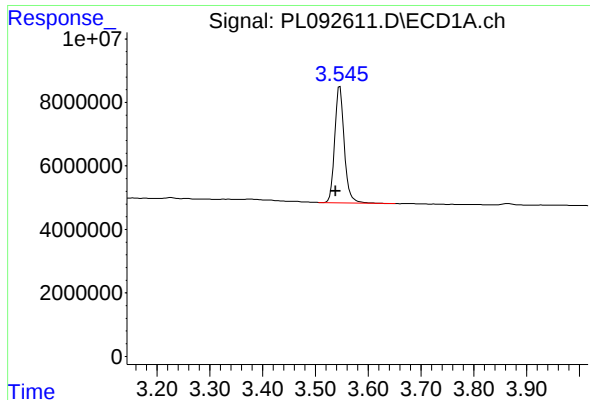


#1 Tetrachloro-m-xylene

R.T.: 3.546 min
Delta R.T.: 0.008 min
Response: 46024411
Conc: 17.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB164365BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2024
Supervised By :Ankita Jodhani 10/28/2024

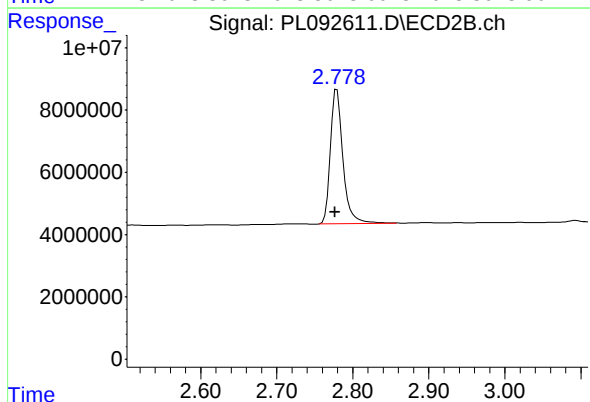


#1 Tetrachloro-m-xylene

R.T.: 2.778 min
Delta R.T.: 0.000 min
Response: 49643329
Conc: 17.87 ng/ml

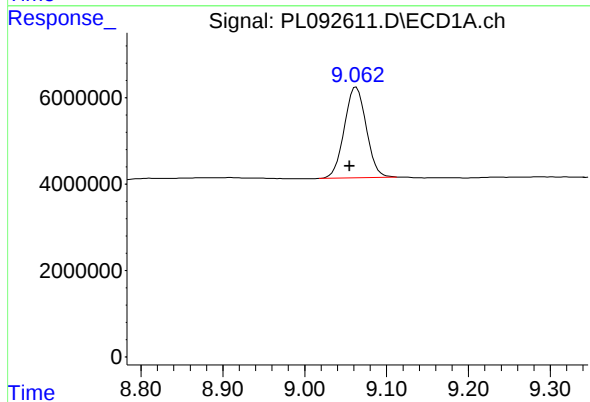

#28 Decachlorobiphenyl

R.T.: 9.062 min
Delta R.T.: 0.007 min
Response: 39184875
Conc: 19.29 ng/ml

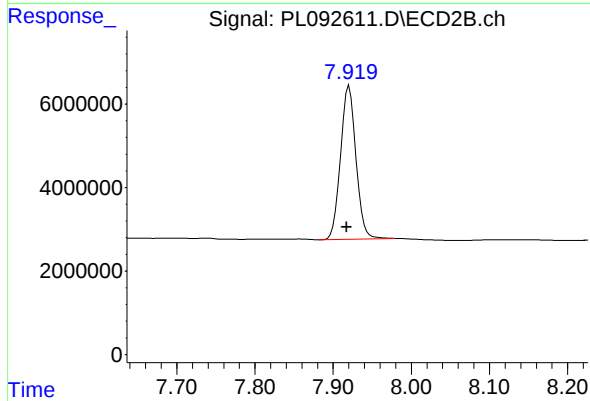

#28 Decachlorobiphenyl

R.T.: 7.921 min
Delta R.T.: 0.003 min
Response: 50381807
Conc: 19.12 ng/ml