

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
 Data File : PL092616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Oct 2024 18:05
 Operator : AR\AJ
 Sample : P4508-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 BP-F23

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/25/2024
 Supervised By : Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 02:24:14 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
 Quant Title : GC Extractables
 QLast Update : Mon Oct 21 17:09:23 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.777	43511884	47753206	16.152m	17.193m
28) SA Decachlor...	9.057	7.919	30756418	40325725	15.142	15.304
Target Compounds						
6) B beta-BHC	4.533	3.915	597581	548271	0.385m	0.314

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102424\
Data File : PL092616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Oct 2024 18:05
Operator : AR\AJ
Sample : P4508-05
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
BP-F23


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/25/2024
Supervised By : Ankita Jodhani 10/28/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 02:24:14 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102124.M
Quant Title : GC Extractables
QLast Update : Mon Oct 21 17:09:23 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

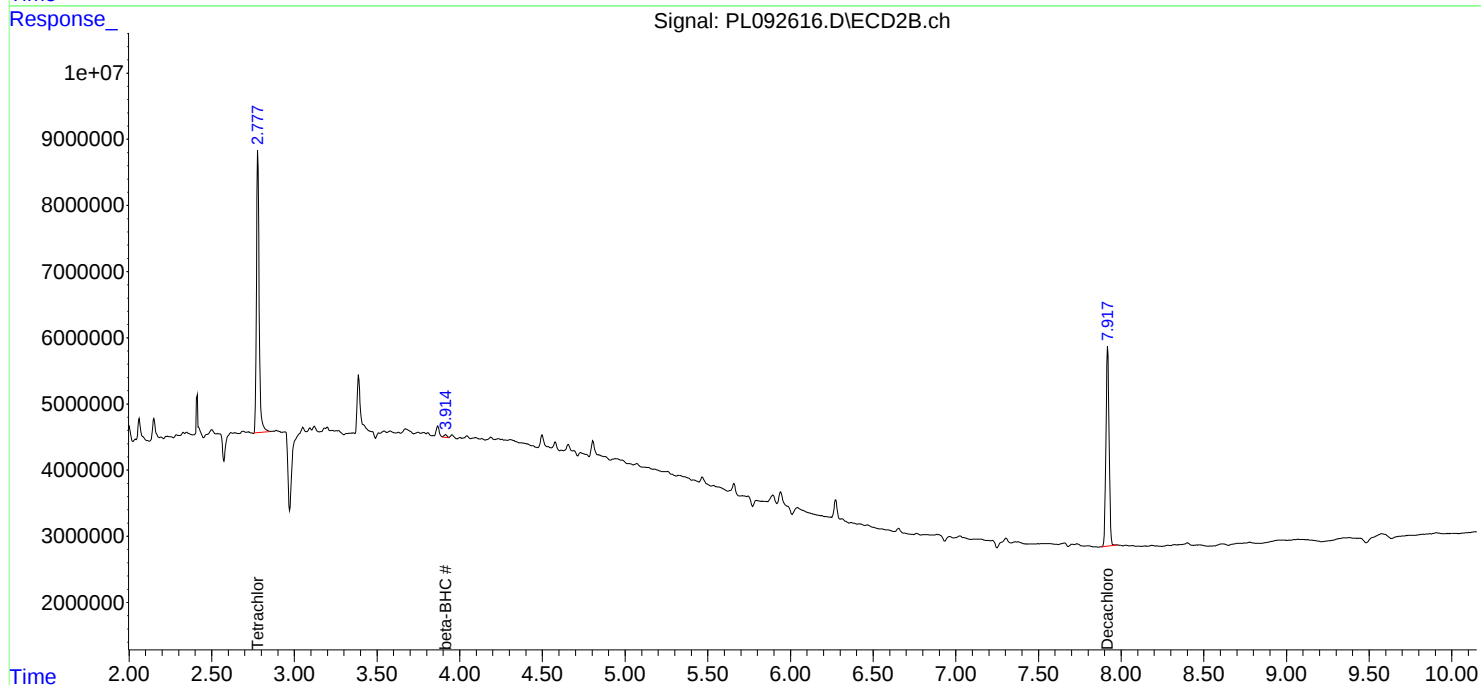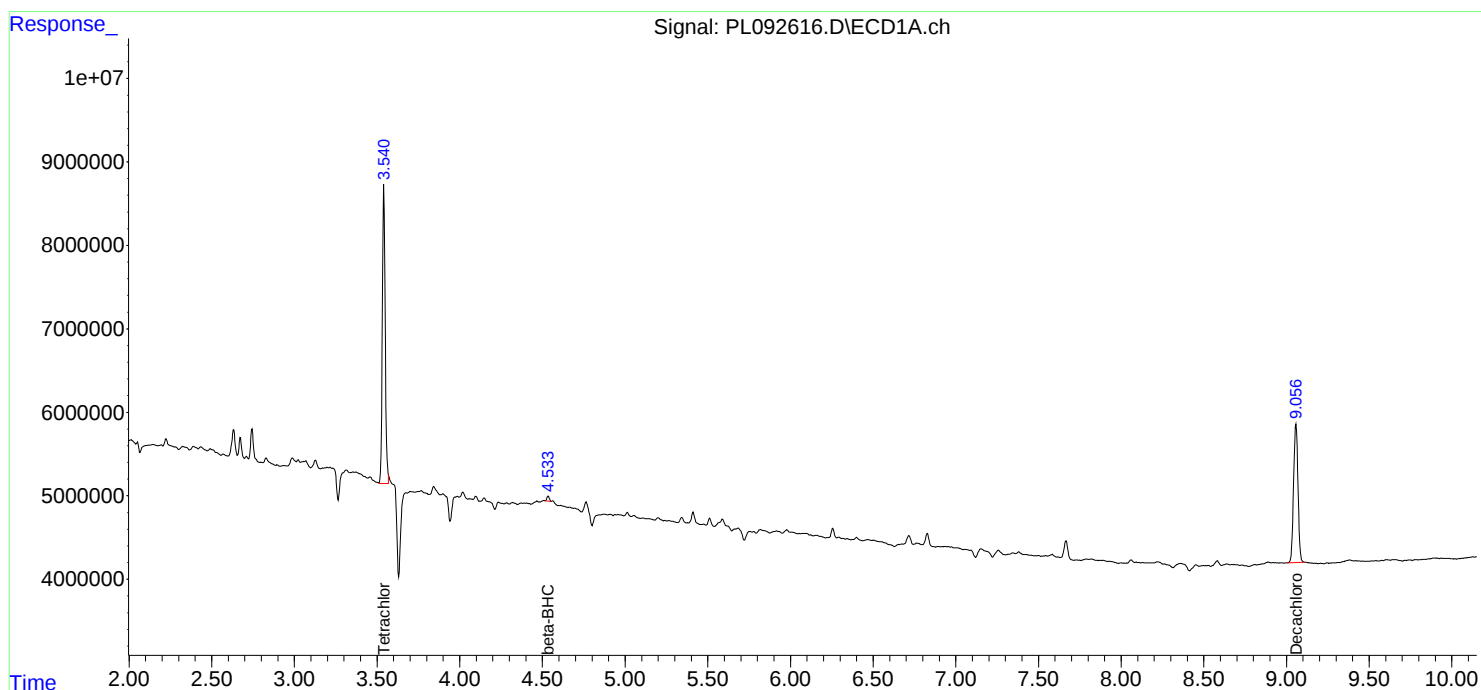

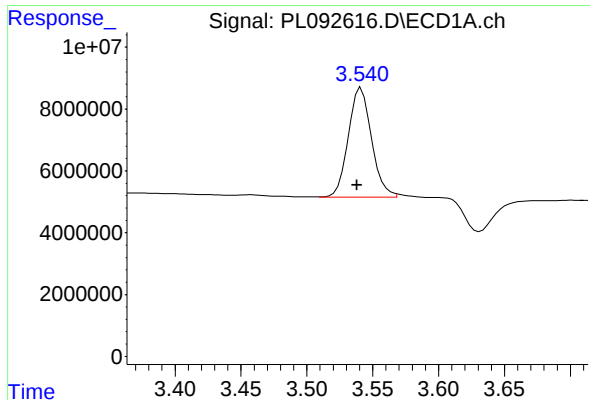


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: 0.002 min
Response: 43511884
Conc: 16.15 ng/ml

Instrument :
ECD_L
ClientSampleId :
BP-F23


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2024
Supervised By :Ankita Jodhani 10/28/2024

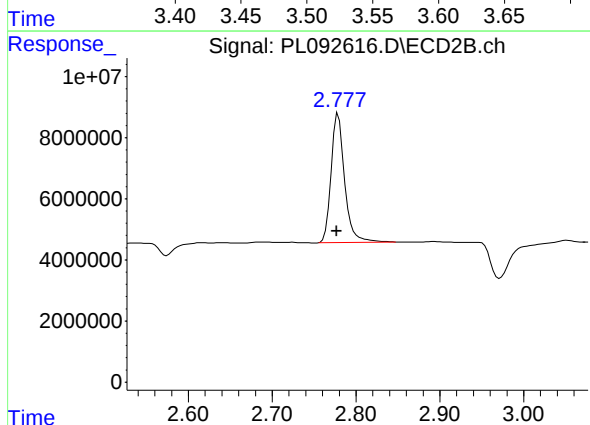


#1 Tetrachloro-m-xylene

R.T.: 2.777 min
Delta R.T.: 0.000 min
Response: 47753206
Conc: 17.19 ng/ml

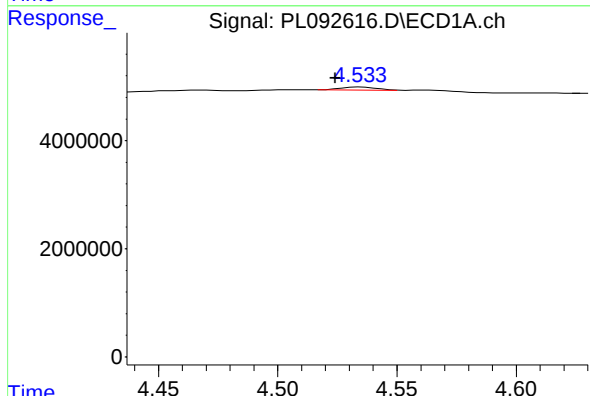


#6 beta-BHC

R.T.: 4.533 min
Delta R.T.: 0.009 min
Response: 597581
Conc: 0.38 ng/ml

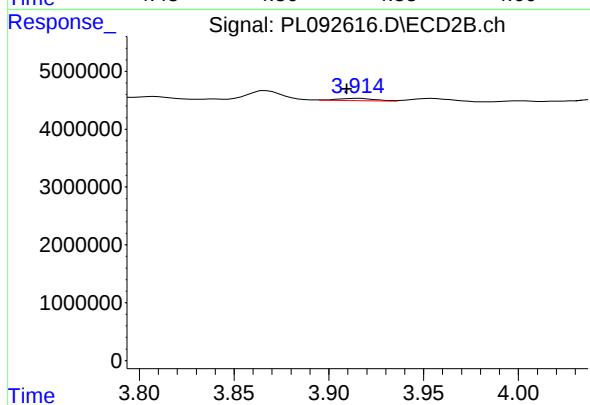

#6 beta-BHC

R.T.: 3.915 min
Delta R.T.: 0.006 min
Response: 548271
Conc: 0.31 ng/ml

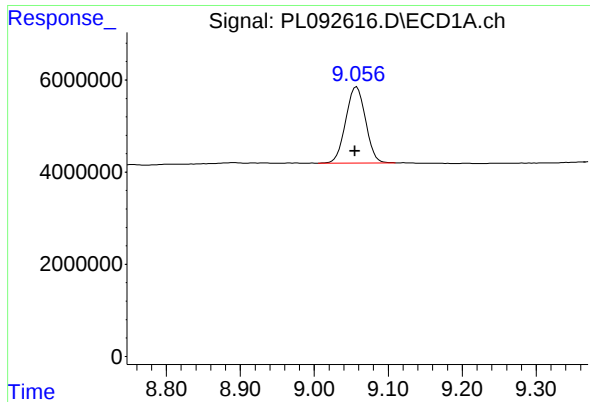


#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: 0.002 min
Response: 30756418
Conc: 15.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
BP-F23

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/25/2024
Supervised By :Ankita Jodhani 10/28/2024

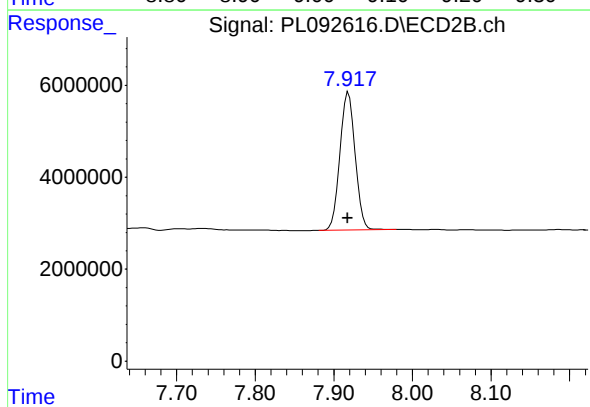

#28 Decachlorobiphenyl

R.T.: 7.919 min
Delta R.T.: 0.001 min
Response: 40325725
Conc: 15.30 ng/ml