

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041340.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 10:54
 Operator : AJ\SJ
 Sample : 5 PPB MIREX
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 5 PPB MIREX

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 03:57:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) A	alpha-BHC	3.910	0.000	3836655	0	0.484	N.D.	#
6) B	beta-BHC	0.000	4.995f	0	2707368	N.D.	1.689	#
16) A	4,4'-DDD	6.231f	0.000	2229038	0	0.493	N.D.	#
23)	Chlordane-1	4.395	0.000	4667472	0	18.288	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041340.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 10:54
Operator : AJ\SJ
Sample : 5 PPB MIREX
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
5 PPB MIREX

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 03:57:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

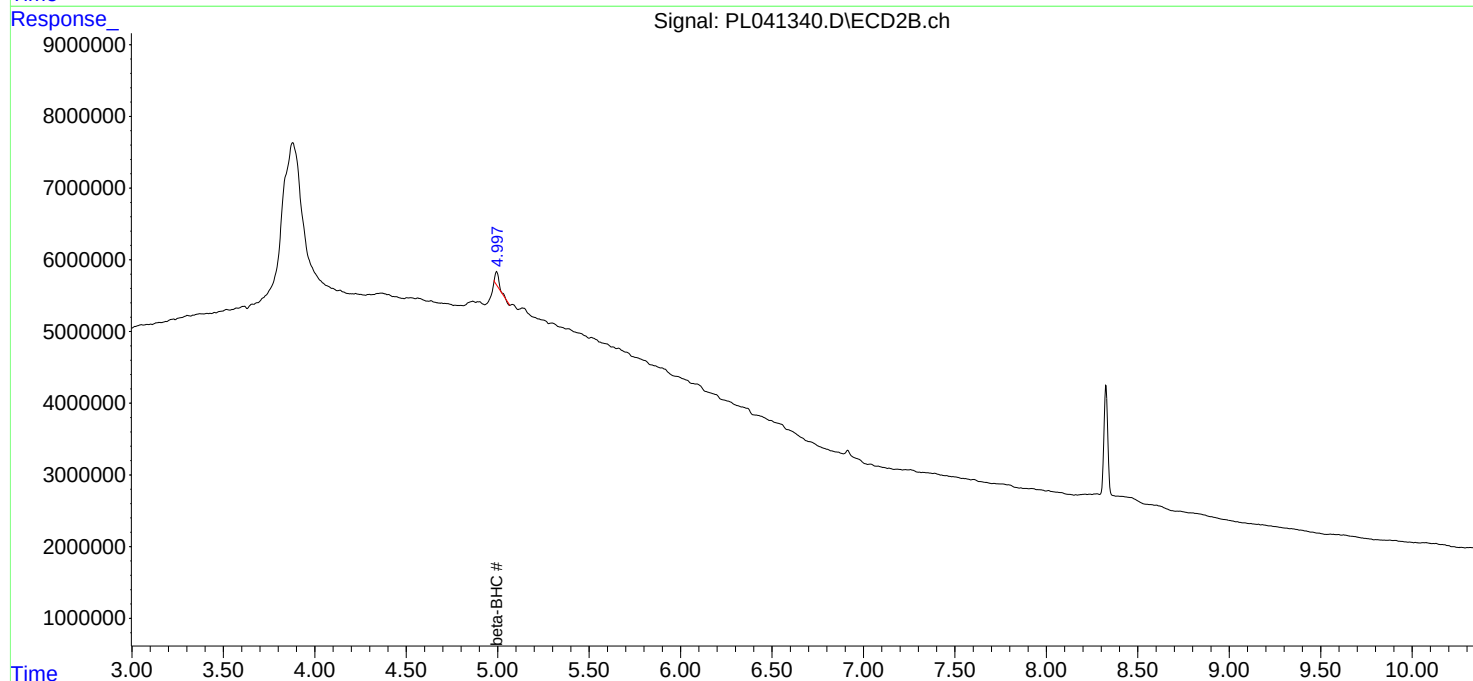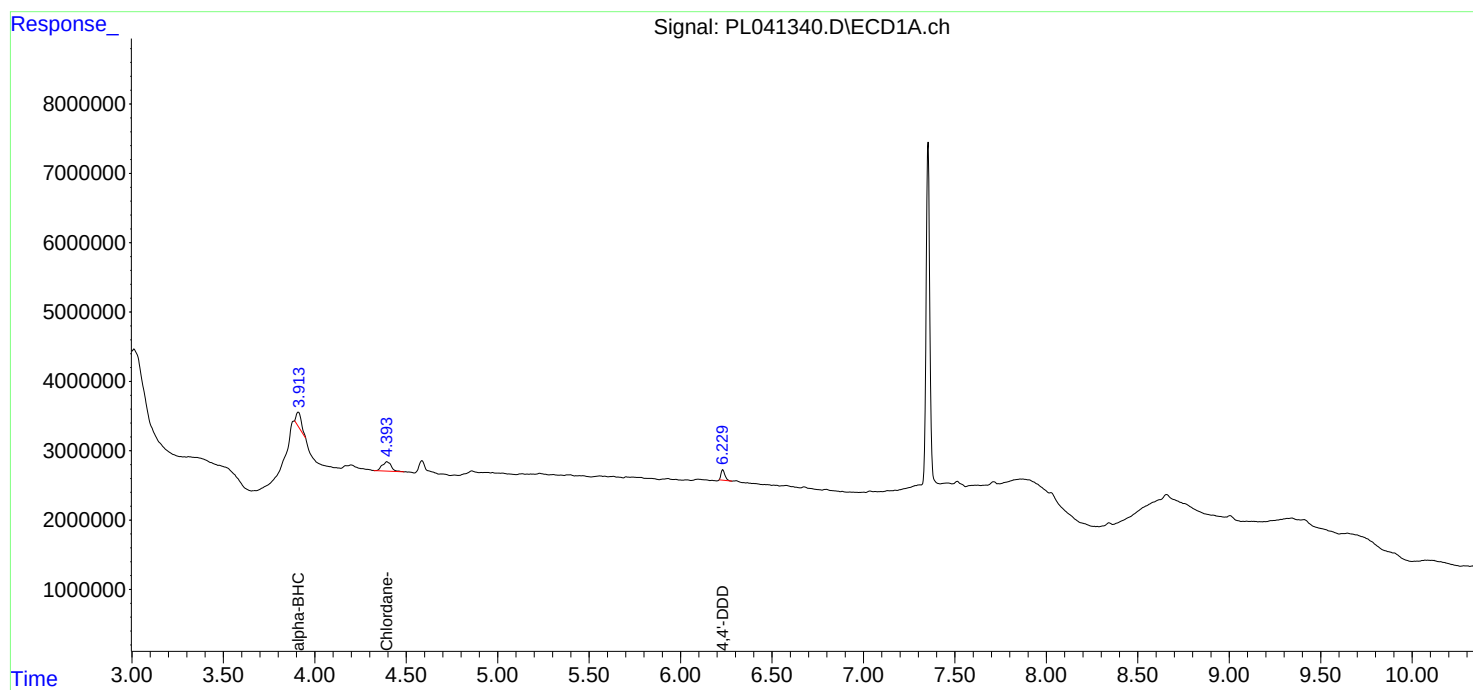


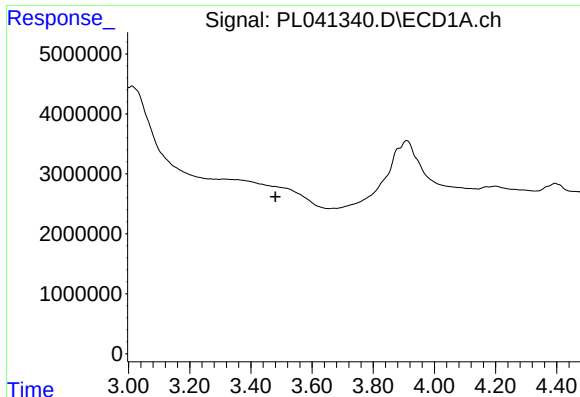

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T.: 3.480 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
5 PPB MIREX

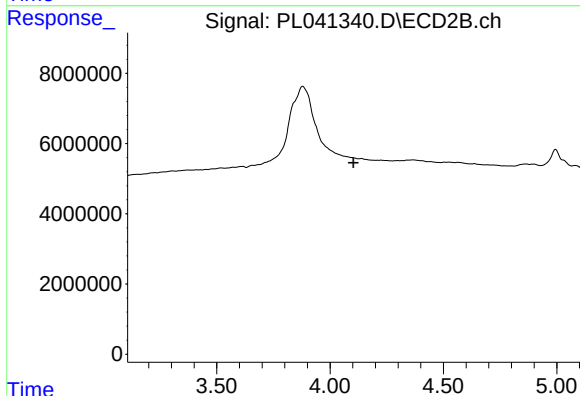


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T.: 4.104 min
Response: 0
Conc: N.D.

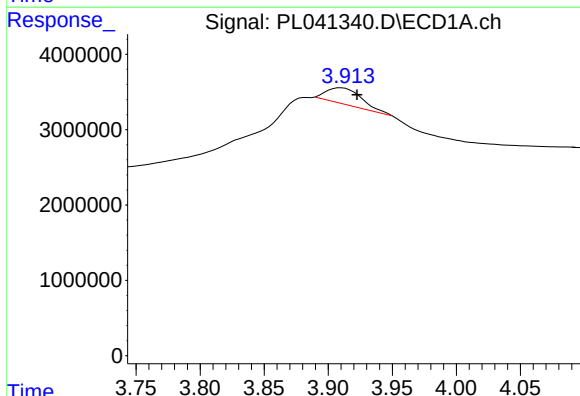


#2 alpha-BHC

R.T.: 3.910 min
Delta R.T.: -0.012 min
Response: 3836655
Conc: 0.48 ng/ml

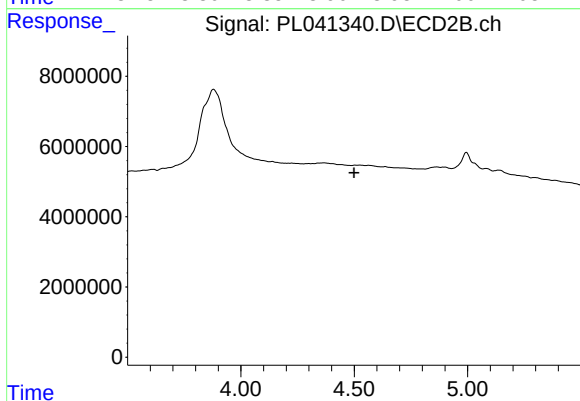

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.499 min
Response: 0
Conc: N.D.

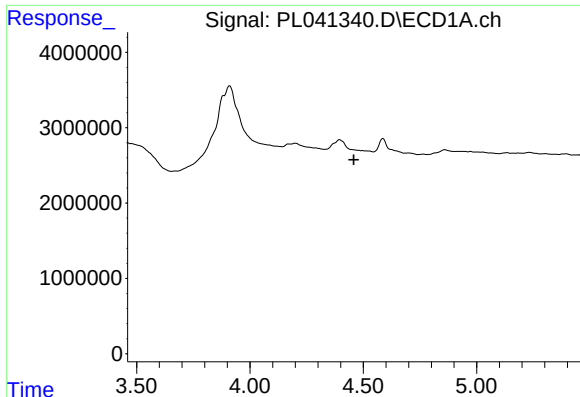

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
5 PPB MIREX

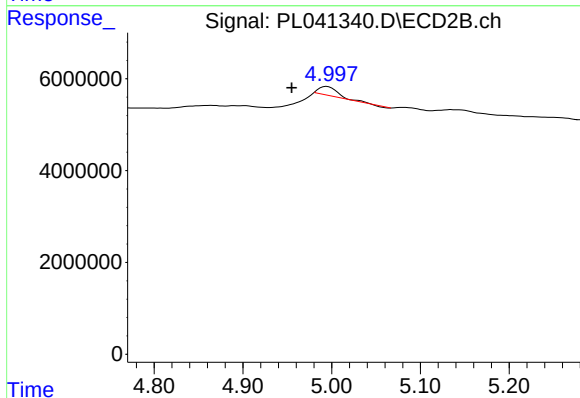


#6 beta-BHC

R.T.: 4.995 min
Delta R.T.: 0.040 min
Response: 2707368
Conc: 1.69 ng/ml

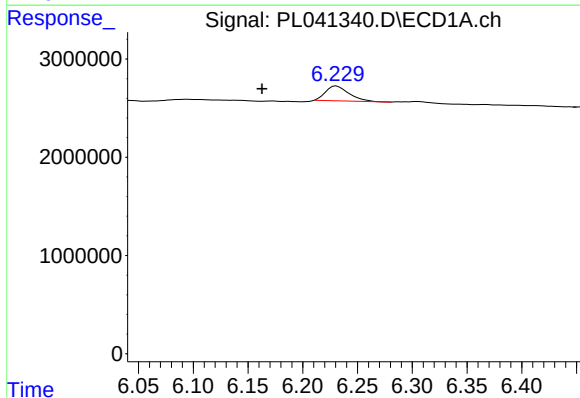


#16 4,4'-DDD

R.T.: 6.231 min
Delta R.T.: 0.068 min
Response: 2229038
Conc: 0.49 ng/ml

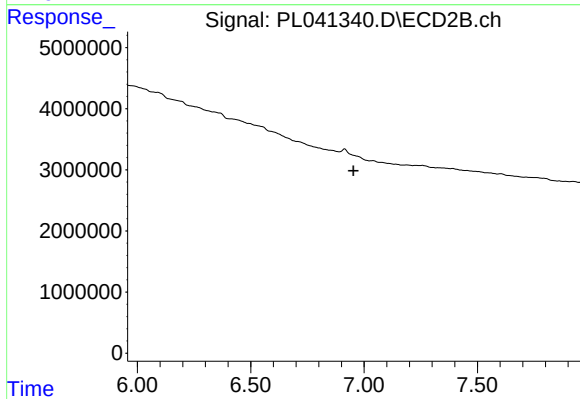

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.954 min
Response: 0
Conc: N.D.

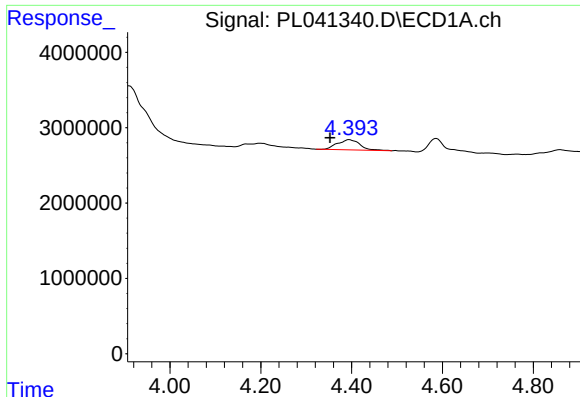

#23 Chlordane-1


R.T.: 4.395 min
Delta R.T.: 0.042 min
Response: 4667472
Conc: 18.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
5 PPB MIREX

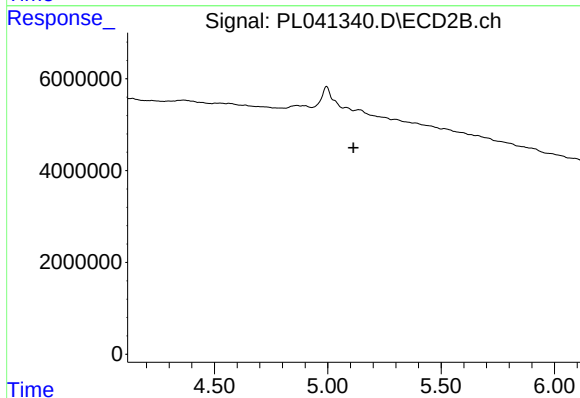


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

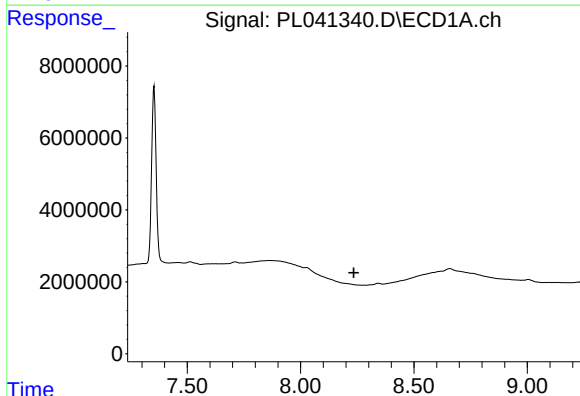

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.234 min
Response: 0
Conc: N.D.

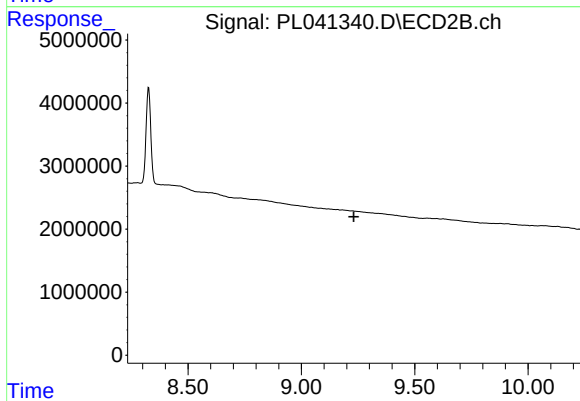

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.231 min
Response: 0
Conc: N.D.