

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041352.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 15:21
 Operator : AJ\SJ
 Sample : J5649-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DL-02B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:00:37 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.104	107.8E6	57206234	19.661	20.517
28)	SA Decachlor...	8.221	9.236	102.7E6	43367845	19.757	16.771
Target Compounds							
4)	MA Heptachlor	4.481	5.356f	2073914	3207776	0.281	0.948 #
6)	B beta-BHC	4.481	4.997f	2073914	2804402	0.654	1.750 #
12)	B 4,4'-DDE	5.655	0.000	3611567	0	0.635	N.D. #
15)	B Endosulfa...	6.246f	0.000	5702761	0	1.017	N.D. #
20)	A Methoxychlor	6.982	0.000	458047	0	0.176	N.D. #
23)	Chlordane-1	4.369	0.000	2685930	0	10.524	N.D. #
24)	Chlordane-2	4.817	0.000	994616	0	3.685	N.D. #
27)	Chlordane-5	6.246	0.000	5702761	0	26.314	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041352.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 15:21
Operator : AJ\SJ
Sample : J5649-04
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
DL-02B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:00:37 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

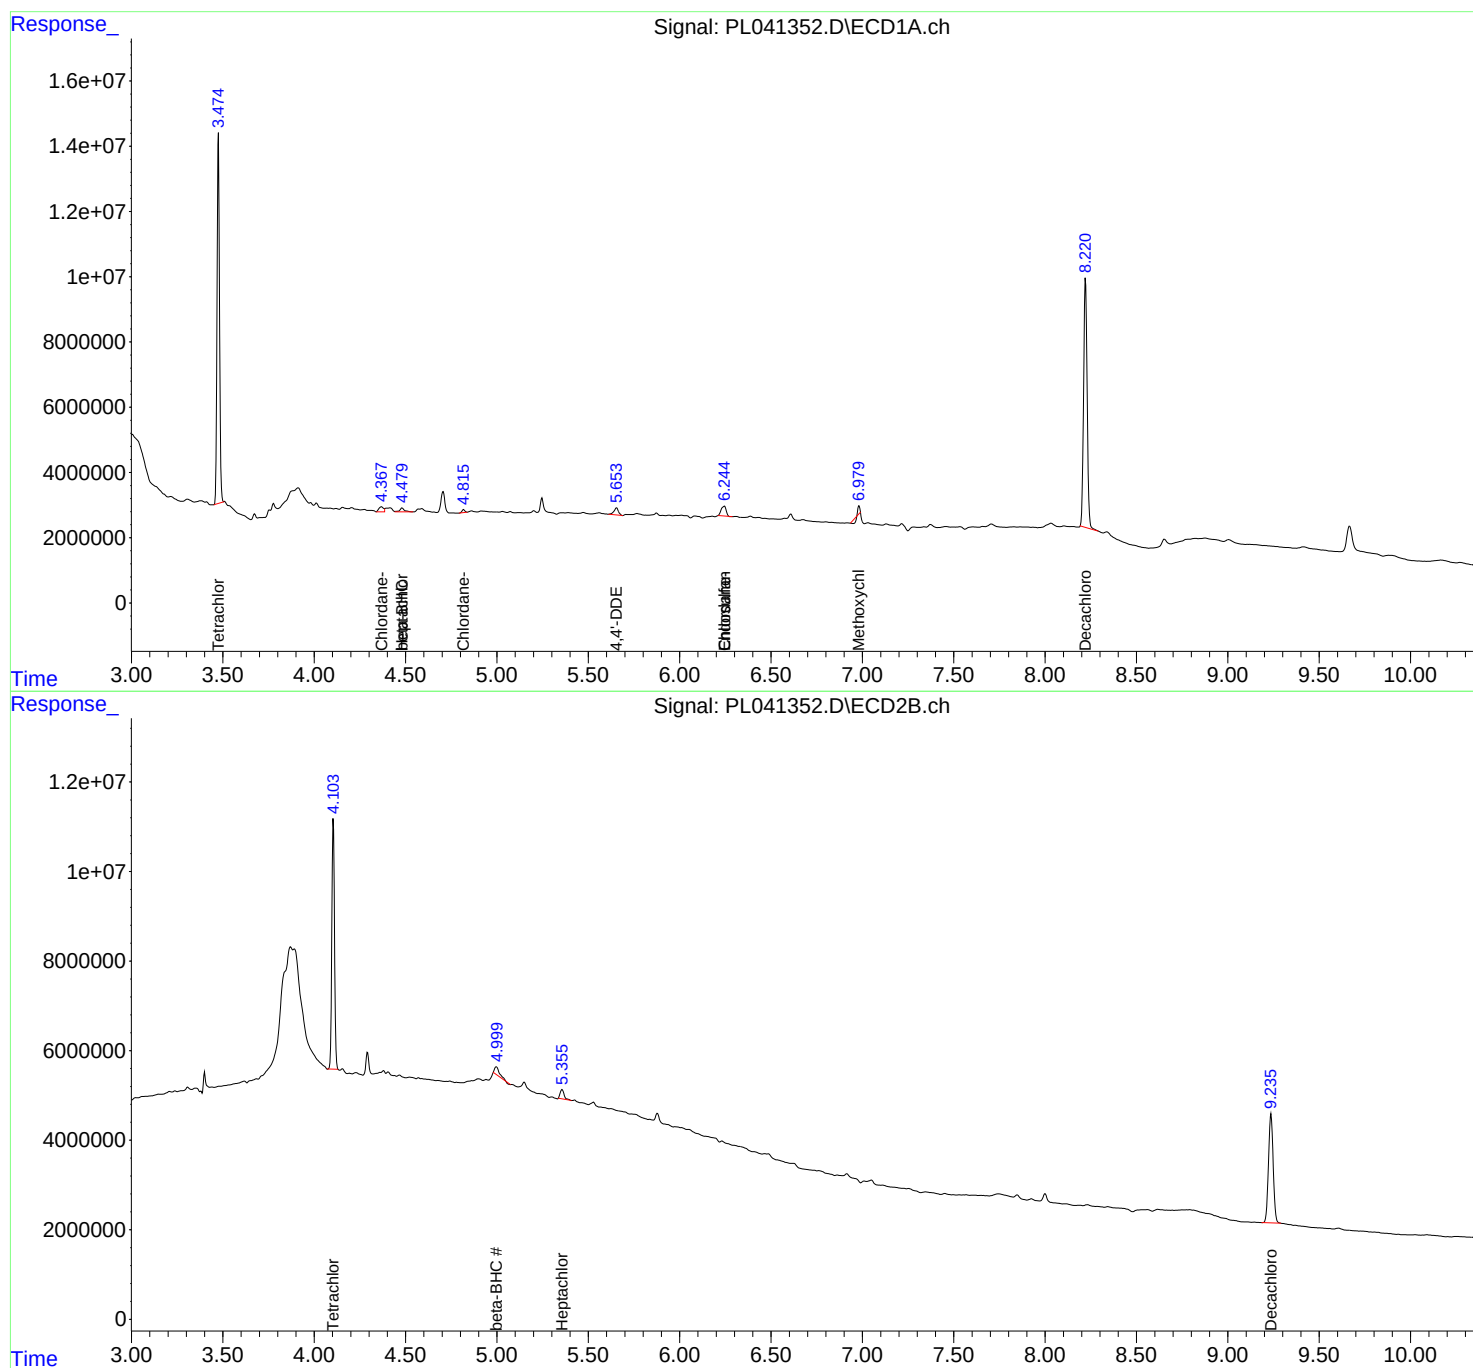


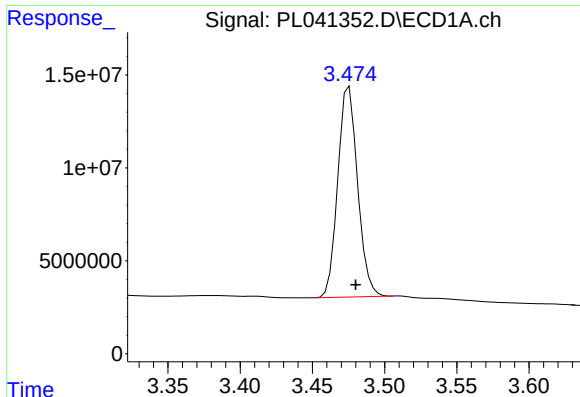

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 107754373
Conc: 19.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-02B

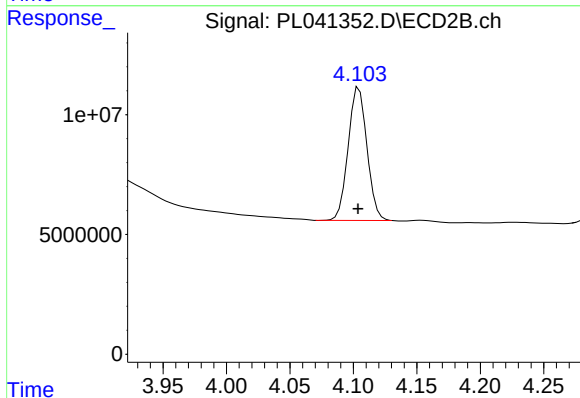


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 57206234
Conc: 20.52 ng/ml

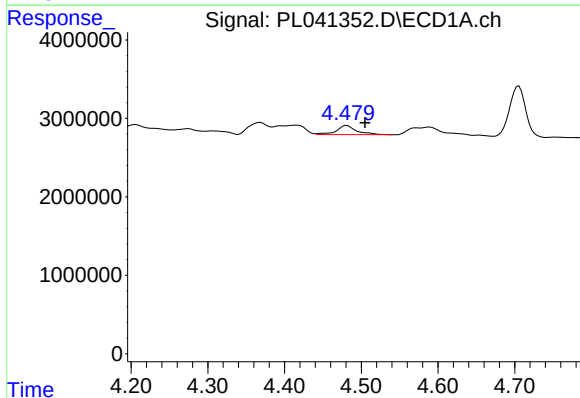


#4 Heptachlor

R.T.: 4.481 min
Delta R.T.: -0.024 min
Response: 2073914
Conc: 0.28 ng/ml

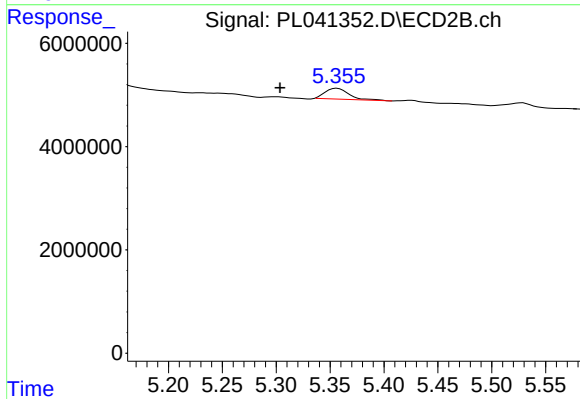

#4 Heptachlor


R.T.: 5.356 min
Delta R.T.: 0.053 min
Response: 3207776
Conc: 0.95 ng/ml

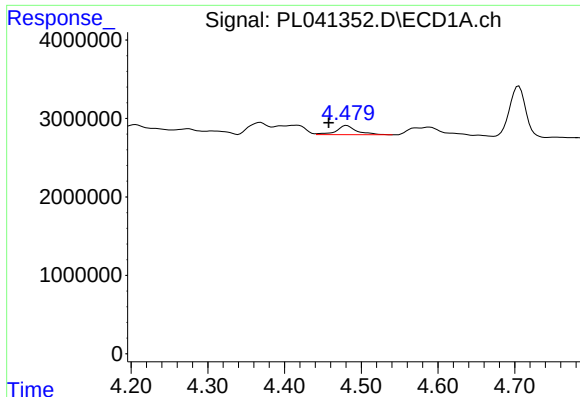

#6 beta-BHC


R.T.: 4.481 min
Delta R.T.: 0.023 min
Response: 2073914
Conc: 0.65 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-02B

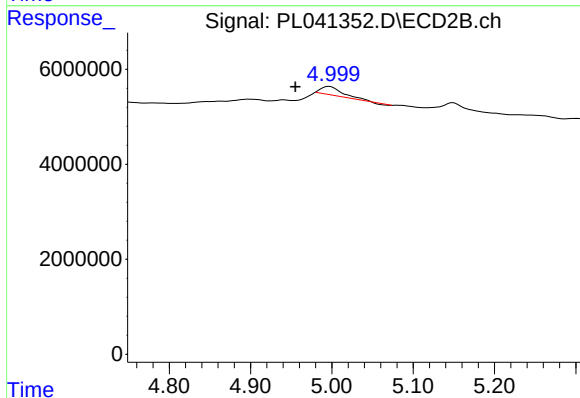


#6 beta-BHC

R.T.: 4.997 min
Delta R.T.: 0.042 min
Response: 2804402
Conc: 1.75 ng/ml

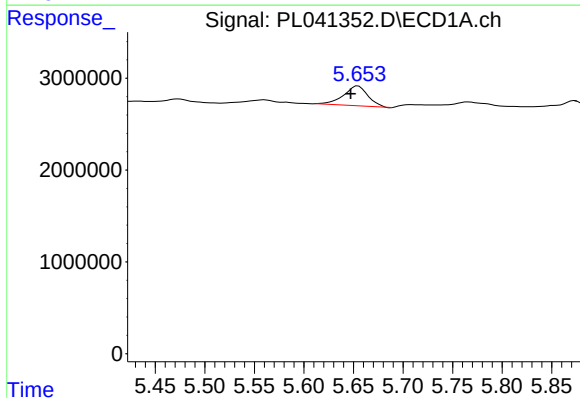


#12 4,4'-DDE

R.T.: 5.655 min
Delta R.T.: 0.007 min
Response: 3611567
Conc: 0.64 ng/ml

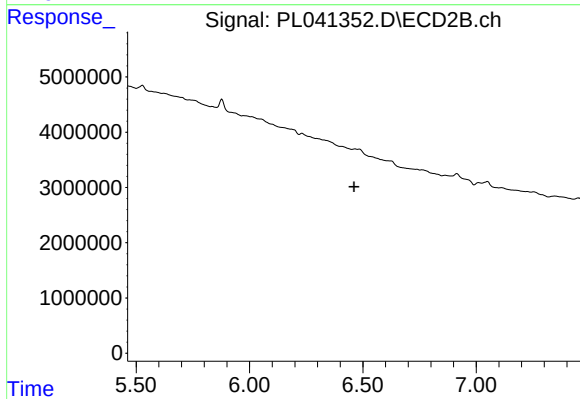

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.462 min
Response: 0
Conc: N.D.

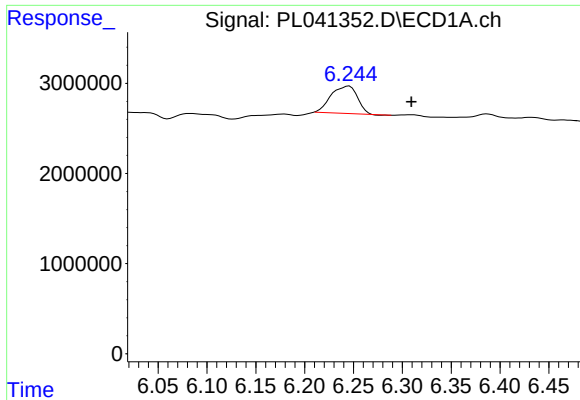

#15 Endosulfan II


R.T.: 6.246 min
Delta R.T.: -0.063 min
Response: 5702761
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-02B

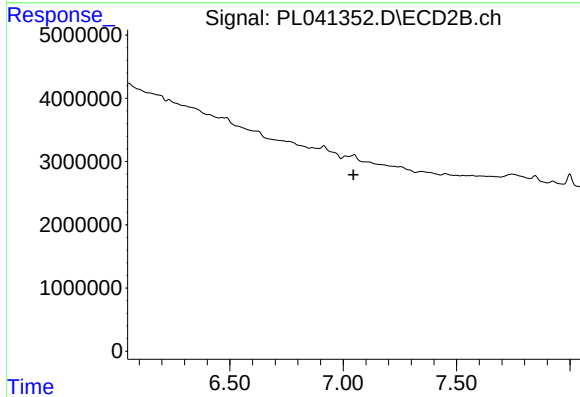


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 7.045 min
Response: 0
Conc: N.D.

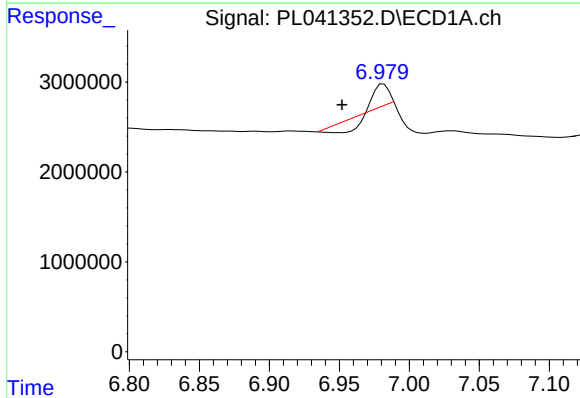


#20 Methoxychlor

R.T.: 6.982 min
Delta R.T.: 0.030 min
Response: 458047
Conc: 0.18 ng/ml

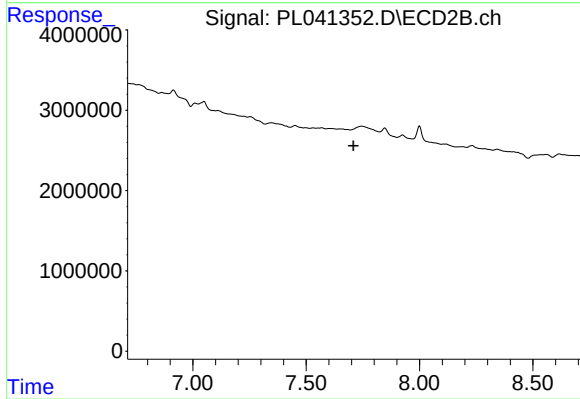

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

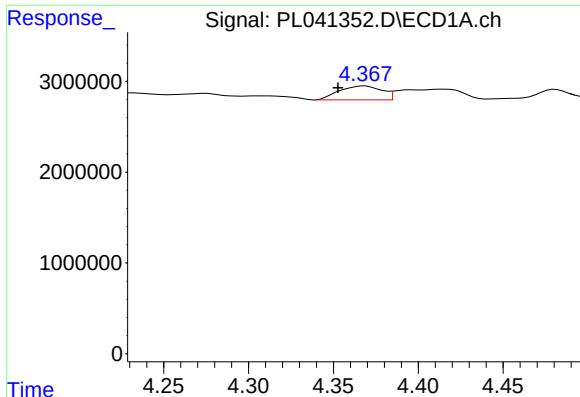

#23 Chlordane-1


R.T.: 4.369 min
Delta R.T.: 0.016 min
Response: 2685930
Conc: 10.52 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-02B

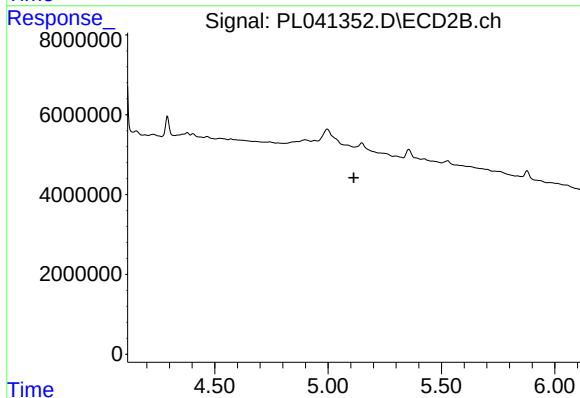


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

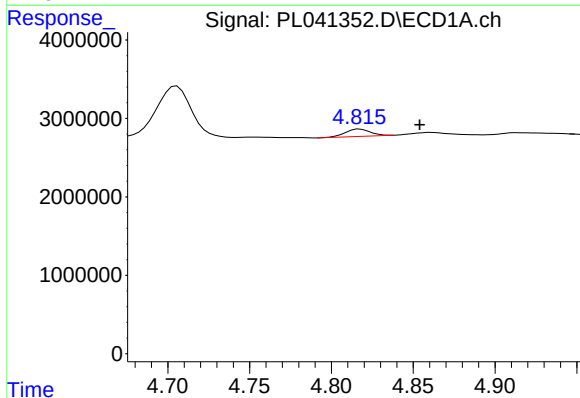


#24 Chlordane-2

R.T.: 4.817 min
Delta R.T.: -0.037 min
Response: 994616
Conc: 3.69 ng/ml

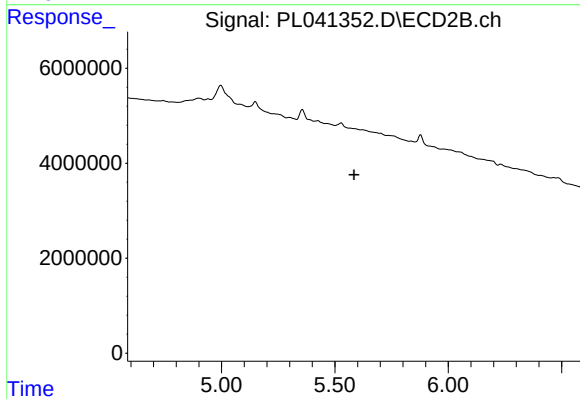

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.584 min
Response: 0
Conc: N.D.

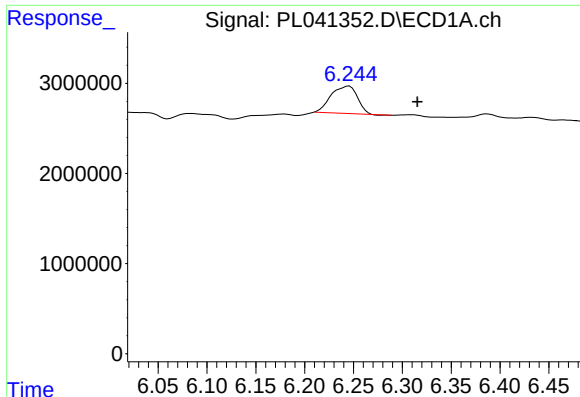

#27 Chlordane-5


R.T.: 6.246 min
Delta R.T.: -0.070 min
Response: 5702761
Conc: 26.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-02B

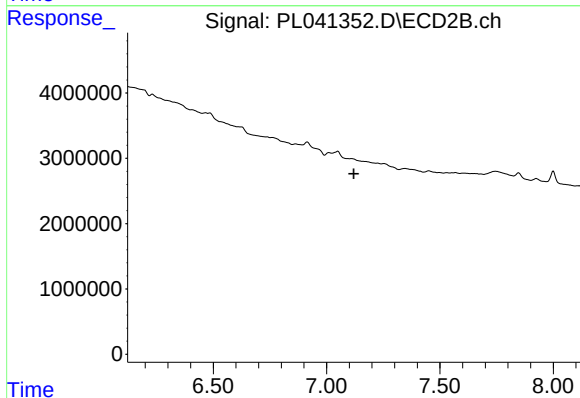


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.120 min
Response: 0
Conc: N.D.

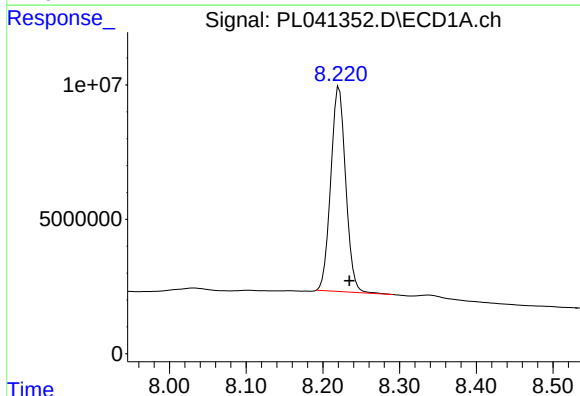

#28 Decachlorobiphenyl

R.T.: 8.221 min
Delta R.T.: -0.013 min
Response: 102725083
Conc: 19.76 ng/ml

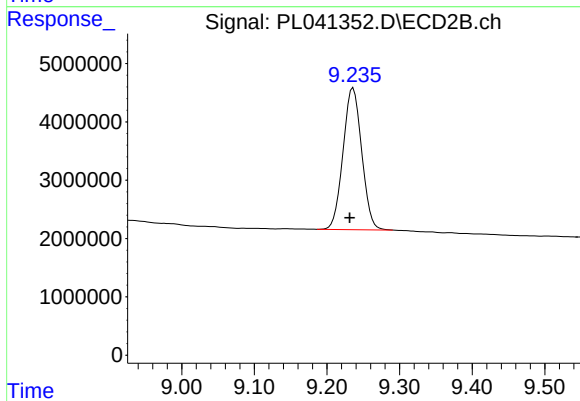

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.005 min
Response: 43367845
Conc: 16.77 ng/ml