

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041362.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 17:45
 Operator : AJ\SJ
 Sample : J5649-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DL-04B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:01:58 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.104	78674558	42071693	14.355	15.089
28)	SA Decachlor...	8.220	9.234	62038367	25063843	11.932	9.693
Target Compounds							
4)	MA Heptachlor	0.000	5.354f	0	1992277	N.D.	0.589 #
6)	B beta-BHC	0.000	4.995f	0	883021	N.D.	0.551 #
12)	B 4,4'-DDE	5.654	0.000	2281767	0	0.401	N.D. #
20)	A Methoxychlor	6.980	0.000	917253	0	0.353	N.D. #
23)	Chlordane-1	4.369	0.000	1143148	0	4.479	N.D. #
24)	Chlordane-2	4.817	0.000	919201	0	3.406	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041362.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 17:45
Operator : AJ\SJ
Sample : J5649-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DL-04B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:01:58 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

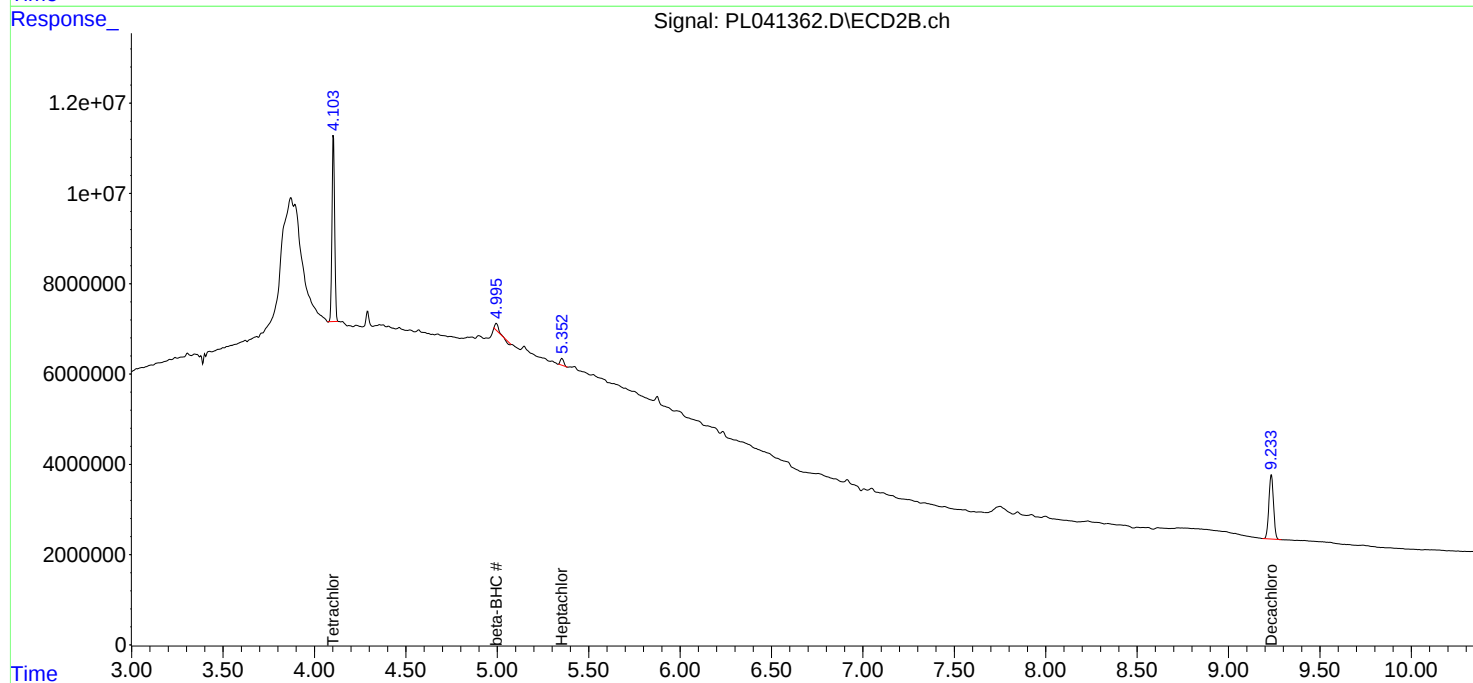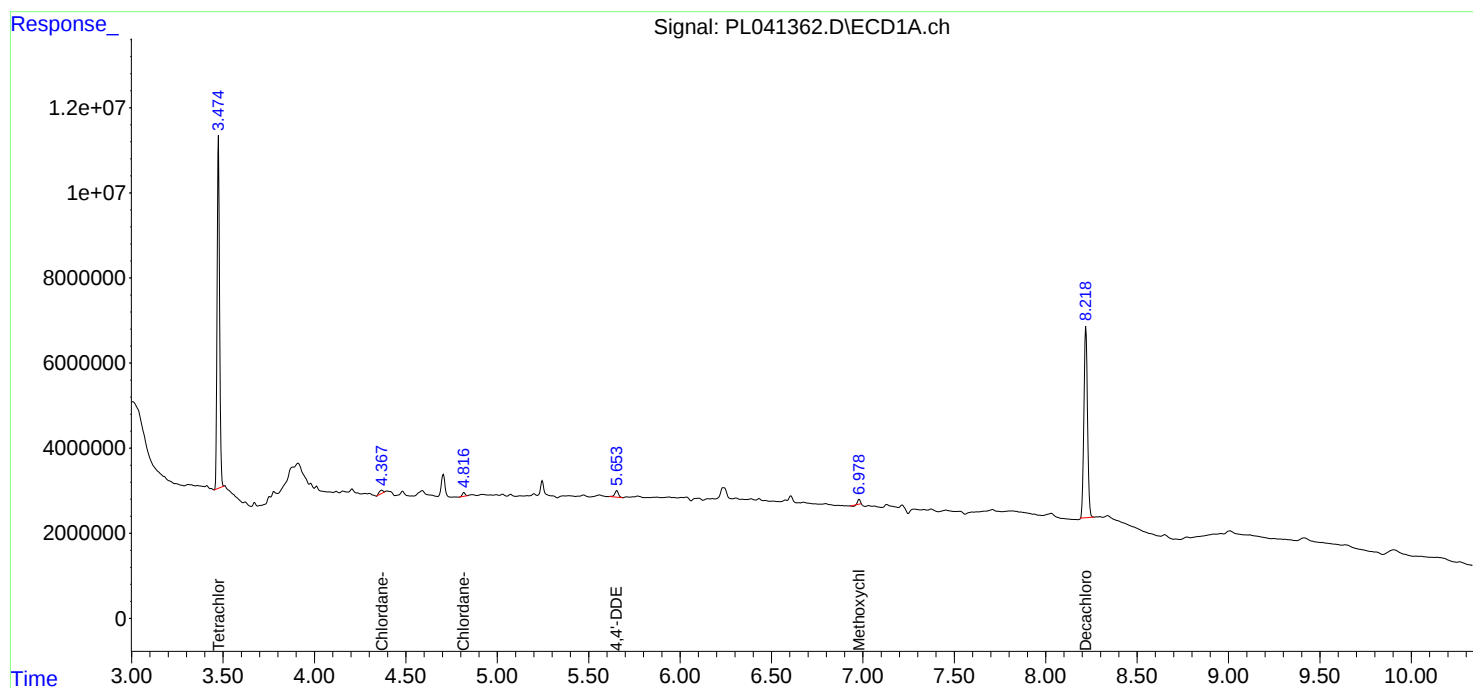


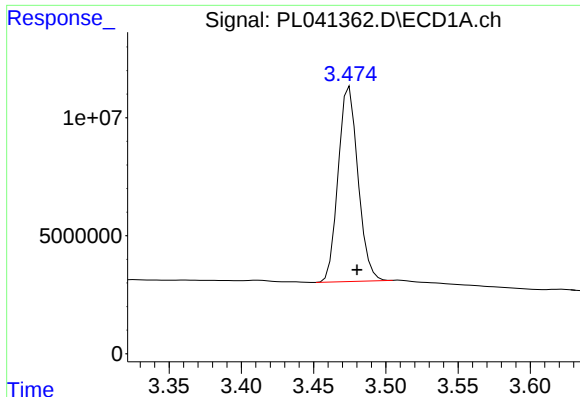

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 78674558
Conc: 14.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-04B

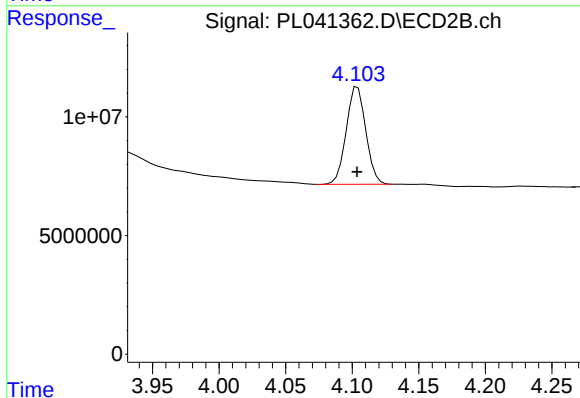


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 42071693
Conc: 15.09 ng/ml

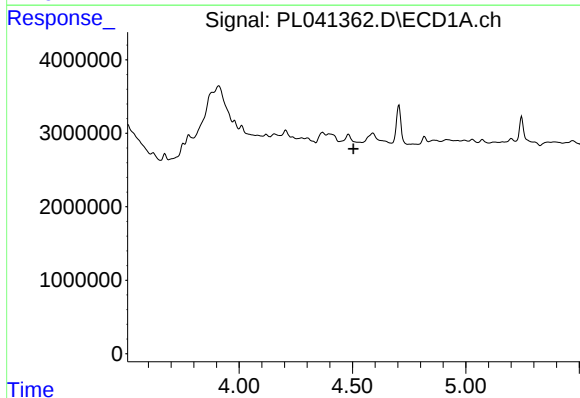


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.505 min
Response: 0
Conc: N.D.

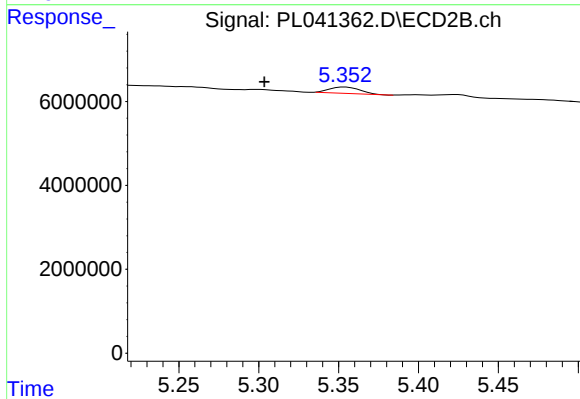

#4 Heptachlor


R.T.: 5.354 min
Delta R.T.: 0.050 min
Response: 1992277
Conc: 0.59 ng/ml

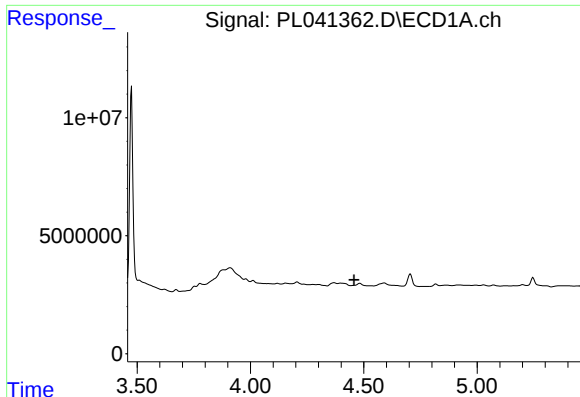

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
DL-04B

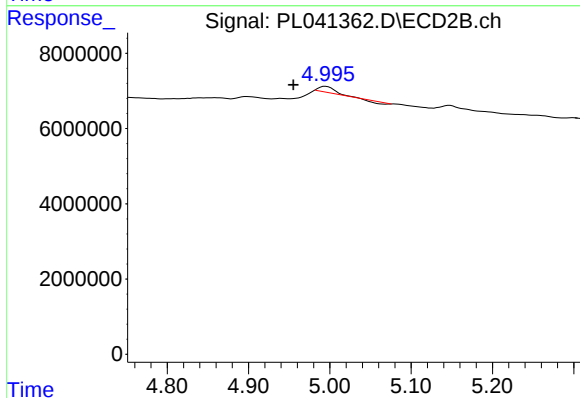


#6 beta-BHC

R.T.: 4.995 min
Delta R.T.: 0.040 min
Response: 883021
Conc: 0.55 ng/ml

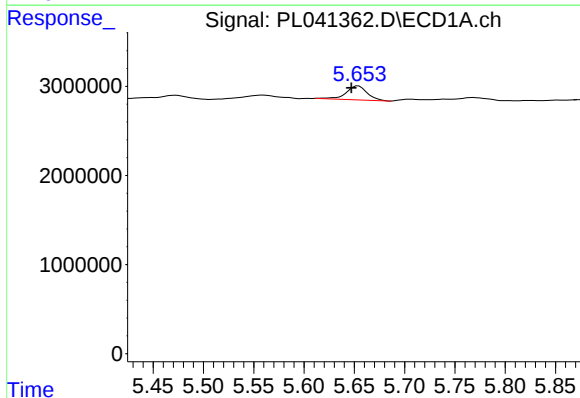


#12 4,4'-DDE

R.T.: 5.654 min
Delta R.T.: 0.007 min
Response: 2281767
Conc: 0.40 ng/ml

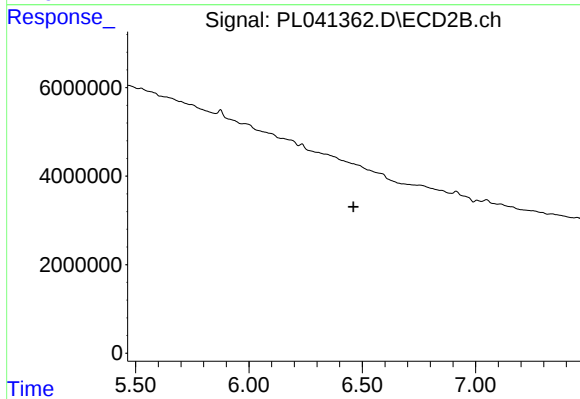

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 6.462 min
Response: 0
Conc: N.D.

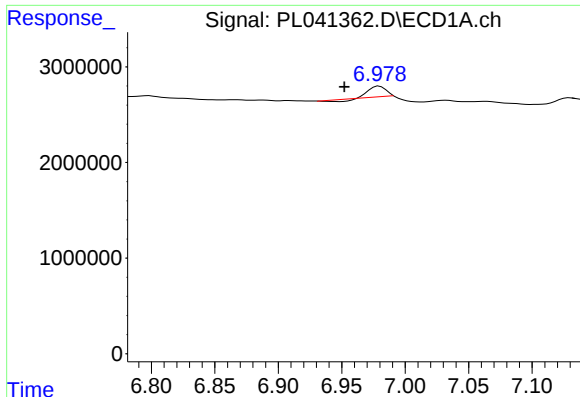

#20 Methoxychlor


R.T.: 6.980 min
Delta R.T.: 0.027 min
Response: 917253
Conc: 0.35 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-04B

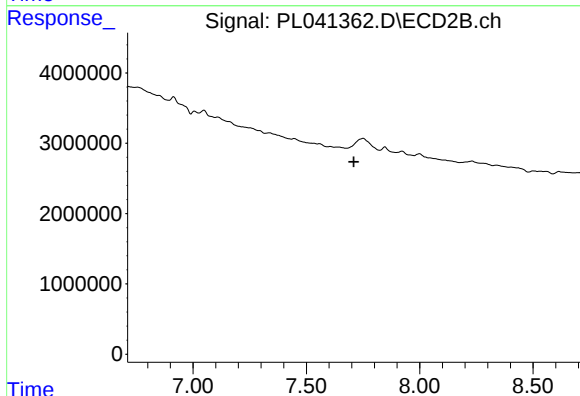


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

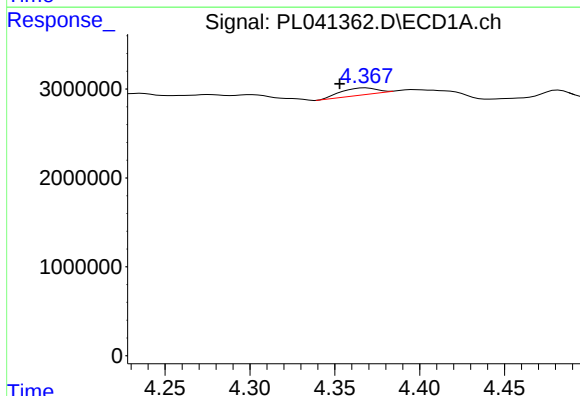


#23 Chlordane-1

R.T.: 4.369 min
Delta R.T.: 0.016 min
Response: 1143148
Conc: 4.48 ng/ml

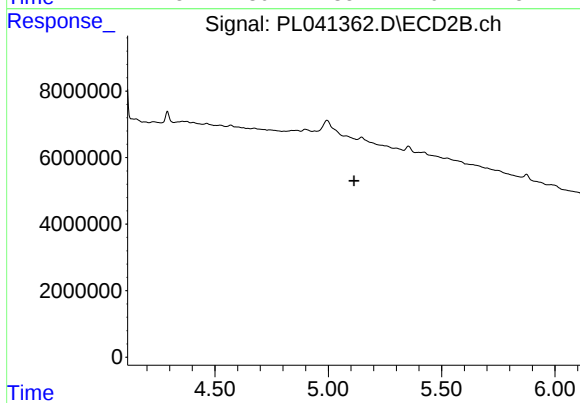

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

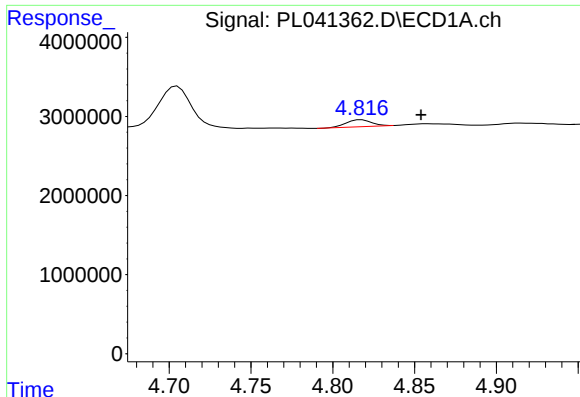

#24 Chlordane-2


R.T.: 4.817 min
Delta R.T.: -0.036 min
Response: 919201
Conc: 3.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-04B

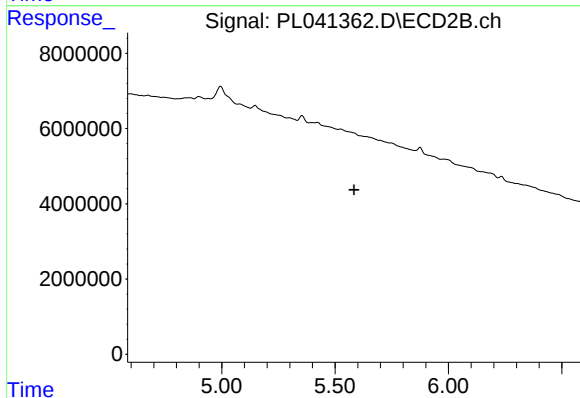


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.584 min
Response: 0
Conc: N.D.

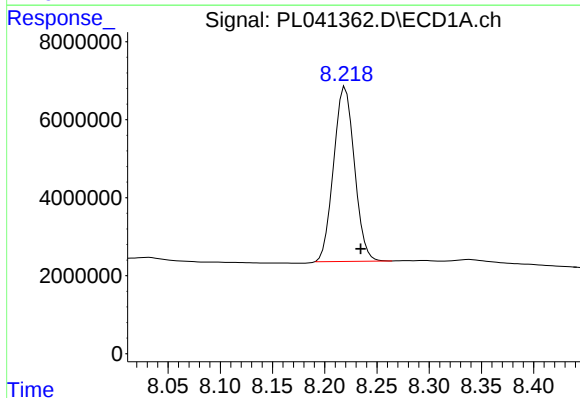

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.015 min
Response: 62038367
Conc: 11.93 ng/ml

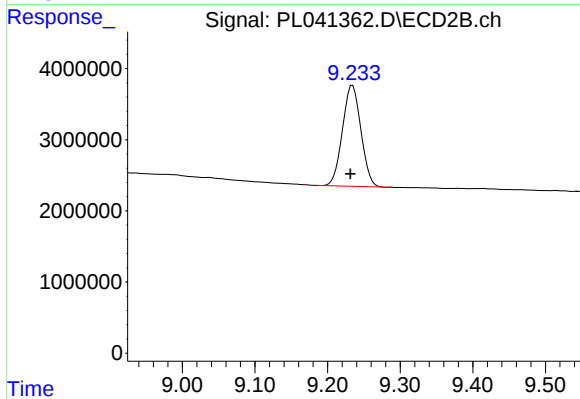

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.003 min
Response: 25063843
Conc: 9.69 ng/ml