

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041363.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 17:59
 Operator : AJ\SJ
 Sample : J5649-12
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DL-05A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:02:04 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.104	52838127	28024574	9.641	10.051
28)	SA Decachlor...	8.220	9.235	63214417	25069628	12.158	9.695
Target Compounds							
6)	B beta-BHC	0.000	4.996f	0	2066868	N.D.	1.290 #
17)	MA 4,4'-DDT	6.385	0.000	2661155	0	0.584	N.D. #
18)	B Endrin al...	6.428f	0.000	1068462	0	0.255	N.D. #
19)	B Endosulfa...	6.672	0.000	1982101	0	0.390	N.D. #
20)	A Methoxychlor	6.917f	0.000	2865022	0	1.101	N.D. #
21)	B Endrin ke...	7.248f	7.827f	3292590	2256306	0.629	0.959 #
23)	Chlordane-1	4.397	0.000	4036819	0	15.817	N.D. #
27)	Chlordane-5	6.385	0.000	2661155	0	12.279	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041363.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 17:59
Operator : AJ\SJ
Sample : J5649-12
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DL-05A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:02:04 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

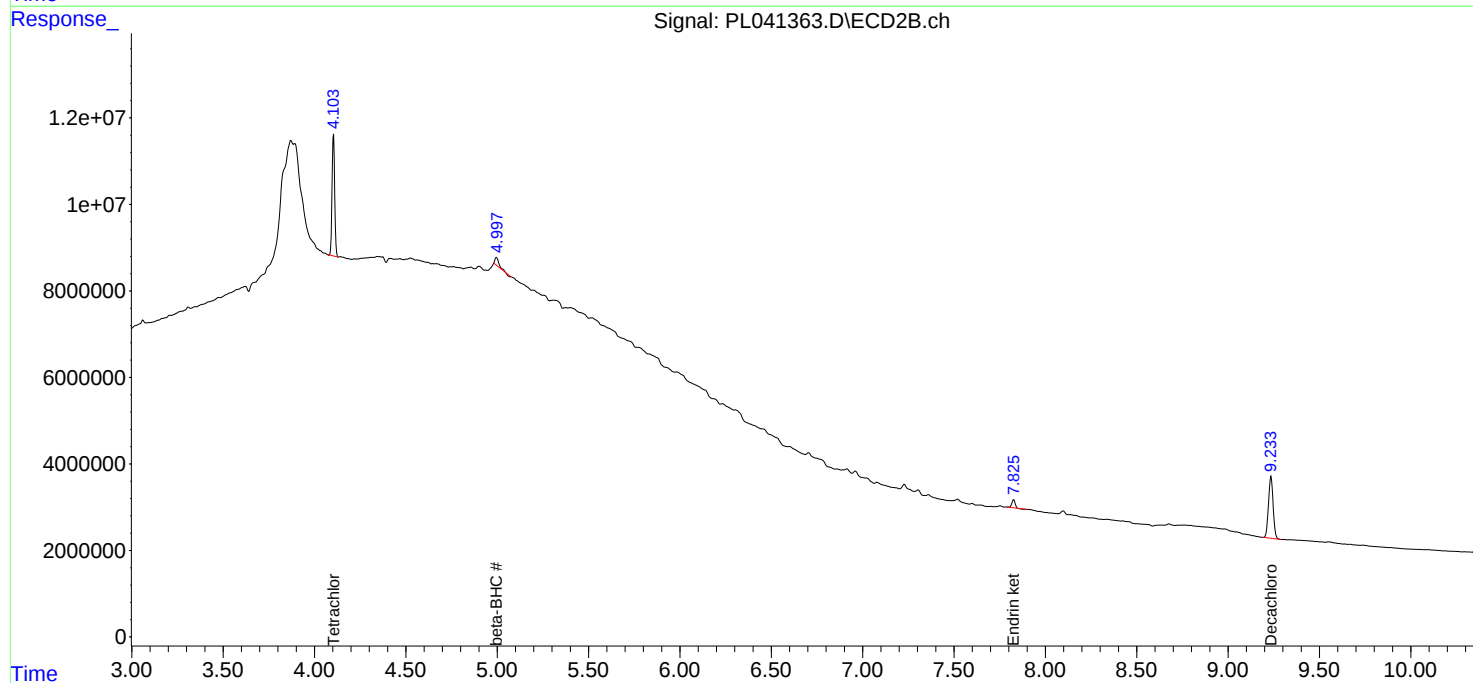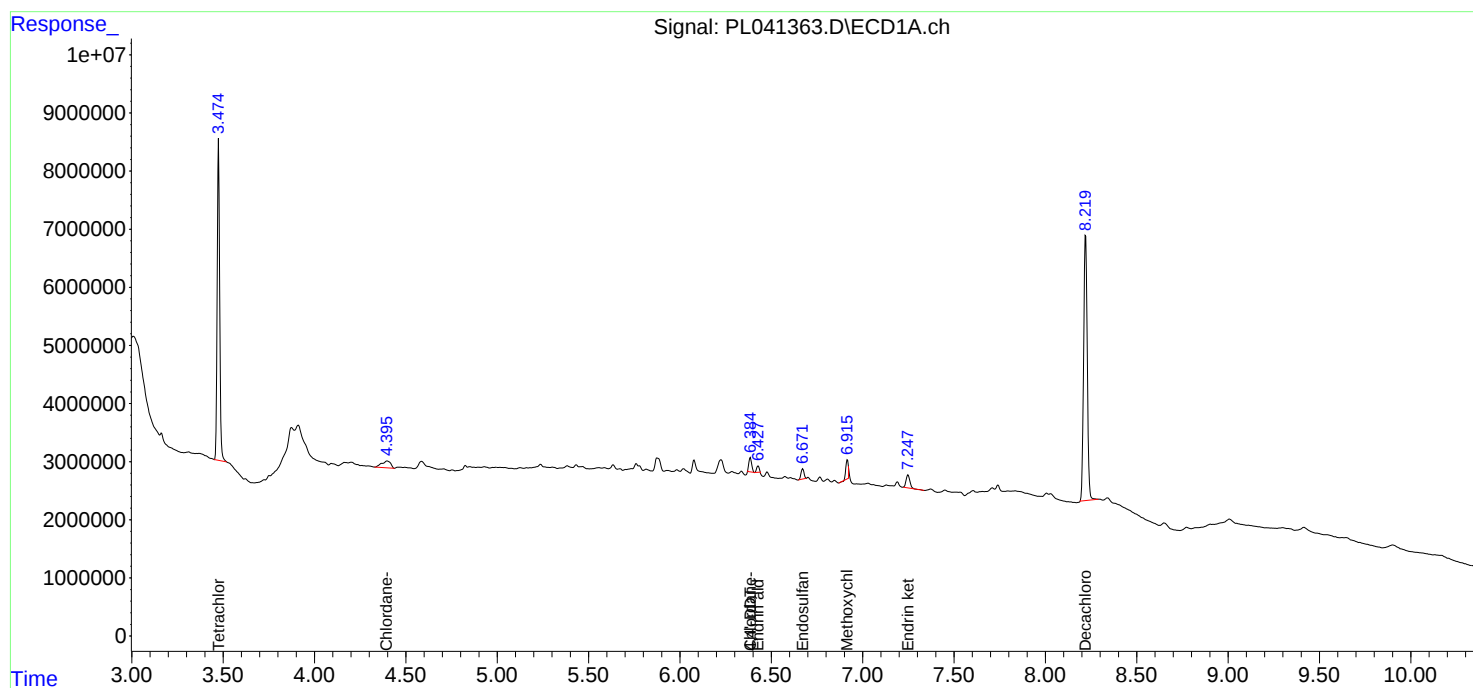


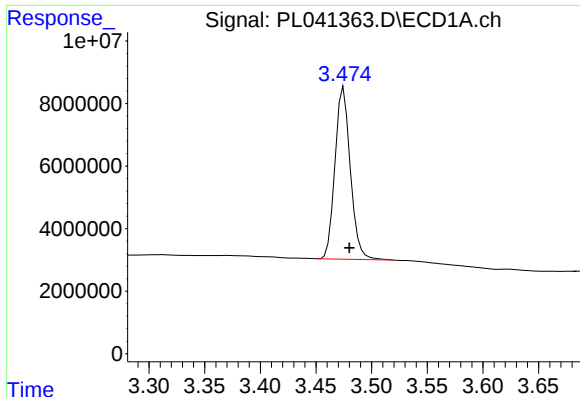

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 52838127
Conc: 9.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-05A

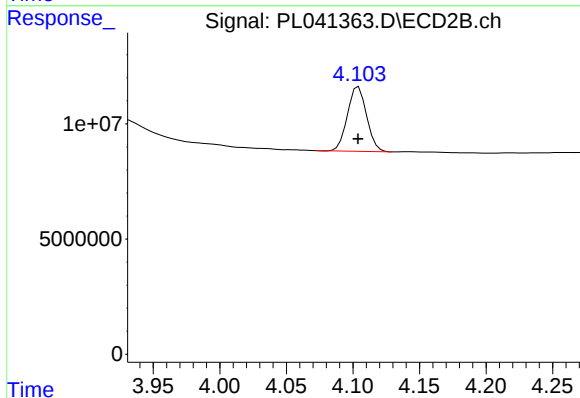


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 28024574
Conc: 10.05 ng/ml

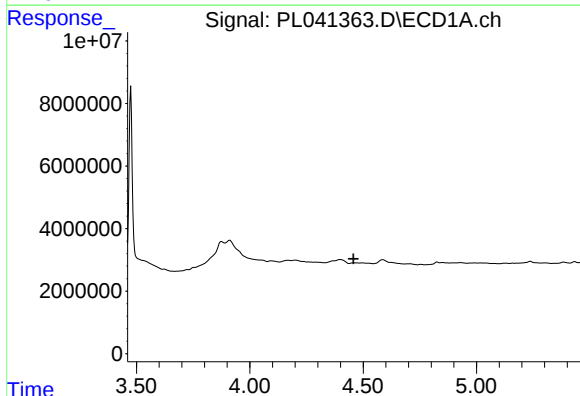


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.458 min
Response: 0
Conc: N.D.

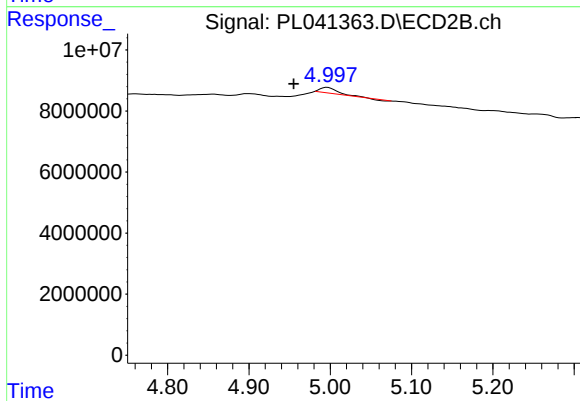

#6 beta-BHC


R.T.: 4.996 min
Delta R.T.: 0.041 min
Response: 2066868
Conc: 1.29 ng/ml

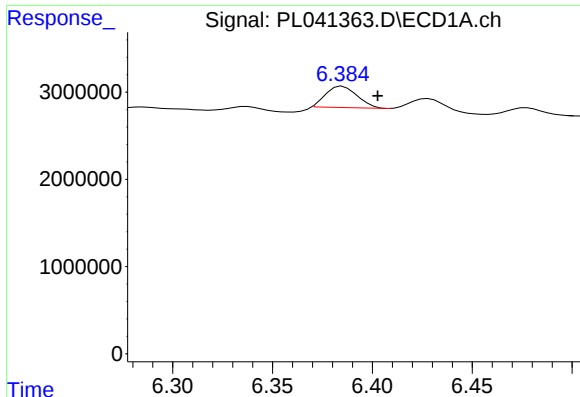

#17 4,4'-DDT


R.T.: 6.385 min
Delta R.T.: -0.018 min
Response: 2661155
Conc: 0.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-05A

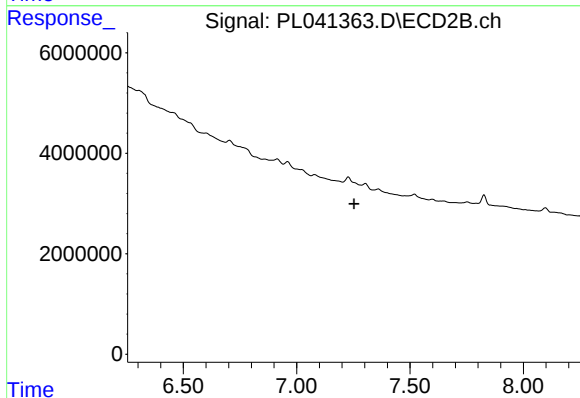


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

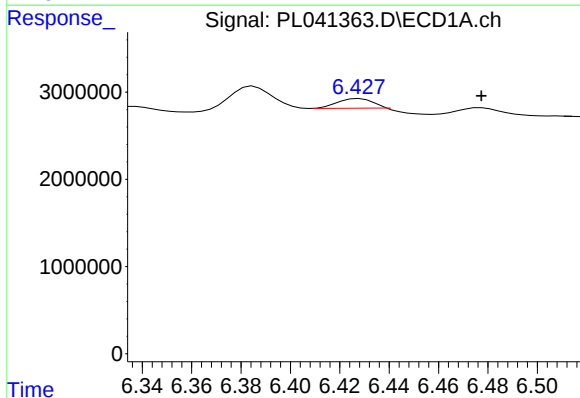


#18 Endrin aldehyde

R.T.: 6.428 min
Delta R.T.: -0.049 min
Response: 1068462
Conc: 0.25 ng/ml

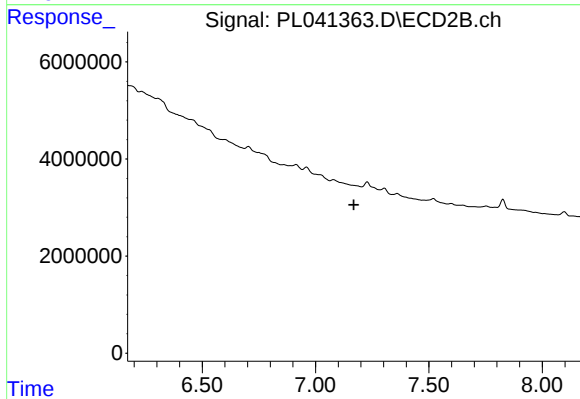

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T. : 7.169 min
Response: 0
Conc: N.D.

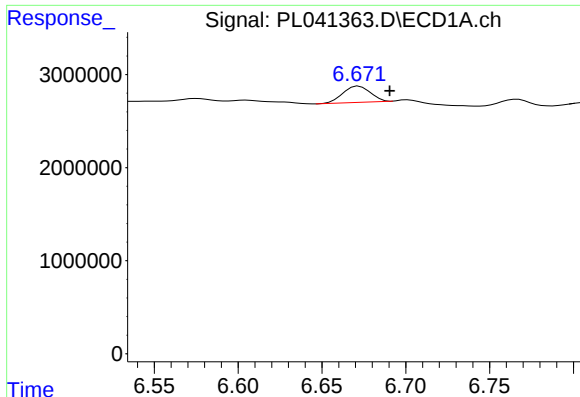

#19 Endosulfan Sulfate


R.T.: 6.672 min
Delta R.T.: -0.018 min
Response: 1982101
Conc: 0.39 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-05A

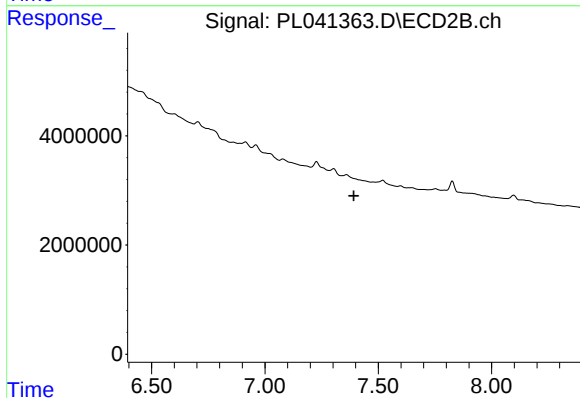


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

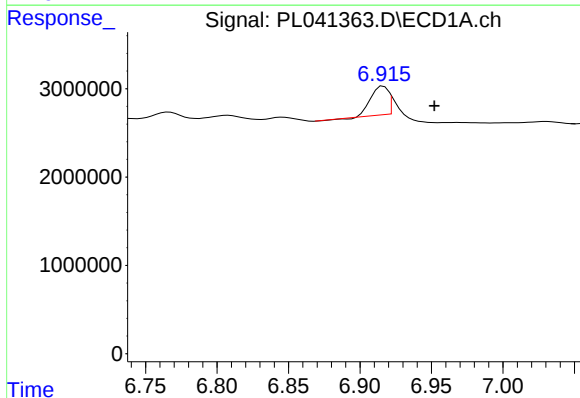


#20 Methoxychlor

R.T.: 6.917 min
Delta R.T.: -0.036 min
Response: 2865022
Conc: 1.10 ng/ml

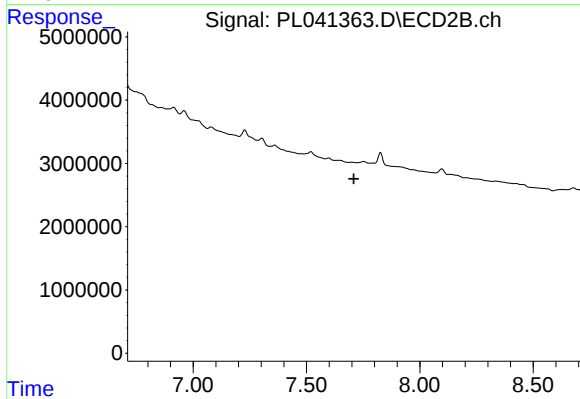

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

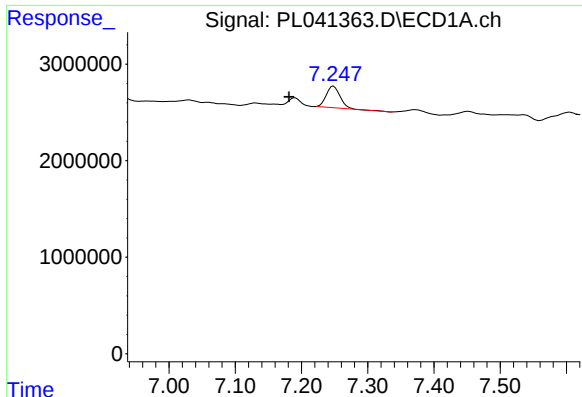

#21 Endrin ketone


R.T.: 7.248 min
Delta R.T.: 0.067 min
Response: 3292590
Conc: 0.63 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-05A

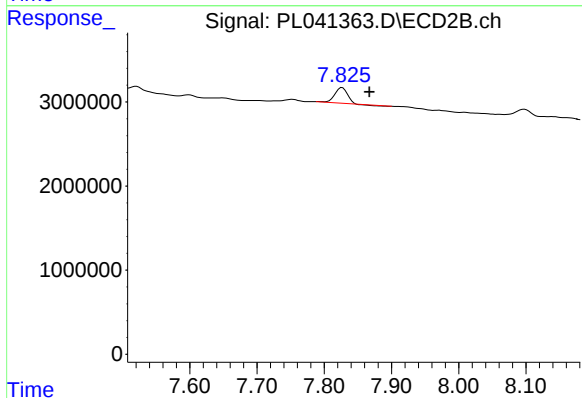


#21 Endrin ketone

R.T.: 7.827 min
Delta R.T.: -0.041 min
Response: 2256306
Conc: 0.96 ng/ml

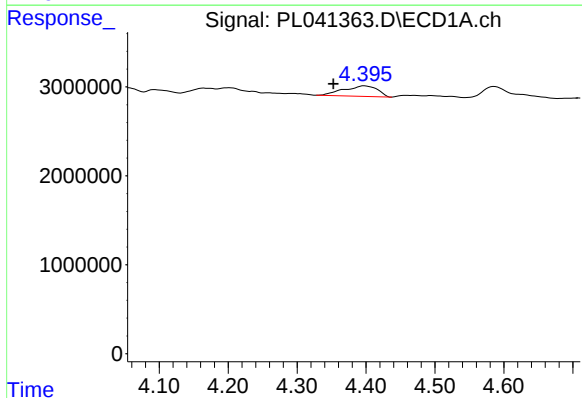


#23 Chlordane-1

R.T.: 4.397 min
Delta R.T.: 0.045 min
Response: 4036819
Conc: 15.82 ng/ml

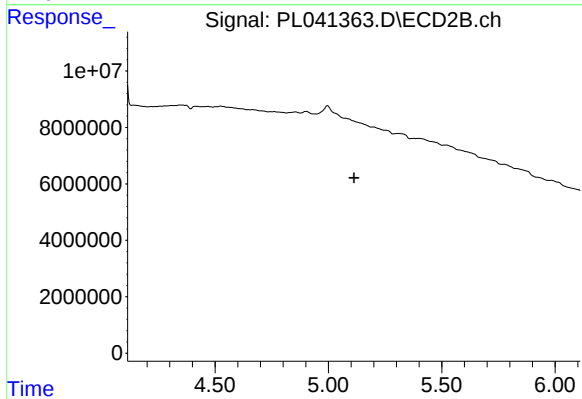

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.114 min
Response: 0
Conc: N.D.

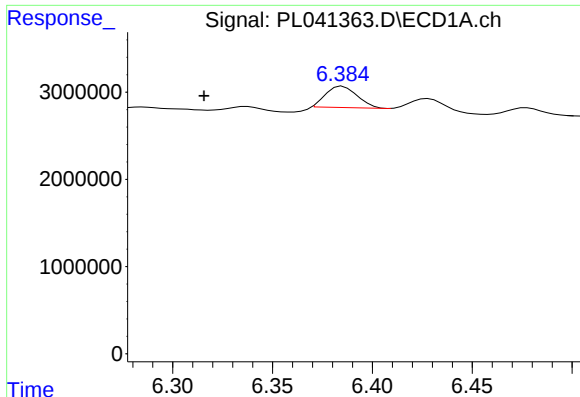

#27 Chlordane-5


R.T.: 6.385 min
Delta R.T.: 0.069 min
Response: 2661155
Conc: 12.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-05A

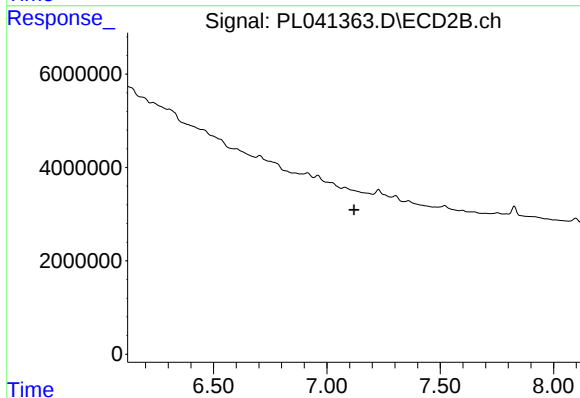


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 7.120 min
Response: 0
Conc: N.D.

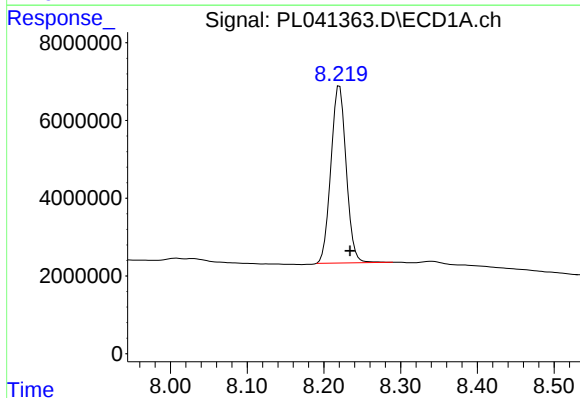

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 63214417
Conc: 12.16 ng/ml

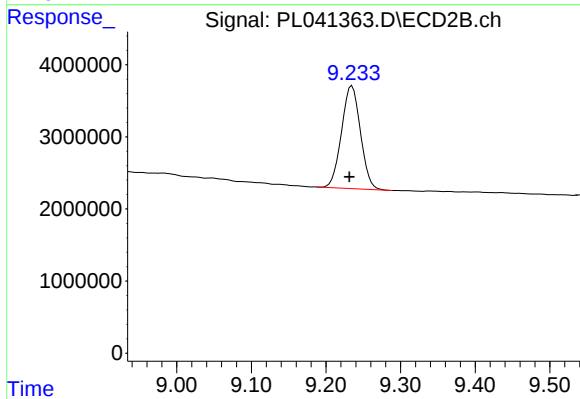

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.003 min
Response: 25069628
Conc: 9.69 ng/ml