

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 18:13
 Operator : AJ\SJ
 Sample : J5649-13
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 DL-05B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:02:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.105	99141819	52542548	18.089	18.844
28)	SA Decachlor...	8.221	9.236	96829038	39527255	18.623	15.286
Target Compounds							
4)	MA Heptachlor	4.569f	0.000	4848920	0	0.658	N.D. #
6)	B beta-BHC	0.000	4.996f	0	2217414	N.D.	1.384 #
7)	B delta-BHC	4.694f	0.000	754036	0	0.113	N.D. #
16)	A 4,4'-DDD	6.232f	0.000	3145236	0	0.696	N.D. #
20)	A Methoxychlor	6.981	0.000	542950	0	0.209	N.D. #
23)	Chlordane-1	4.370	0.000	533177	0	2.089	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 18:13
Operator : AJ\SJ
Sample : J5649-13
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
DL-05B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:02:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

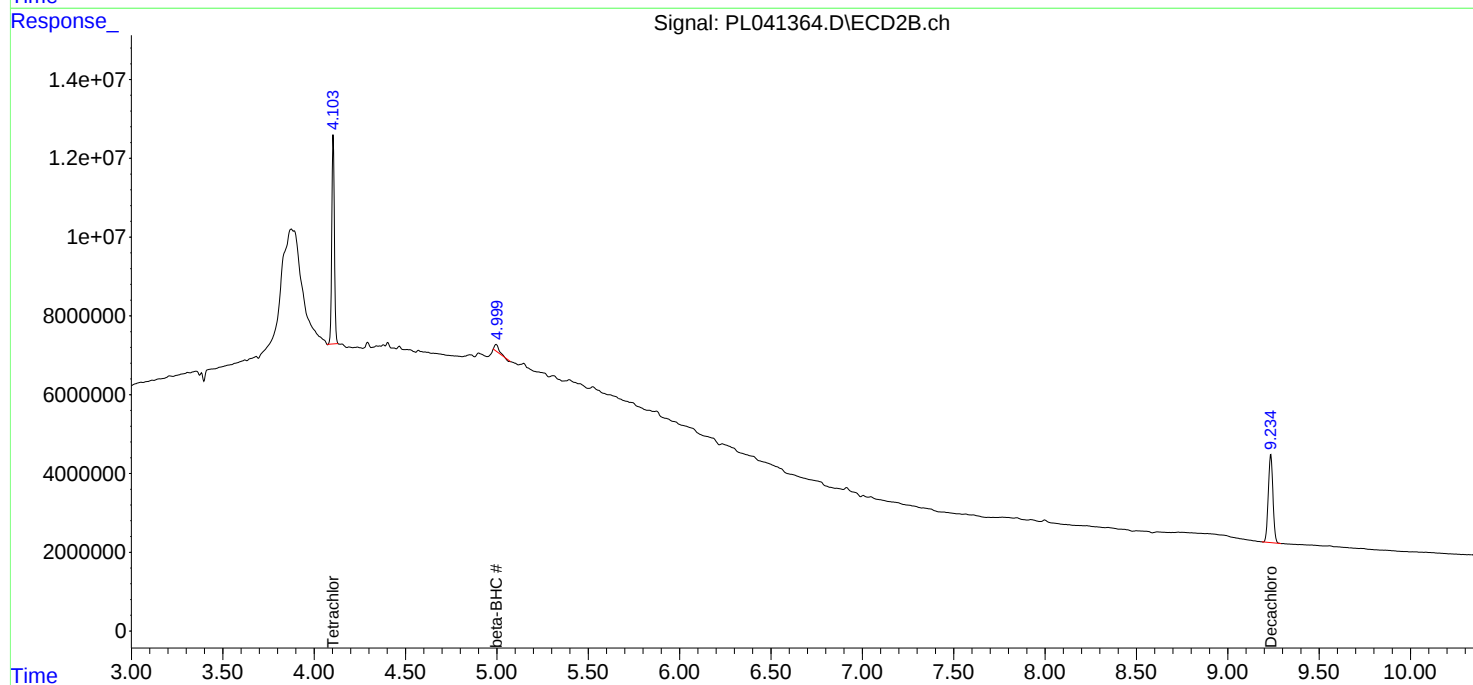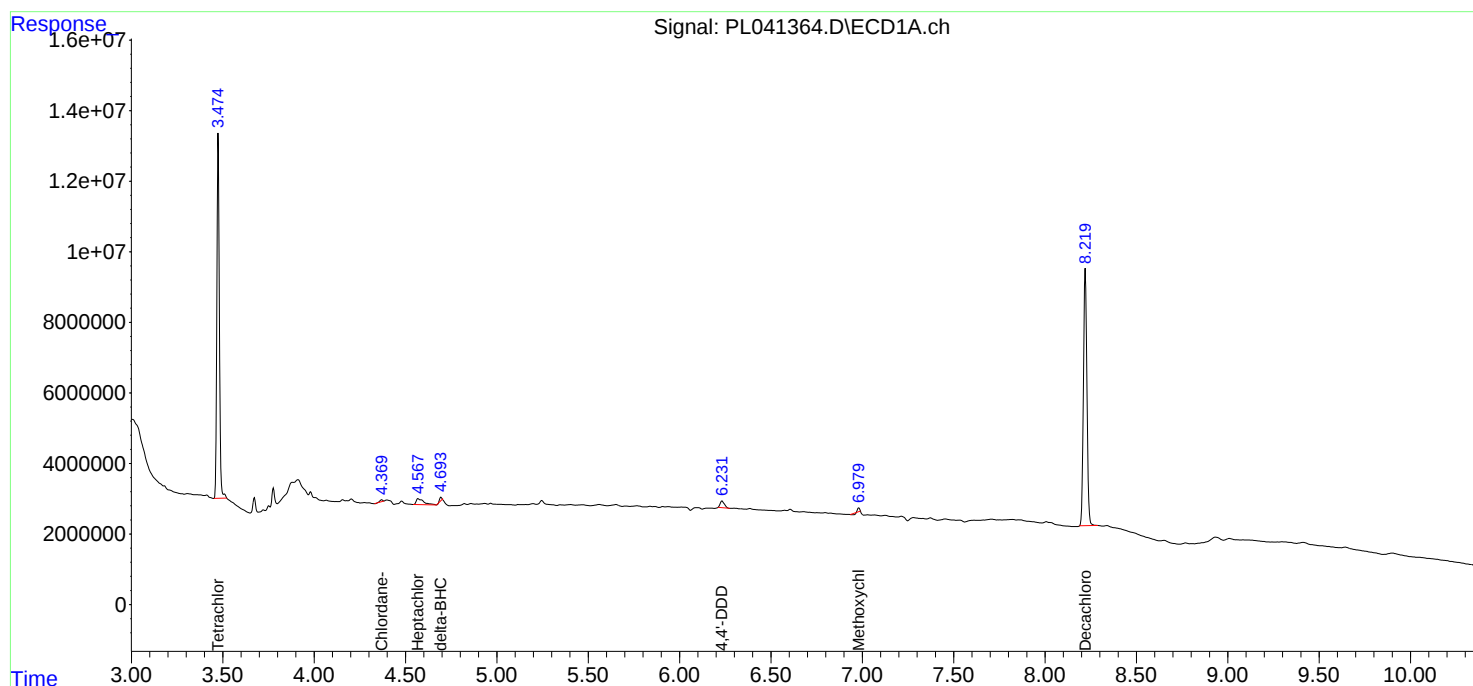


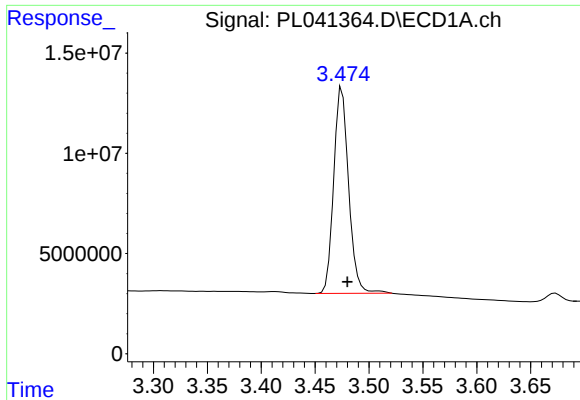

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 99141819
Conc: 18.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-05B

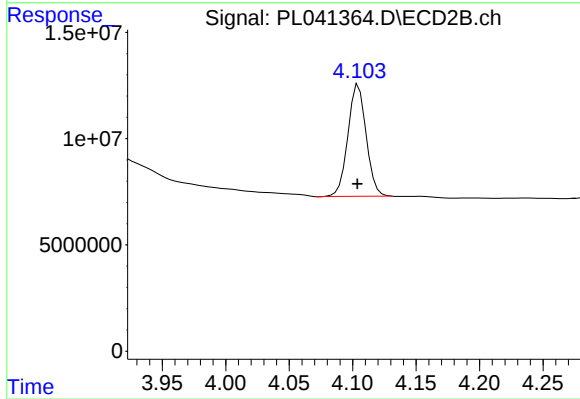


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.000 min
Response: 52542548
Conc: 18.84 ng/ml

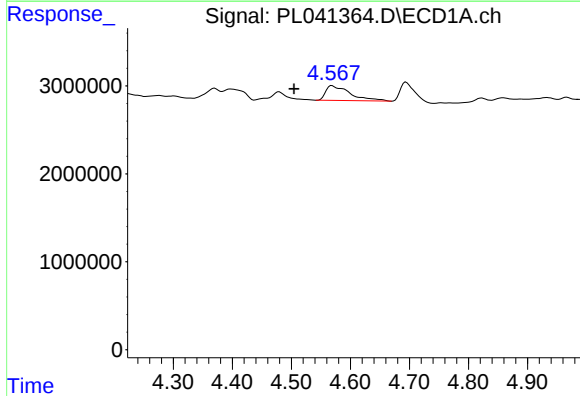


#4 Heptachlor

R.T.: 4.569 min
Delta R.T.: 0.064 min
Response: 4848920
Conc: 0.66 ng/ml

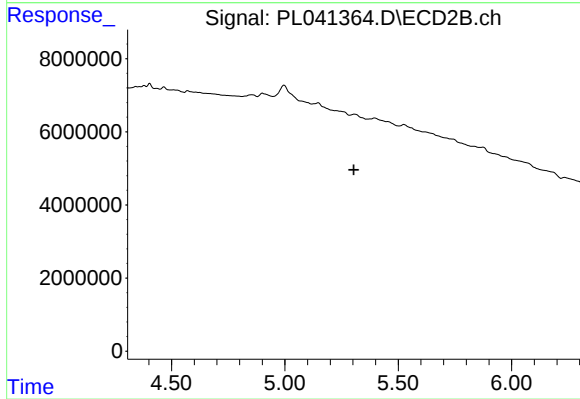

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.304 min
Response: 0
Conc: N.D.

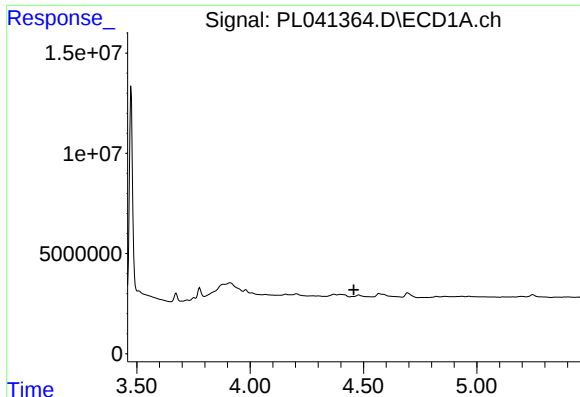

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
DL-05B

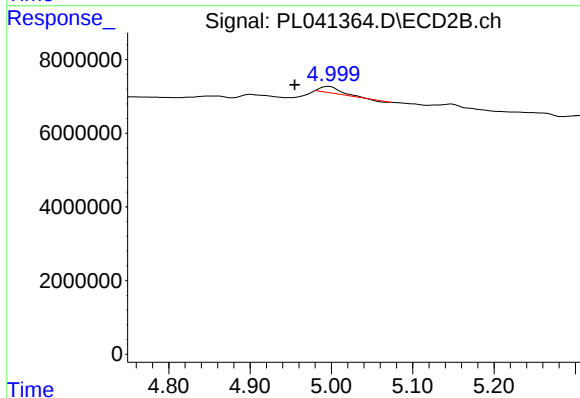


#6 beta-BHC

R.T.: 4.996 min
Delta R.T.: 0.041 min
Response: 2217414
Conc: 1.38 ng/ml

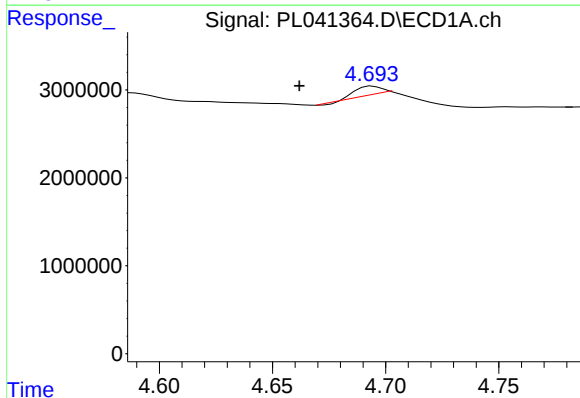


#7 delta-BHC

R.T.: 4.694 min
Delta R.T.: 0.032 min
Response: 754036
Conc: 0.11 ng/ml

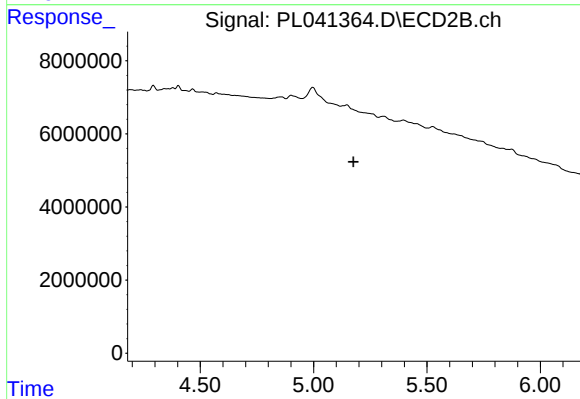

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 5.176 min
Response: 0
Conc: N.D.

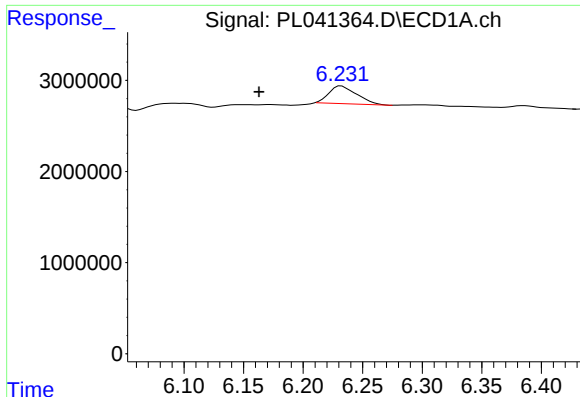

#16 4,4'-DDD


R.T.: 6.232 min
Delta R.T.: 0.069 min
Response: 3145236
Conc: 0.70 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-05B

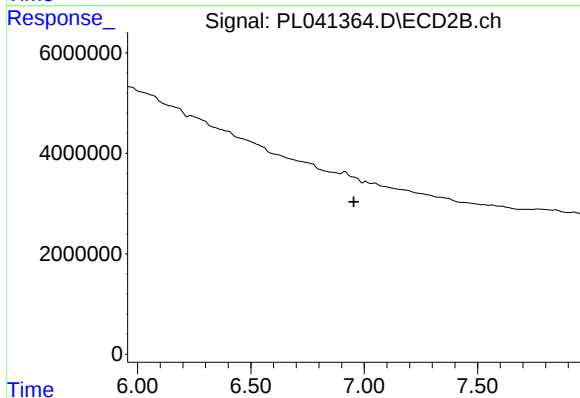


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.954 min
Response: 0
Conc: N.D.

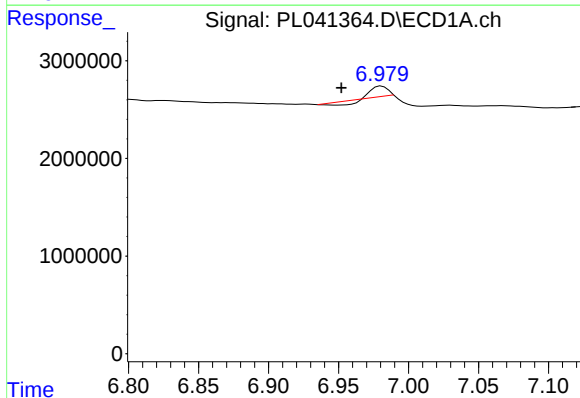


#20 Methoxychlor

R.T.: 6.981 min
Delta R.T.: 0.029 min
Response: 542950
Conc: 0.21 ng/ml

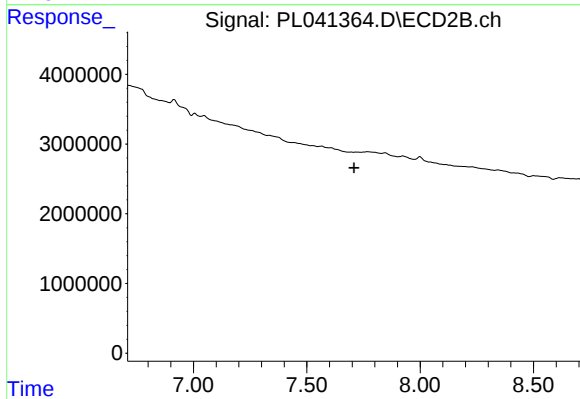

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

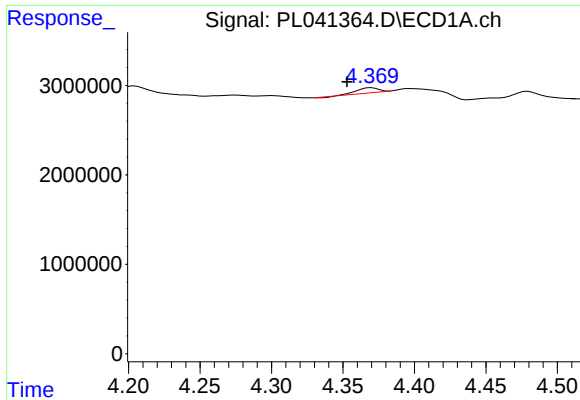

#23 Chlordane-1


R.T.: 4.370 min
Delta R.T.: 0.017 min
Response: 533177
Conc: 2.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
DL-05B

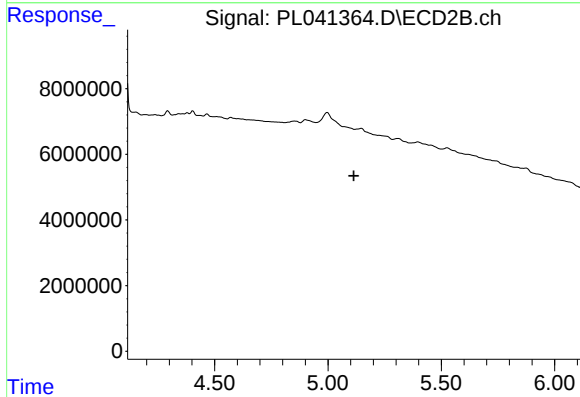


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

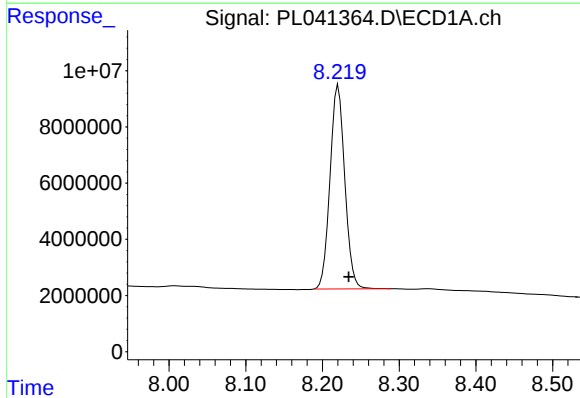

#28 Decachlorobiphenyl

R.T.: 8.221 min
Delta R.T.: -0.014 min
Response: 96829038
Conc: 18.62 ng/ml

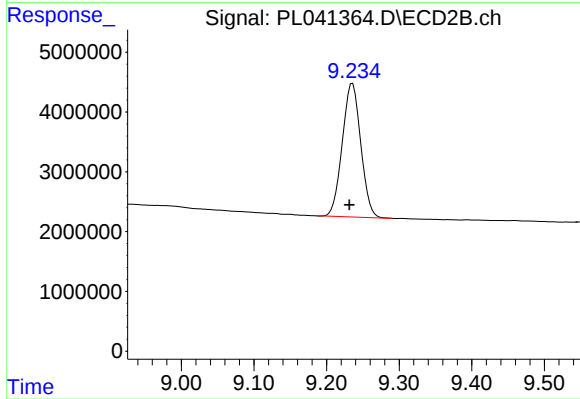

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.004 min
Response: 39527255
Conc: 15.29 ng/ml