

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041371.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 19:52
 Operator : AJ\SJ
 Sample : J5661-01
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VB44949

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:03:03 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.105	126.5E6	65522028	23.090	23.499
28)	SA Decachlor...	8.220	9.236	123.9E6	52798977	23.833	20.418
Target Compounds							
6)	B beta-BHC	0.000	4.998f	0	1553188	N.D.	0.969 #
14)	MA Endrin	6.103f	0.000	1683925	0	0.293	N.D. #
15)	B Endosulfa...	0.000	7.040	0	3799606	N.D.	1.600 #
16)	A 4,4'-DDD	6.103f	0.000	1683925	0	0.373	N.D. #
17)	MA 4,4'-DDT	0.000	7.278	0	2683006	N.D.	1.290 #
23)	Chlordane-1	4.352	0.000	490725	0	1.923	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041371.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 19:52
Operator : AJ\SJ
Sample : J5661-01
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
VB44949

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:03:03 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

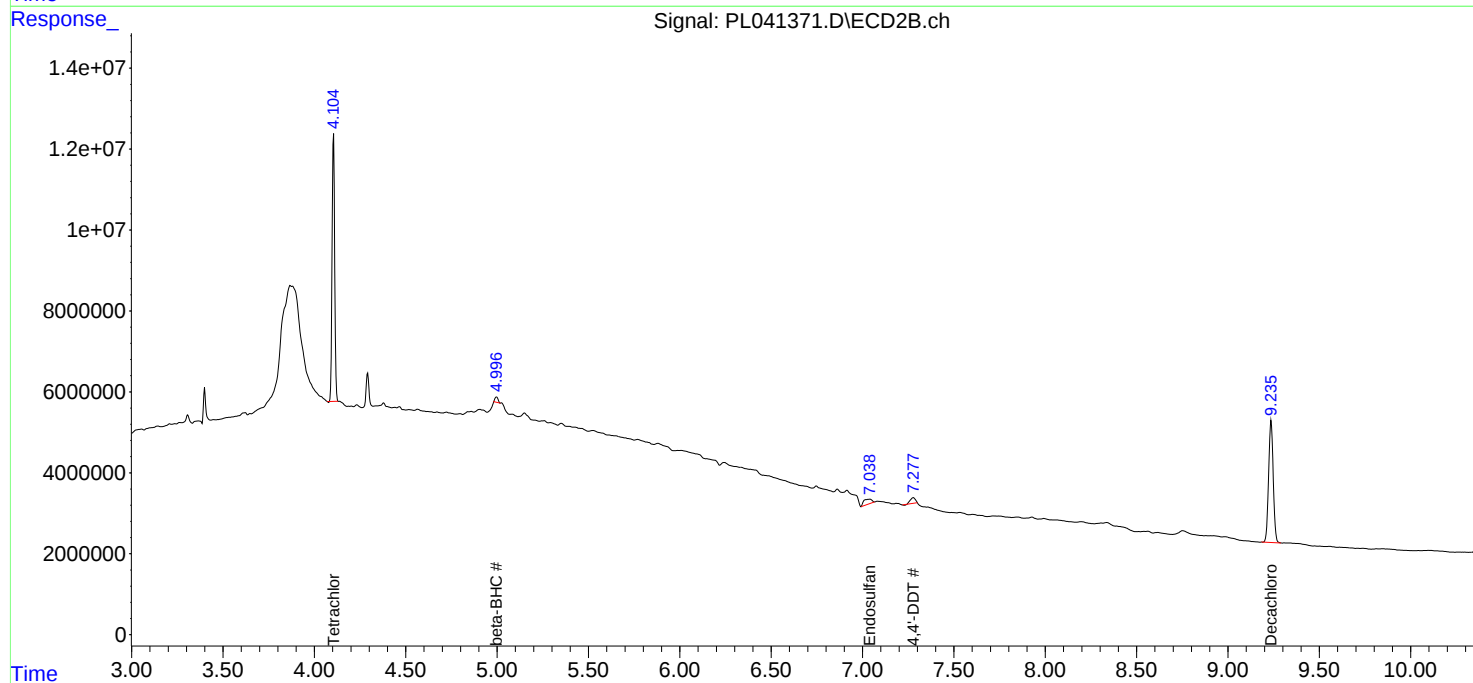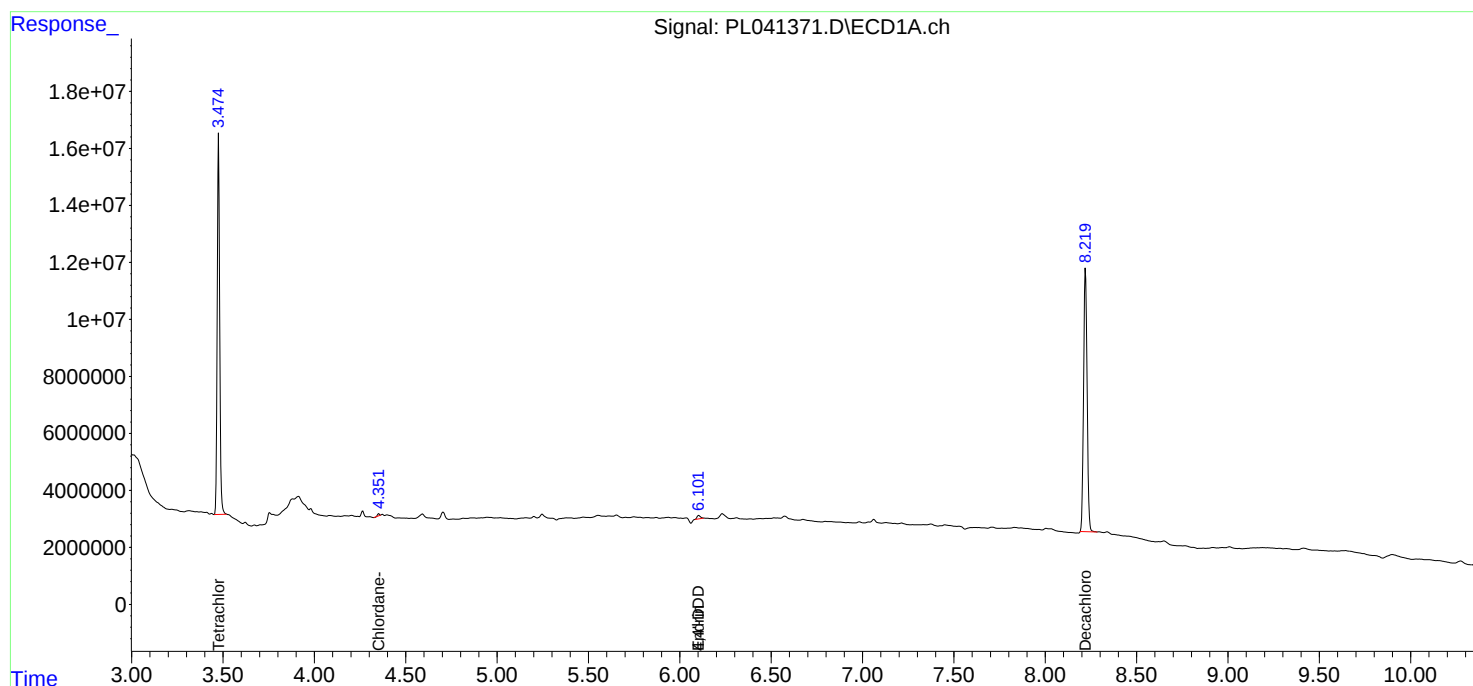


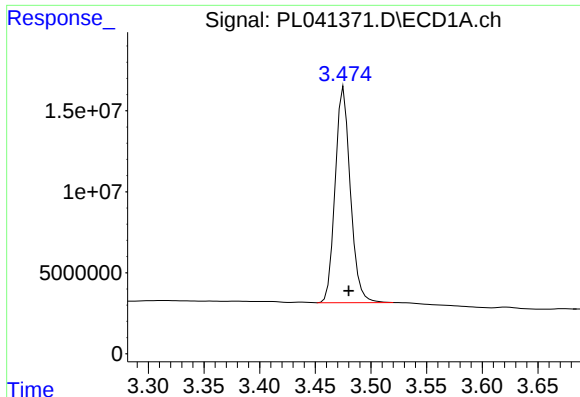

#1 Tetrachloro-m-xylene


R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 126549089
Conc: 23.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB44949

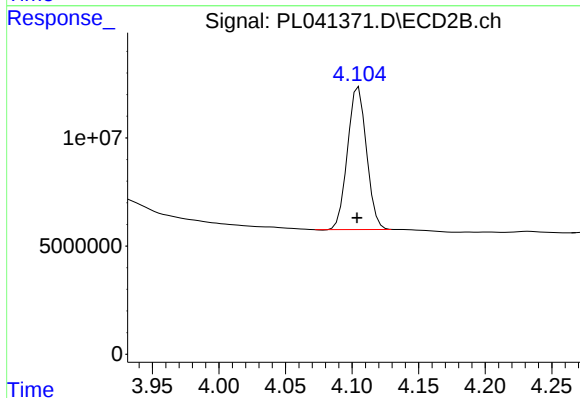


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.001 min
Response: 65522028
Conc: 23.50 ng/ml

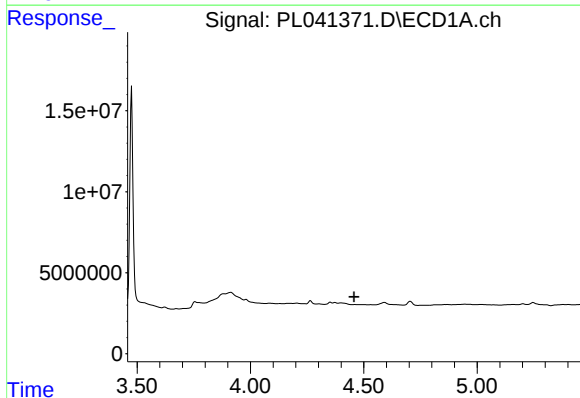


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.458 min
Response: 0
Conc: N.D.

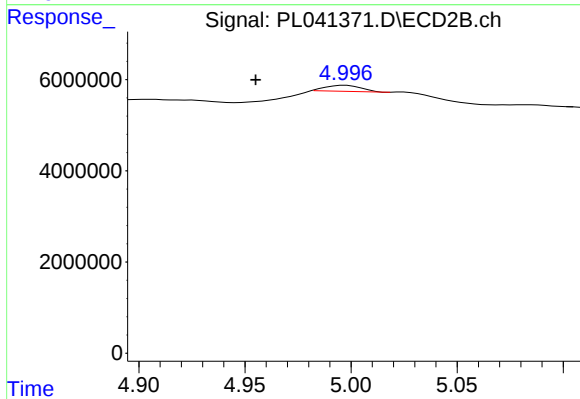

#6 beta-BHC


R.T.: 4.998 min
Delta R.T.: 0.042 min
Response: 1553188
Conc: 0.97 ng/ml

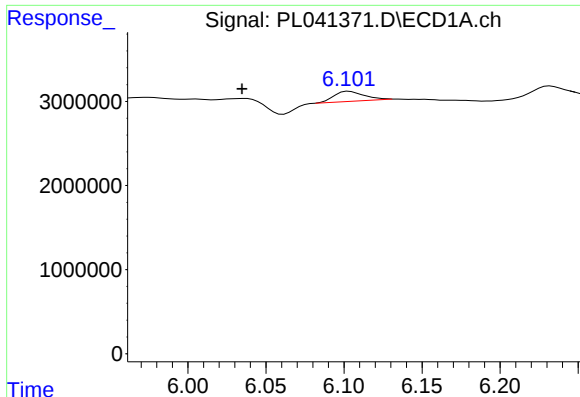

#14 Endrin


R.T.: 6.103 min
Delta R.T.: 0.069 min
Response: 1683925
Conc: 0.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB44949

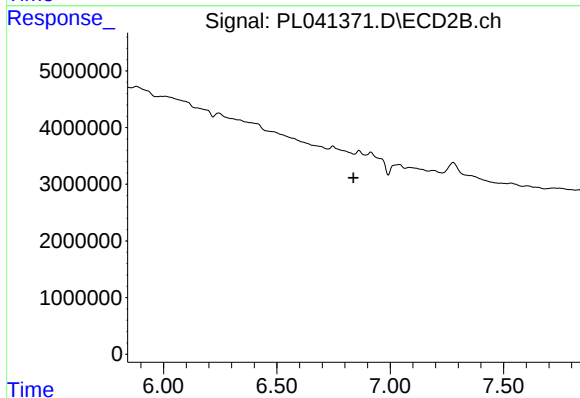


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.838 min
Response: 0
Conc: N.D.

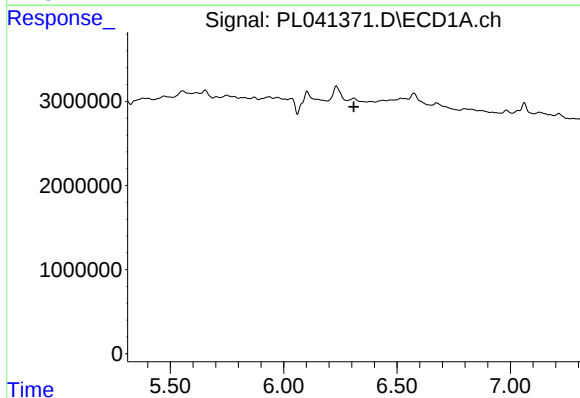


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.309 min
Response: 0
Conc: N.D.

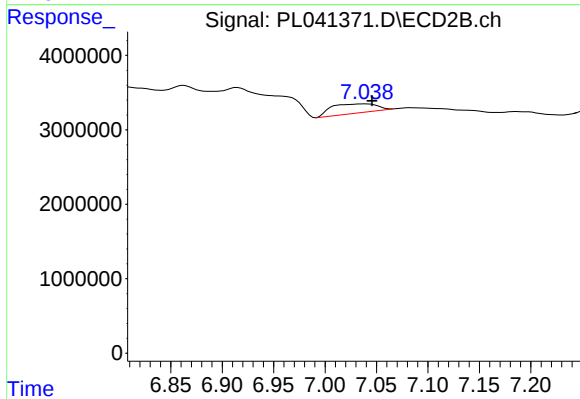

#15 Endosulfan II


R.T.: 7.040 min
Delta R.T.: -0.006 min
Response: 3799606
Conc: 1.60 ng/ml

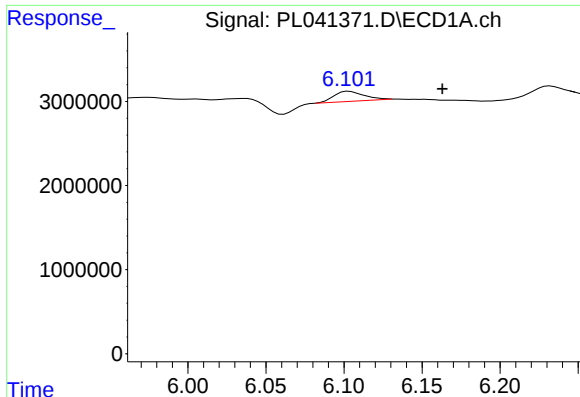

#16 4,4'-DDD


R.T.: 6.103 min
Delta R.T.: -0.060 min
Response: 1683925
Conc: 0.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB44949

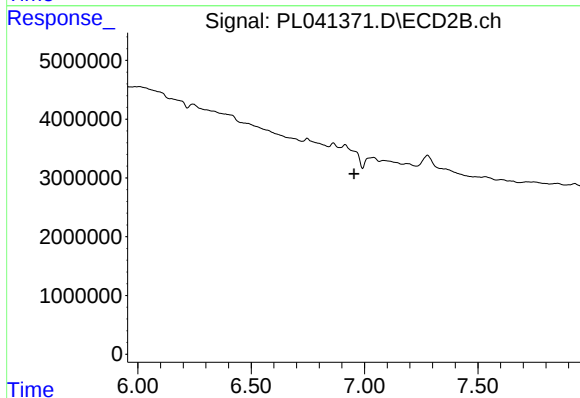


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.954 min
Response: 0
Conc: N.D.

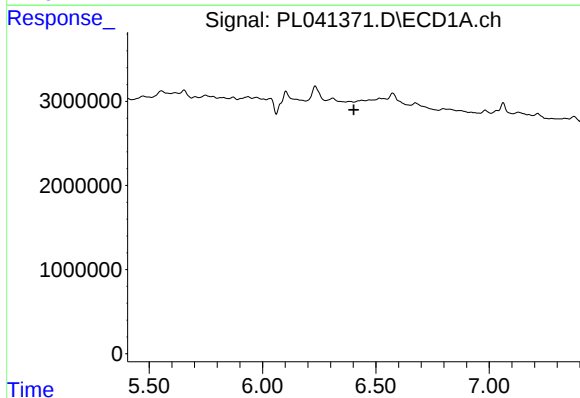


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.403 min
Response: 0
Conc: N.D.

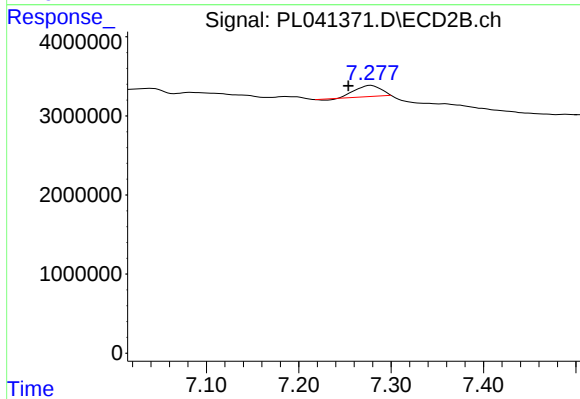

#17 4,4'-DDT


R.T.: 7.278 min
Delta R.T.: 0.024 min
Response: 2683006
Conc: 1.29 ng/ml

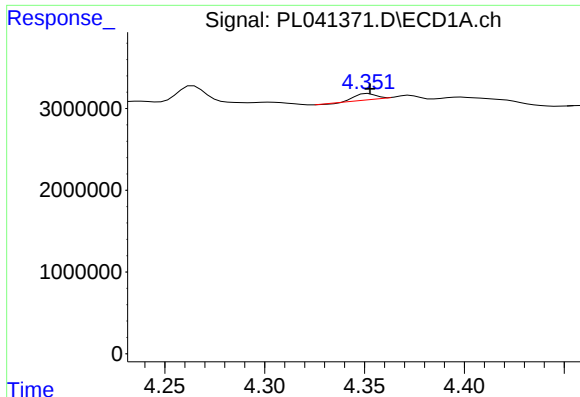

#23 Chlordane-1


R.T.: 4.352 min
Delta R.T.: 0.000 min
Response: 490725
Conc: 1.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB44949

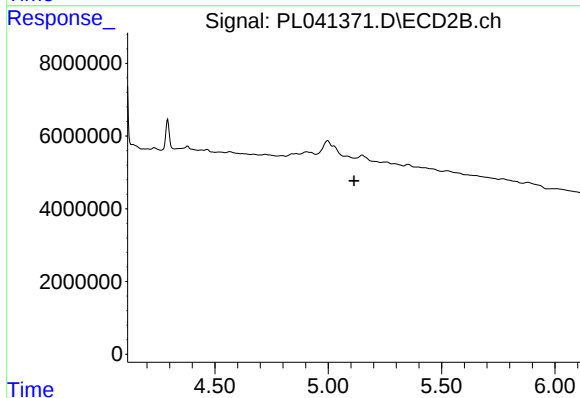


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T.: 5.114 min
Response: 0
Conc: N.D.

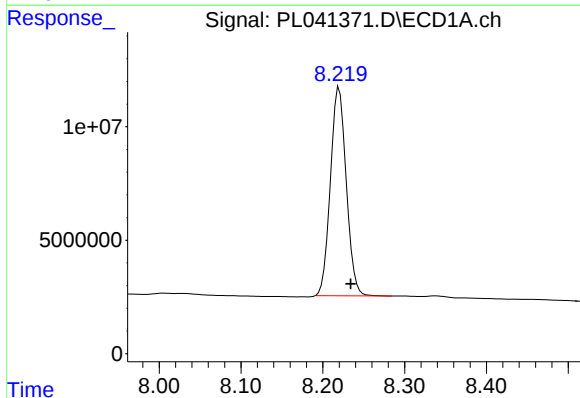

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 123918187
Conc: 23.83 ng/ml

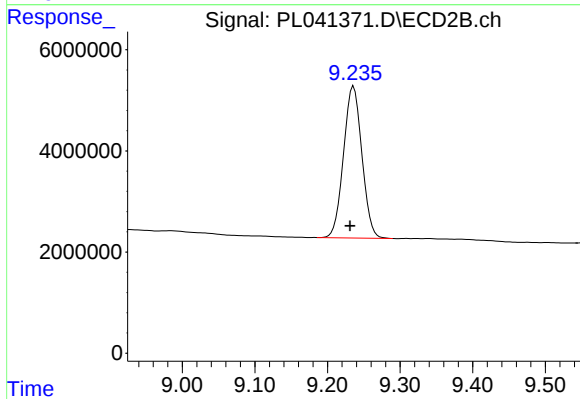

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.005 min
Response: 52798977
Conc: 20.42 ng/ml