

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041366.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 18:41
 Operator : AJ\SJ
 Sample : J5652-02 (Sig #1); J5651-02 (Sig #2)
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VB16206-VB16207-V236-VB16209-V

Manual Integrations
 APPROVED

Sohil
 10/26/2018 5:26:10 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:02:26 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.103	82954457	43584232	15.136	15.631m
28)	SA Decachlor...	8.218	9.235	69896153	28291152	13.443m	10.941

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041366.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 18:41
Operator : AJ\SJ
Sample : J5652-02 (Sig #1); J5651-02 (Sig #2)
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VB16206-VB16207-V236-VB16209-V


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:10 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:02:26 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

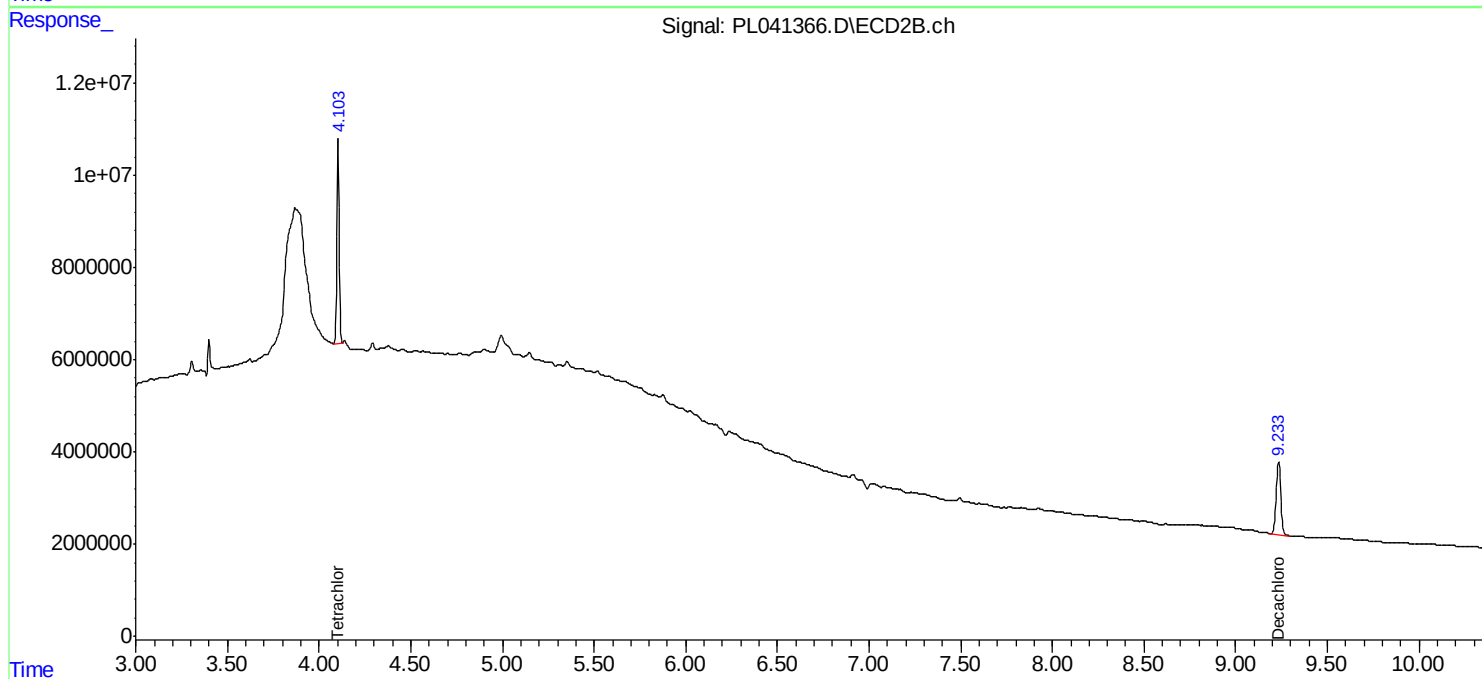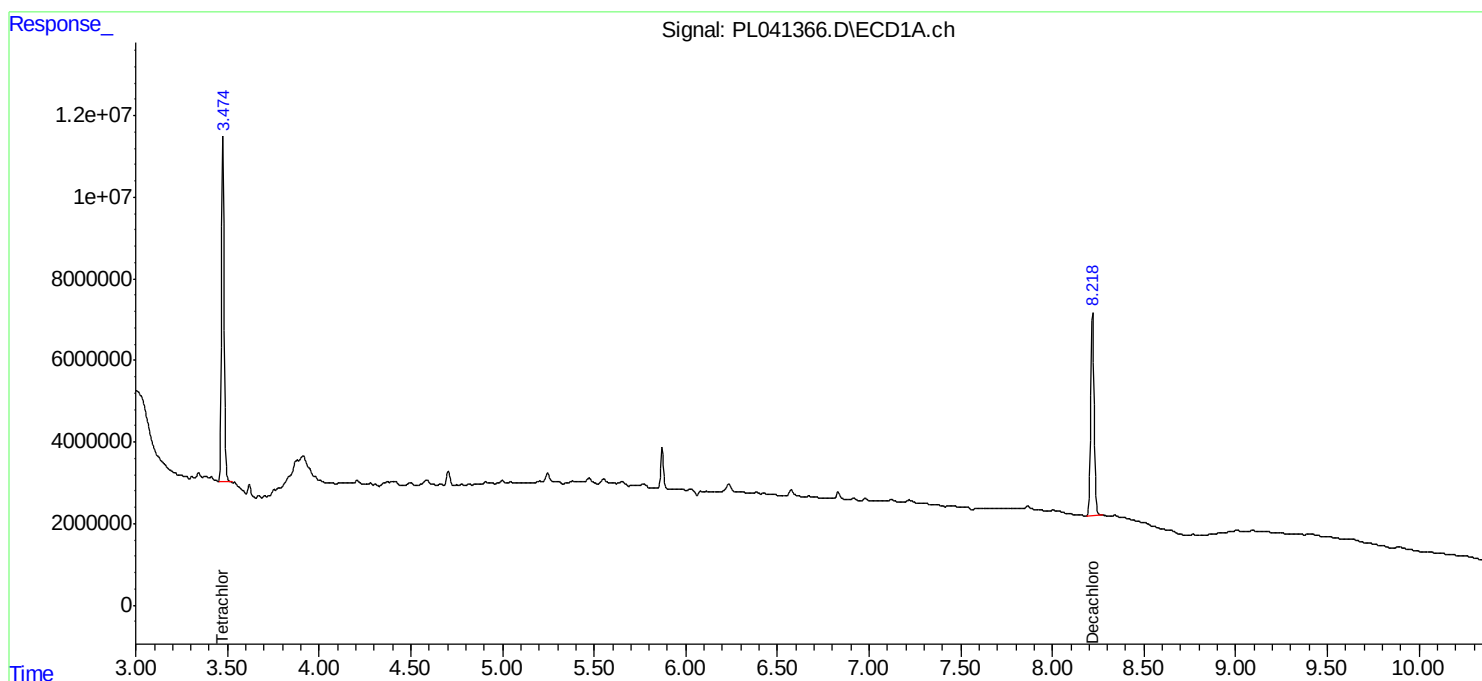

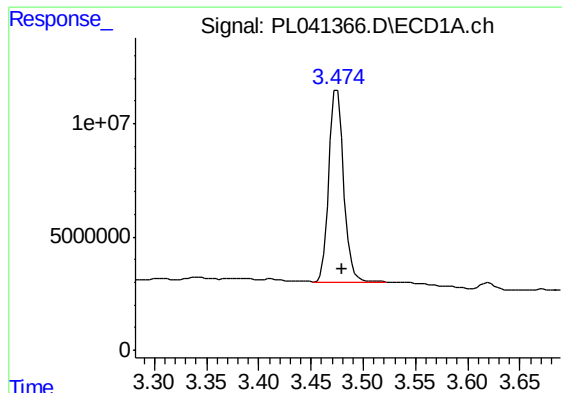


#1 Tetrachloro-m-xylene

R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 82954457
Conc: 15.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
VB16206-VB16207-V236-VB16209-V


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:10 PM

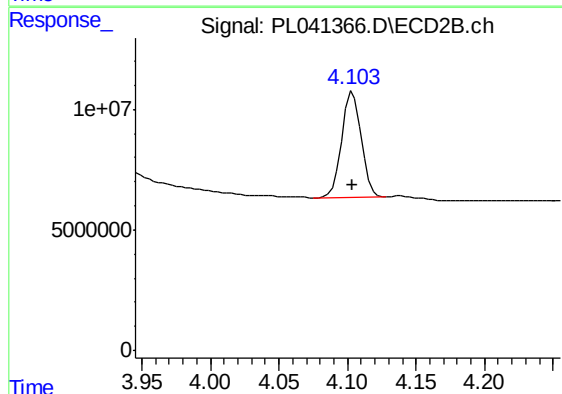


#1 Tetrachloro-m-xylene

R.T.: 4.103 min
Delta R.T.: -0.001 min
Response: 43584232
Conc: 15.63 ng/ml m

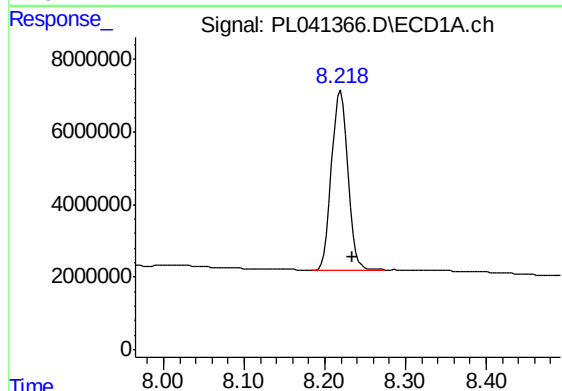

#28 Decachlorobiphenyl

R.T.: 8.218 min
Delta R.T.: -0.016 min
Response: 69896153
Conc: 13.44 ng/ml m

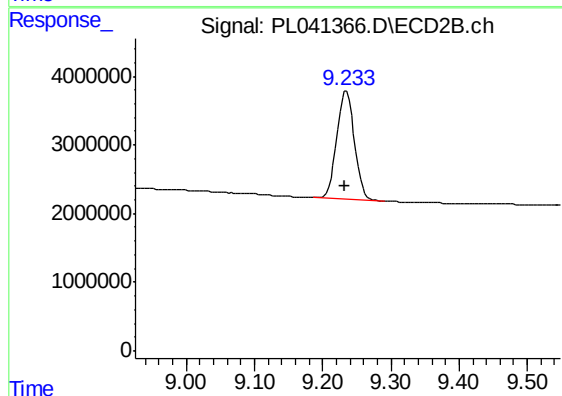

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.003 min
Response: 28291152
Conc: 10.94 ng/ml