

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
 Data File : PL041373.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2018 20:20
 Operator : AJ\SJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PSTDCCC050

Manual Integrations
 APPROVED

Sohil
 10/26/2018 5:26:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:03:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.476	4.105	267.9E6	139.2E6	48.882	49.923
28)	SA Decachlor...	8.220	9.236	257.1E6	110.8E6	49.443	42.866
Target Compounds							
2)	A alpha-BHC	3.917	4.499	414.7E6	211.1E6	52.336	54.562m
3)	MA gamma-BHC...	4.200	4.789	379.7E6	192.3E6	52.003	54.003
4)	MA Heptachlor	4.497	5.305	384.1E6	183.9E6	52.117	54.337
5)	MB Aldrin	4.742	5.614	356.3E6	171.6E6	51.911m	56.850
6)	B beta-BHC	4.452	4.957	159.3E6	78372496	50.200	48.900
7)	B delta-BHC	4.656	5.178	357.8E6	184.5E6	53.694	56.221
8)	B Heptachlor...	5.187	6.000	335.1E6	168.6E6	51.093	58.784m
9)	A Endosulfan I	5.525	6.361	306.1E6	138.0E6	51.101	53.897
10)	B gamma-Chl...	5.412	6.236	339.4E6	151.4E6	51.617m	53.990
11)	B alpha-Chl...	5.471	6.310	328.7E6	148.2E6	50.530	53.385
12)	B 4,4'-DDE	5.635	6.464	297.7E6	144.8E6	52.385m	54.737
13)	MA Dieldrin	5.767	6.620	330.4E6	144.6E6	52.255	54.305
14)	MA Endrin	6.023	6.839	280.8E6	100.5E6	48.881m	45.016
15)	B Endosulfa...	6.299	7.048	286.5E6	124.7E6	51.107	52.503
16)	A 4,4'-DDD	6.151	6.954	242.9E6	113.2E6	53.778m	54.025m
17)	MA 4,4'-DDT	6.389	7.256	242.2E6	110.8E6	53.182m	53.270
18)	B Endrin al...	6.466	7.172	228.1E6	103.6E6	54.398m	52.191
19)	B Endosulfa...	6.680	7.395	261.0E6	115.1E6	51.289	51.491
20)	A Methoxychlor	6.937	7.710	132.8E6	57335716	51.071m	48.707m
21)	B Endrin ke...	7.168	7.868	303.3E6	125.4E6	57.943m	53.330m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102518\
Data File : PL041373.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2018 20:20
Operator : AJ\SJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:03:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

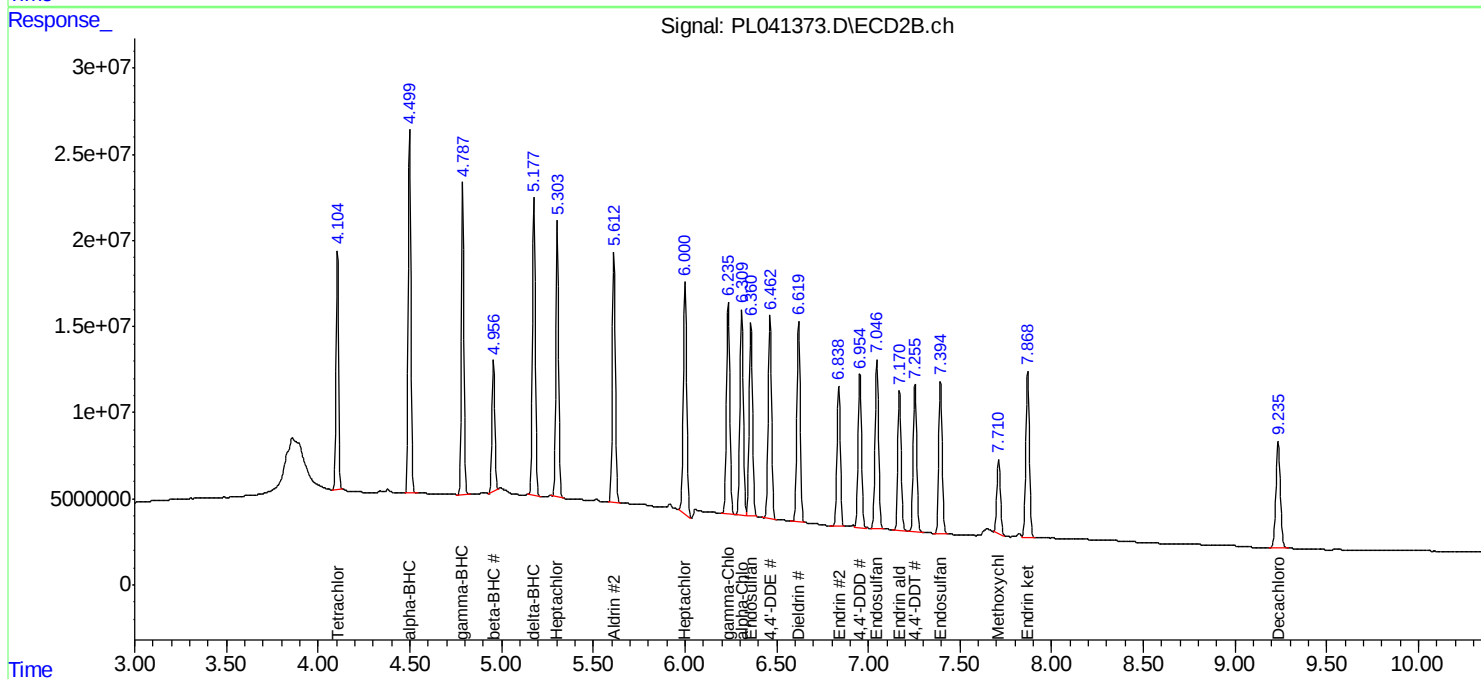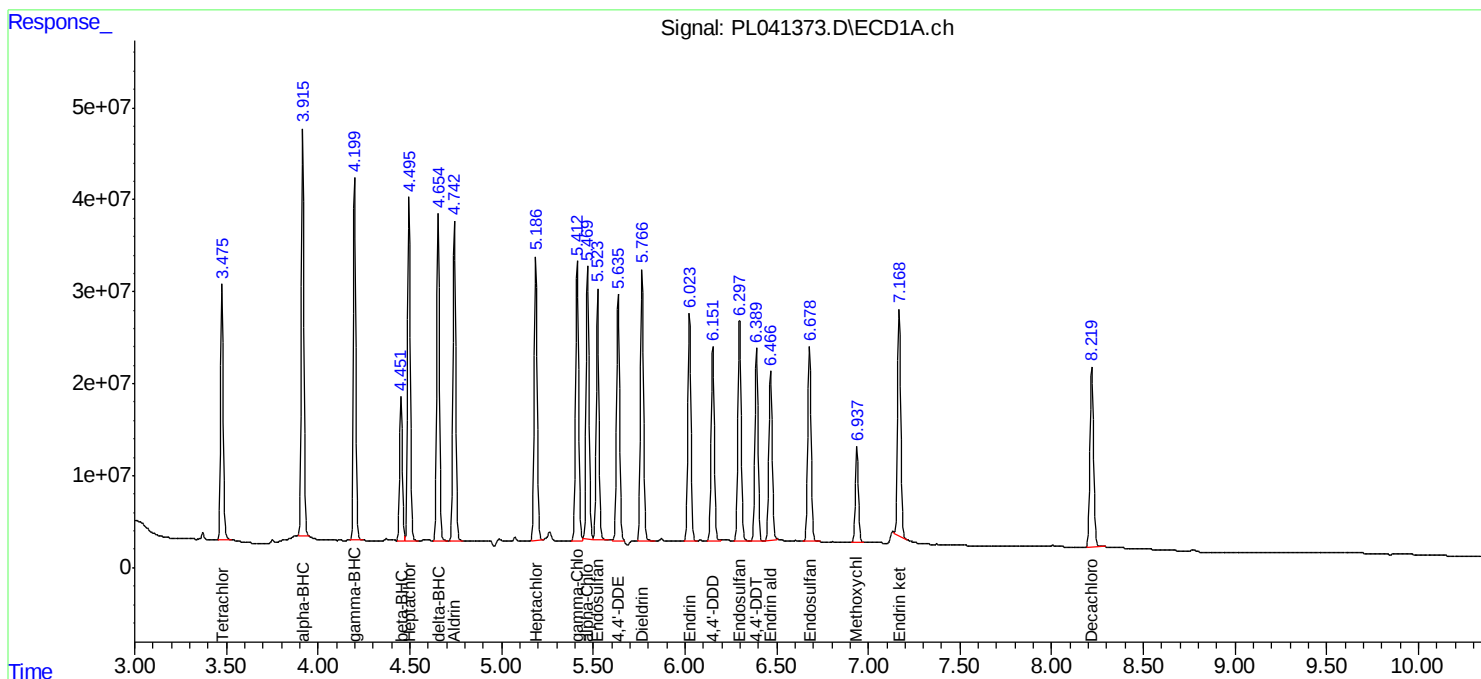




#1 Tetrachloro-m-xylene

R.T.: 3.476 min
Delta R.T.: -0.004 min
Response: 267907516
Conc: 48.88 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

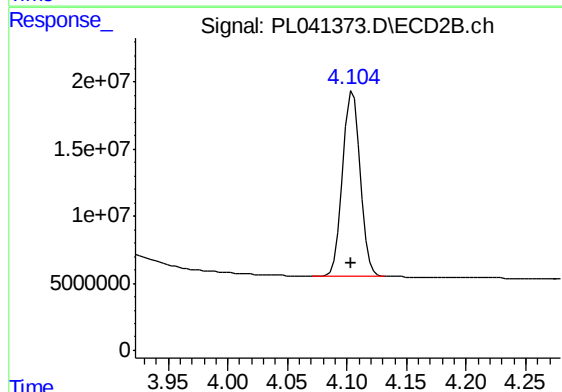


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.001 min
Response: 139200428
Conc: 49.92 ng/ml

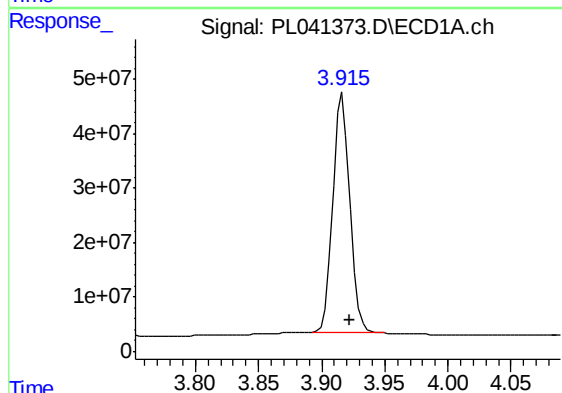


#2 alpha-BHC

R.T.: 3.917 min
Delta R.T.: -0.006 min
Response: 414693720
Conc: 52.34 ng/ml

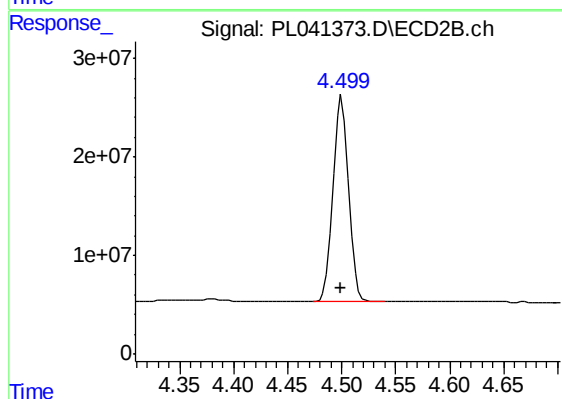

#2 alpha-BHC

R.T.: 4.499 min
Delta R.T.: 0.000 min
Response: 211115887
Conc: 54.56 ng/ml m

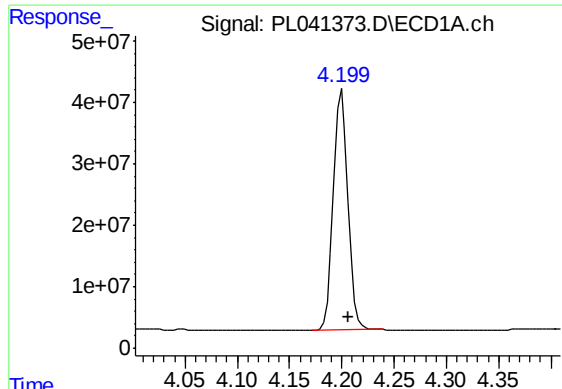


#3 gamma-BHC (Lindane)

R.T.: 4.200 min
Delta R.T.: -0.006 min
Response: 379725765
Conc: 52.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

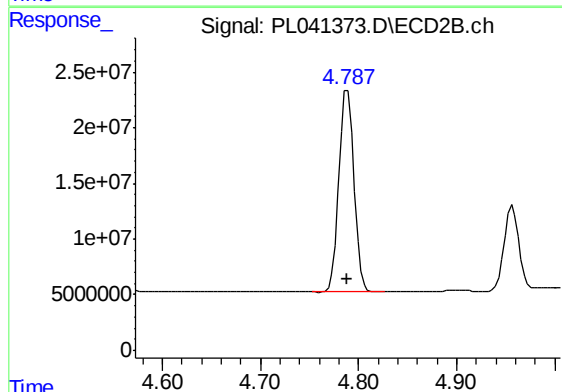


#3 gamma-BHC (Lindane)

R.T.: 4.789 min
Delta R.T.: 0.000 min
Response: 192291506
Conc: 54.00 ng/ml




#4 Heptachlor

R.T.: 4.497 min
Delta R.T.: -0.008 min
Response: 384053560
Conc: 52.12 ng/ml

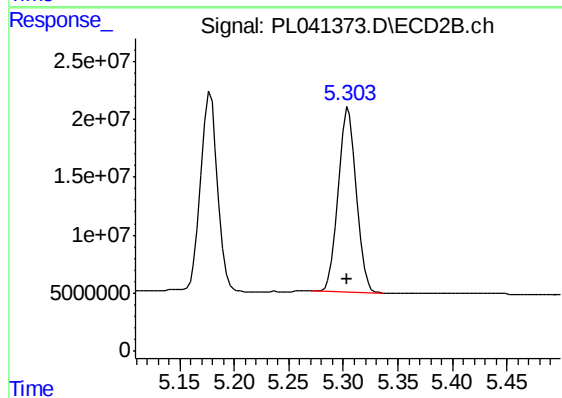

#4 Heptachlor

R.T.: 5.305 min
Delta R.T.: 0.001 min
Response: 183911776
Conc: 54.34 ng/ml




#5 Aldrin

R.T.: 4.742 min
Delta R.T.: -0.010 min
Response: 356336407
Conc: 51.91 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

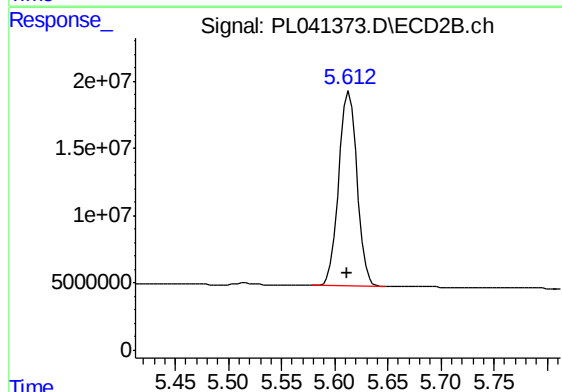


#5 Aldrin

R.T.: 5.614 min
Delta R.T.: 0.001 min
Response: 171580081
Conc: 56.85 ng/ml




#6 beta-BHC

R.T.: 4.452 min
Delta R.T.: -0.005 min
Response: 159286065
Conc: 50.20 ng/ml

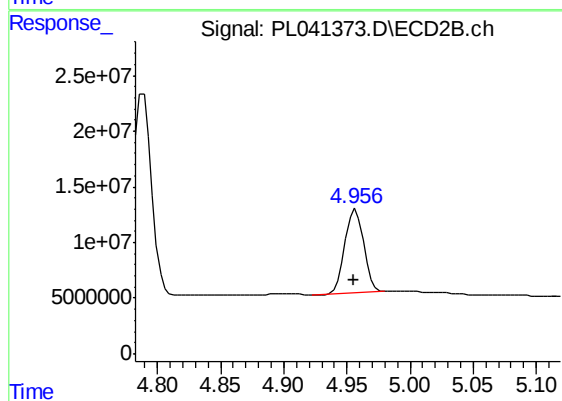

#6 beta-BHC

R.T.: 4.957 min
Delta R.T.: 0.002 min
Response: 78372496
Conc: 48.90 ng/ml

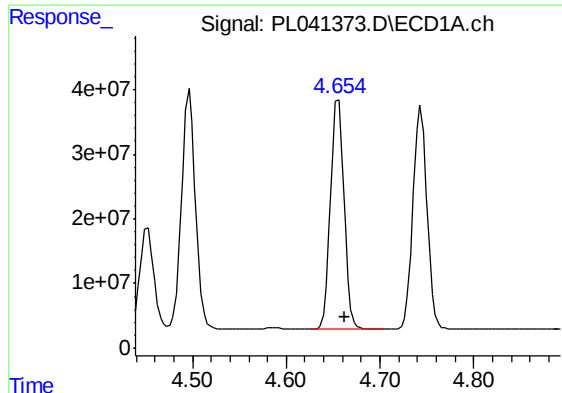


#7 delta-BHC

R.T.: 4.656 min
Delta R.T.: -0.006 min
Response: 357806127
Conc: 53.69 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

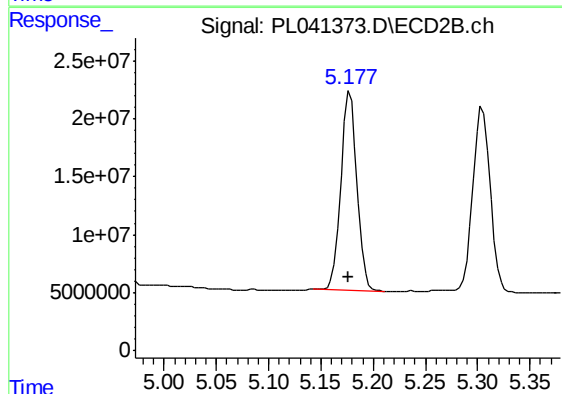


#7 delta-BHC

R.T.: 5.178 min
Delta R.T.: 0.002 min
Response: 184545648
Conc: 56.22 ng/ml

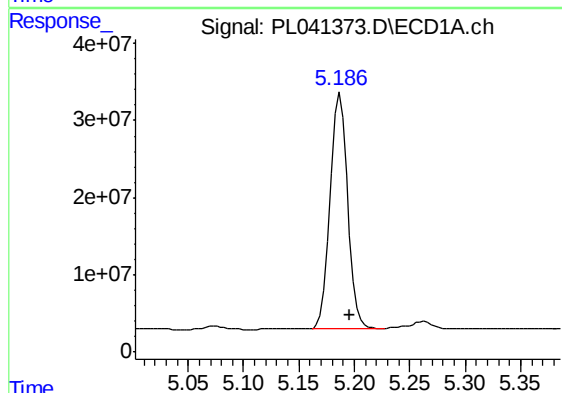


#8 Heptachlor epoxide

R.T.: 5.187 min
Delta R.T.: -0.009 min
Response: 335107228
Conc: 51.09 ng/ml

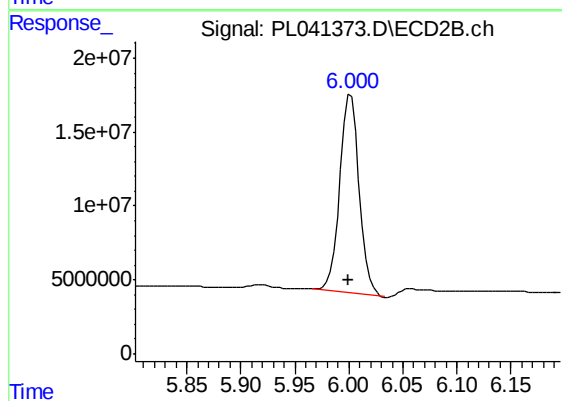

#8 Heptachlor epoxide

R.T.: 6.000 min
Delta R.T.: 0.000 min
Response: 168600624
Conc: 58.78 ng/ml m

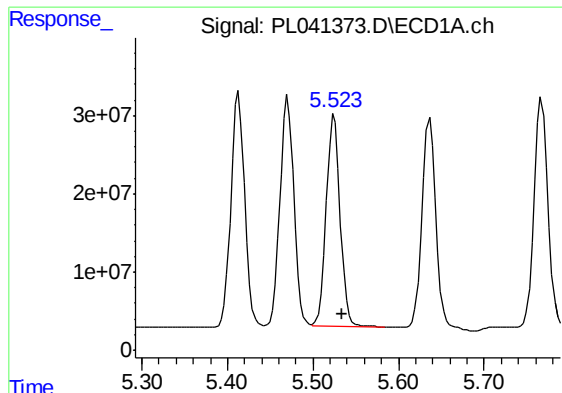


#9 Endosulfan I

R.T.: 5.525 min
Delta R.T.: -0.010 min
Response: 306143412
Conc: 51.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

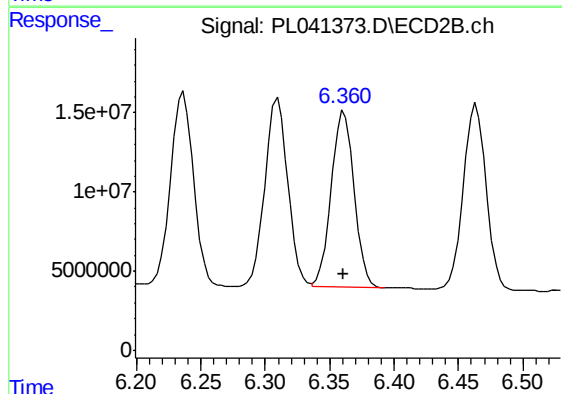


#9 Endosulfan I

R.T.: 6.361 min
Delta R.T.: 0.000 min
Response: 138043817
Conc: 53.90 ng/ml

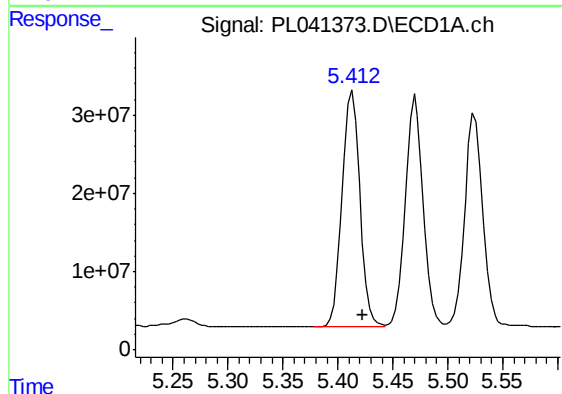


#10 gamma-Chlordane

R.T.: 5.412 min
Delta R.T.: -0.011 min
Response: 339446893
Conc: 51.62 ng/ml m

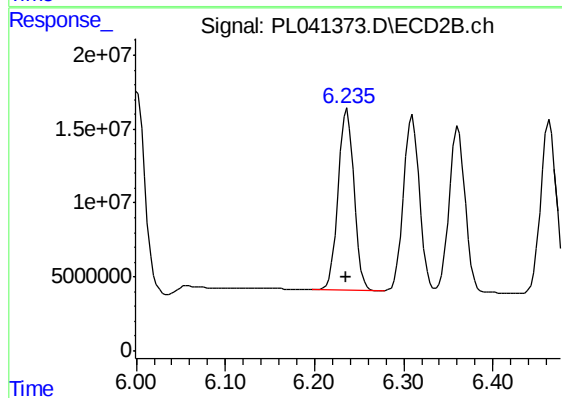

#10 gamma-Chlordane

R.T.: 6.236 min
Delta R.T.: 0.002 min
Response: 151423978
Conc: 53.99 ng/ml




#11 alpha-Chlordane

R.T.: 5.471 min
Delta R.T.: -0.010 min
Response: 328746999
Conc: 50.53 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

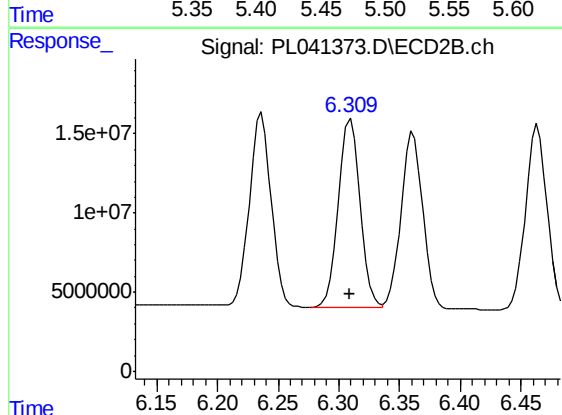


#11 alpha-Chlordane

R.T.: 6.310 min
Delta R.T.: 0.001 min
Response: 148174622
Conc: 53.38 ng/ml

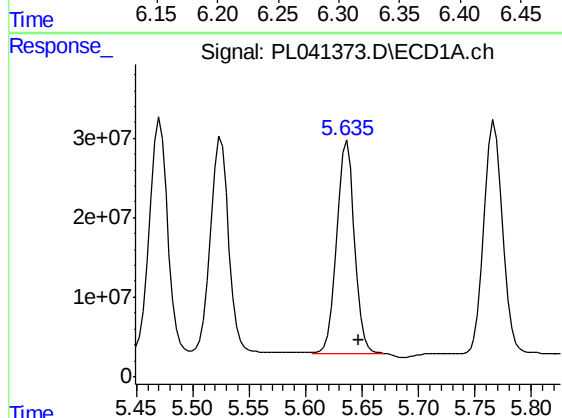


#12 4,4'-DDE

R.T.: 5.635 min
Delta R.T.: -0.012 min
Response: 297749312
Conc: 52.39 ng/ml m

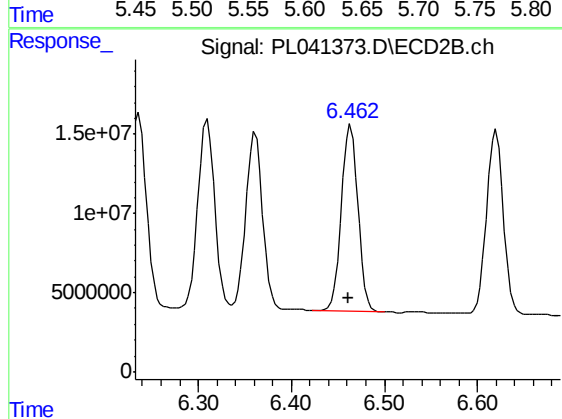

#12 4,4'-DDE

R.T.: 6.464 min
Delta R.T.: 0.002 min
Response: 144795823
Conc: 54.74 ng/ml




#13 Dieldrin

R.T.: 5.767 min
Delta R.T.: -0.011 min
Response: 330377333
Conc: 52.25 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

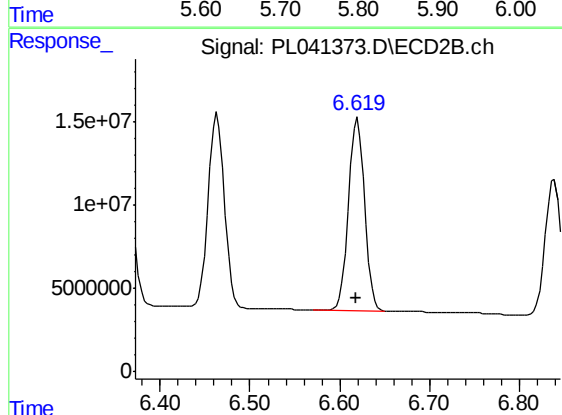


#13 Dieldrin

R.T.: 6.620 min
Delta R.T.: 0.002 min
Response: 144582118
Conc: 54.30 ng/ml

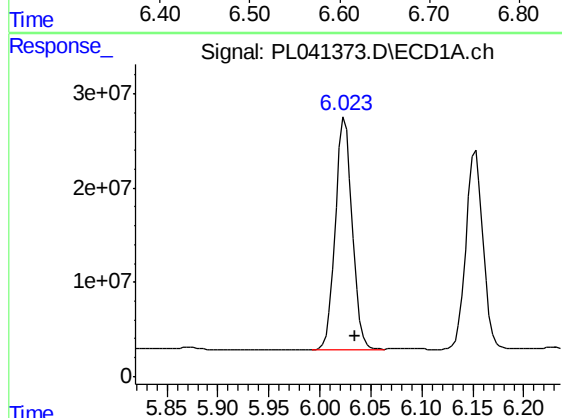


#14 Endrin

R.T.: 6.023 min
Delta R.T.: -0.012 min
Response: 280776098
Conc: 48.88 ng/ml m

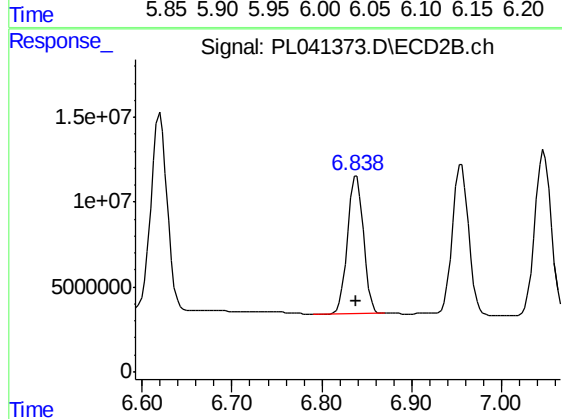

#14 Endrin

R.T.: 6.839 min
Delta R.T.: 0.000 min
Response: 100481792
Conc: 45.02 ng/ml




#15 Endosulfan II

R.T.: 6.299 min
Delta R.T.: -0.010 min
Response: 286450394
Conc: 51.11 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

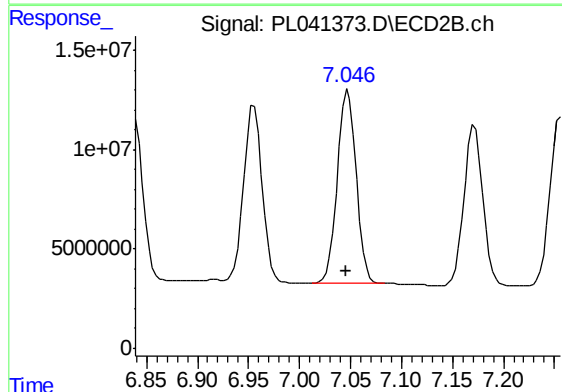


#15 Endosulfan II

R.T.: 7.048 min
Delta R.T.: 0.002 min
Response: 124696986
Conc: 52.50 ng/ml

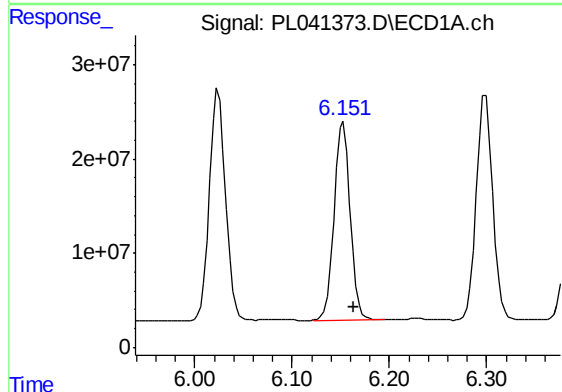


#16 4,4'-DDD

R.T.: 6.151 min
Delta R.T.: -0.012 min
Response: 242911041
Conc: 53.78 ng/ml m

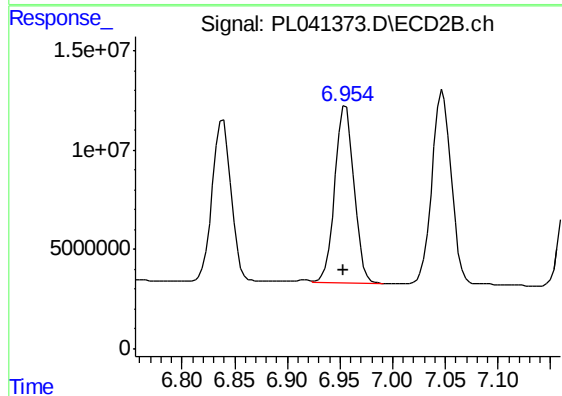

#16 4,4'-DDD

R.T.: 6.954 min
Delta R.T.: 0.000 min
Response: 113166227
Conc: 54.02 ng/ml m




#17 4,4'-DDT

R.T.: 6.389 min
Delta R.T.: -0.013 min
Response: 242224102
Conc: 53.18 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

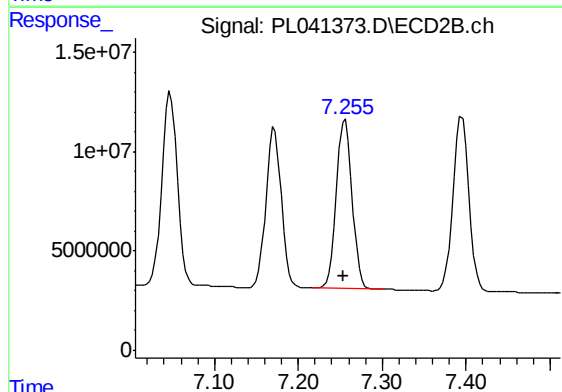


#17 4,4'-DDT

R.T.: 7.256 min
Delta R.T.: 0.002 min
Response: 110808398
Conc: 53.27 ng/ml

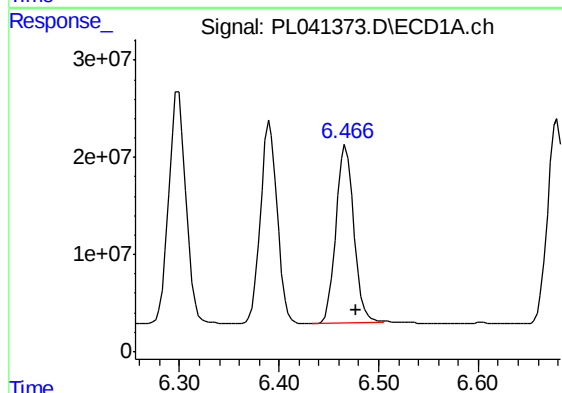


#18 Endrin aldehyde

R.T.: 6.466 min
Delta R.T.: -0.011 min
Response: 228082847
Conc: 54.40 ng/ml m

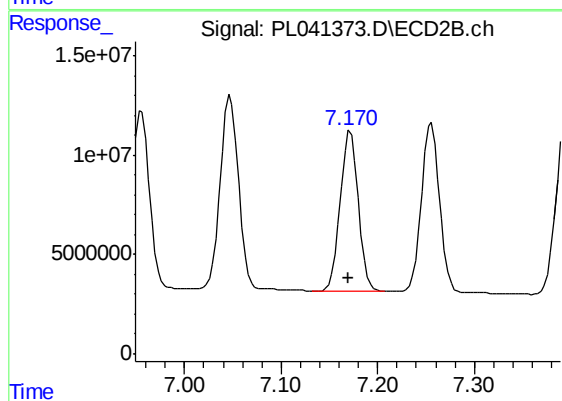

#18 Endrin aldehyde

R.T.: 7.172 min
Delta R.T.: 0.002 min
Response: 103553522
Conc: 52.19 ng/ml

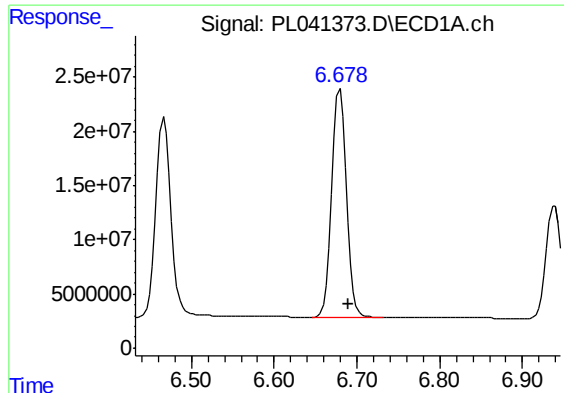


#19 Endosulfan Sulfate

R.T.: 6.680 min
Delta R.T.: -0.011 min
Response: 260953007
Conc: 51.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

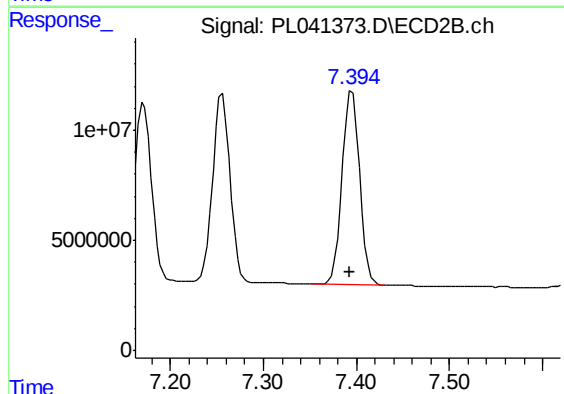


#19 Endosulfan Sulfate

R.T.: 7.395 min
Delta R.T.: 0.003 min
Response: 115052644
Conc: 51.49 ng/ml

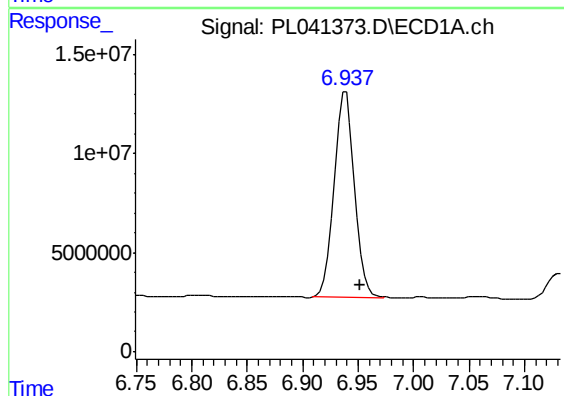


#20 Methoxychlor

R.T.: 6.937 min
Delta R.T.: -0.015 min
Response: 132846287
Conc: 51.07 ng/ml m

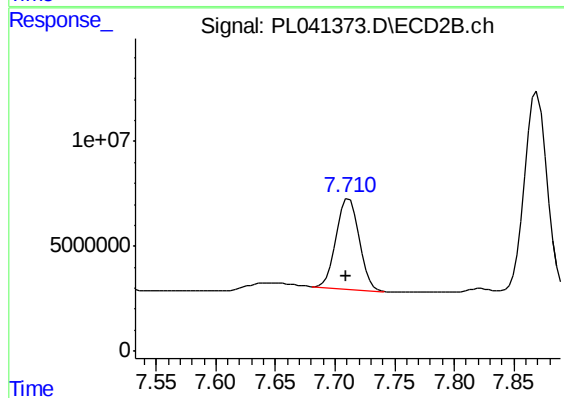

#20 Methoxychlor

R.T.: 7.710 min
Delta R.T.: 0.000 min
Response: 57335716
Conc: 48.71 ng/ml m




#21 Endrin ketone

R.T.: 7.168 min
Delta R.T.: -0.013 min
Response: 303318001
Conc: 57.94 ng/ml m

Instrument :
ECD_L
ClientSampleId :
PSTDCCC050


Manual Integrations
APPROVED

Sohil
10/26/2018 5:26:22 PM

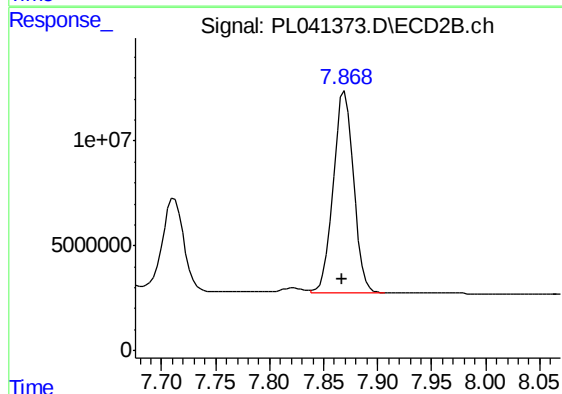


#21 Endrin ketone

R.T.: 7.868 min
Delta R.T.: 0.001 min
Response: 125407505
Conc: 53.33 ng/ml m



#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 257079704
Conc: 49.44 ng/ml

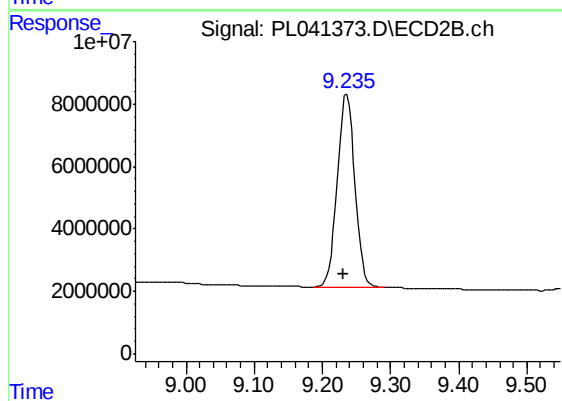

#28 Decachlorobiphenyl

R.T.: 9.236 min
Delta R.T.: 0.005 min
Response: 110845314
Conc: 42.87 ng/ml