

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
 Data File : PL053750.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2019 15:42
 Operator : SG\AJ
 Sample : K5542-21
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 16:17:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.044	196.1E6	45118459	18.087	18.030
28)	SA Decachlor...	8.327	9.122	121.6E6	35642785	12.395	12.657
Target Compounds							
6)	B beta-BHC	4.495f	0.000	10781860	0	1.636	N.D. #
8)	B Heptachlo...	0.000	5.902f	0	2847104	N.D.	0.976 #
9)	A Endosulfan I	0.000	6.308f	0	1066629	N.D.	0.393 #
10)	B gamma-Chl...	5.512	0.000	3110652	0	0.228	N.D. #
12)	B 4,4'-DDE	0.000	6.416f	0	634999	N.D.	0.225 #
16)	A 4,4'-DDD	6.243	0.000	4864035	0	0.547	N.D. #
17)	MA 4,4'-DDT	0.000	7.147f	0	895071	N.D.	0.387 #
25)	Chlordane-3	5.512	0.000	3110652	0	2.699	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
Data File : PL053750.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2019 15:42
Operator : SG\AJ
Sample : K5542-21
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 16:17:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

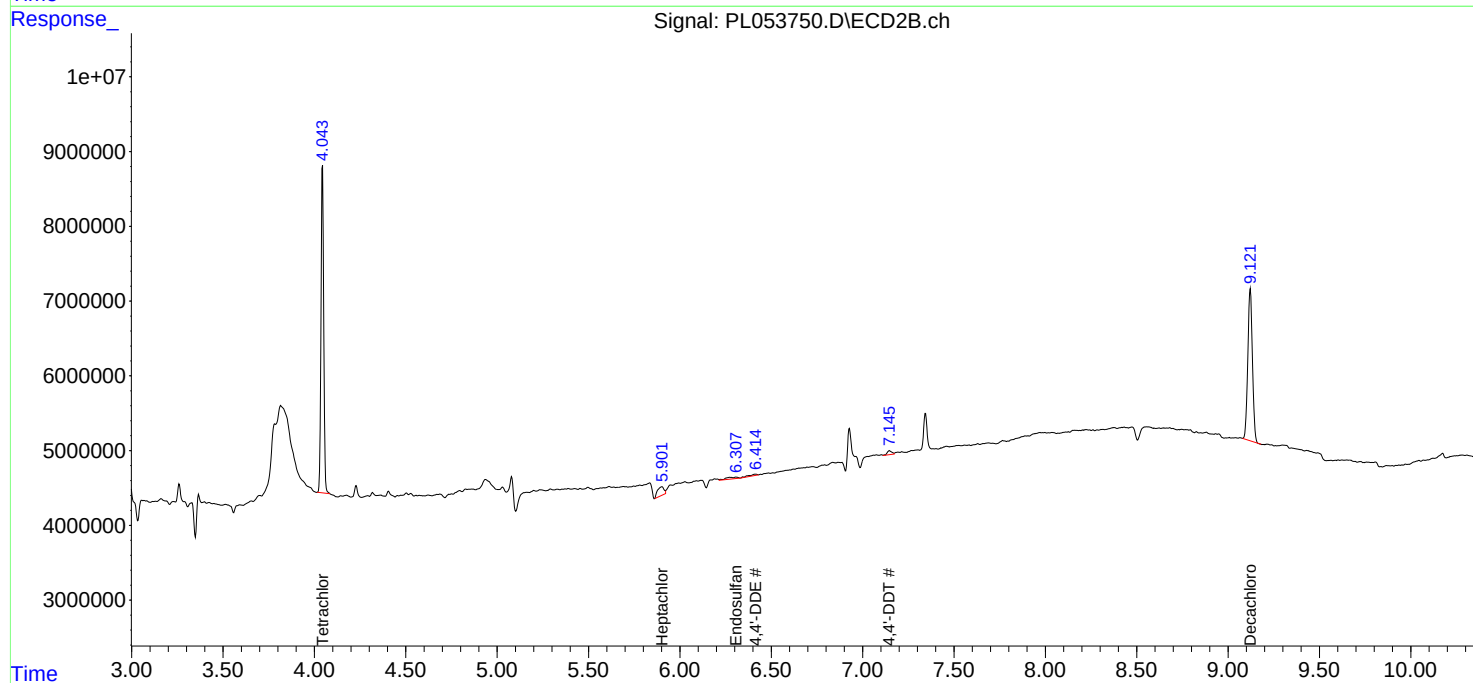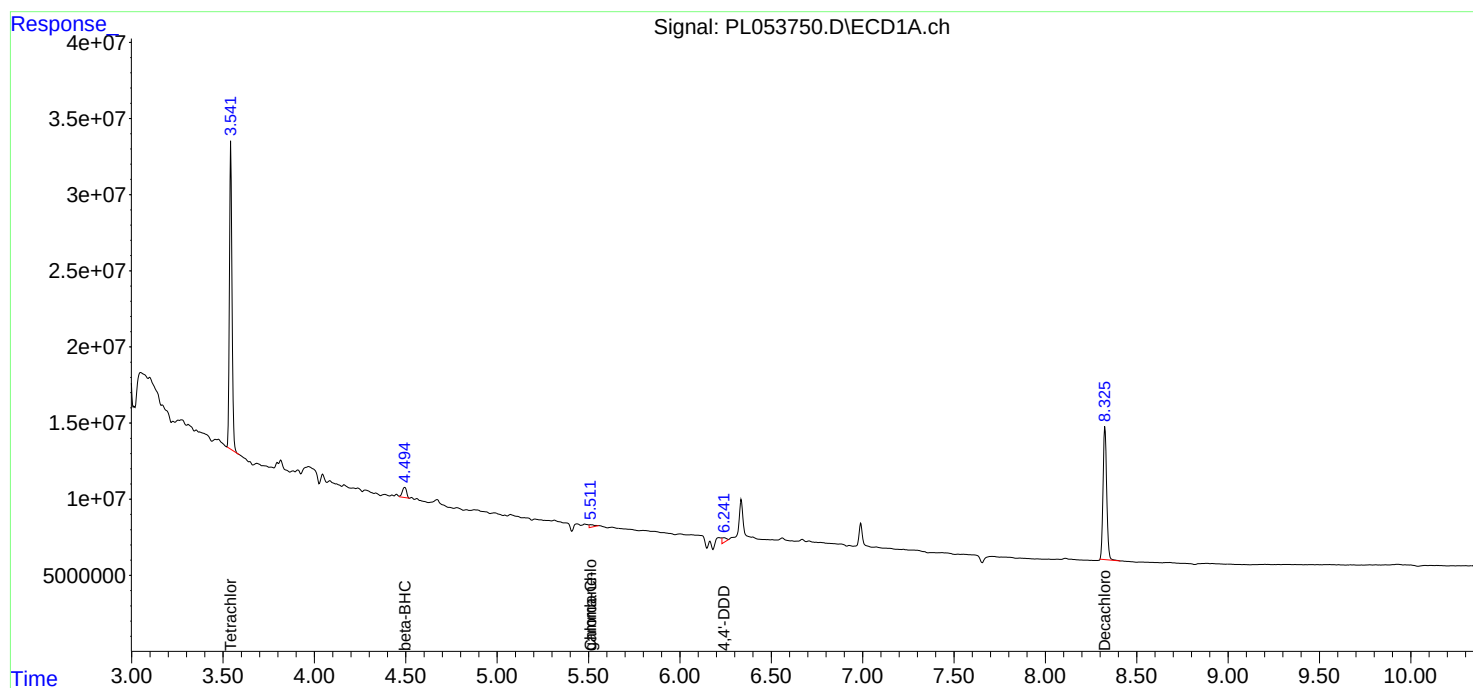


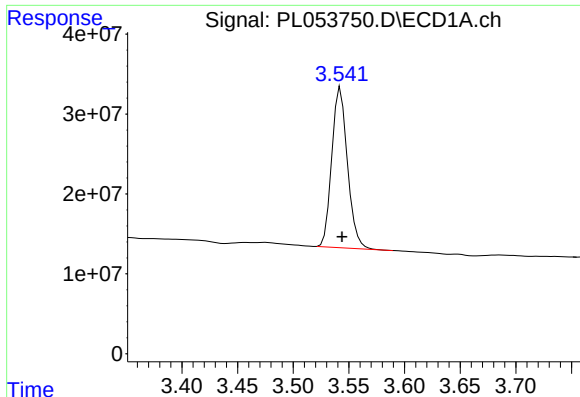

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 196053107
Conc: 18.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

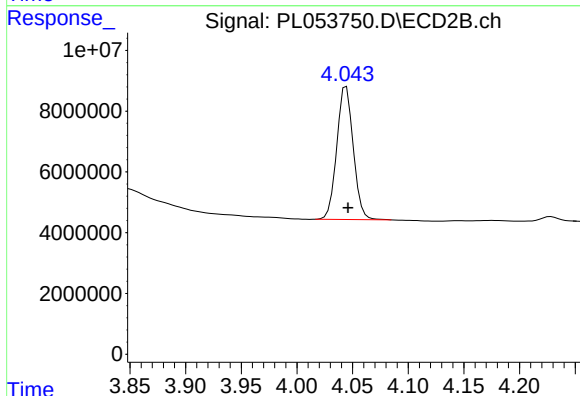


#1 Tetrachloro-m-xylene

R.T.: 4.044 min
Delta R.T.: -0.001 min
Response: 45118459
Conc: 18.03 ng/ml

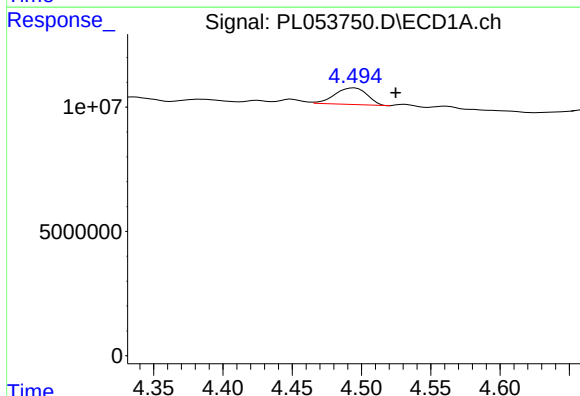


#6 beta-BHC

R.T.: 4.495 min
Delta R.T.: -0.030 min
Response: 10781860
Conc: 1.64 ng/ml

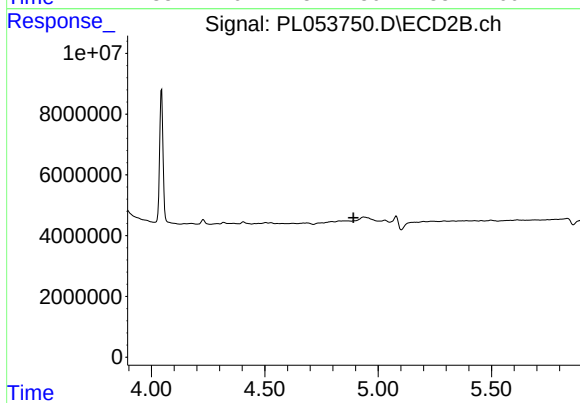

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.892 min
Response: 0
Conc: N.D.

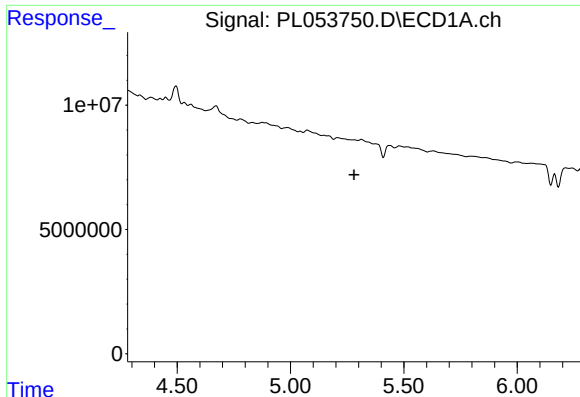

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T.: 5.280 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

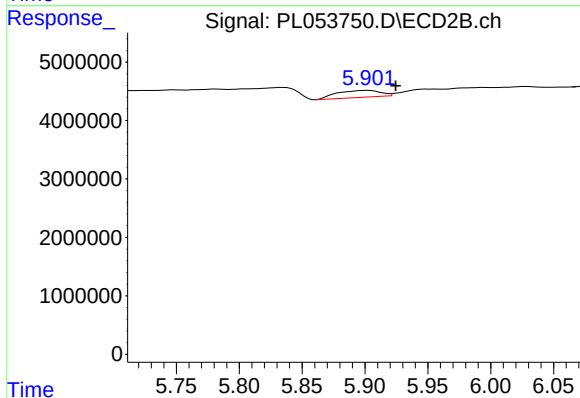


#8 Heptachlor epoxide

R.T.: 5.902 min
Delta R.T.: -0.022 min
Response: 2847104
Conc: 0.98 ng/ml

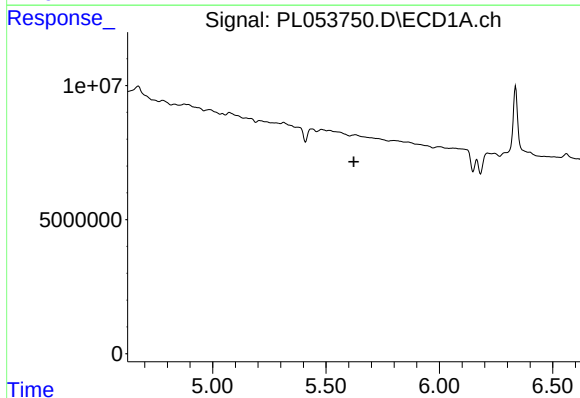


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 5.623 min
Response: 0
Conc: N.D.

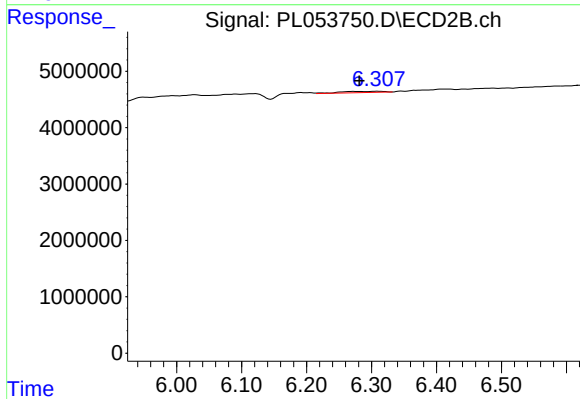

#9 Endosulfan I


R.T.: 6.308 min
Delta R.T.: 0.027 min
Response: 1066629
Conc: 0.39 ng/ml

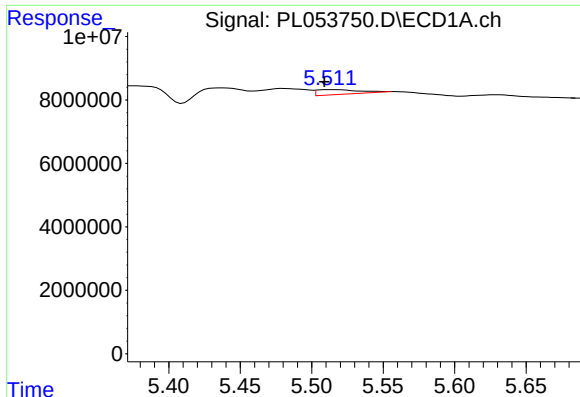

#10 gamma-Chlordane


R.T.: 5.512 min
Delta R.T.: 0.003 min
Response: 3110652
Conc: 0.23 ng/ml

Instrument :
ECD_L
ClientSampleId :

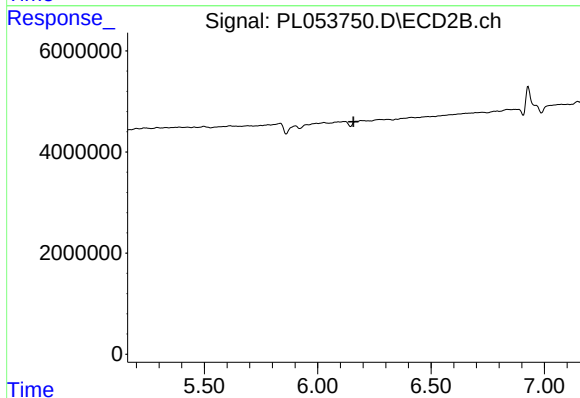


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

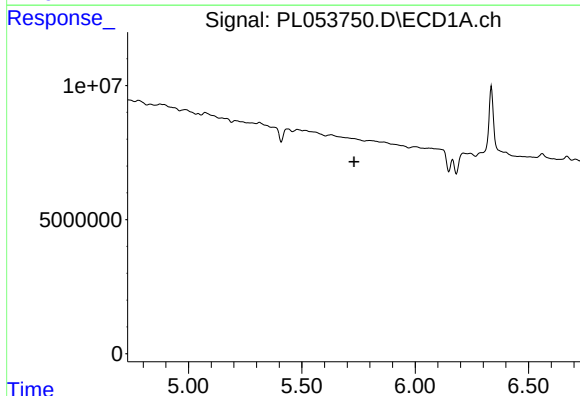


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 5.731 min
Response: 0
Conc: N.D.

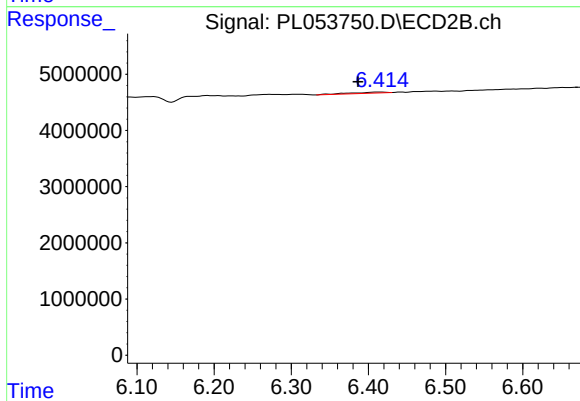

#12 4,4'-DDE


R.T.: 6.416 min
Delta R.T.: 0.029 min
Response: 634999
Conc: 0.23 ng/ml

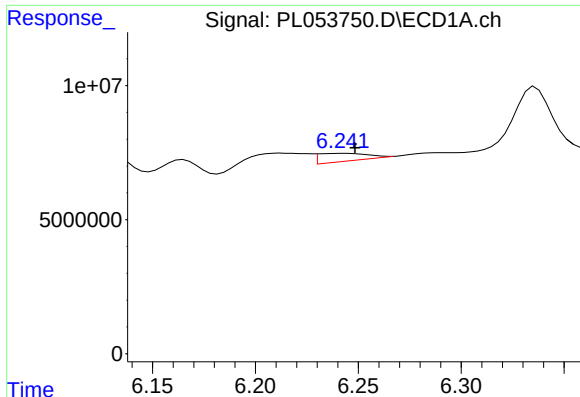

#16 4,4'-DDD


R.T.: 6.243 min
Delta R.T.: -0.005 min
Response: 4864035
Conc: 0.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

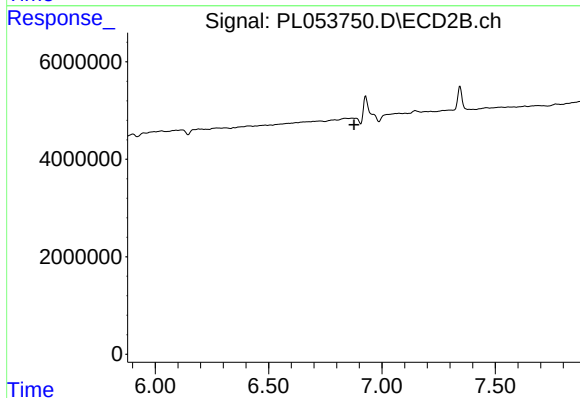


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.877 min
Response: 0
Conc: N.D.

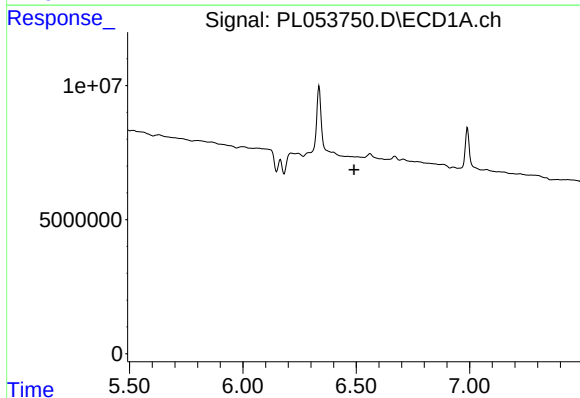


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.491 min
Response: 0
Conc: N.D.

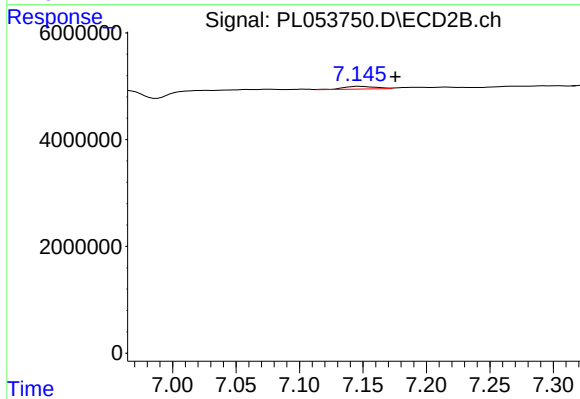

#17 4,4'-DDT


R.T.: 7.147 min
Delta R.T.: -0.029 min
Response: 895071
Conc: 0.39 ng/ml

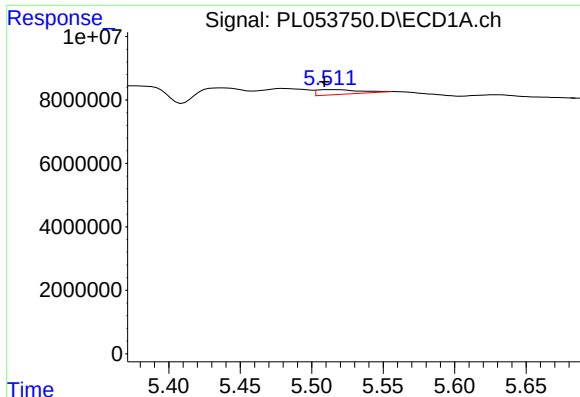

#25 Chlordane-3


R.T.: 5.512 min
Delta R.T.: 0.003 min
Response: 3110652
Conc: 2.70 ng/ml

Instrument :
ECD_L
ClientSampleId :

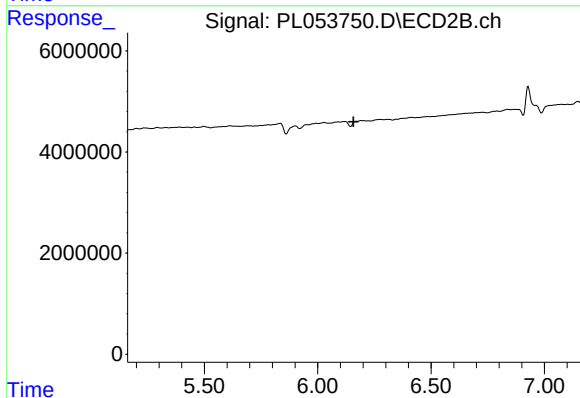


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.158 min
Response: 0
Conc: N.D.

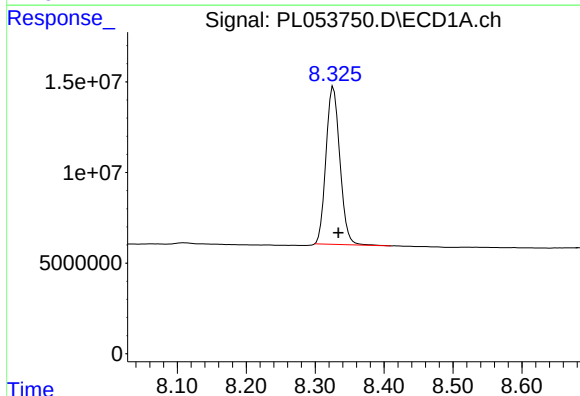

#28 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: -0.007 min
Response: 121613211
Conc: 12.39 ng/ml

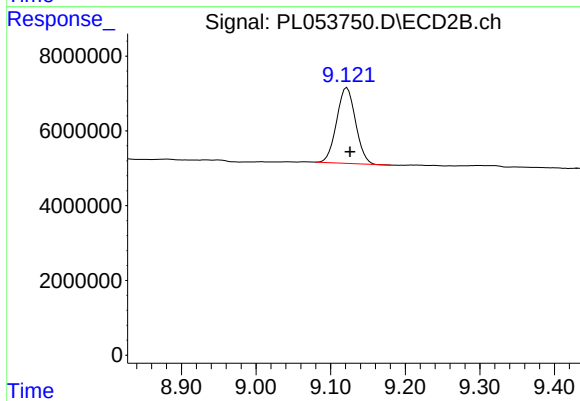

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 35642785
Conc: 12.66 ng/ml