

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
 Data File : PL053786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2019 00:32
 Operator : SG\AJ
 Sample : K5540-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 00:49:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.543	4.045	197.5E6	44701424	18.222	17.864
28)	SA Decachlor...	8.327	9.123	87319635	25056019	8.900	8.898
Target Compounds							
6)	B beta-BHC	4.501f	0.000	10205363	0	1.549	N.D. #
12)	B 4,4'-DDE	0.000	6.401	0	3438665	N.D.	1.221 #
13)	MA Dieldrin	5.877	0.000	11363028	0	0.872	N.D. #
15)	B Endosulfa...	0.000	6.973	0	2076661	N.D.	0.813 #
16)	A 4,4'-DDD	6.245	0.000	3498954	0	0.393	N.D. #
17)	MA 4,4'-DDT	0.000	7.150f	0	3348008	N.D.	1.448 #
18)	B Endrin al...	6.575	0.000	8051215	0	0.878	N.D. #
23)	Chlordane-1	4.428	0.000	2448009	0	6.902	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
Data File : PL053786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2019 00:32
Operator : SG\AJ
Sample : K5540-01
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 00:49:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

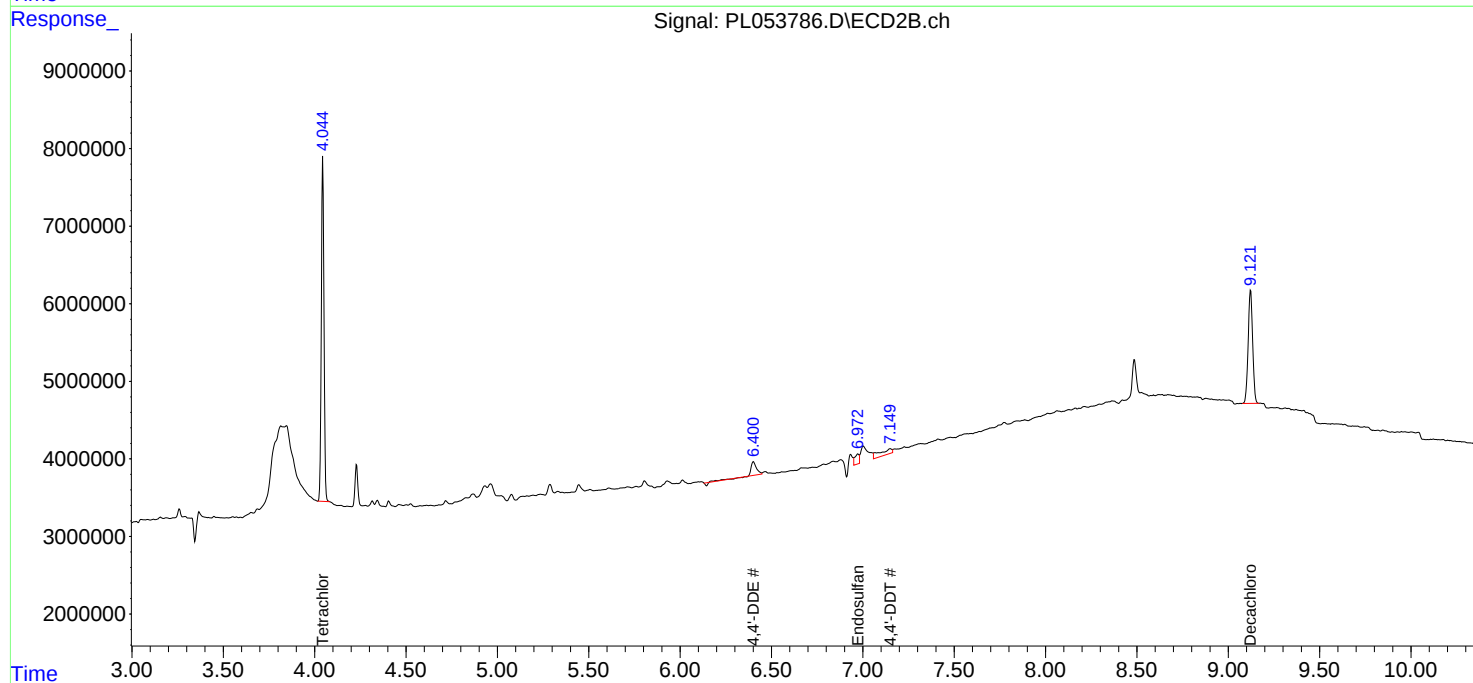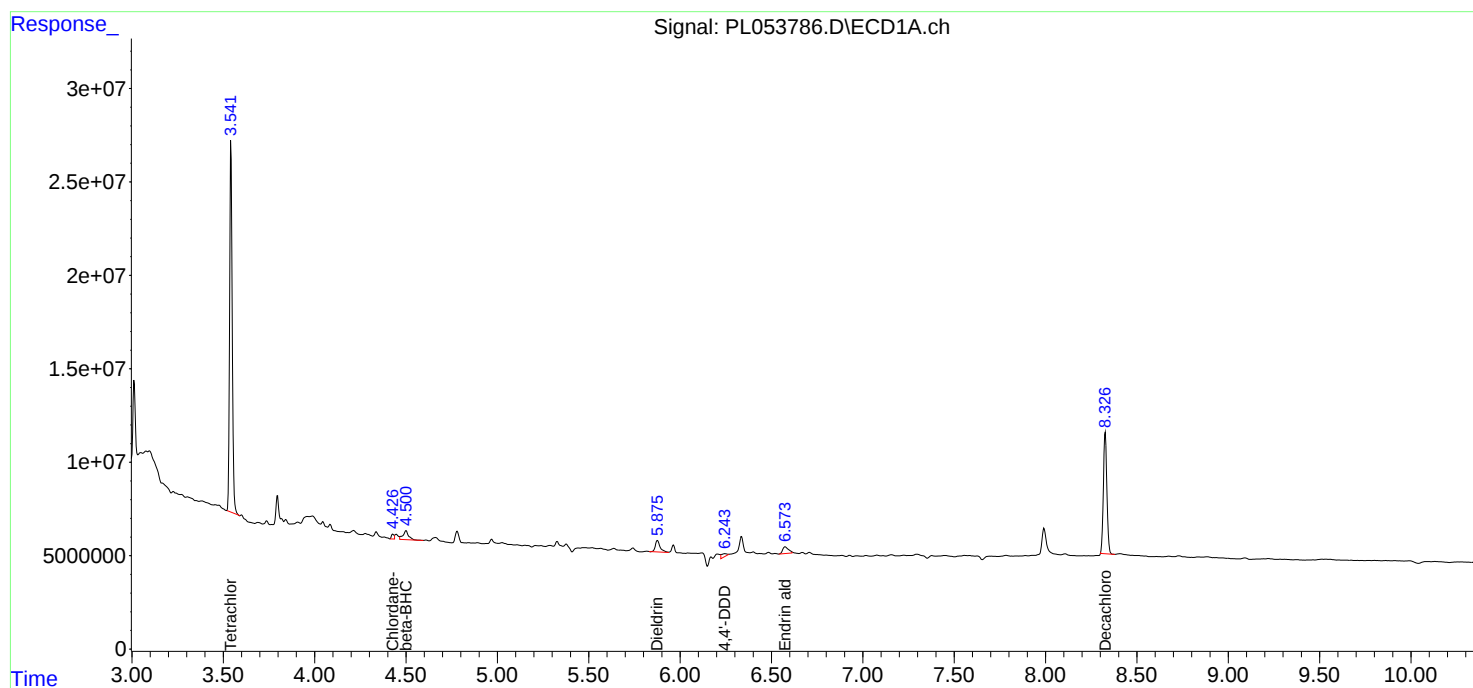


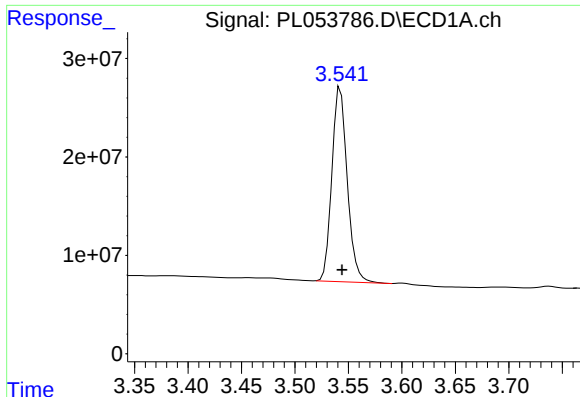

#1 Tetrachloro-m-xylene


R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 197511045
Conc: 18.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

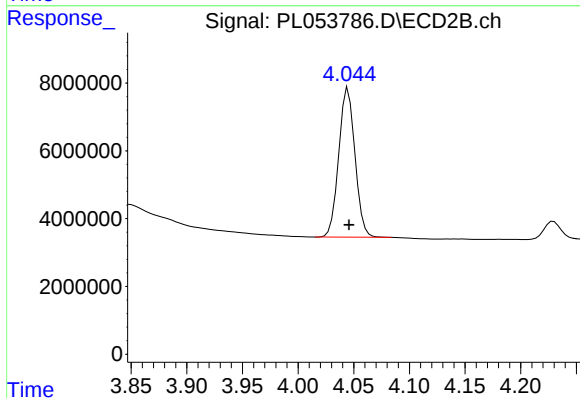


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 44701424
Conc: 17.86 ng/ml

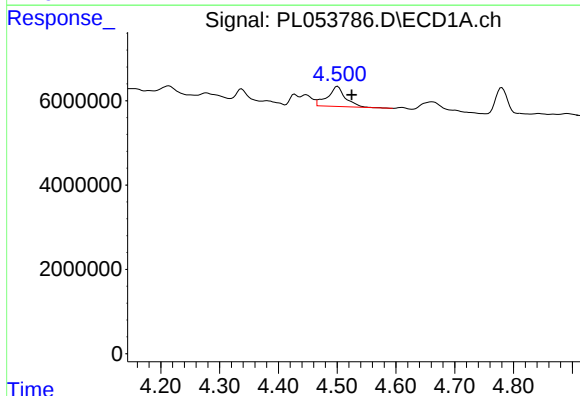


#6 beta-BHC

R.T.: 4.501 min
Delta R.T.: -0.024 min
Response: 10205363
Conc: 1.55 ng/ml

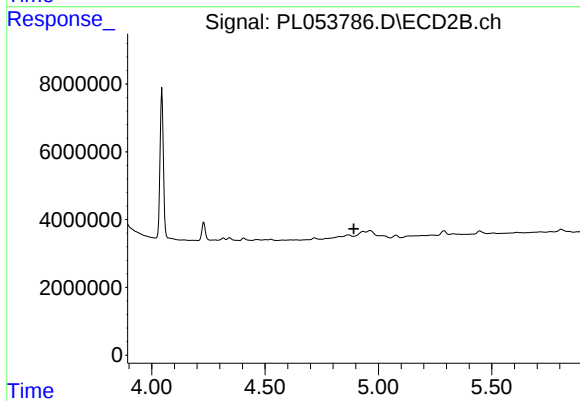

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.892 min
Response: 0
Conc: N.D.

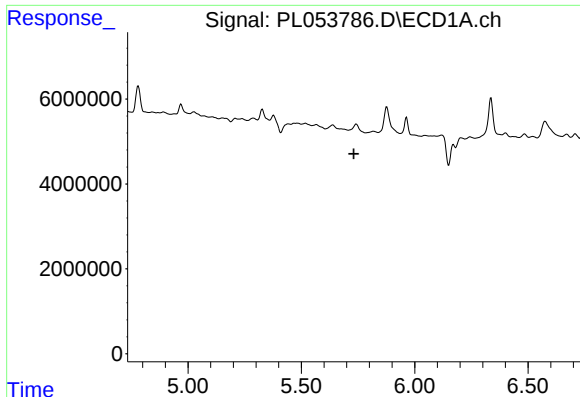

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T.: 5.731 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

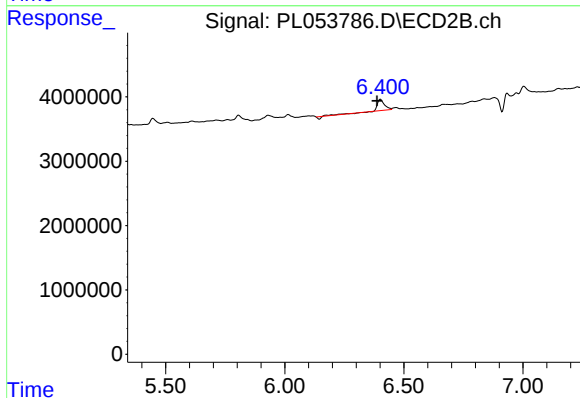


#12 4,4'-DDE

R.T.: 6.401 min
Delta R.T.: 0.015 min
Response: 3438665
Conc: 1.22 ng/ml

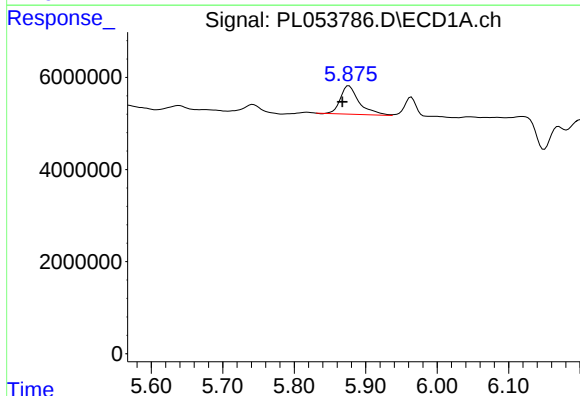


#13 Dieldrin

R.T.: 5.877 min
Delta R.T.: 0.009 min
Response: 11363028
Conc: 0.87 ng/ml

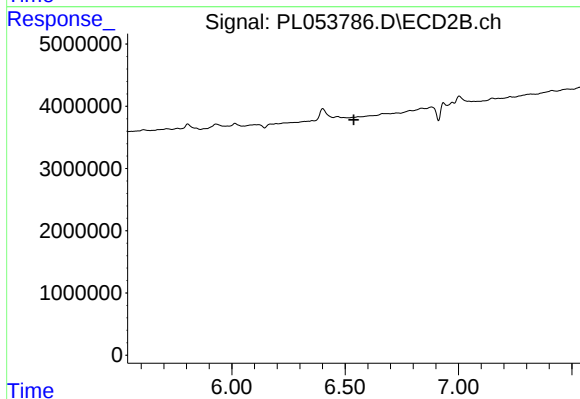

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.538 min
Response: 0
Conc: N.D.

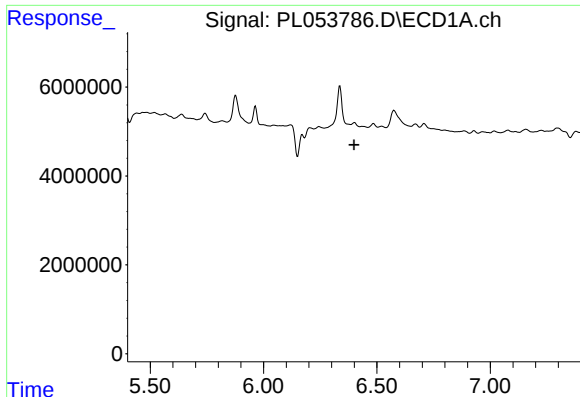

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.399 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

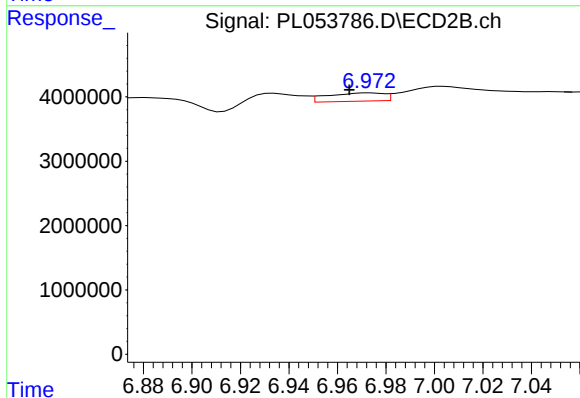


#15 Endosulfan II

R.T.: 6.973 min
Delta R.T.: 0.008 min
Response: 2076661
Conc: 0.81 ng/ml

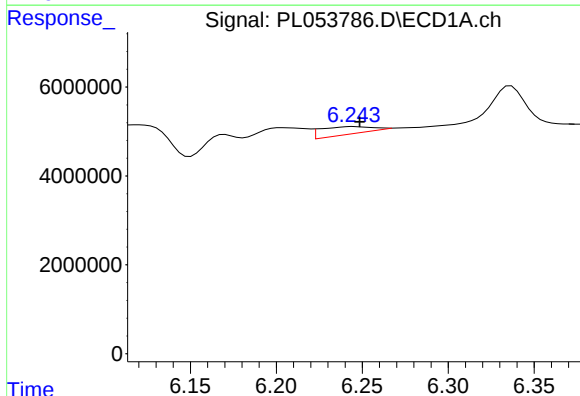


#16 4,4'-DDD

R.T.: 6.245 min
Delta R.T.: -0.004 min
Response: 3498954
Conc: 0.39 ng/ml

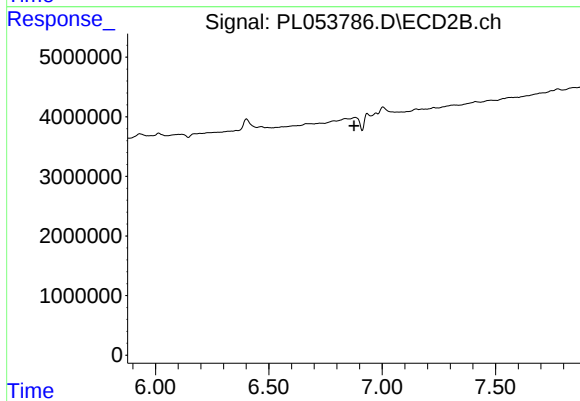

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.877 min
Response: 0
Conc: N.D.

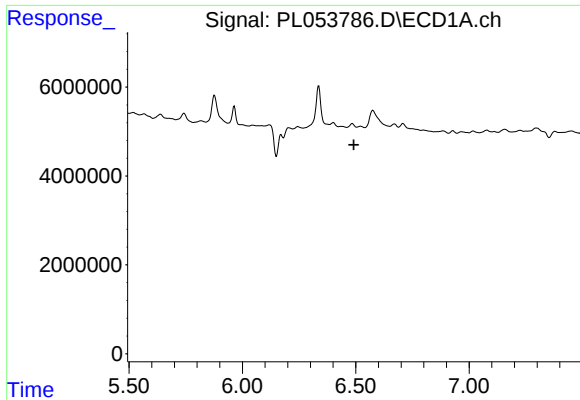

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.491 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

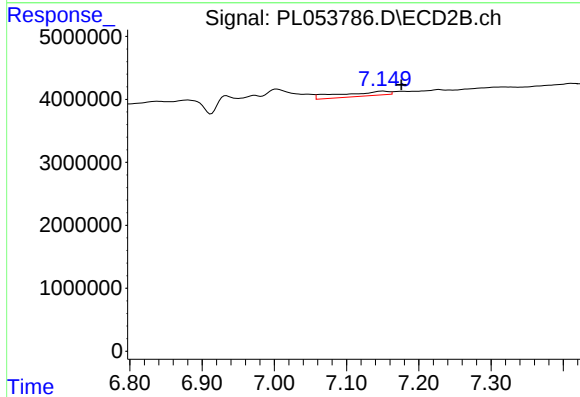


#17 4,4'-DDT

R.T.: 7.150 min
Delta R.T.: -0.025 min
Response: 3348008
Conc: 1.45 ng/ml

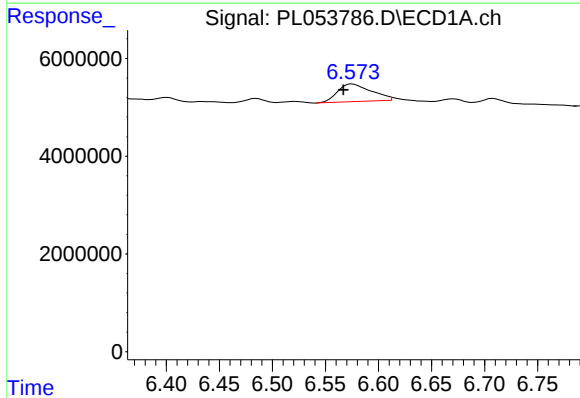


#18 Endrin aldehyde

R.T.: 6.575 min
Delta R.T.: 0.008 min
Response: 8051215
Conc: 0.88 ng/ml

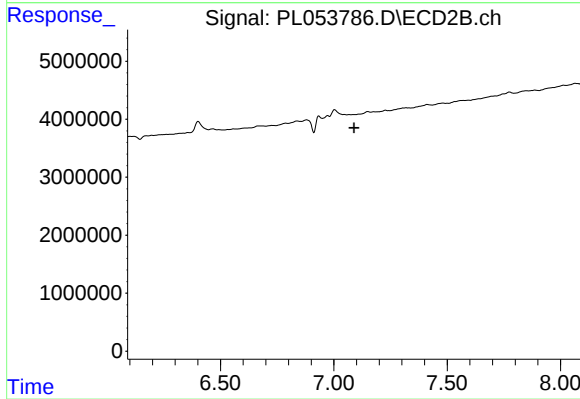

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 7.089 min
Response: 0
Conc: N.D.

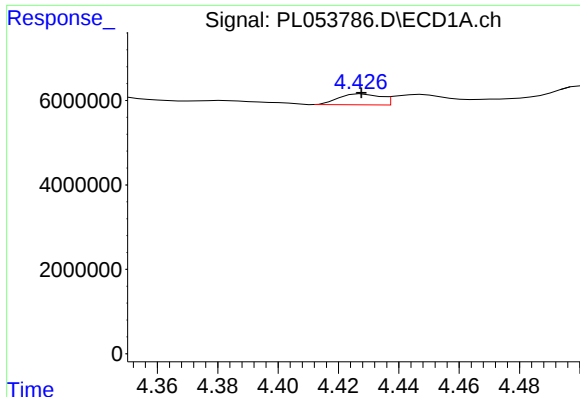

#23 Chlordane-1


R.T.: 4.428 min
Delta R.T.: 0.000 min
Response: 2448009
Conc: 6.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

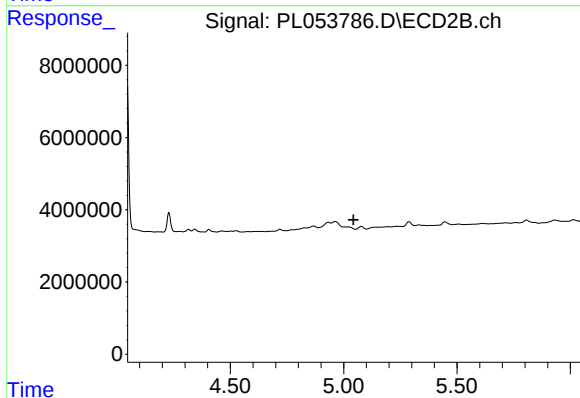


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.043 min
Response: 0
Conc: N.D.

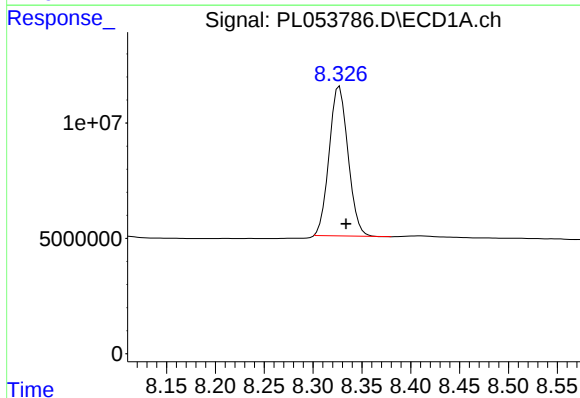

#28 Decachlorobiphenyl

R.T.: 8.327 min
Delta R.T.: -0.007 min
Response: 87319635
Conc: 8.90 ng/ml

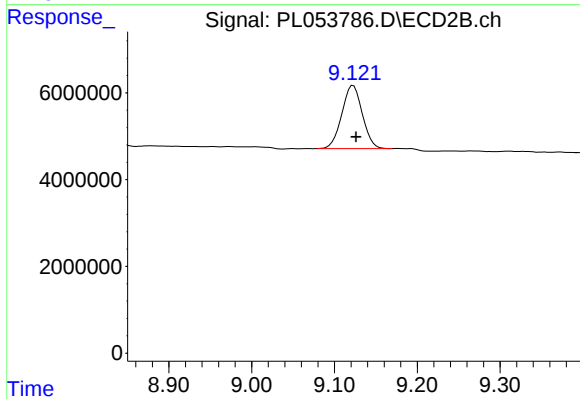

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 25056019
Conc: 8.90 ng/ml