

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
 Data File : PL053789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2019 01:14
 Operator : SG\AJ
 Sample : K5540-03
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 155-40-(0-1.1)

Manual Integrations
 APPROVED

Ankita
 10/28/2019 12:30:29 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 03:33:09 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.045	97129050	22618788	8.961	9.039
28)	SA Decachlor...	8.325	9.122	114.9E6	30711830	11.713m	10.906
Target Compounds							
12)	B 4,4'-DDE	5.727	6.384	77305128	20690536	6.506	7.347
17)	MA 4,4'-DDT	6.486	7.173	98975060	17480527	9.991	7.559

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
Data File : PL053789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2019 01:14
Operator : SG\AJ
Sample : K5540-03
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
155-40-(0-1.1)


Manual Integrations
APPROVED

Ankita
10/28/2019 12:30:29 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 03:33:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

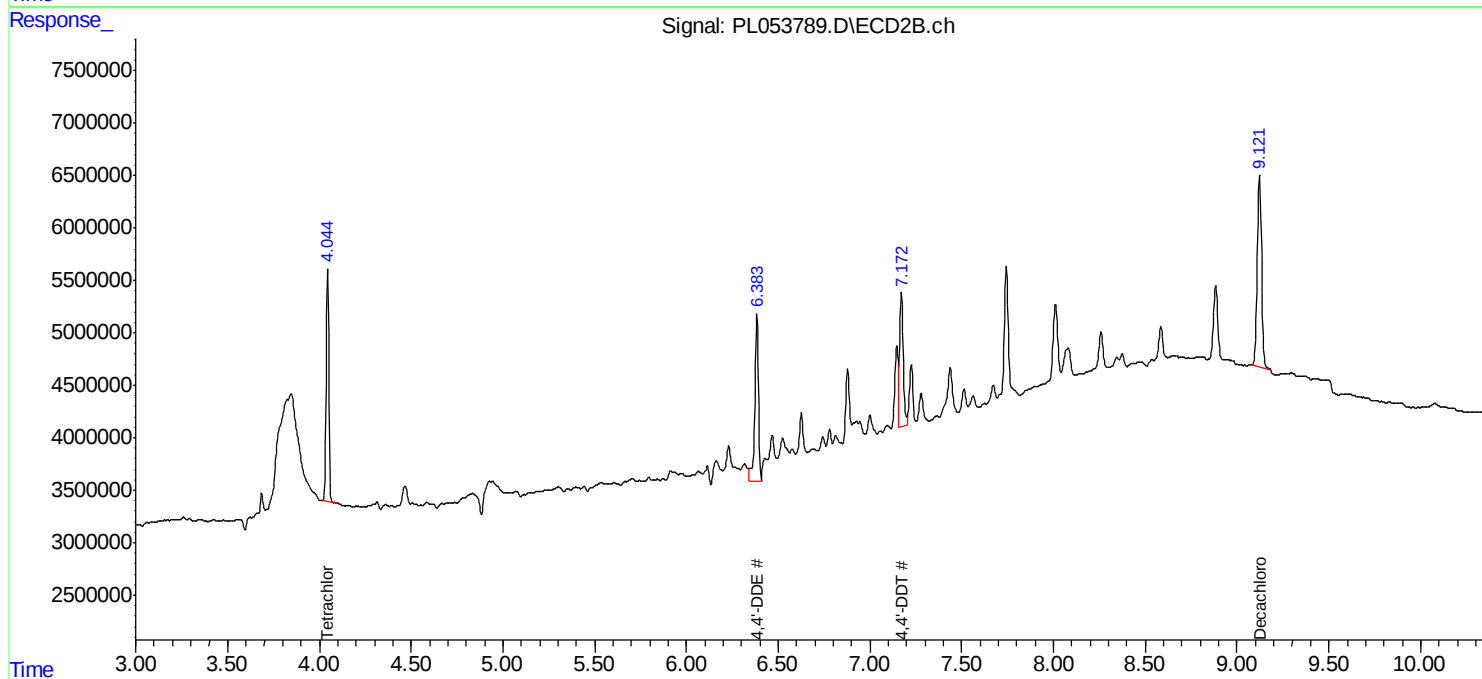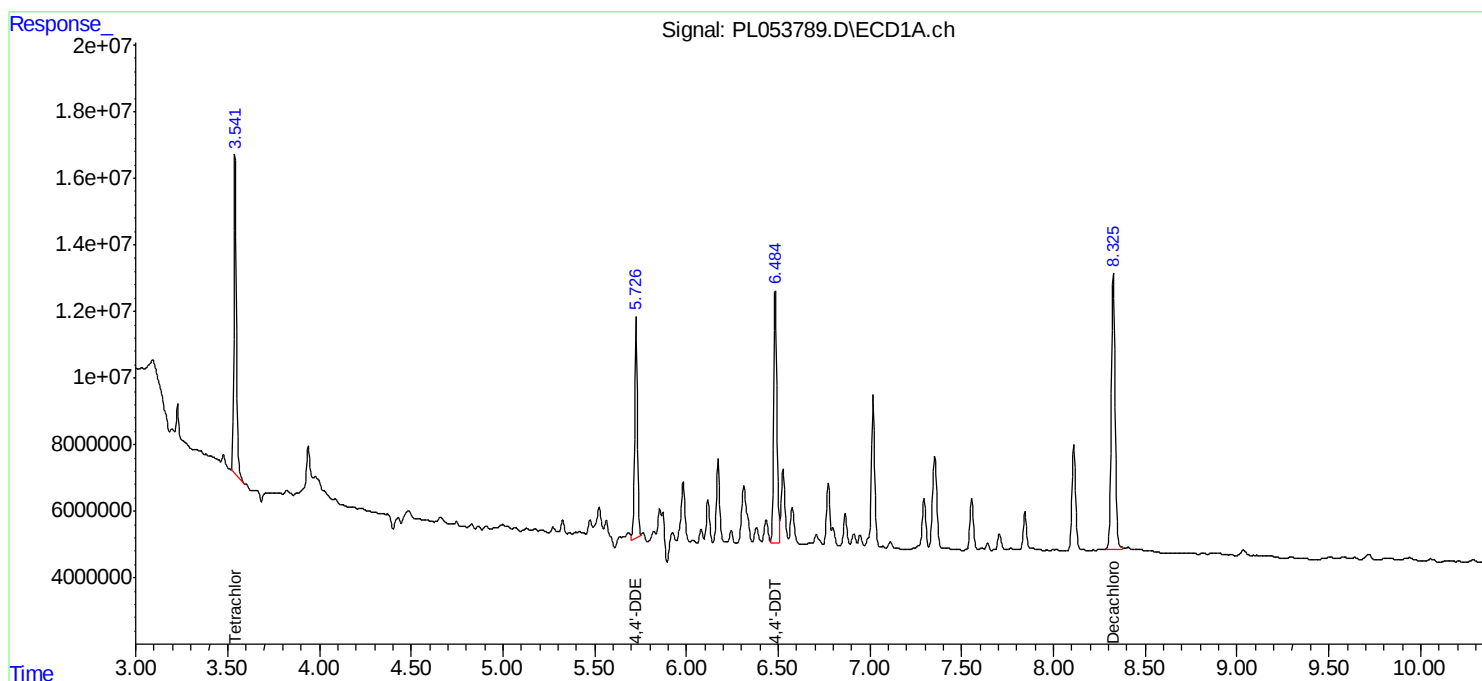

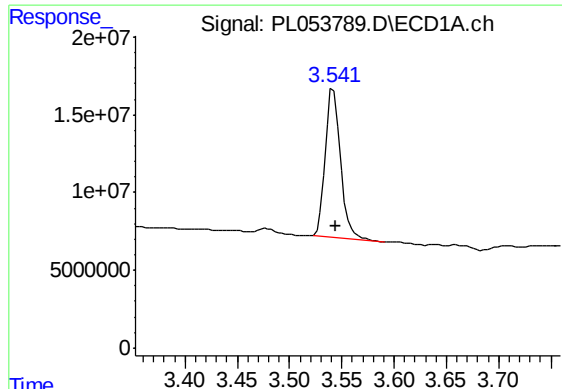


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 97129050
Conc: 8.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
155-40-(0-1.1)


Manual Integrations
APPROVED

Ankita
10/28/2019 12:30:29 PM

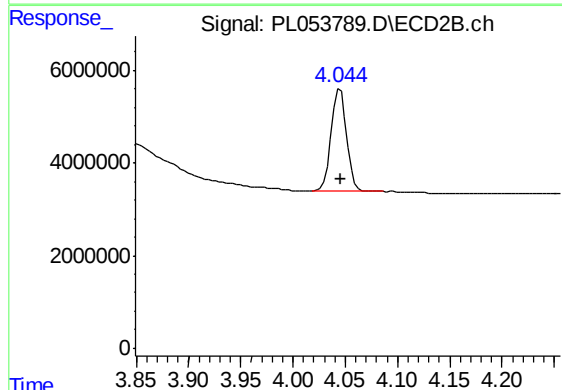


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 22618788
Conc: 9.04 ng/ml

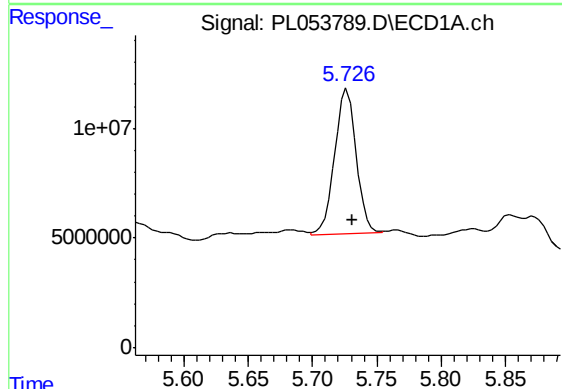


#12 4,4'-DDE

R.T.: 5.727 min
Delta R.T.: -0.004 min
Response: 77305128
Conc: 6.51 ng/ml

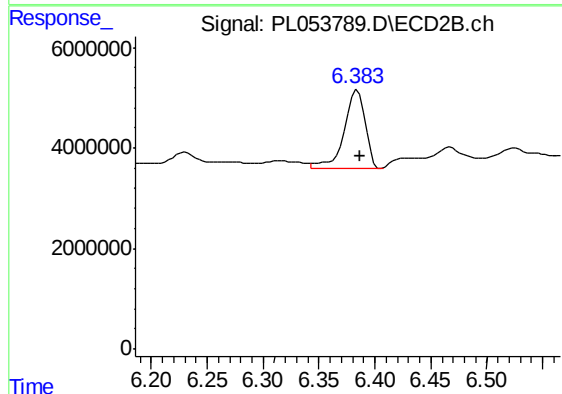

#12 4,4'-DDE

R.T.: 6.384 min
Delta R.T.: -0.003 min
Response: 20690536
Conc: 7.35 ng/ml

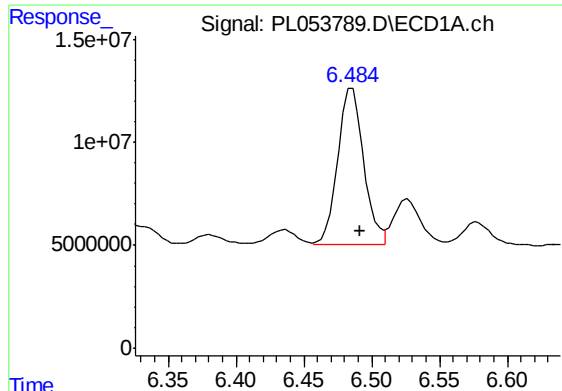


#17 4,4'-DDT

R.T.: 6.486 min
Delta R.T.: -0.005 min
Response: 98975060
Conc: 9.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
155-40-(0-1.1)


Manual Integrations
APPROVED

Ankita
10/28/2019 12:30:29 PM

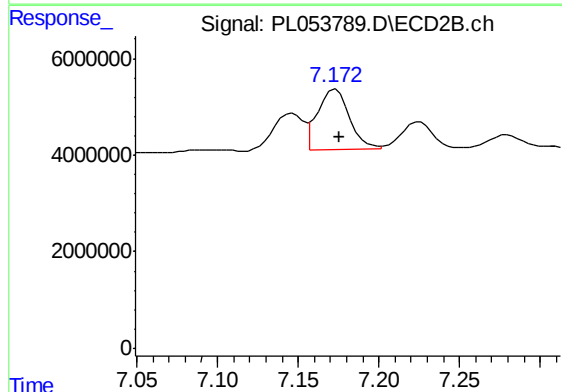


#17 4,4'-DDT

R.T.: 7.173 min
Delta R.T.: -0.002 min
Response: 17480527
Conc: 7.56 ng/ml

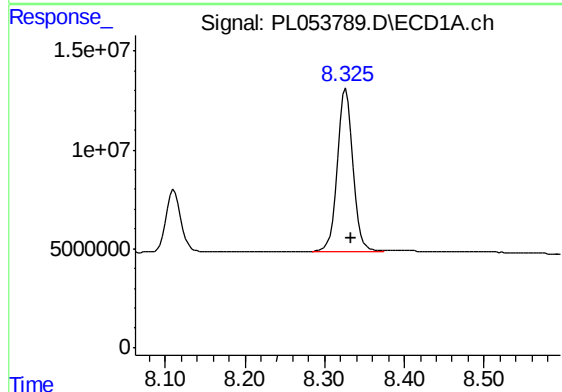

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 114924045
Conc: 11.71 ng/ml m

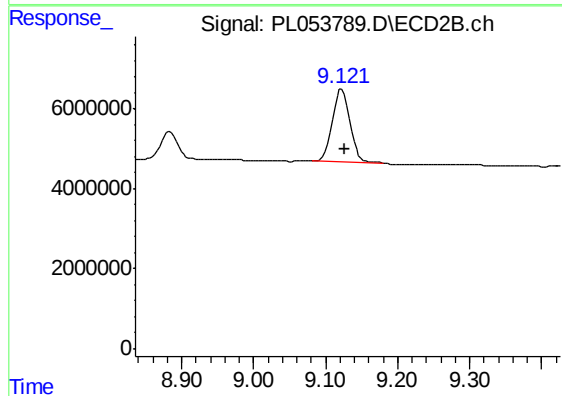

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 30711830
Conc: 10.91 ng/ml