

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
 Data File : PL053797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2019 03:05
 Operator : SG\AJ
 Sample : K5540-19
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 160-04-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/28/2019 2:39:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 03:34:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.045	194.5E6	43580622	17.943	17.416
28)	SA Decachlor...	8.325	9.123	113.7E6	31071648	11.592m	11.034
Target Compounds							
12)	B 4,4'-DDE	5.725	6.384	37181450	5277117	3.129	1.874 #
16)	A 4,4'-DDD	6.244	6.877	27504574	12776256	3.090	6.131 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
Data File : PL053797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2019 03:05
Operator : SG\AJ
Sample : K5540-19
Misc :
ALS Vial : 56 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
160-04-(0-1)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:39:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 03:34:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

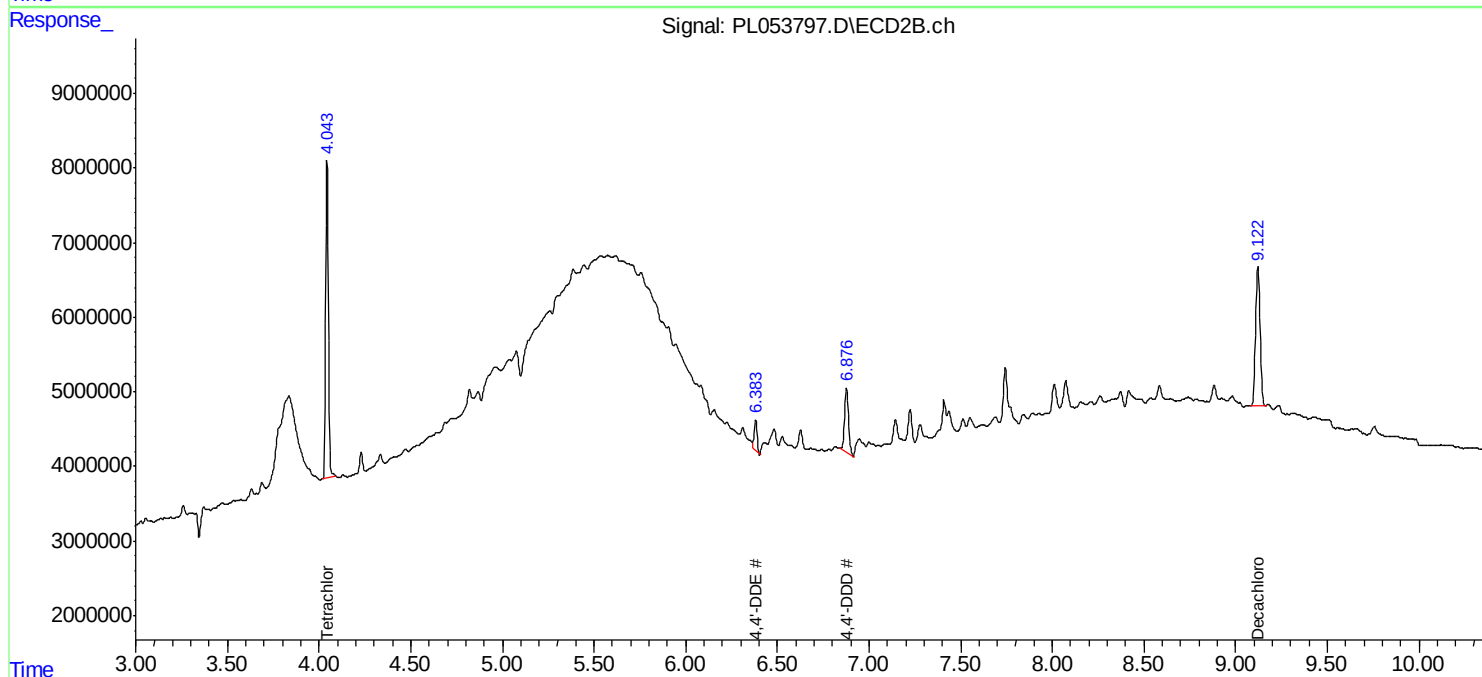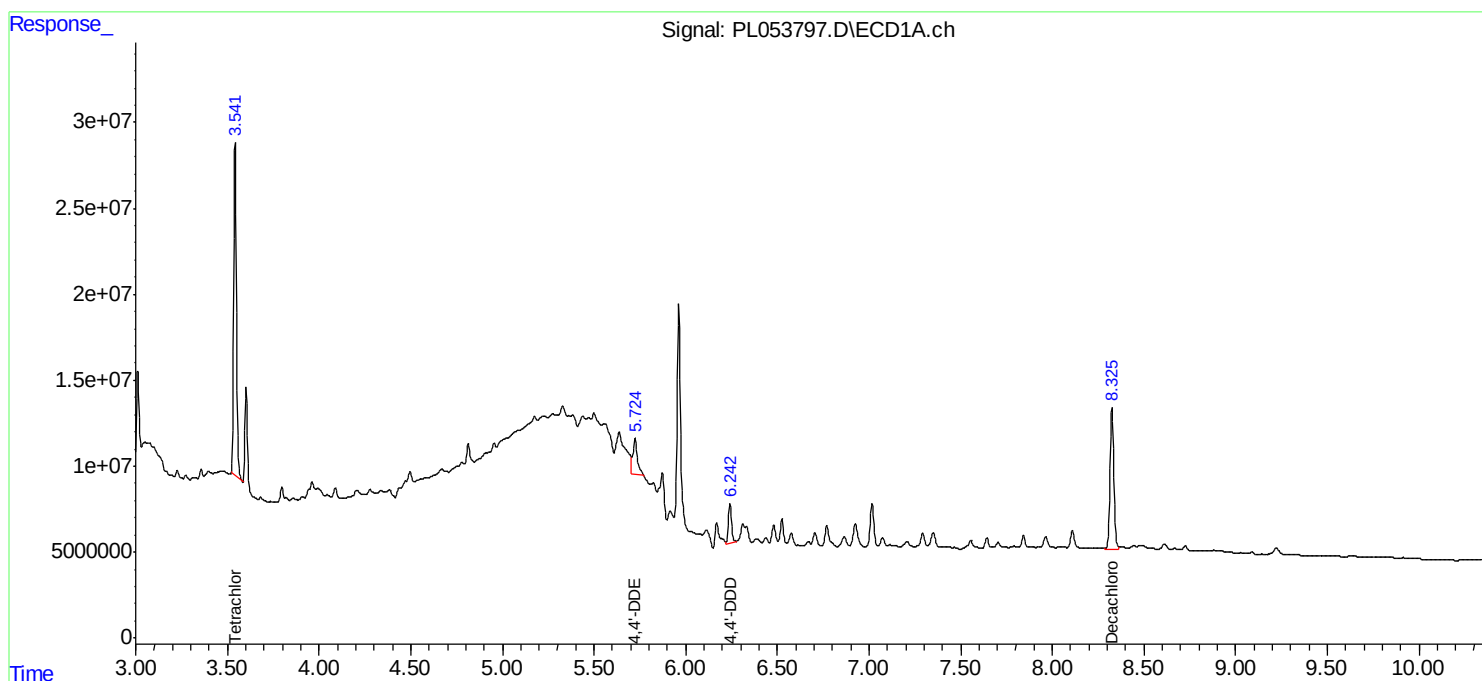

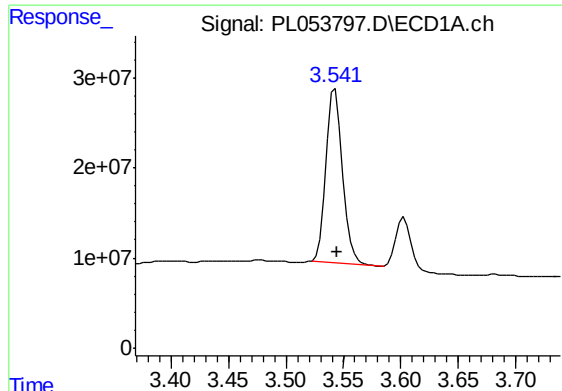


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 194485698
Conc: 17.94 ng/ml

Instrument :
ECD_L
ClientSampleId :
160-04-(0-1)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:39:53 PM

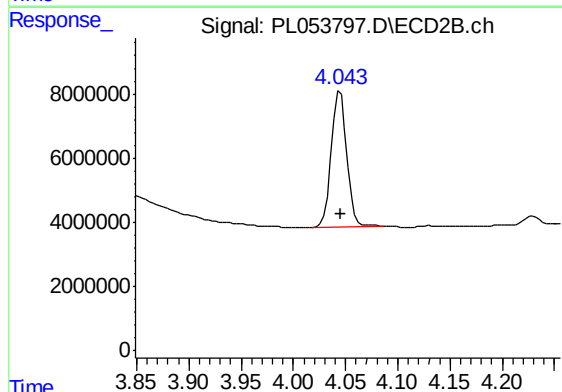


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 43580622
Conc: 17.42 ng/ml

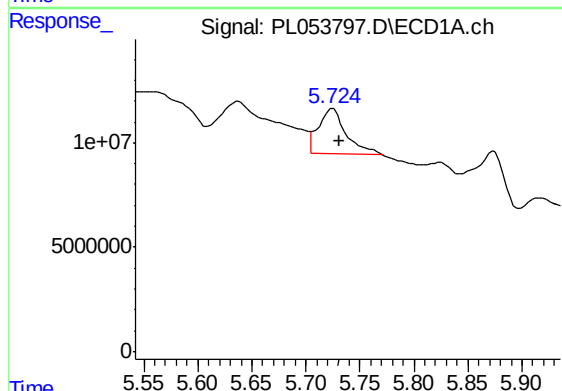


#12 4,4'-DDE

R.T.: 5.725 min
Delta R.T.: -0.006 min
Response: 37181450
Conc: 3.13 ng/ml

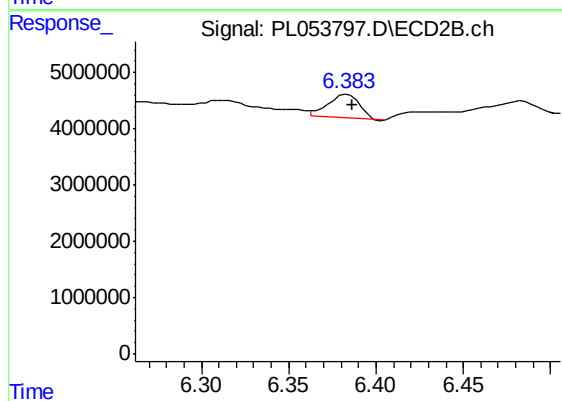

#12 4,4'-DDE

R.T.: 6.384 min
Delta R.T.: -0.003 min
Response: 5277117
Conc: 1.87 ng/ml

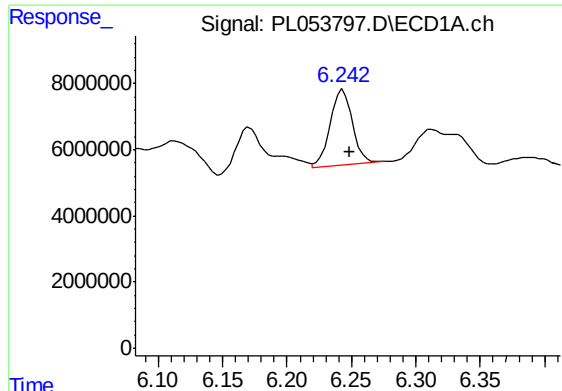


#16 4,4'-DDD

R.T.: 6.244 min
Delta R.T.: -0.005 min
Response: 27504574
Conc: 3.09 ng/ml

Instrument :
ECD_L
ClientSampleId :
160-04-(0-1)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:39:53 PM

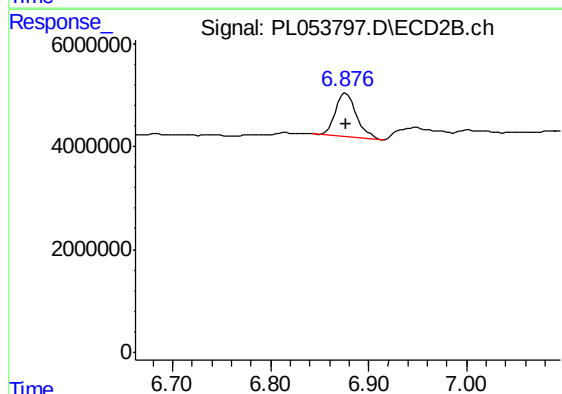


#16 4,4'-DDD

R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 12776256
Conc: 6.13 ng/ml

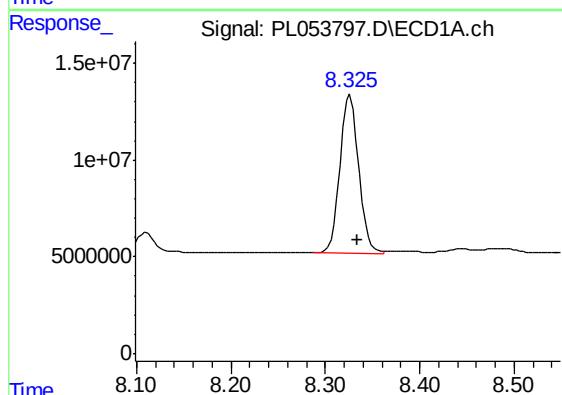

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 113740454
Conc: 11.59 ng/ml m

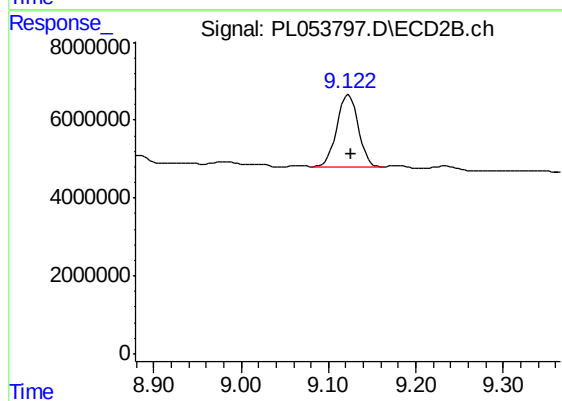

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 31071648
Conc: 11.03 ng/ml