

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
 Data File : PL053798.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2019 03:19
 Operator : SG\AJ
 Sample : K5541-01
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 154-24-(0-2)

Manual Integrations
 APPROVED

Ankita
 10/28/2019 2:39:55 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 03:35:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.542	4.045	107.3E6	25279961	9.903	10.102
28)	SA Decachlor...	8.325	9.122	62782119	17079076	6.399m	6.065
Target Compounds							
12)	B 4,4'-DDE	5.726	6.384	18453970	6249456	1.553	2.219 #
17)	MA 4,4'-DDT	6.483	7.174	36103480	4413821	3.644m	1.909 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
Data File : PL053798.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2019 03:19
Operator : SG\AJ
Sample : K5541-01
Misc :
ALS Vial : 57 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
154-24-(0-2)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:39:55 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 03:35:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

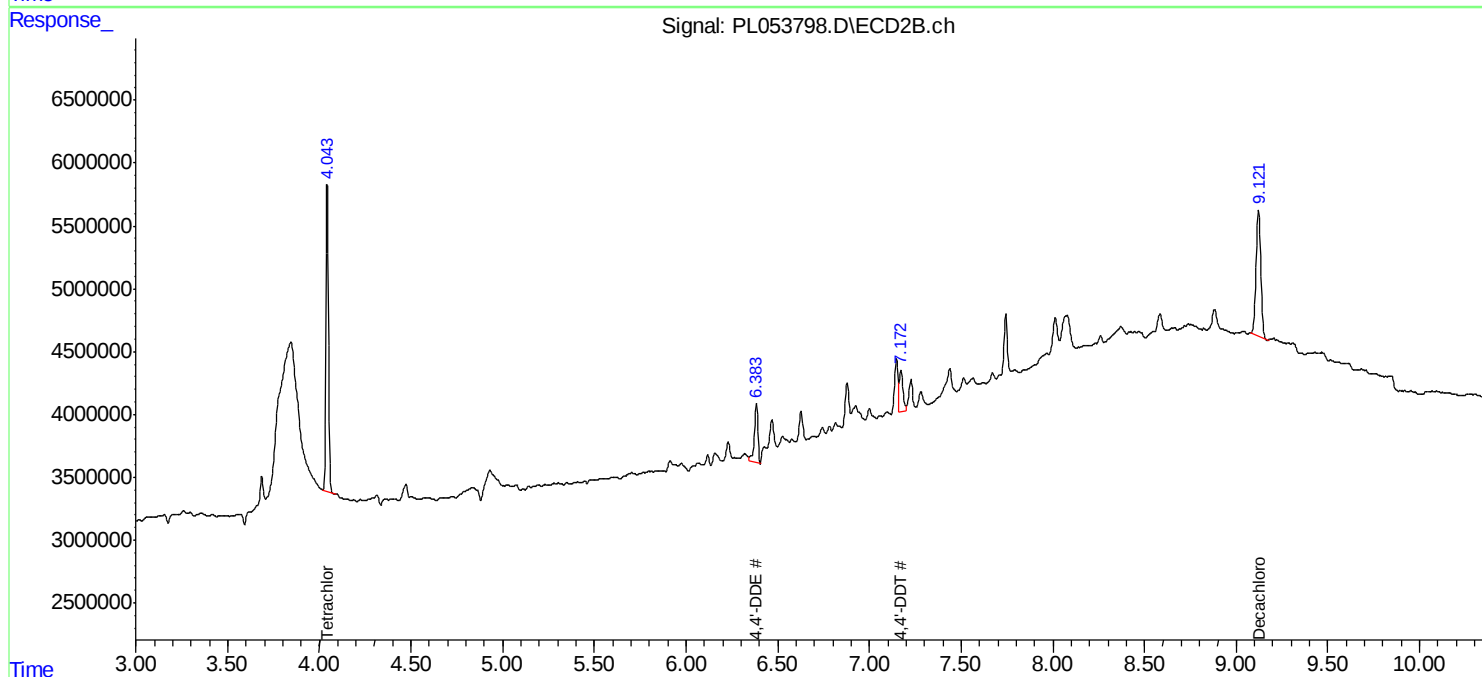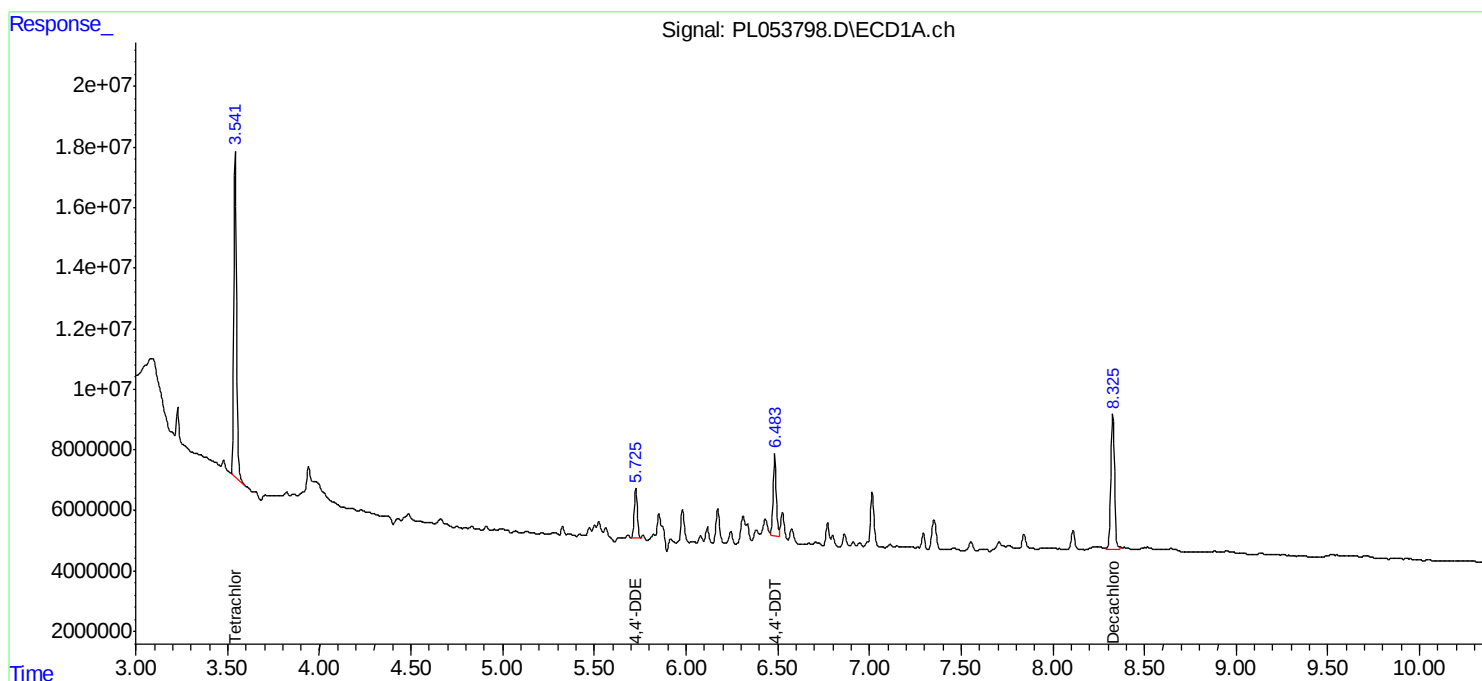

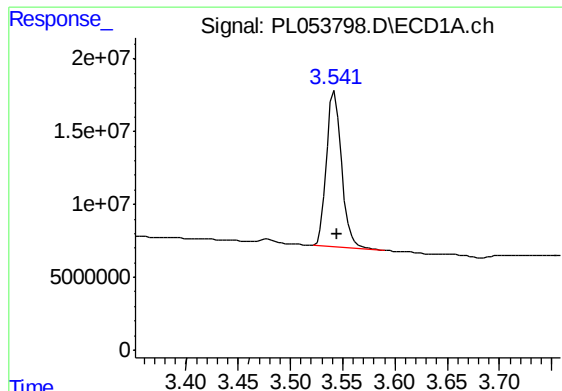


#1 Tetrachloro-m-xylene

R.T.: 3.542 min
Delta R.T.: -0.002 min
Response: 107342960
Conc: 9.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
154-24-(0-2)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:39:55 PM

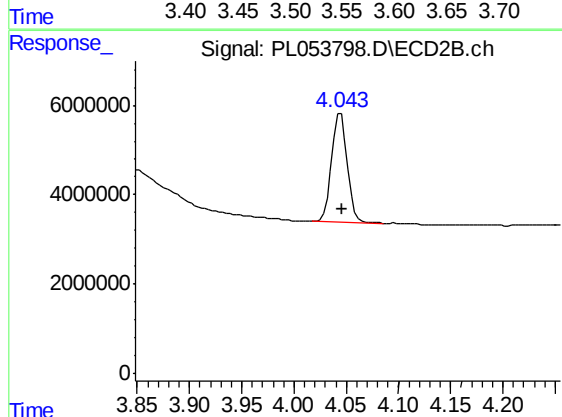


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: -0.001 min
Response: 25279961
Conc: 10.10 ng/ml

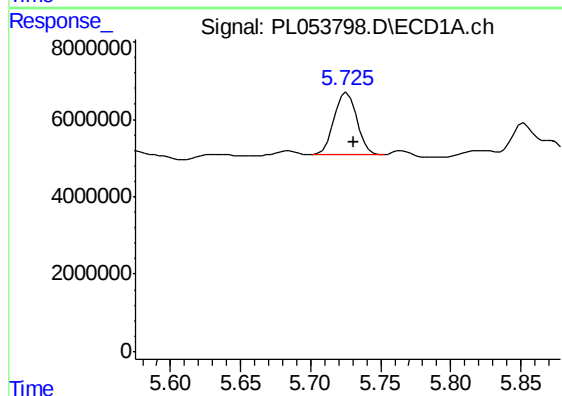


#12 4,4'-DDE

R.T.: 5.726 min
Delta R.T.: -0.005 min
Response: 18453970
Conc: 1.55 ng/ml

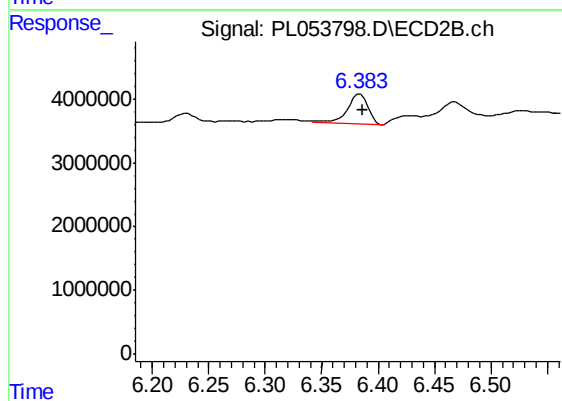

#12 4,4'-DDE

R.T.: 6.384 min
Delta R.T.: -0.002 min
Response: 6249456
Conc: 2.22 ng/ml

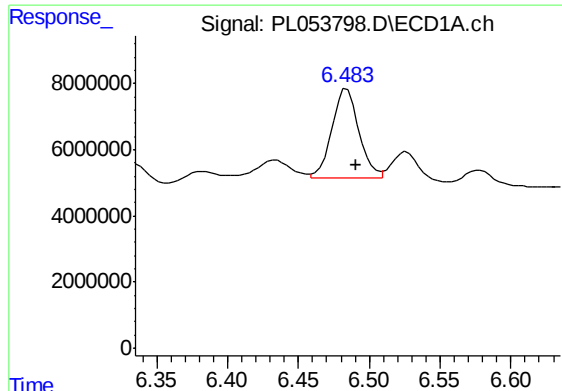


#17 4,4'-DDT

R.T.: 6.483 min
Delta R.T.: -0.008 min
Response: 36103480
Conc: 3.64 ng/ml m

Instrument :
ECD_L
ClientSampleId :
154-24-(0-2)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:39:55 PM

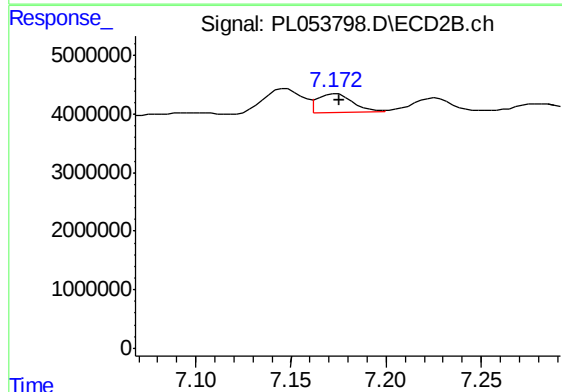


#17 4,4'-DDT

R.T.: 7.174 min
Delta R.T.: -0.002 min
Response: 4413821
Conc: 1.91 ng/ml

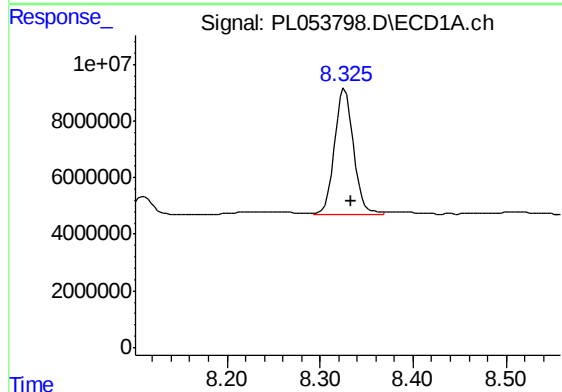

#28 Decachlorobiphenyl

R.T.: 8.325 min
Delta R.T.: -0.009 min
Response: 62782119
Conc: 6.40 ng/ml m

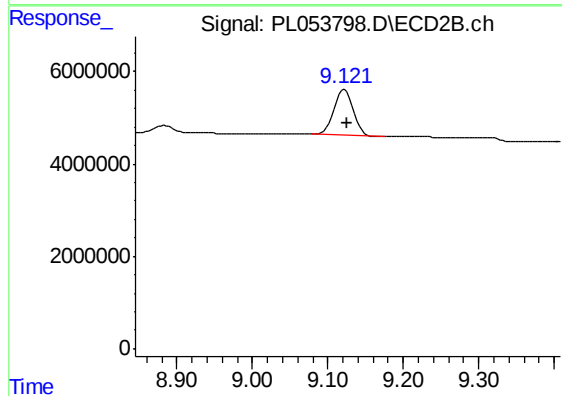

#28 Decachlorobiphenyl

R.T.: 9.122 min
Delta R.T.: -0.004 min
Response: 17079076
Conc: 6.06 ng/ml