

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
 Data File : PL053801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2019 04:01
 Operator : SG\AJ
 Sample : K5541-07
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 152-50-(0-1)

Manual Integrations
 APPROVED

Ankita
 10/28/2019 2:40:03 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 04:18:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
 Quant Title : GC Extractables
 QLast Update : Fri Oct 18 13:56:08 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.543	4.045	117.8E6	27934672	10.868	11.163
28) SA Decachlor...	8.324	9.123	86768078	23633998	8.843m	8.393
Target Compounds						
12) B 4,4'-DDE	5.727	6.388	29592229	4447178	2.490	1.579 #
17) MA 4,4'-DDT	6.485	7.174	89370613	13465447	9.022	5.823 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102519\
Data File : PL053801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2019 04:01
Operator : SG\AJ
Sample : K5541-07
Misc :
ALS Vial : 60 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
152-50-(0-1)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:40:03 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 04:18:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101919.M
Quant Title : GC Extractables
QLast Update : Fri Oct 18 13:56:08 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

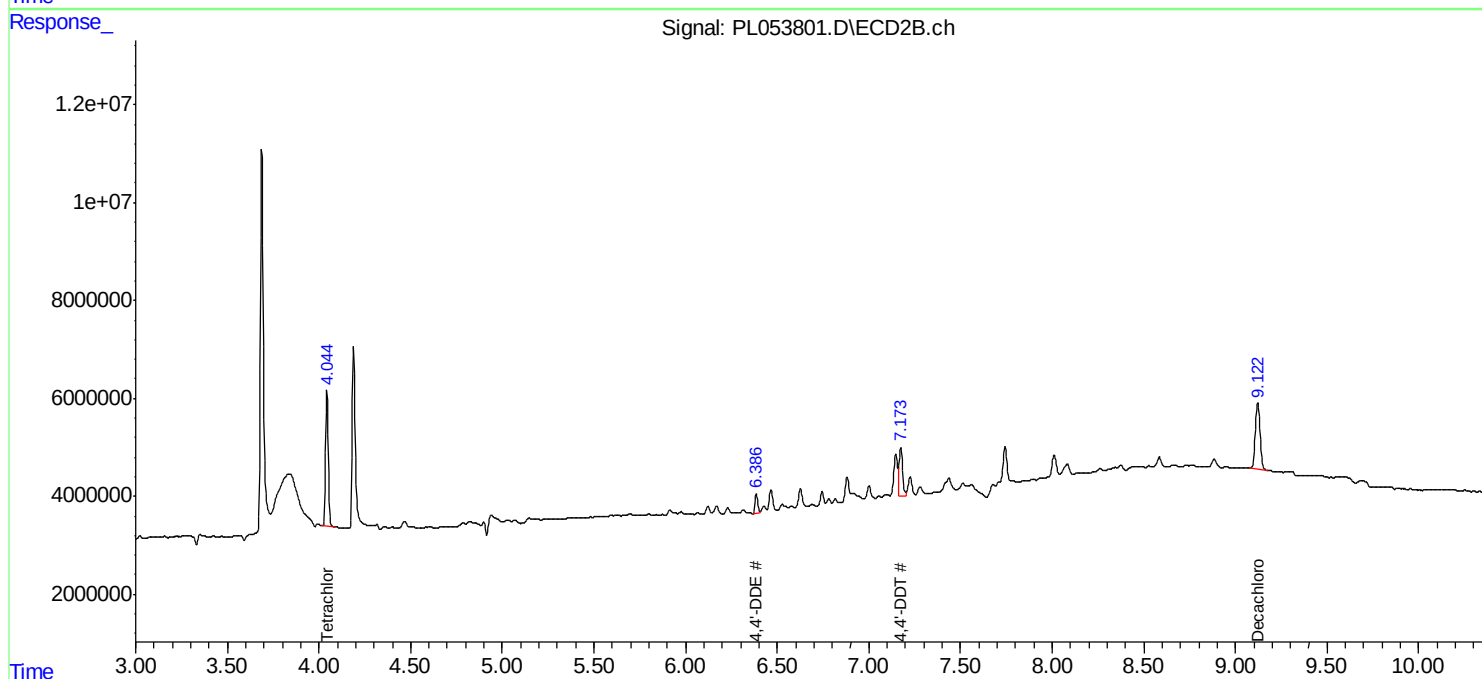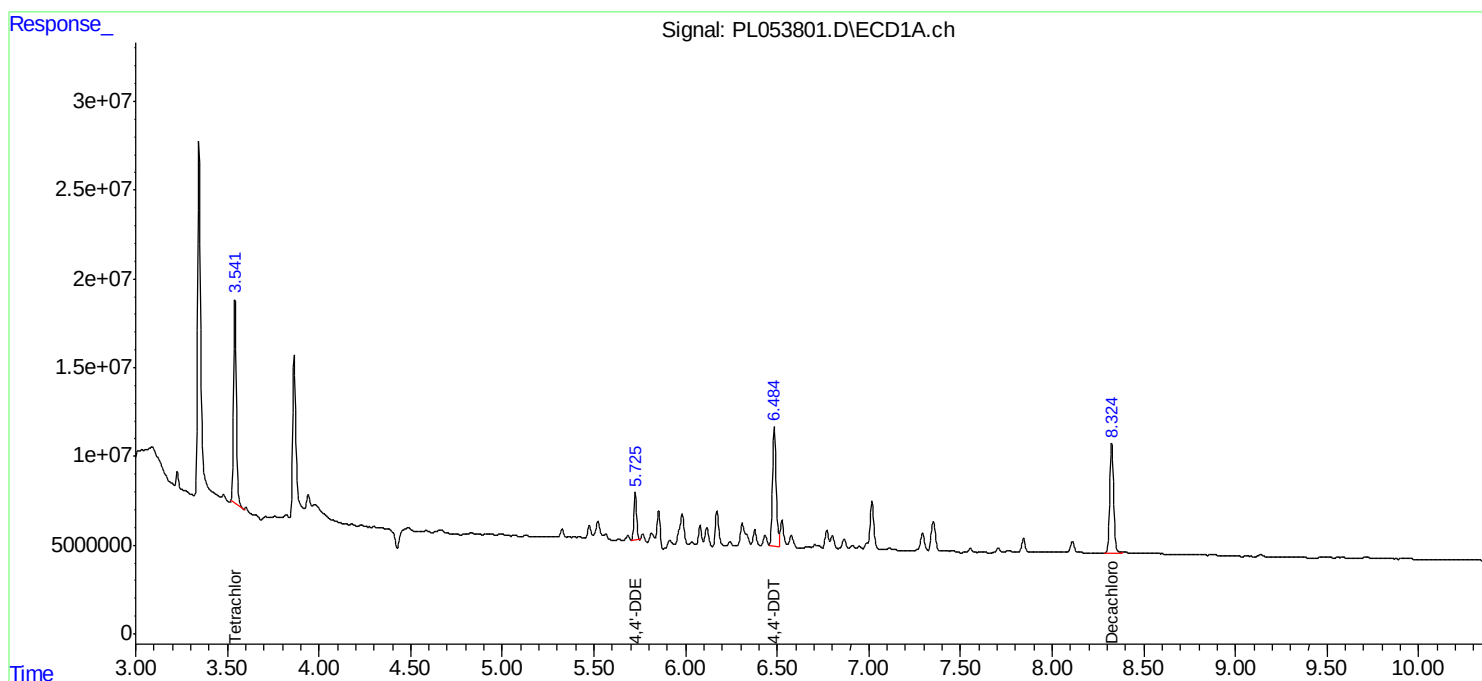

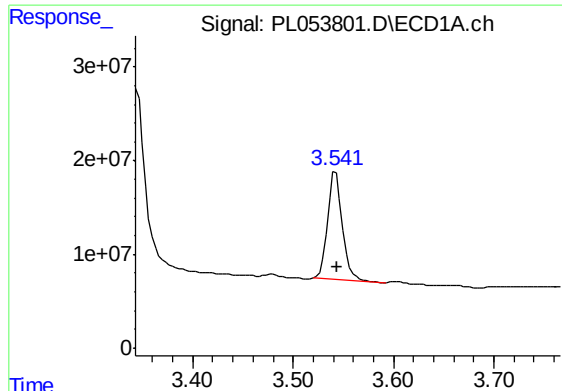


#1 Tetrachloro-m-xylene

R.T.: 3.543 min
Delta R.T.: -0.001 min
Response: 117801314
Conc: 10.87 ng/ml

Instrument :
ECD_L
ClientSampleId :
152-50-(0-1)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:40:03 PM

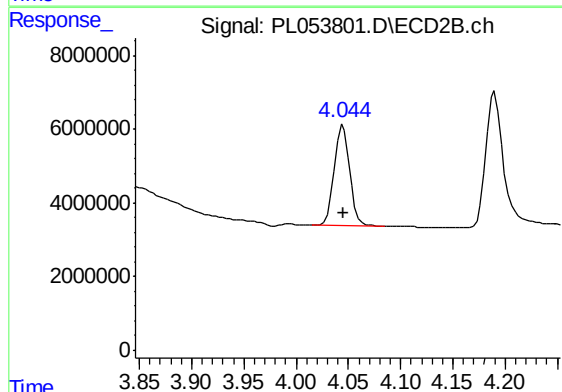


#1 Tetrachloro-m-xylene

R.T.: 4.045 min
Delta R.T.: 0.000 min
Response: 27934672
Conc: 11.16 ng/ml

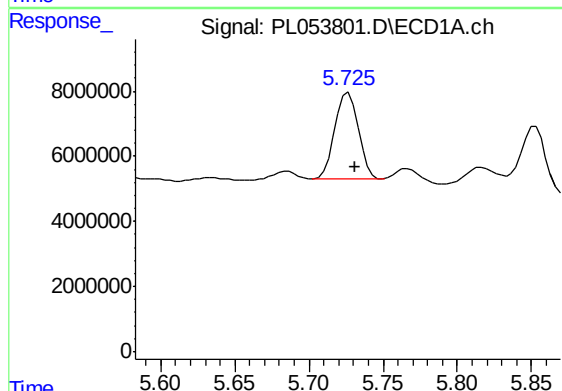


#12 4,4'-DDE

R.T.: 5.727 min
Delta R.T.: -0.004 min
Response: 29592229
Conc: 2.49 ng/ml

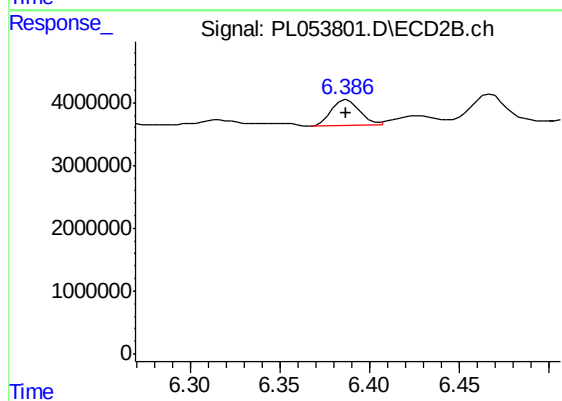

#12 4,4'-DDE

R.T.: 6.388 min
Delta R.T.: 0.000 min
Response: 4447178
Conc: 1.58 ng/ml

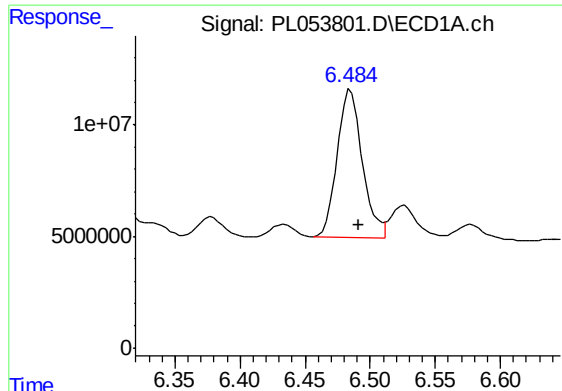


#17 4,4'-DDT

R.T.: 6.485 min
Delta R.T.: -0.006 min
Response: 89370613
Conc: 9.02 ng/ml

Instrument :
ECD_L
ClientSampleId :
152-50-(0-1)


Manual Integrations
APPROVED

Ankita
10/28/2019 2:40:03 PM

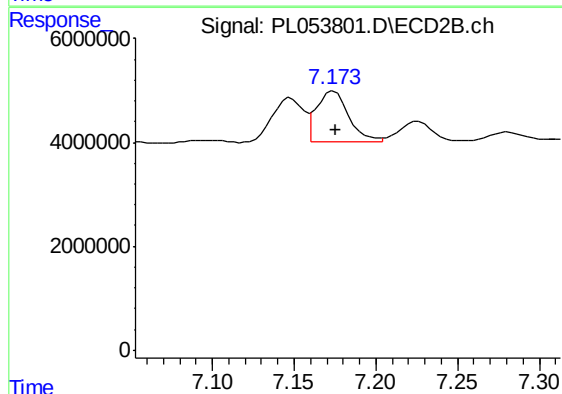


#17 4,4'-DDT

R.T.: 7.174 min
Delta R.T.: -0.001 min
Response: 13465447
Conc: 5.82 ng/ml

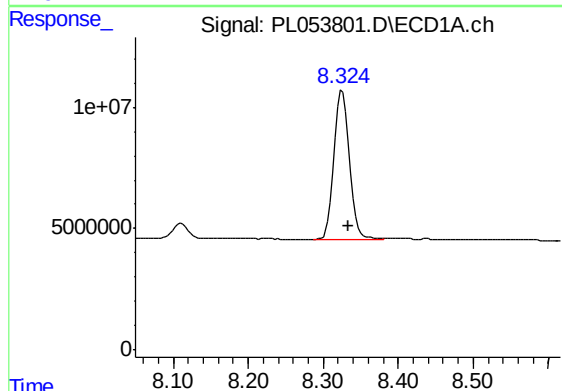

#28 Decachlorobiphenyl

R.T.: 8.324 min
Delta R.T.: -0.010 min
Response: 86768078
Conc: 8.84 ng/ml m

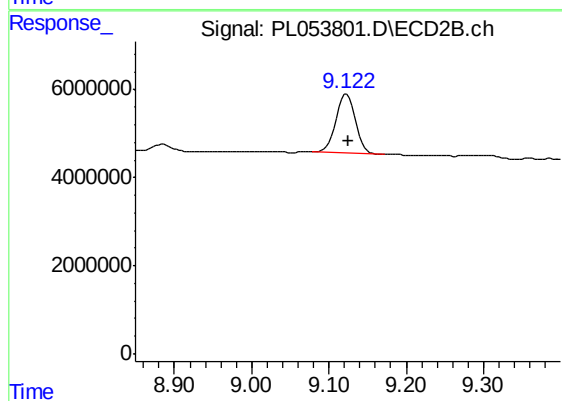

#28 Decachlorobiphenyl

R.T.: 9.123 min
Delta R.T.: -0.003 min
Response: 23633998
Conc: 8.39 ng/ml