

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102521\
 Data File : PL070521.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2021 20:23
 Operator : AR\AJ
 Sample : M4315-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 06:43:43 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.623	5.561	11698790	30716366	23.379	23.224
28)	SA Decachlor...	10.388	11.482	10362105	18920813	14.975	15.635
Target Compounds							
10)	B gamma-Chl...	7.372f	0.000	437483	0	0.604	N.D. #
13)	MA Dieldrin	7.754	0.000	522569	0	0.761	N.D. #
23)	Chlordane-1	5.950	6.945	368309	395633	20.079	8.618 #
25)	Chlordane-3	7.372f	0.000	437483	0	6.394	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102521\
Data File : PL070521.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2021 20:23
Operator : AR\AJ
Sample : M4315-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 06:43:43 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

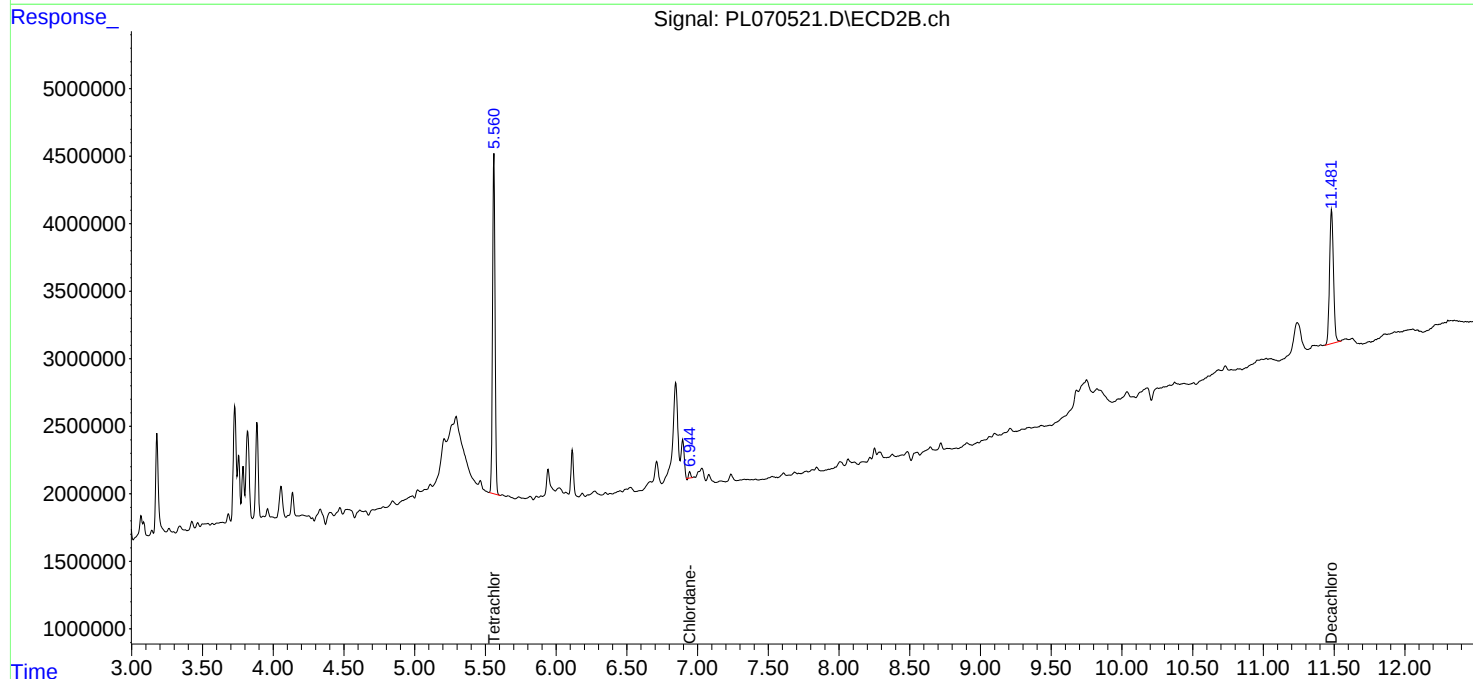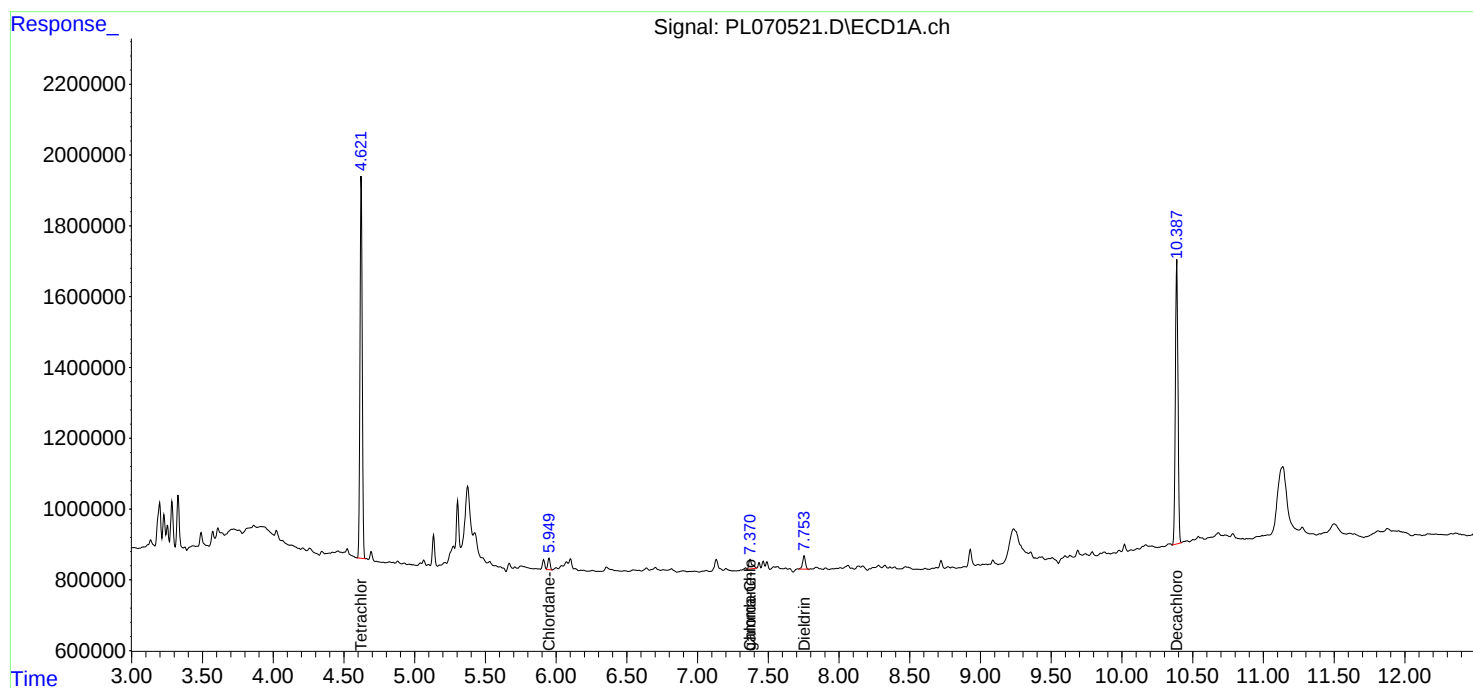


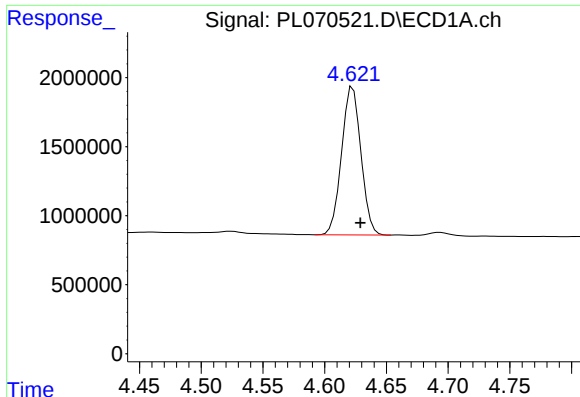

#1 Tetrachloro-m-xylene


R.T.: 4.623 min
Delta R.T.: -0.006 min
Response: 11698790
Conc: 23.38 ng/ml

Instrument :
ECD_L
ClientSampleId :

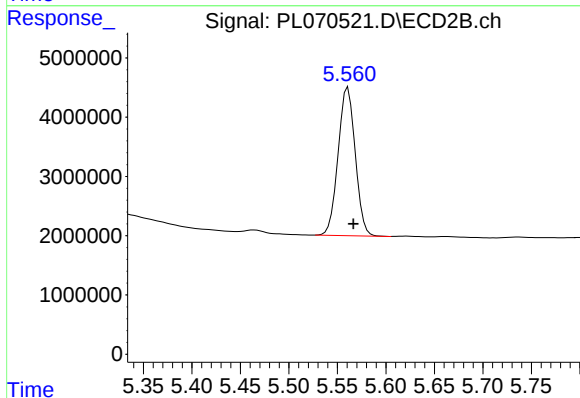


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: -0.006 min
Response: 30716366
Conc: 23.22 ng/ml

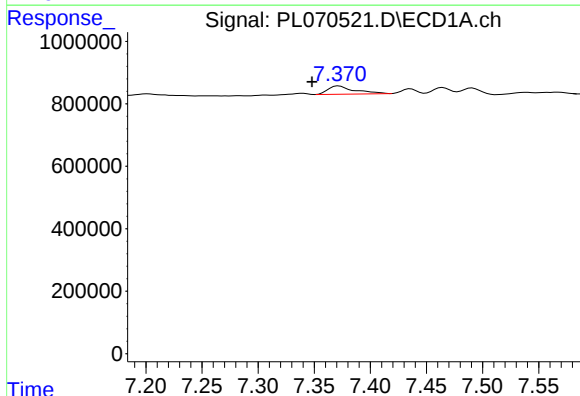


#10 gamma-Chlordane

R.T.: 7.372 min
Delta R.T.: 0.024 min
Response: 437483
Conc: 0.60 ng/ml

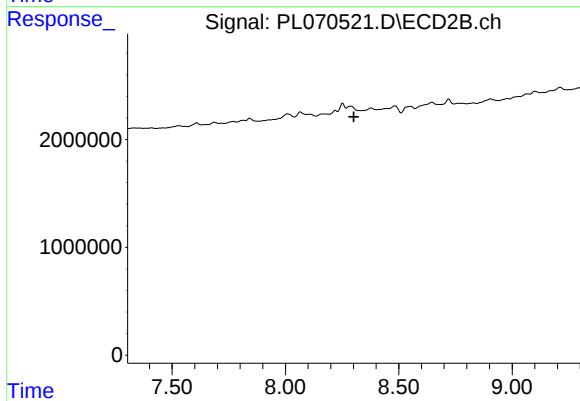

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 8.302 min
Response: 0
Conc: N.D.

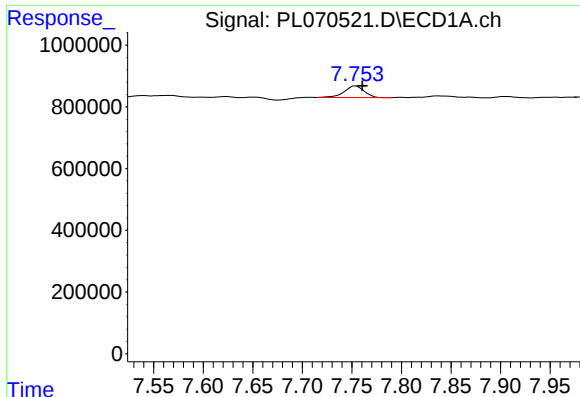

#13 Dieldrin


R.T.: 7.754 min
Delta R.T.: -0.007 min
Response: 522569
Conc: 0.76 ng/ml

Instrument :
ECD_L
ClientSampleId :

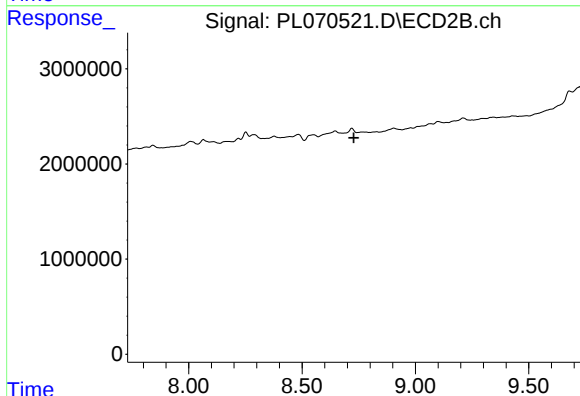


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.728 min
Response: 0
Conc: N.D.

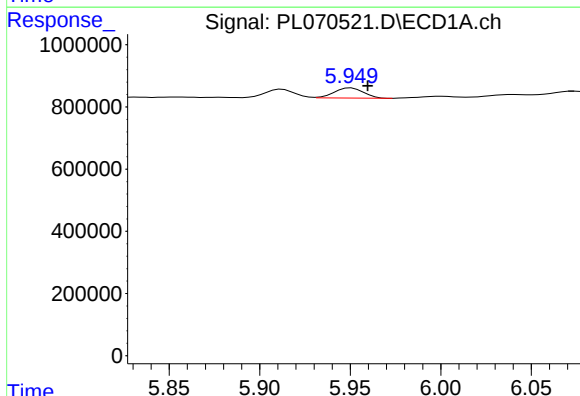


#23 Chlordane-1

R.T.: 5.950 min
Delta R.T.: -0.009 min
Response: 368309
Conc: 20.08 ng/ml

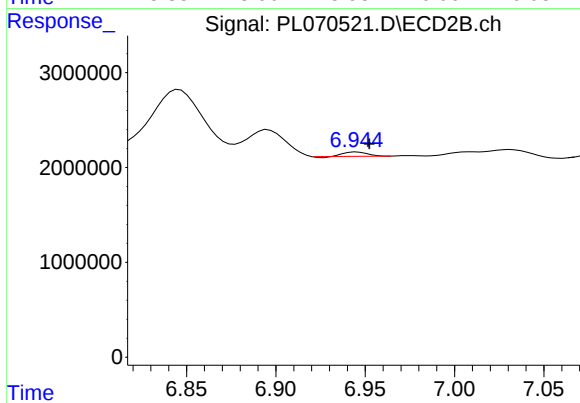

#23 Chlordane-1


R.T.: 6.945 min
Delta R.T.: -0.007 min
Response: 395633
Conc: 8.62 ng/ml

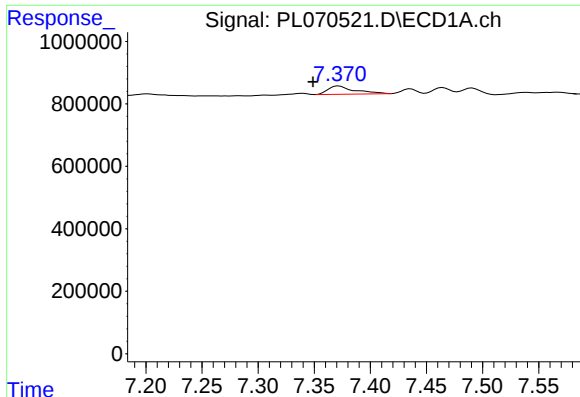

#25 Chlordane-3


R.T.: 7.372 min
Delta R.T.: 0.023 min
Response: 437483
Conc: 6.39 ng/ml

Instrument :
ECD_L
ClientSampleId :

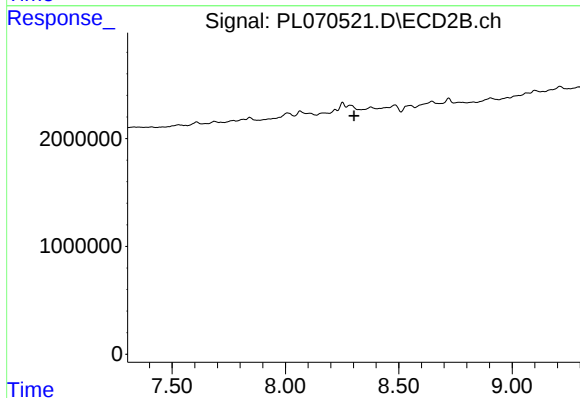


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 8.303 min
Response: 0
Conc: N.D.

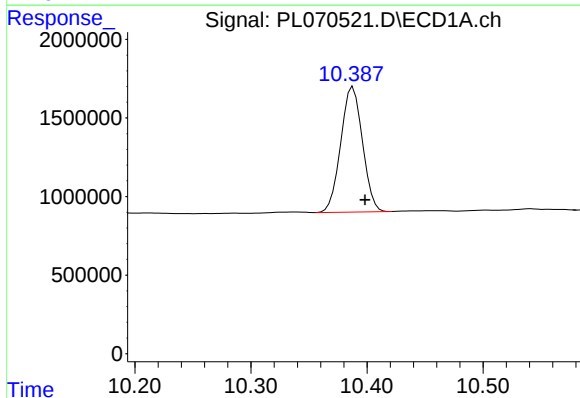

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.010 min
Response: 10362105
Conc: 14.97 ng/ml

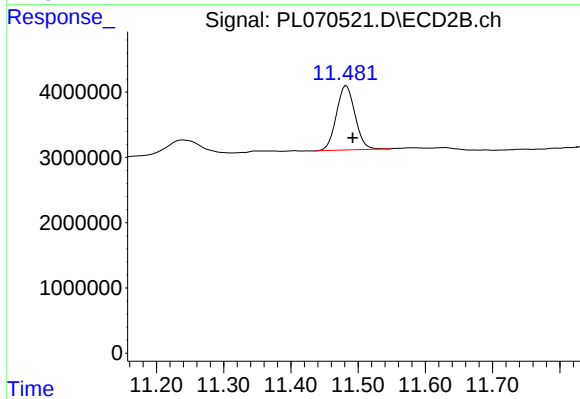

#28 Decachlorobiphenyl

R.T.: 11.482 min
Delta R.T.: -0.009 min
Response: 18920813
Conc: 15.63 ng/ml