

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102521\
 Data File : PL070524.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2021 21:14
 Operator : AR\AJ
 Sample : PB140165BL
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 06:44:33 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 29 09:19:28 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.623	5.561	10475677	27372393	20.935	20.695
28)	SA Decachlor...	10.388	11.482	13325684	23506561	19.257	19.424
Target Compounds							
7)	B delta-BHC	0.000	7.079	0	3388021	N.D.	1.750 #
20)	A Methoxychlor	0.000	9.933f	0	37459	N.D.	0.058 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102521\
Data File : PL070524.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2021 21:14
Operator : AR\AJ
Sample : PB140165BL
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 06:44:33 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL092821.M
Quant Title : GC Extractables
QLast Update : Wed Sep 29 09:19:28 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

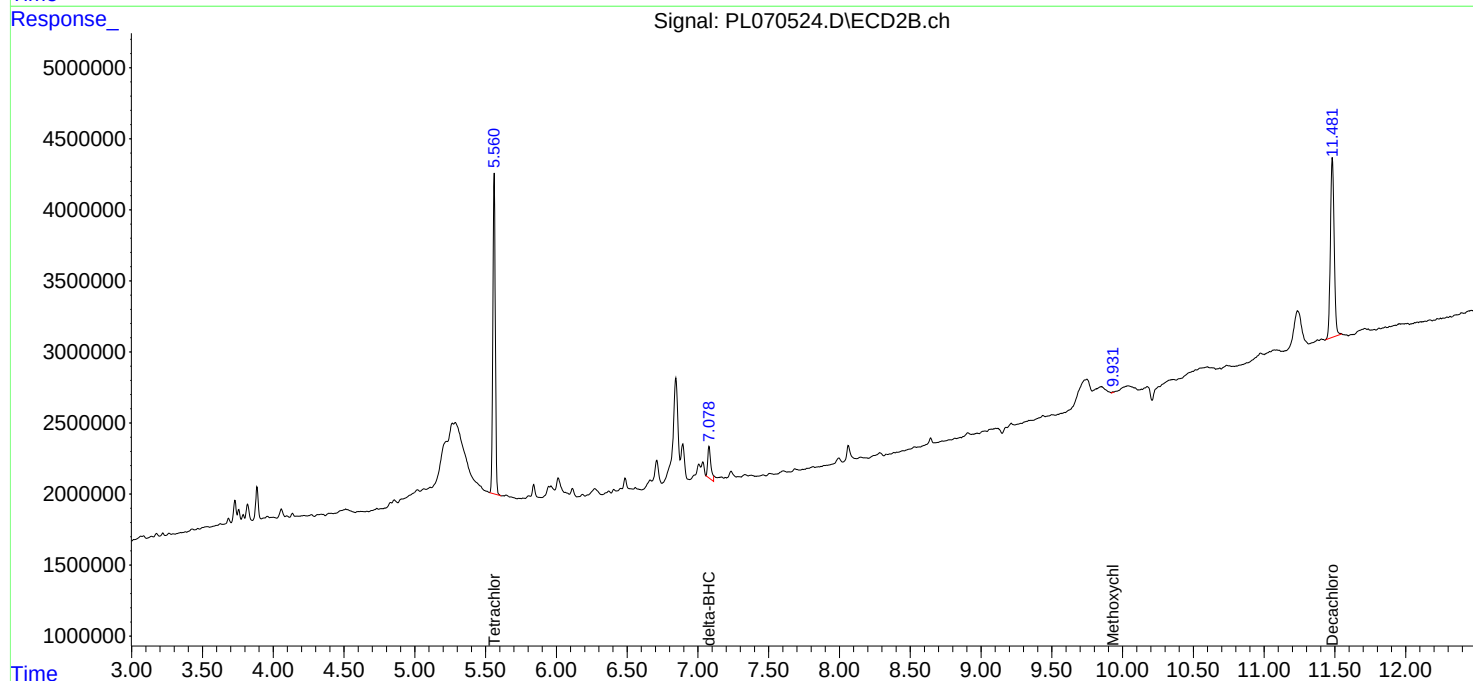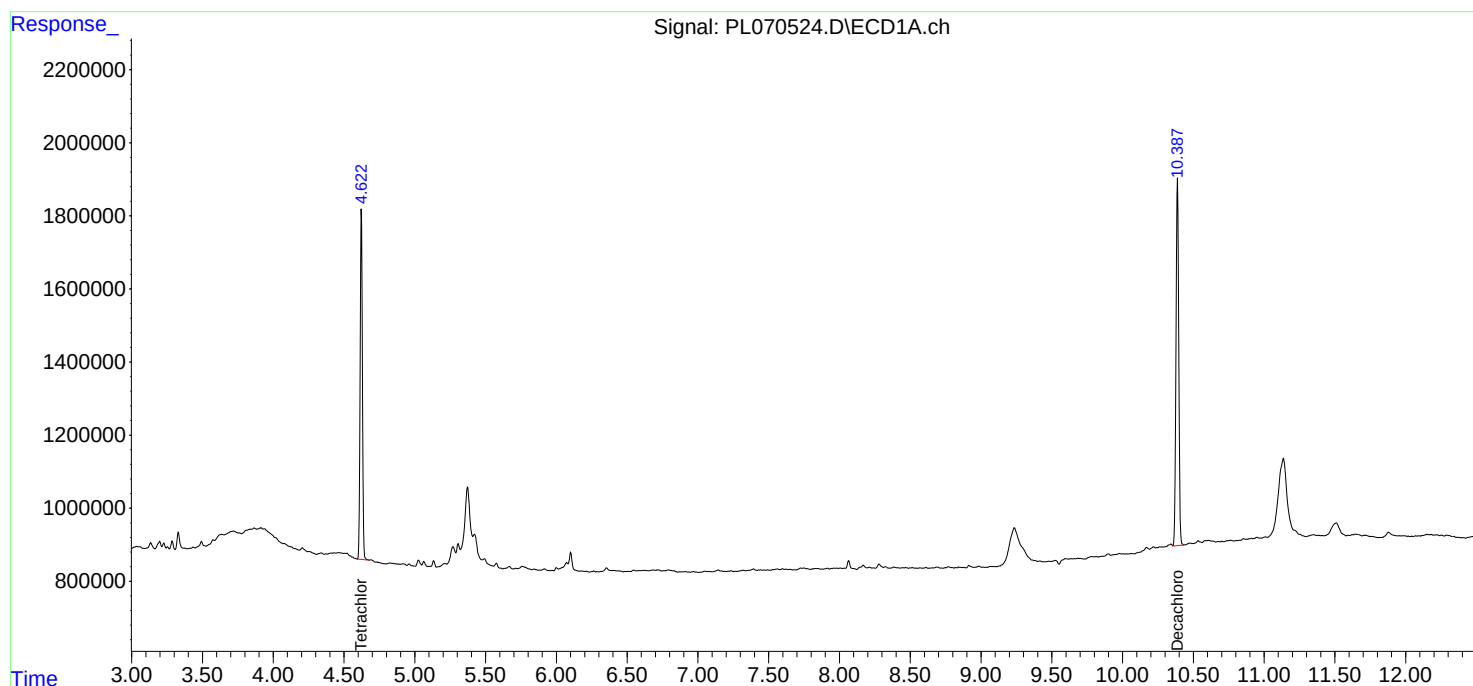


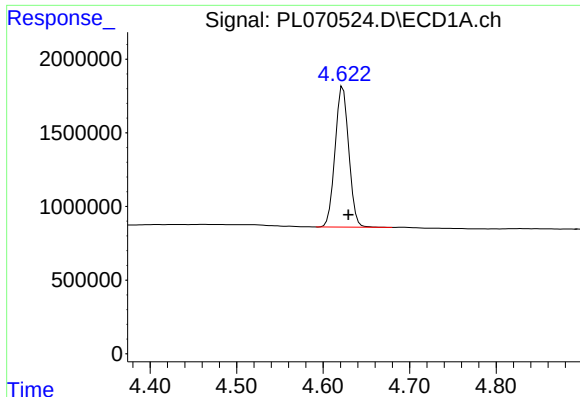

#1 Tetrachloro-m-xylene


R.T.: 4.623 min
Delta R.T.: -0.006 min
Response: 10475677
Conc: 20.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

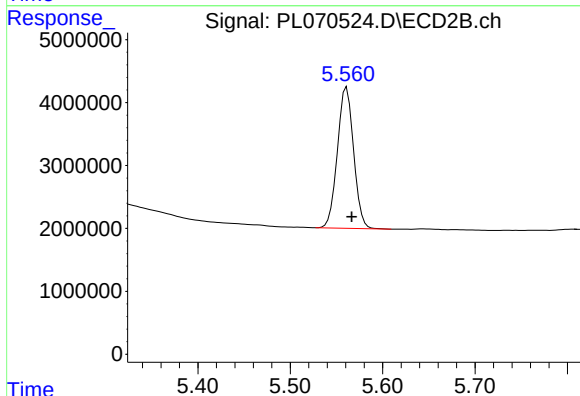


#1 Tetrachloro-m-xylene

R.T.: 5.561 min
Delta R.T.: -0.006 min
Response: 27372393
Conc: 20.70 ng/ml

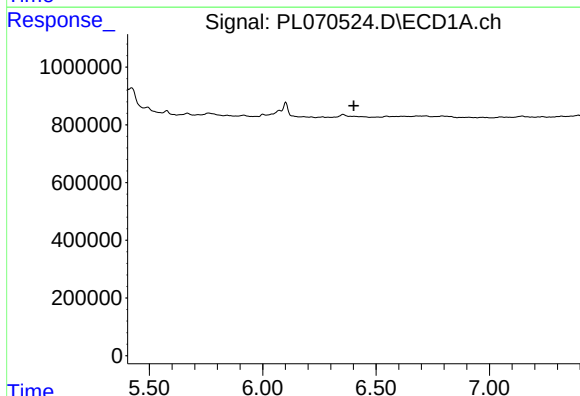


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.401 min
Response: 0
Conc: N.D.

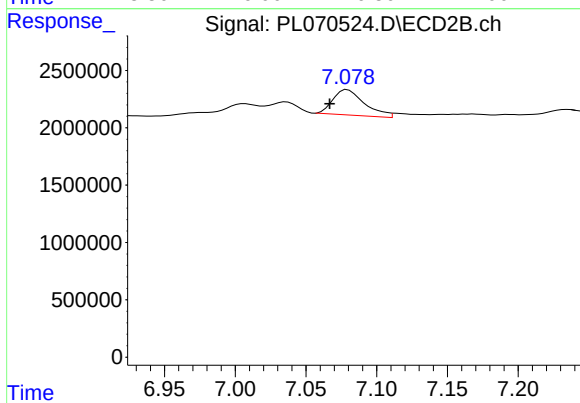

#7 delta-BHC


R.T.: 7.079 min
Delta R.T.: 0.012 min
Response: 3388021
Conc: 1.75 ng/ml

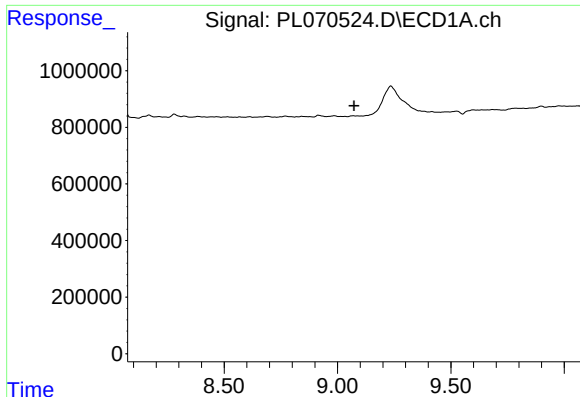

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 9.073 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

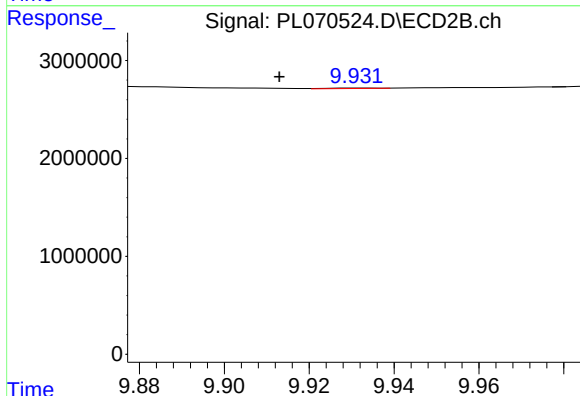


#20 Methoxychlor

R.T.: 9.933 min
Delta R.T.: 0.020 min
Response: 37459
Conc: 0.06 ng/ml

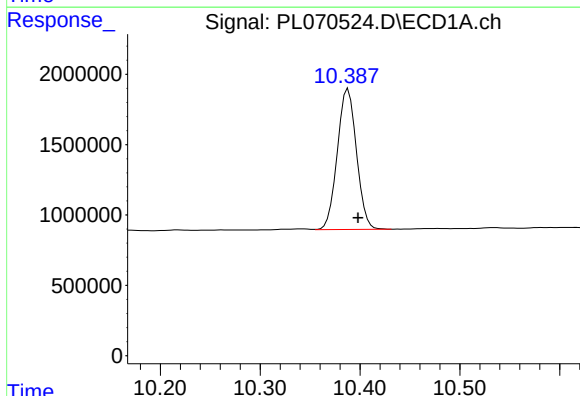

#28 Decachlorobiphenyl

R.T.: 10.388 min
Delta R.T.: -0.010 min
Response: 13325684
Conc: 19.26 ng/ml

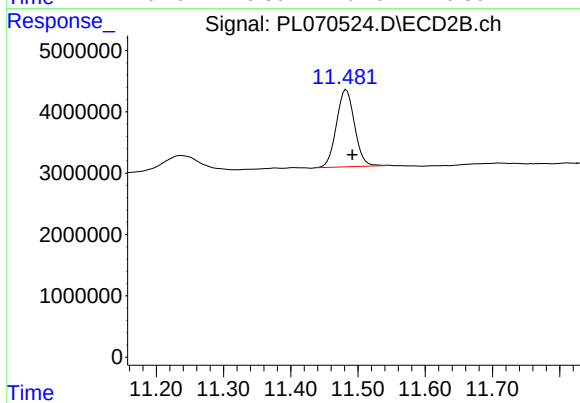

#28 Decachlorobiphenyl

R.T.: 11.482 min
Delta R.T.: -0.009 min
Response: 23506561
Conc: 19.42 ng/ml