

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102523\
 Data File : PL086149.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 13:32
 Operator : AR\AJ
 Sample : 05005-04RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N-3(0-5)RE

Manual Integrations APPROVED

Reviewed By :Abdul Mirza 10/26/2023
 Supervised By :Ankita Jodhani 10/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 15:49:28 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.354	2.620	33002121	10744236	11.096m	11.502
2) SA Decachlor...	8.875f	7.769	1045.3E6	205.0E6	479.915m	222.116 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102523\
Data File : PL086149.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 13:32
Operator : AR\AJ
Sample : 05005-04RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
N-3(0-5)RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/26/2023
Supervised By : Ankita Jodhani 10/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 15:49:28 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

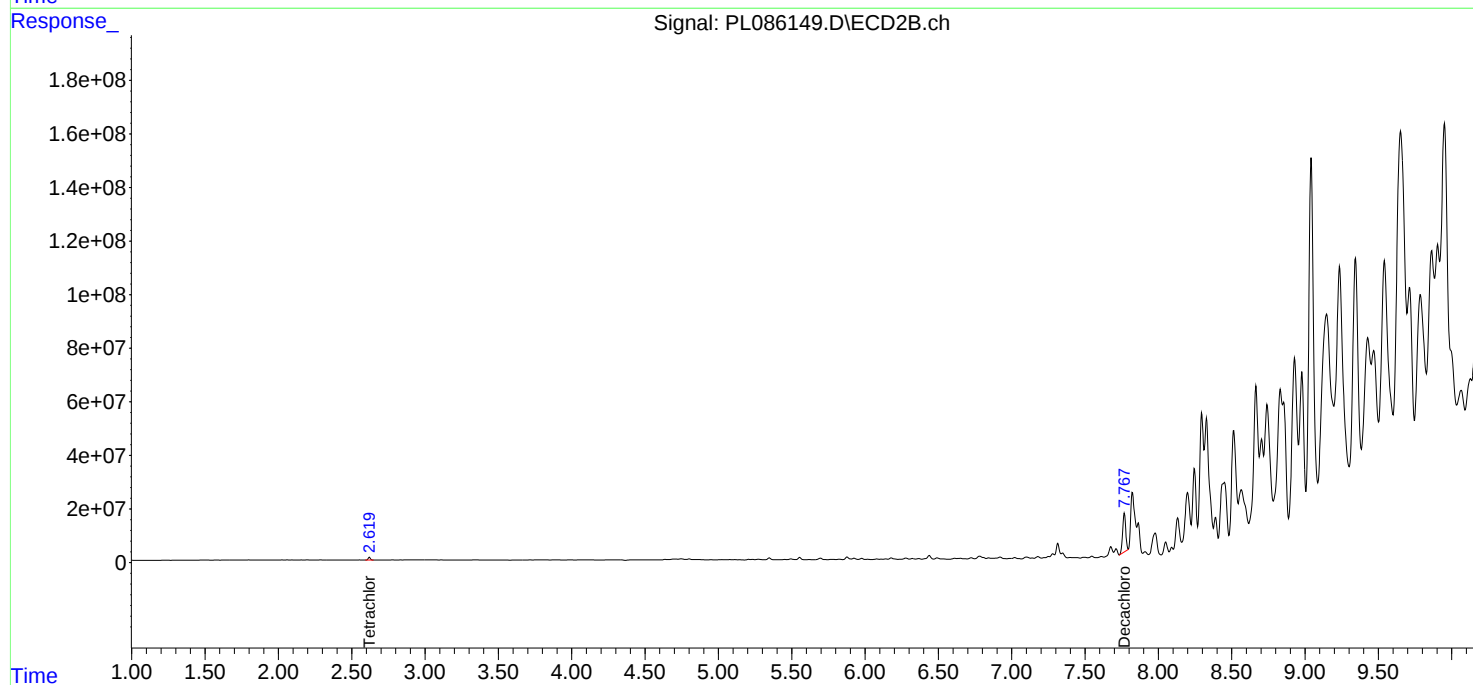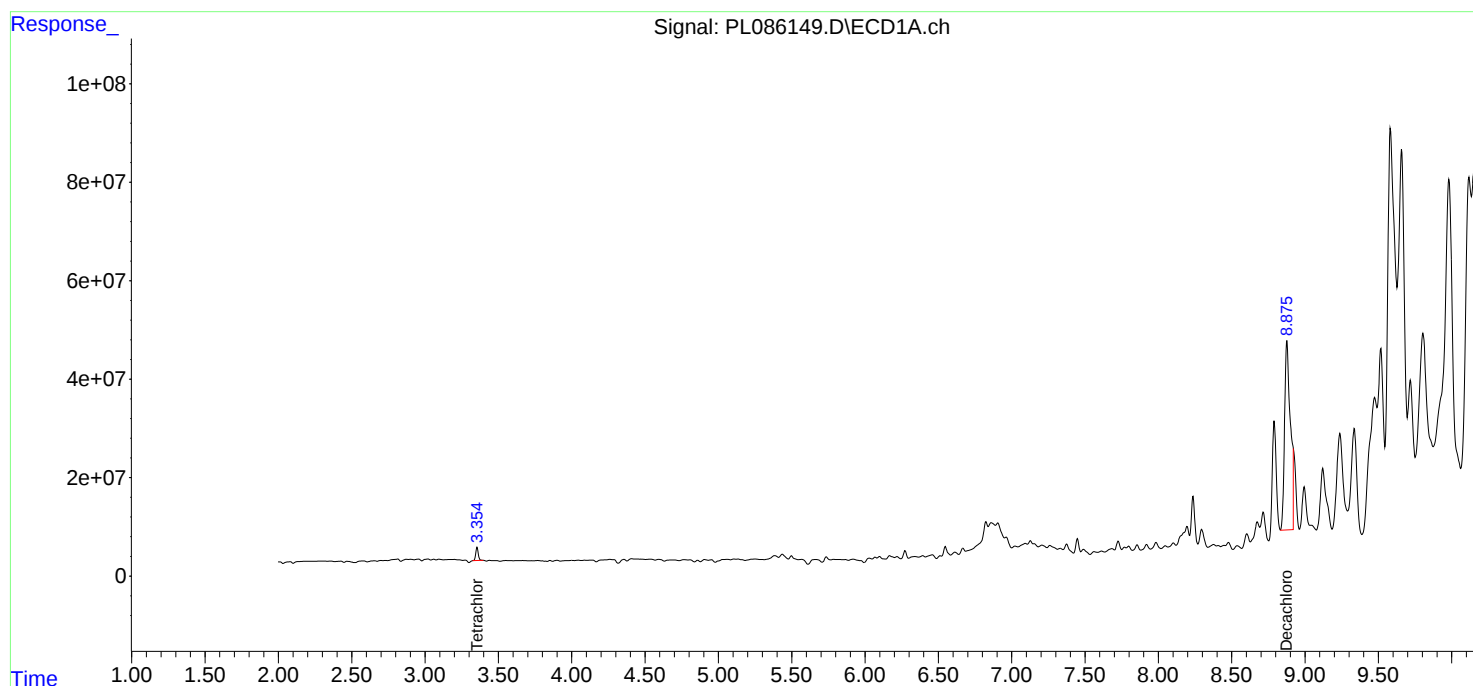

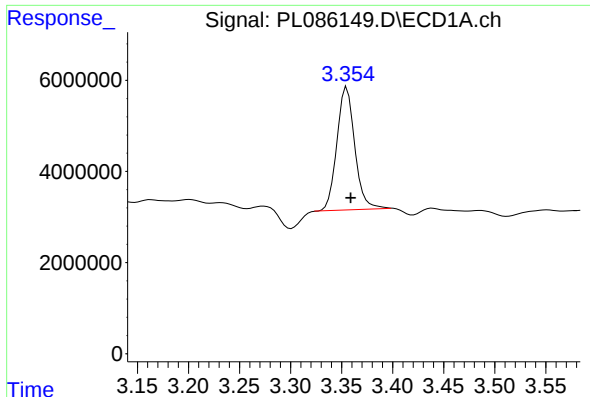


#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: -0.005 min
Response: 33002121
Conc: 11.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
N-3(0-5)RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/26/2023
Supervised By :Ankita Jodhani 10/26/2023

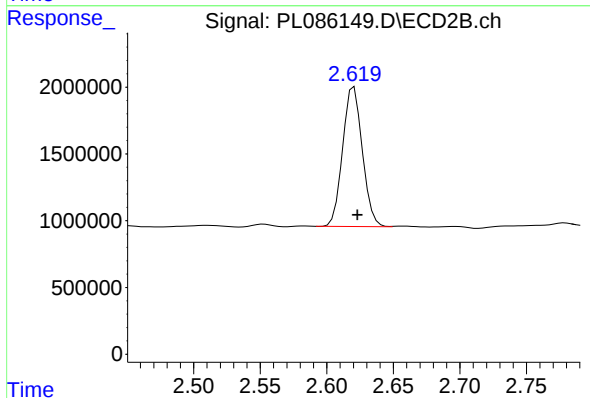


#1 Tetrachloro-m-xylene

R.T.: 2.620 min
Delta R.T.: -0.002 min
Response: 10744236
Conc: 11.50 ng/ml

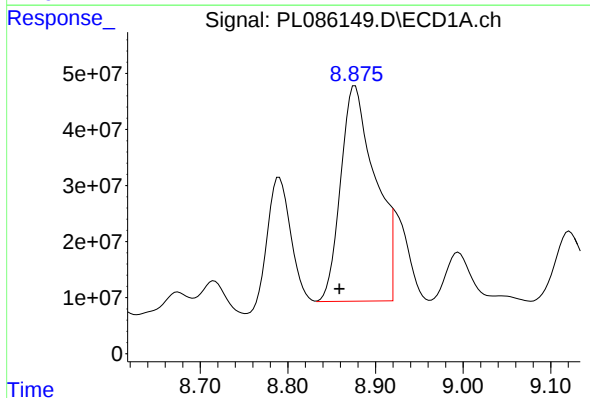

#28 Decachlorobiphenyl

R.T.: 8.875 min
Delta R.T.: 0.017 min
Response: 1045280832
Conc: 479.92 ng/ml m

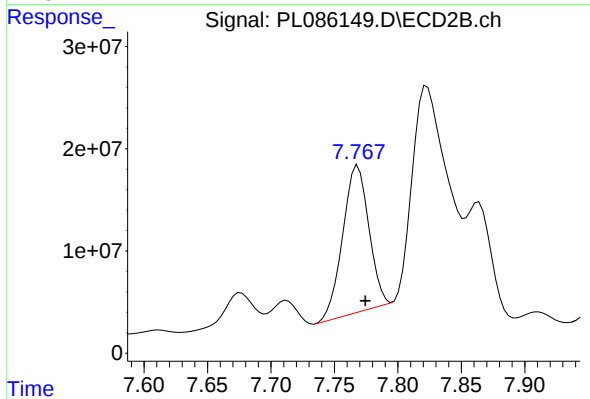

#28 Decachlorobiphenyl

R.T.: 7.769 min
Delta R.T.: -0.006 min
Response: 205009890
Conc: 222.12 ng/ml