

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102523\
 Data File : PL086157.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 16:37
 Operator : AR\AJ
 Sample : 05040-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 M-4(50FT)(0-5)

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 10/26/2023
 Supervised By : Ankita Jodhani 10/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 17:30:23 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.354	2.621	26891136	9136186	9.042m	9.781
28) SA Decachlor...	8.854	7.771	31904274	13272307	14.648	14.380

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102523\
Data File : PL086157.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 16:37
Operator : AR\AJ
Sample : 05040-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
M-4(50FT)(0-5)


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/26/2023
Supervised By : Ankita Jodhani 10/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 17:30:23 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

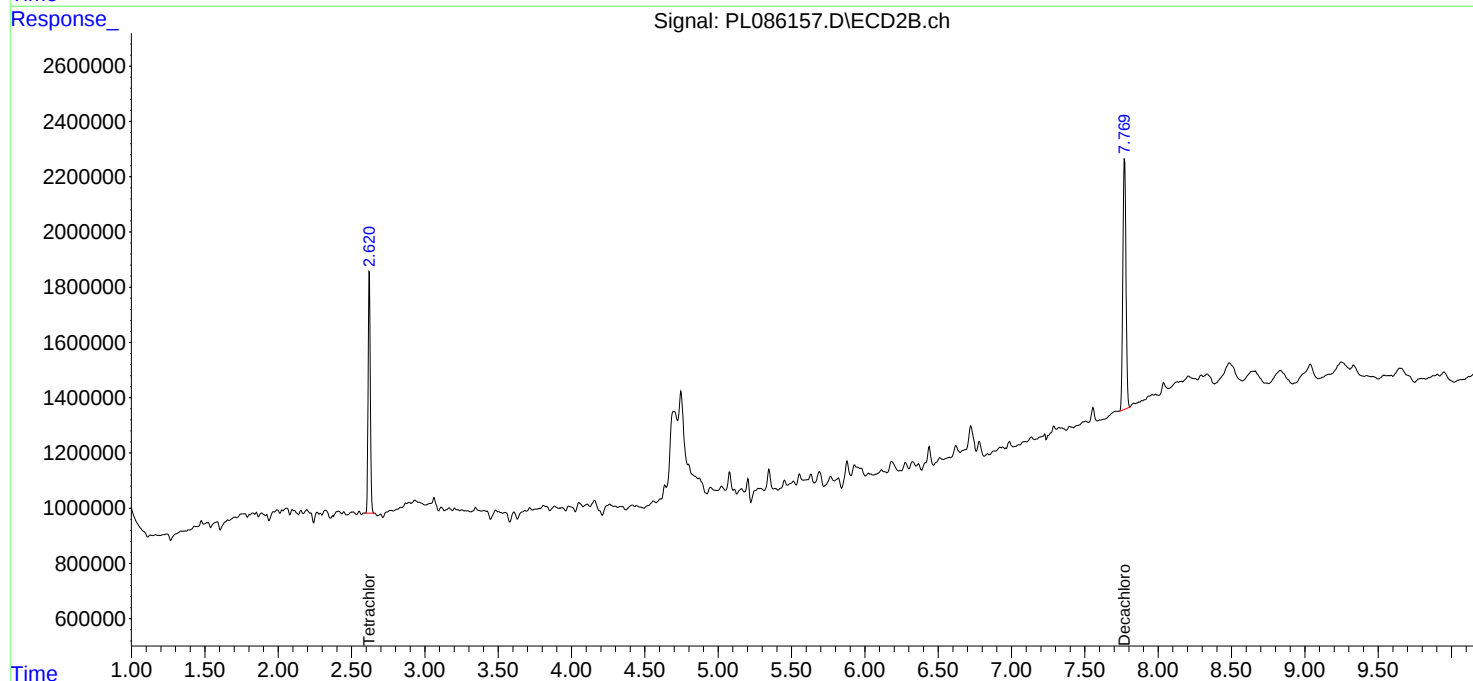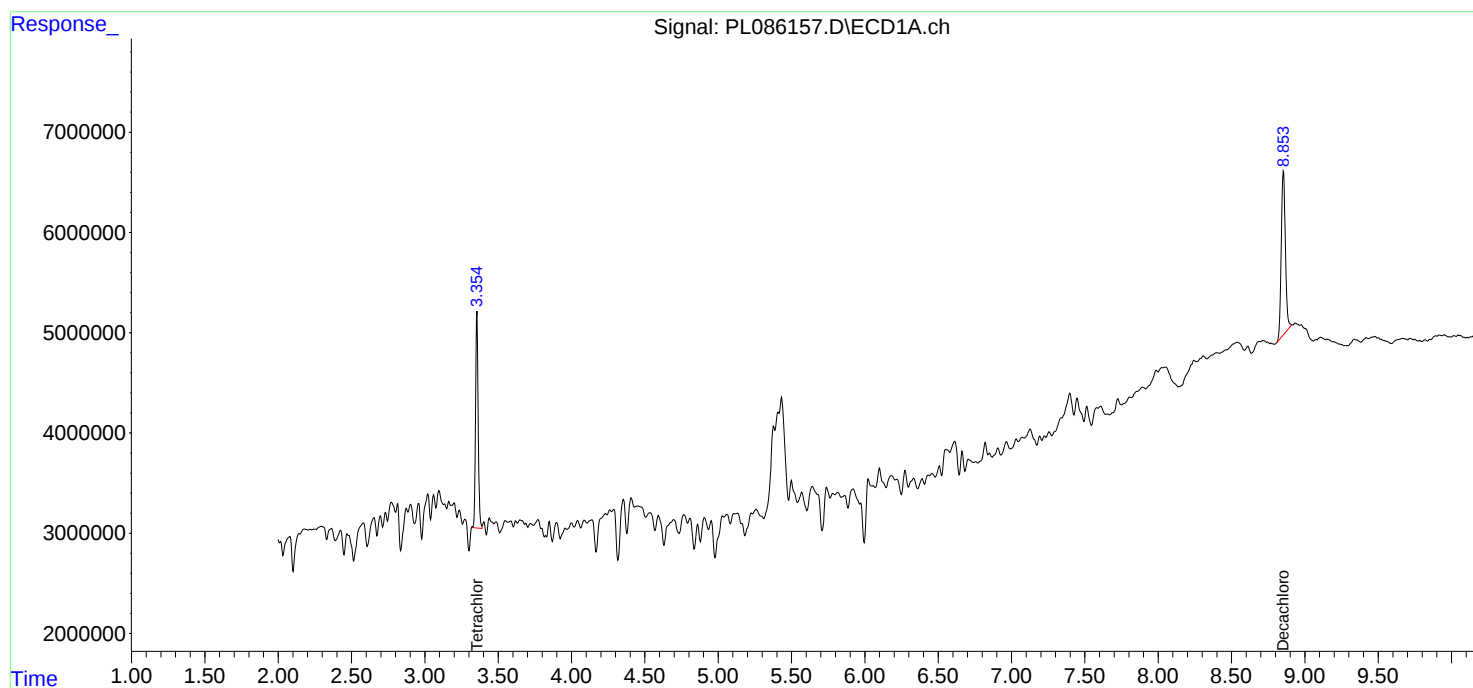

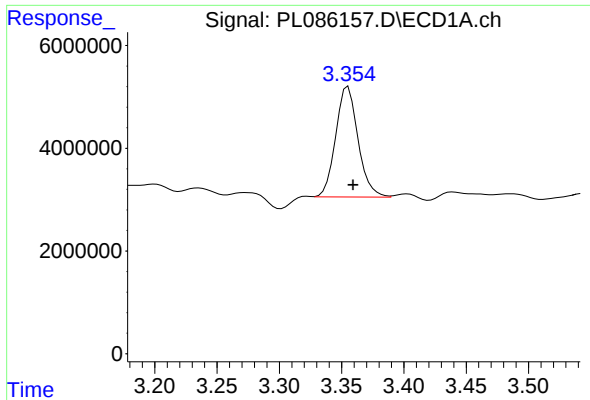

#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: -0.005 min
Response: 26891136
Conc: 9.04 ng/ml

Instrument :

ECD_L


ClientSampleId :

M-4(50FT)(0-5)

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 10/26/2023
Supervised By :Ankita Jodhani 10/26/2023

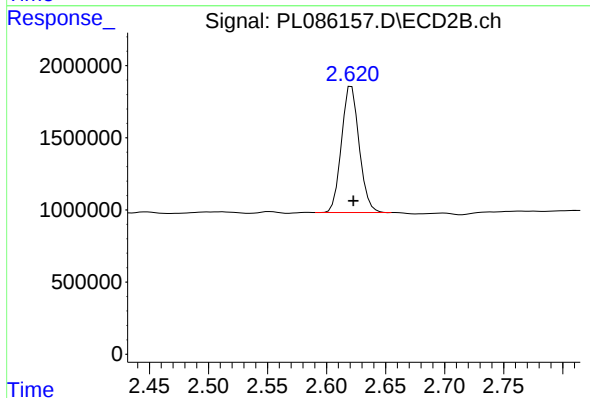


#1 Tetrachloro-m-xylene

R.T.: 2.621 min
Delta R.T.: -0.002 min
Response: 9136186
Conc: 9.78 ng/ml

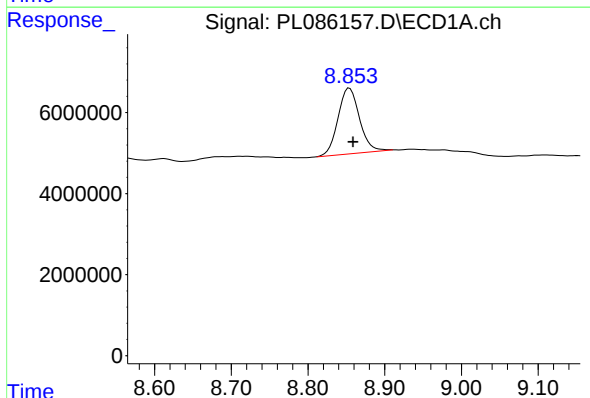

#28 Decachlorobiphenyl

R.T.: 8.854 min
Delta R.T.: -0.005 min
Response: 31904274
Conc: 14.65 ng/ml

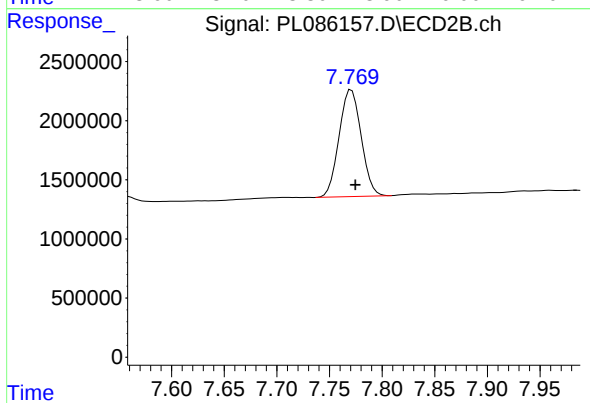

#28 Decachlorobiphenyl

R.T.: 7.771 min
Delta R.T.: -0.004 min
Response: 13272307
Conc: 14.38 ng/ml