

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102523\
 Data File : PL086161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Oct 2023 17:44
 Operator : AR\AJ
 Sample : 05005-04RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 N-3(0-5)RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 10/26/2023
 Supervised By :Ankita Jodhani 10/26/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 25 18:37:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
 Quant Title : GC Extractables
 QLast Update : Wed Oct 04 05:29:39 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.354	2.620	33193328	11086576	11.161m	11.869
28) SA Decachlor...	8.874f	7.768	992.1E6	216.0E6	455.494m	234.029 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102523\
Data File : PL086161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Oct 2023 17:44
Operator : AR\AJ
Sample : 05005-04RE
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
N-3(0-5)RE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 10/26/2023
Supervised By : Ankita Jodhani 10/26/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 25 18:37:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL100323.M
Quant Title : GC Extractables
QLast Update : Wed Oct 04 05:29:39 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

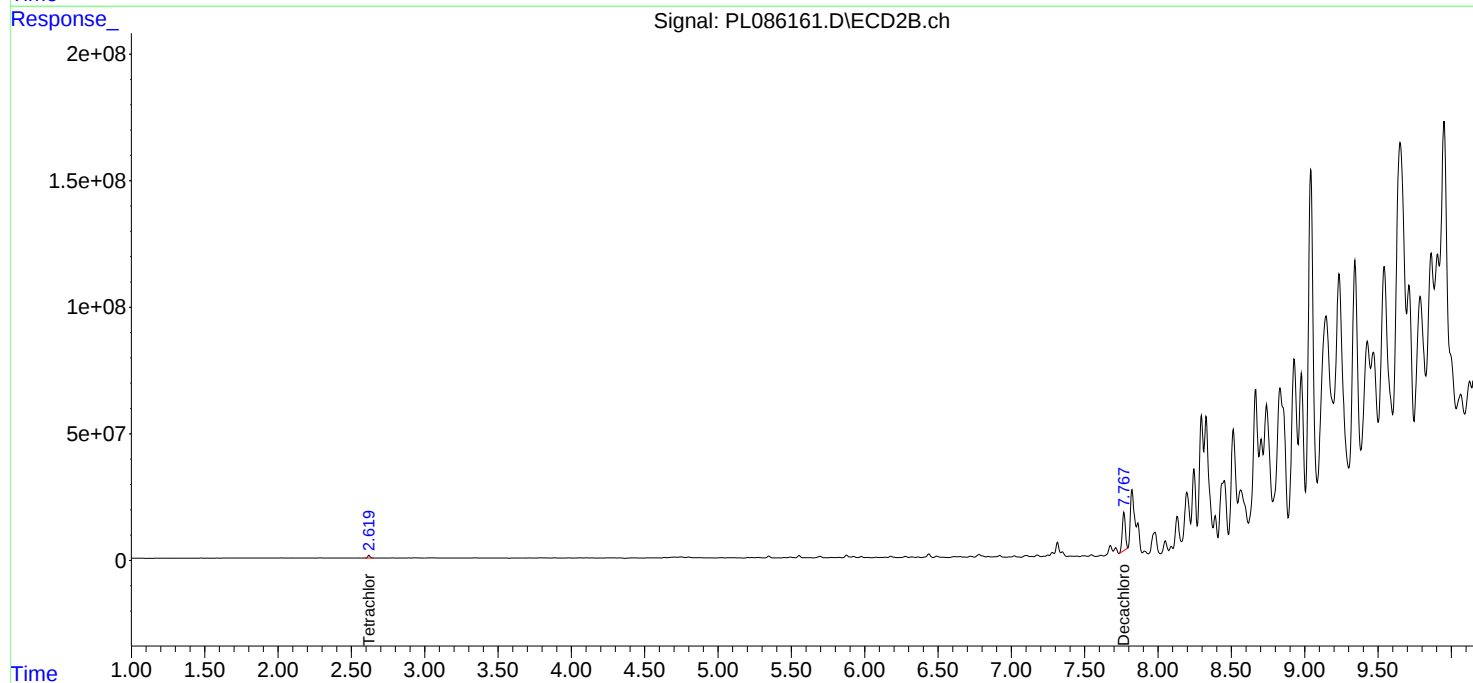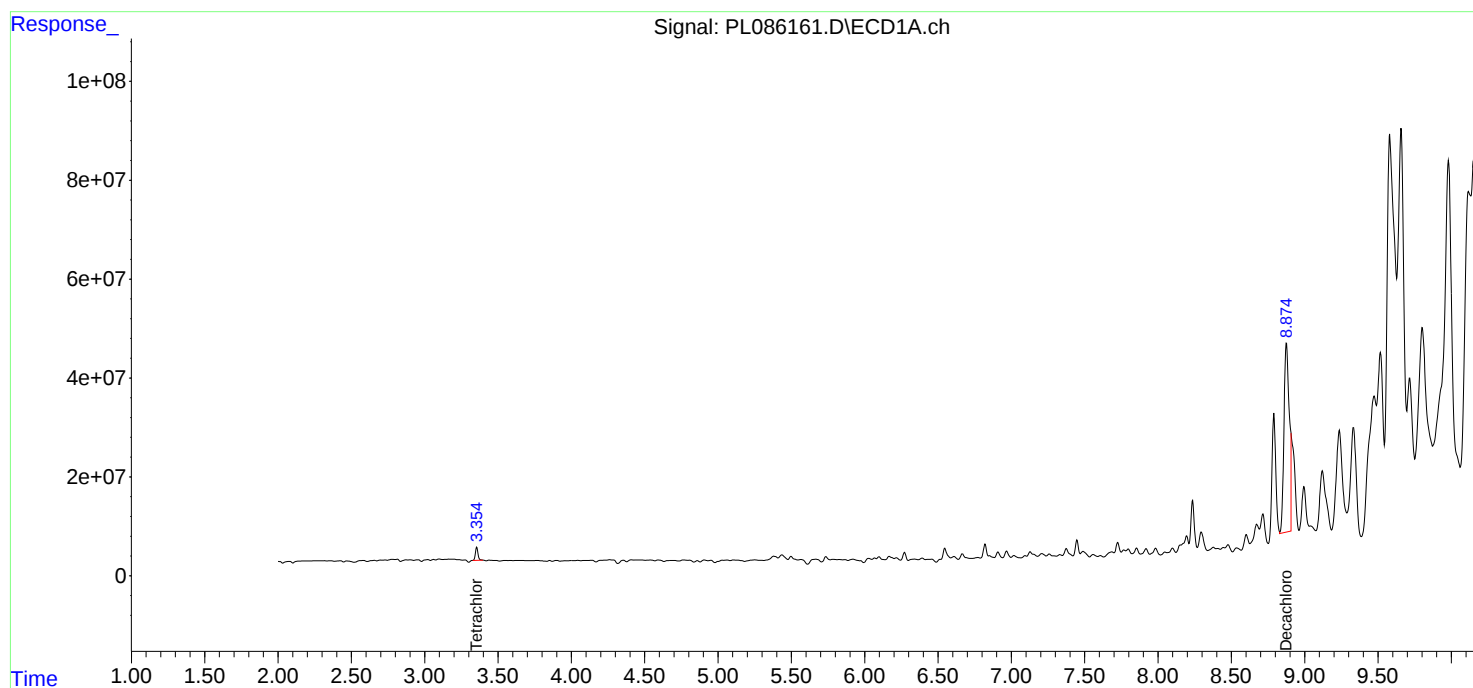

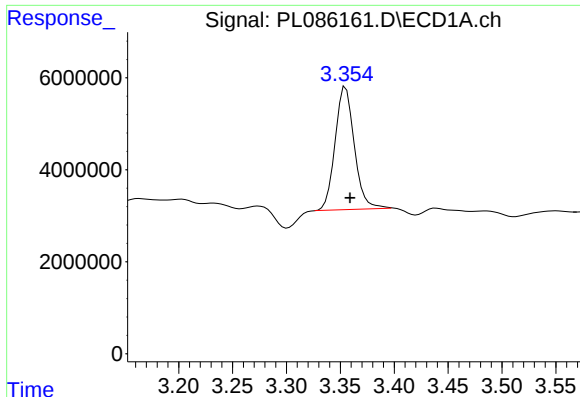


#1 Tetrachloro-m-xylene

R.T.: 3.354 min
Delta R.T.: -0.005 min
Response: 33193328
Conc: 11.16 ng/ml

Instrument :
ECD_L
ClientSampleId :
N-3(0-5)RE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 10/26/2023
Supervised By :Ankita Jodhani 10/26/2023

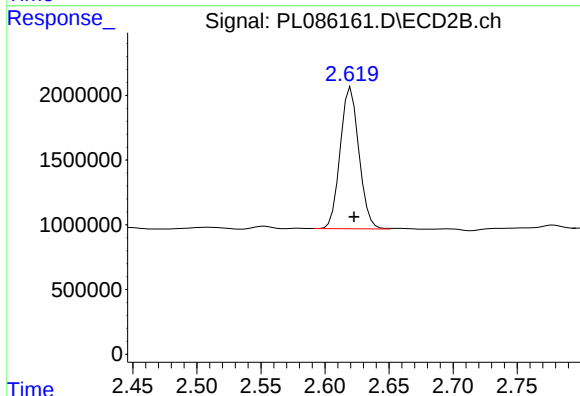


#1 Tetrachloro-m-xylene

R.T.: 2.620 min
Delta R.T.: -0.003 min
Response: 11086576
Conc: 11.87 ng/ml

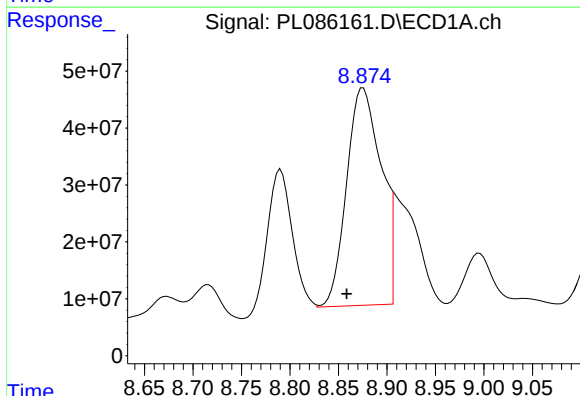

#28 Decachlorobiphenyl

R.T.: 8.874 min
Delta R.T.: 0.015 min
Response: 992089440
Conc: 455.49 ng/ml m

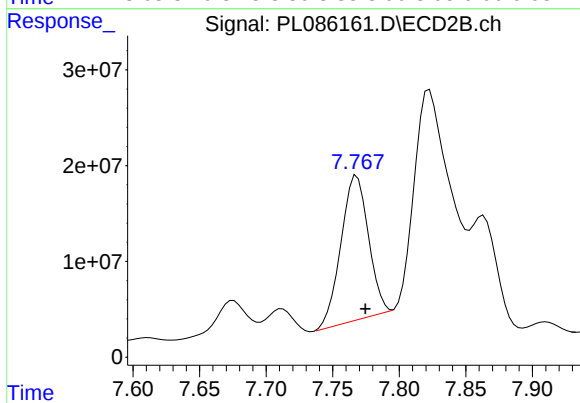

#28 Decachlorobiphenyl

R.T.: 7.768 min
Delta R.T.: -0.006 min
Response: 216005423
Conc: 234.03 ng/ml