

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
 Data File : PL041378.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2018 10:50
 Operator : AJ\SJ
 Sample : J5618-02RE
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 23:29:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.104	62927071	33086049	11.482	11.866
28)	SA Decachlor...	8.220	9.234	89143506	36212558	17.145	14.004
Target Compounds							
2)	A alpha-BHC	3.909	0.000	3710512	0	0.468	N.D. #
6)	B beta-BHC	4.418f	4.997f	11233946	3514325	3.540	2.193 #
7)	B delta-BHC	0.000	5.149f	0	1311143	N.D.	0.399 #
8)	B Heptachlo...	5.262f	0.000	1669061	0	0.254	N.D. #
12)	B 4,4'-DDE	5.635	0.000	3678734	0	0.647	N.D. #
17)	MA 4,4'-DDT	6.389	0.000	1365990	0	0.300	N.D. #
23)	Chlordane-1	4.418	5.149	11233946	1311143	44.018	10.615 #
24)	Chlordane-2	4.883	0.000	7398411	0	27.412	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
Data File : PL041378.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 10:50
Operator : AJ\SJ
Sample : J5618-02RE
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 23:29:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

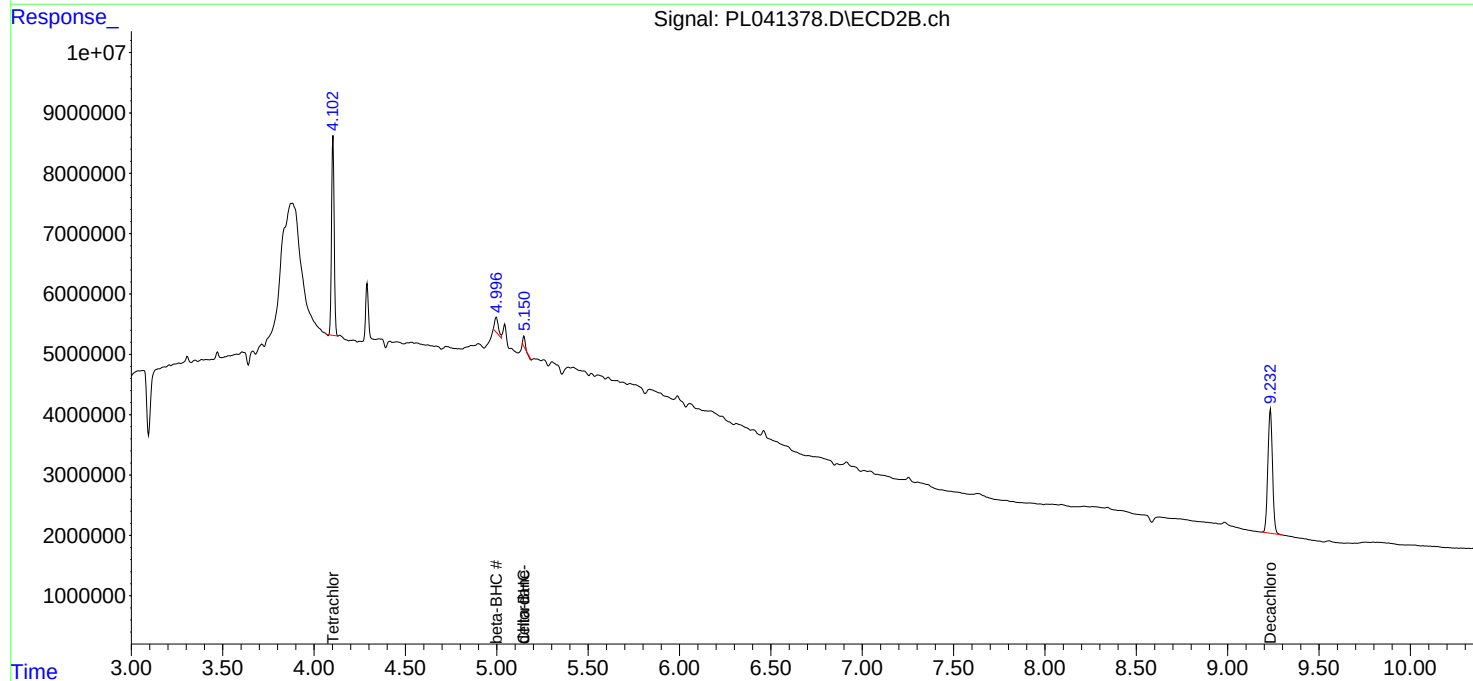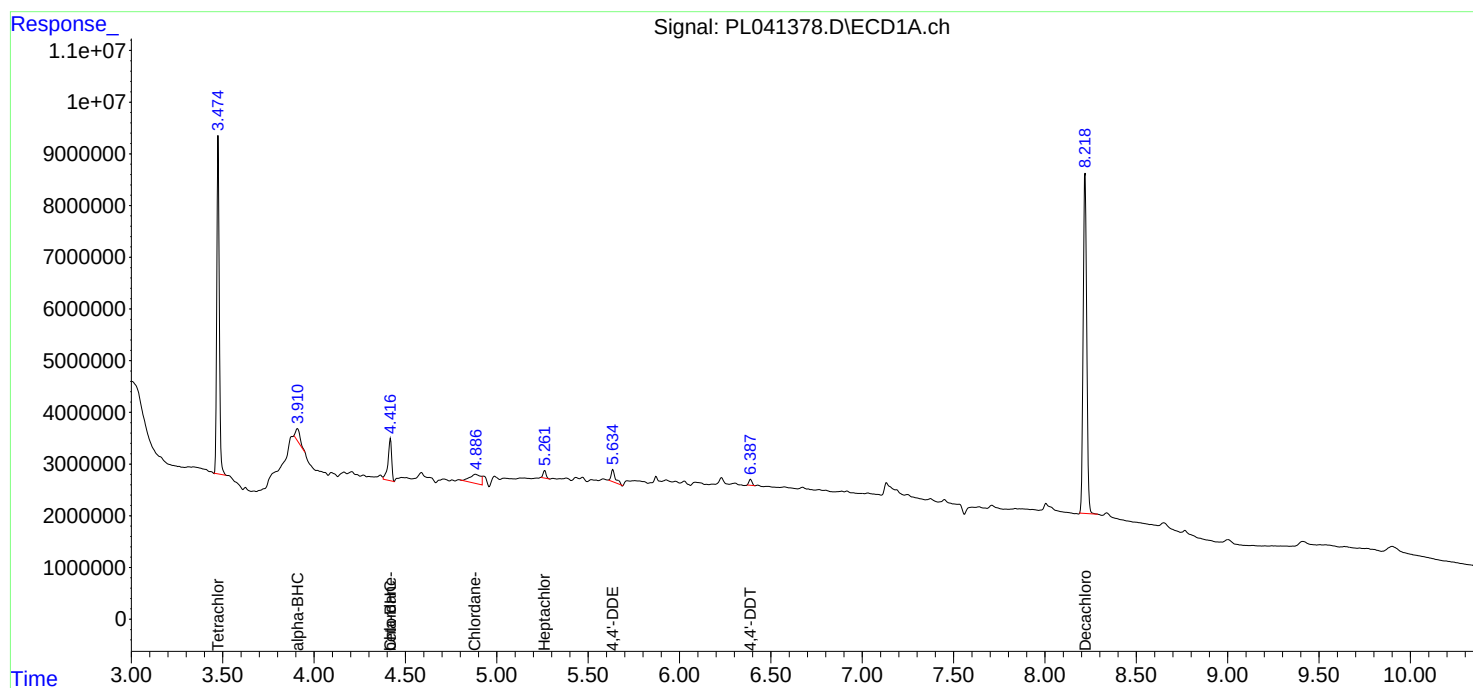


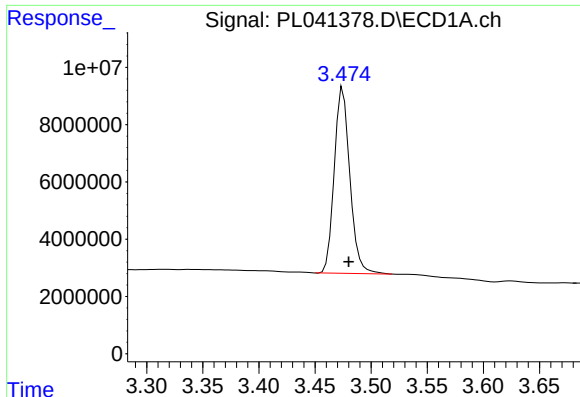

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 62927071
Conc: 11.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

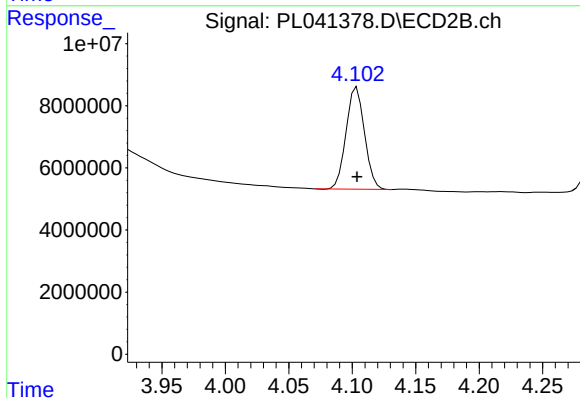


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 33086049
Conc: 11.87 ng/ml

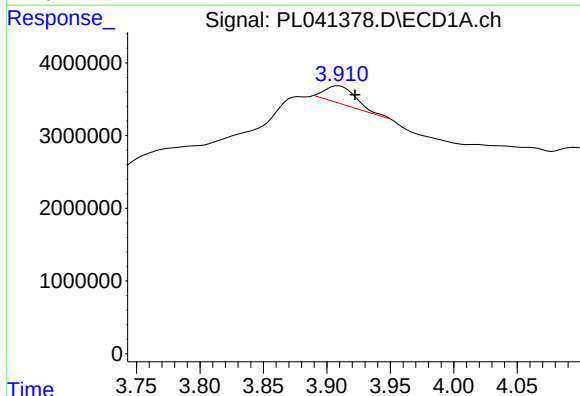


#2 alpha-BHC

R.T.: 3.909 min
Delta R.T.: -0.013 min
Response: 3710512
Conc: 0.47 ng/ml

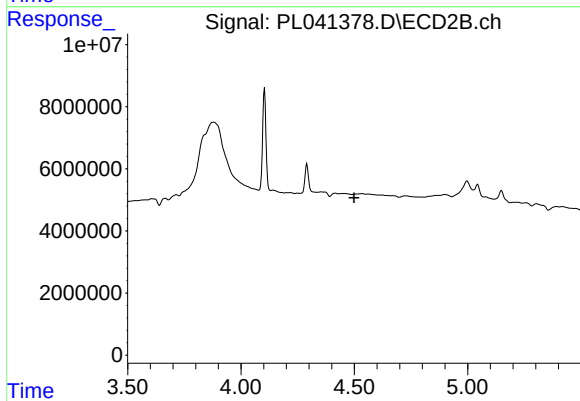

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.499 min
Response: 0
Conc: N.D.

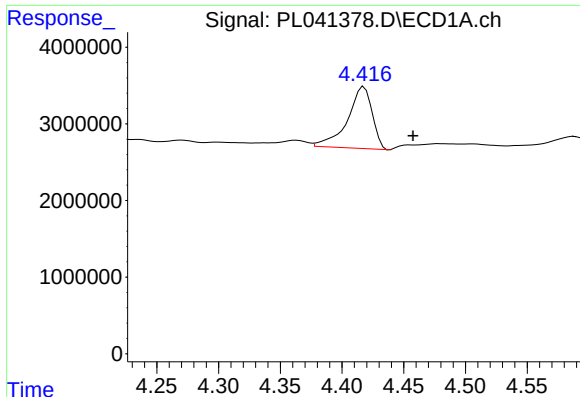

#6 beta-BHC


R.T.: 4.418 min
Delta R.T.: -0.040 min
Response: 11233946
Conc: 3.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

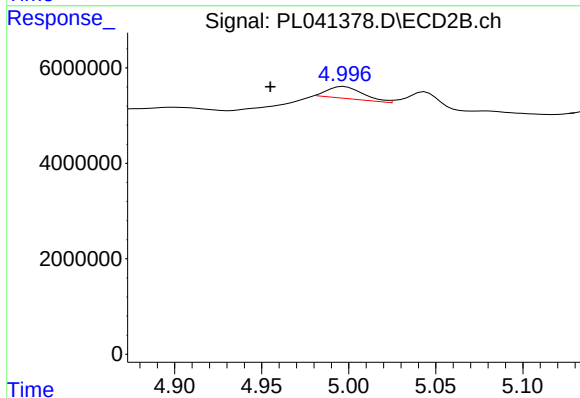


#6 beta-BHC

R.T.: 4.997 min
Delta R.T.: 0.042 min
Response: 3514325
Conc: 2.19 ng/ml

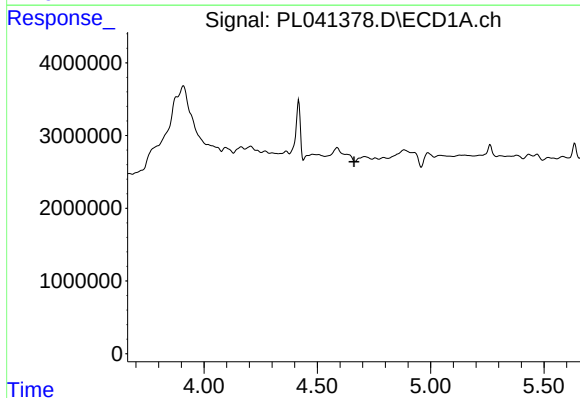


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.662 min
Response: 0
Conc: N.D.

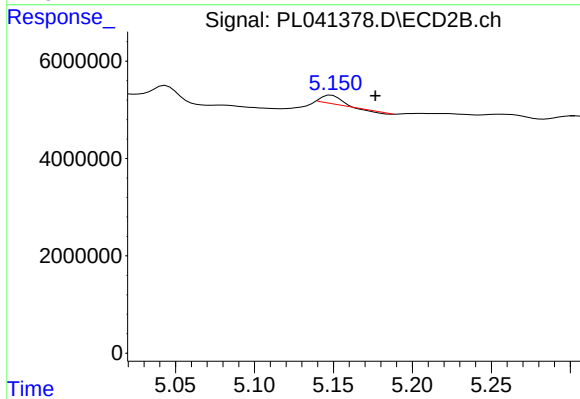

#7 delta-BHC


R.T.: 5.149 min
Delta R.T.: -0.028 min
Response: 1311143
Conc: 0.40 ng/ml

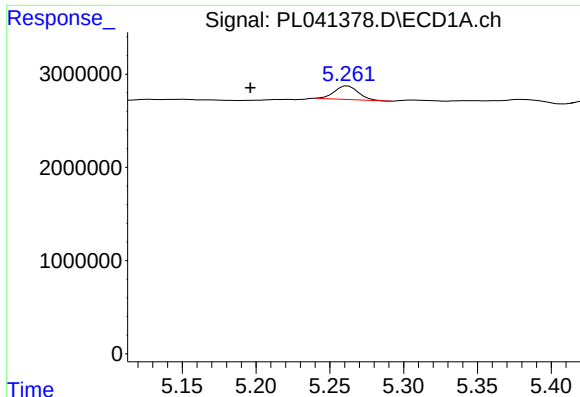

#8 Heptachlor epoxide


R.T.: 5.262 min
Delta R.T.: 0.066 min
Response: 1669061
Conc: 0.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

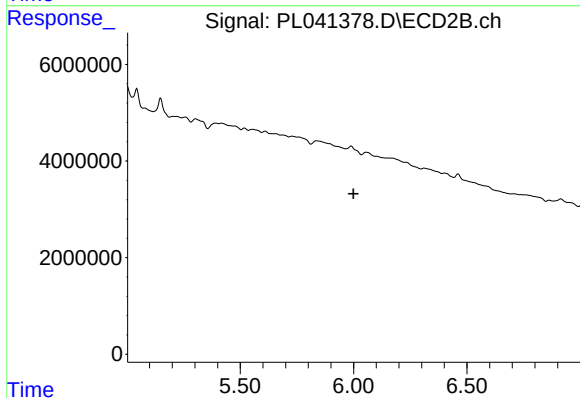


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.000 min
Response: 0
Conc: N.D.

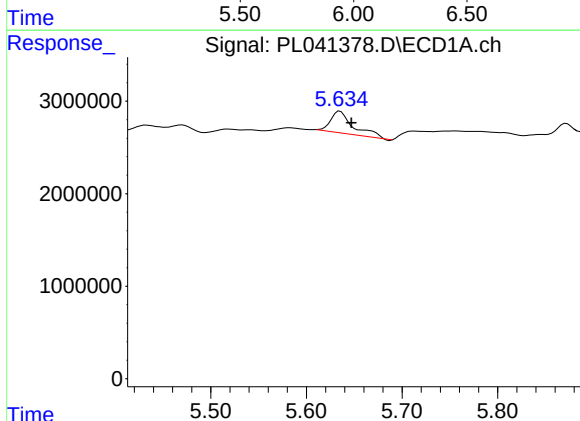


#12 4,4'-DDE

R.T.: 5.635 min
Delta R.T.: -0.012 min
Response: 3678734
Conc: 0.65 ng/ml

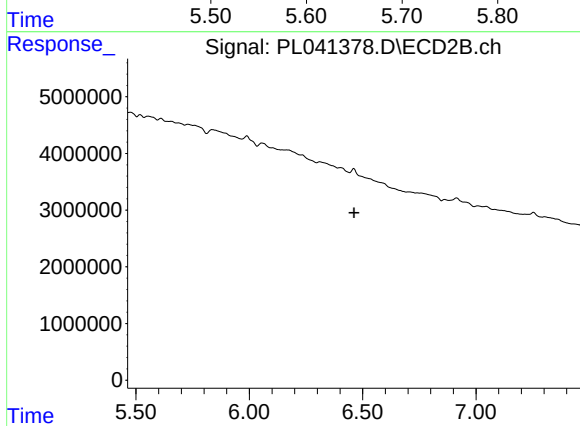

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.462 min
Response: 0
Conc: N.D.

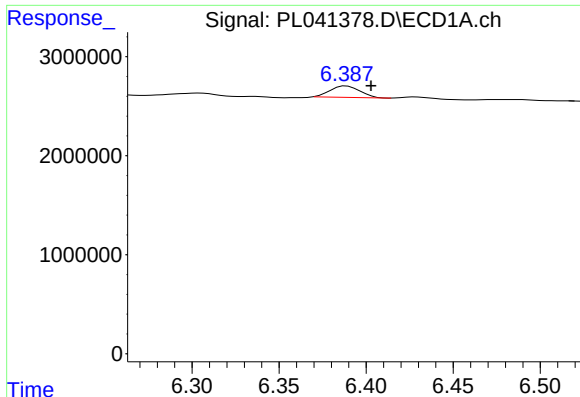

#17 4,4'-DDT


R.T.: 6.389 min
Delta R.T.: -0.014 min
Response: 1365990
Conc: 0.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

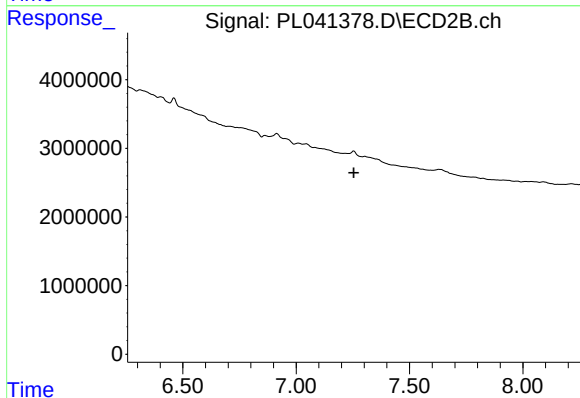


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

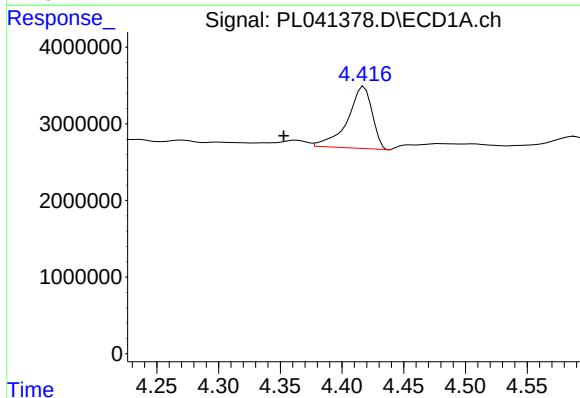


#23 Chlordane-1

R.T.: 4.418 min
Delta R.T.: 0.065 min
Response: 11233946
Conc: 44.02 ng/ml

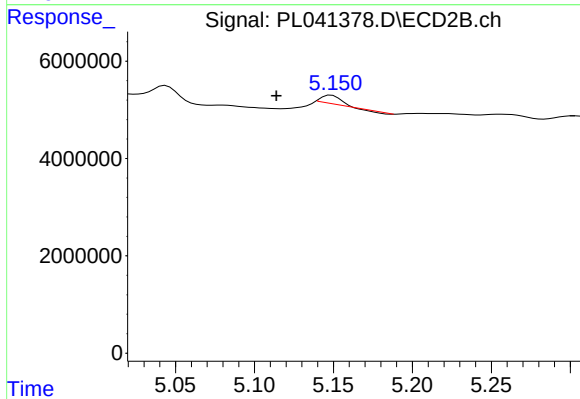

#23 Chlordane-1


R.T.: 5.149 min
Delta R.T.: 0.035 min
Response: 1311143
Conc: 10.62 ng/ml

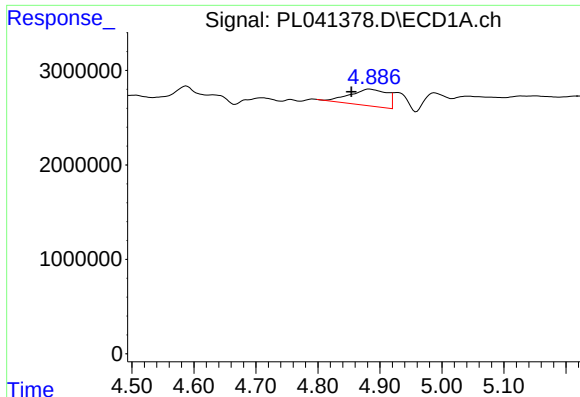

#24 Chlordane-2


R.T.: 4.883 min
Delta R.T.: 0.029 min
Response: 7398411
Conc: 27.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

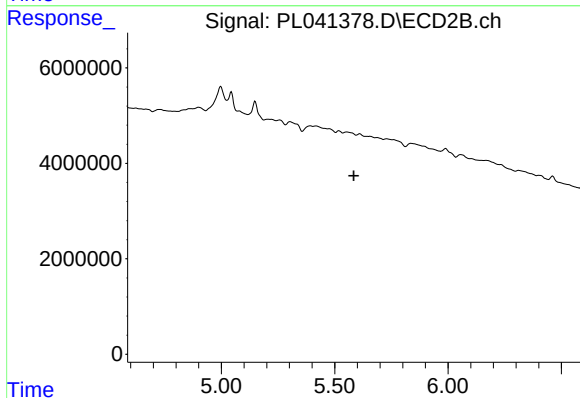


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.584 min
Response: 0
Conc: N.D.

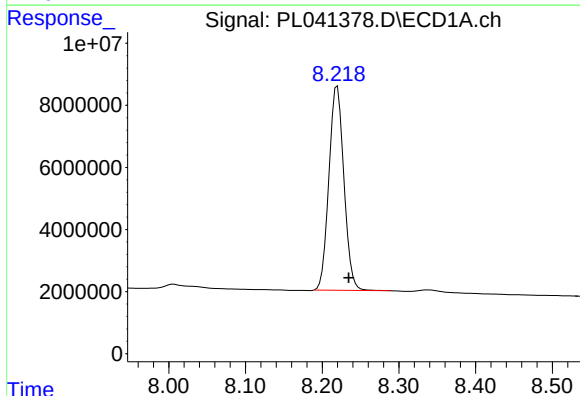

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.015 min
Response: 89143506
Conc: 17.14 ng/ml

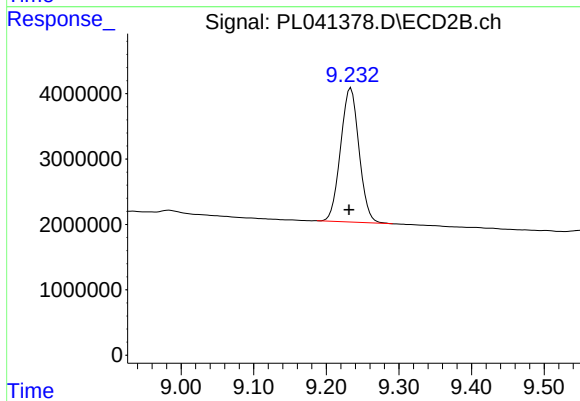

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.002 min
Response: 36212558
Conc: 14.00 ng/ml