

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
 Data File : PL041381.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2018 13:53
 Operator : AJ\SJ
 Sample : J5651-01RE
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 23:30:15 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.483	4.104	30709981	14829688	5.603	5.319
28)	SA Decachlor...	8.229	9.239	48210427	18901370	9.272	7.310
Target Compounds							
2)	A alpha-BHC	3.875f	0.000	1050962	0	0.133	N.D. #
8)	B Heptachlo...	5.127f	5.994	1798776	32527383	0.274	11.341 #
13)	MA Dieldrin	5.730f	0.000	397656	0	0.063	N.D. #
14)	MA Endrin	6.044	6.901f	5018090	3610397	0.874	1.617 #
16)	A 4,4'-DDD	0.000	6.901f	0	3610397	N.D.	1.724 #
17)	MA 4,4'-DDT	6.395	0.000	1453022	0	0.319	N.D. #
20)	A Methoxychlor	0.000	7.652f	0	20659669	N.D.	17.551 #
24)	Chlordane-2	0.000	5.516	0	4651688	N.D.	37.614 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
Data File : PL041381.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 13:53
Operator : AJ\SJ
Sample : J5651-01RE
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 23:30:15 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

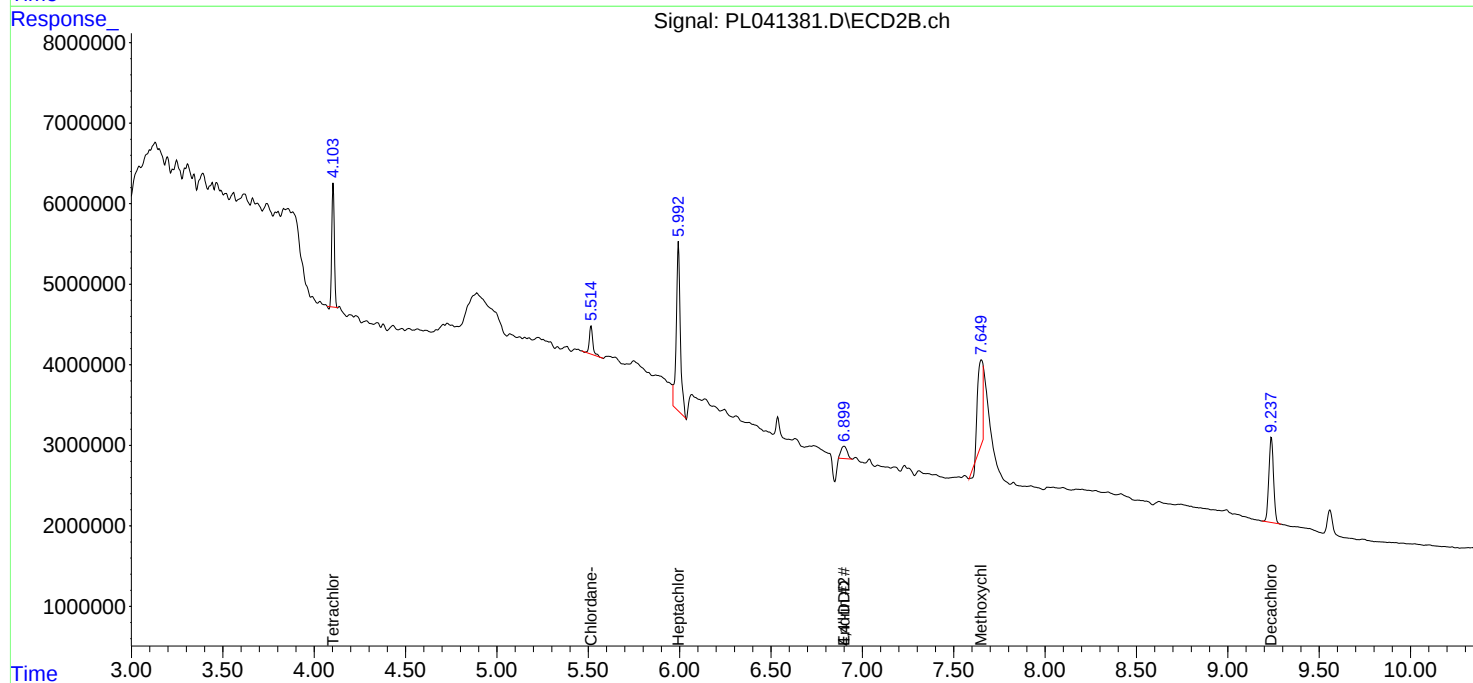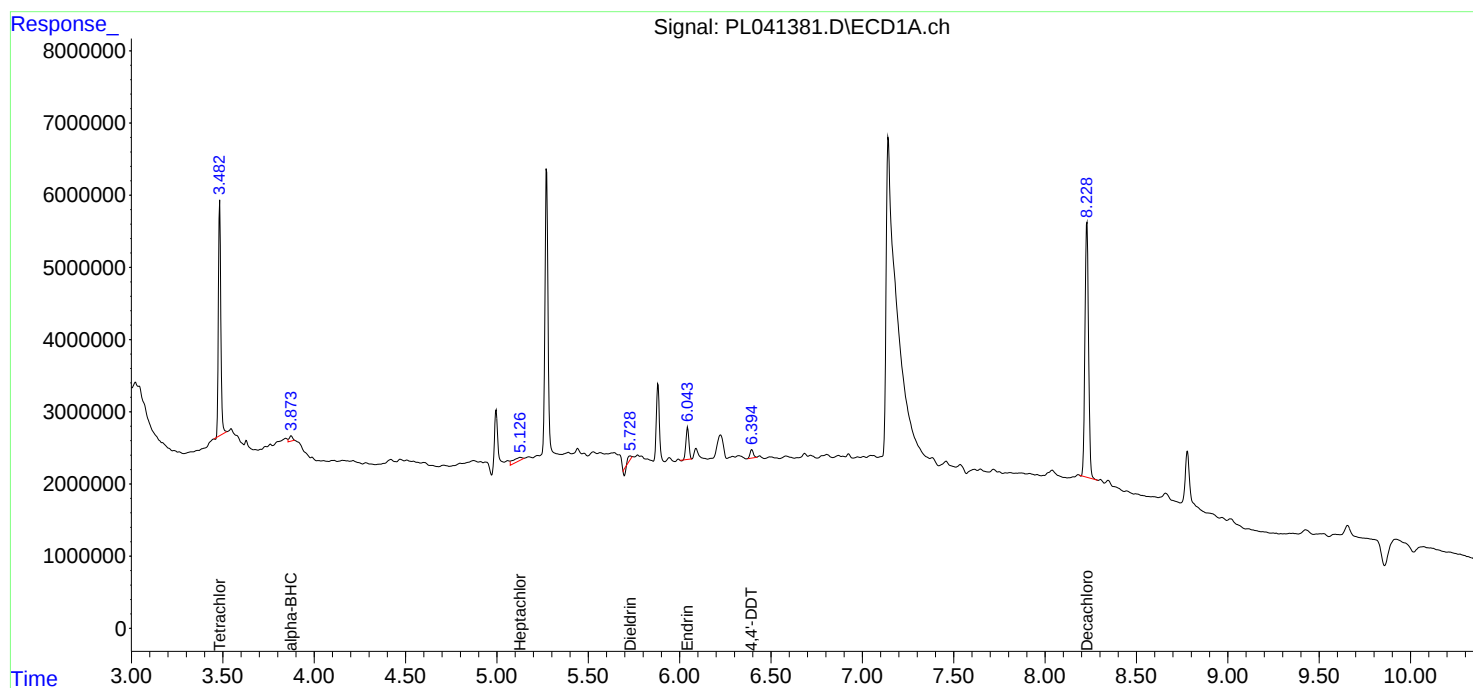


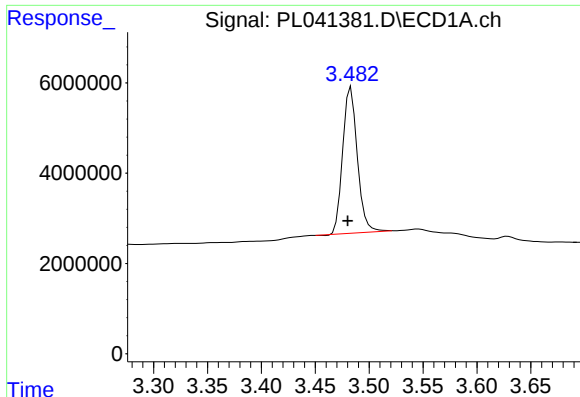

#1 Tetrachloro-m-xylene


R.T.: 3.483 min
Delta R.T.: 0.003 min
Response: 30709981
Conc: 5.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

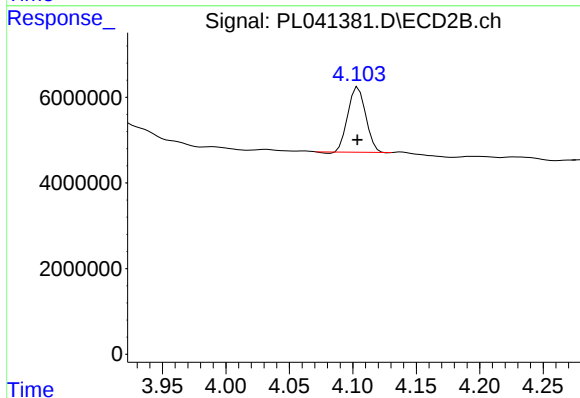


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 14829688
Conc: 5.32 ng/ml

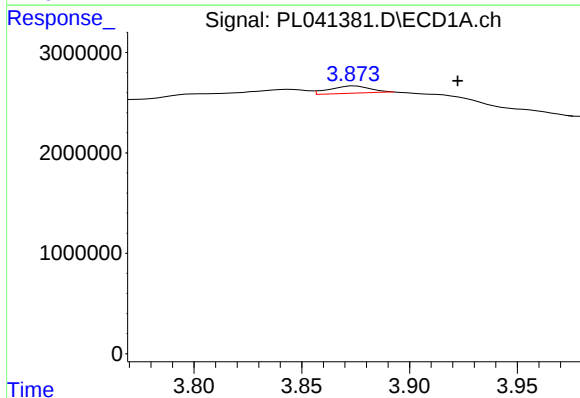


#2 alpha-BHC

R.T.: 3.875 min
Delta R.T.: -0.048 min
Response: 1050962
Conc: 0.13 ng/ml

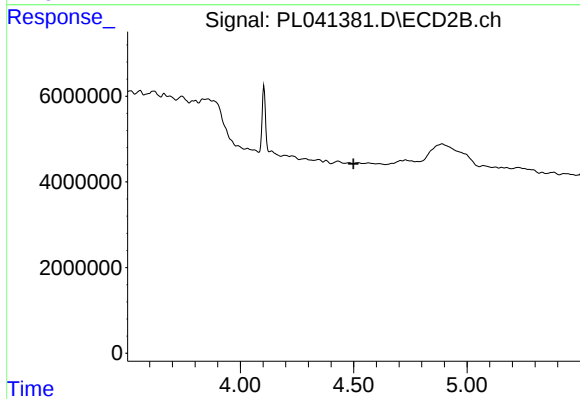

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.499 min
Response: 0
Conc: N.D.

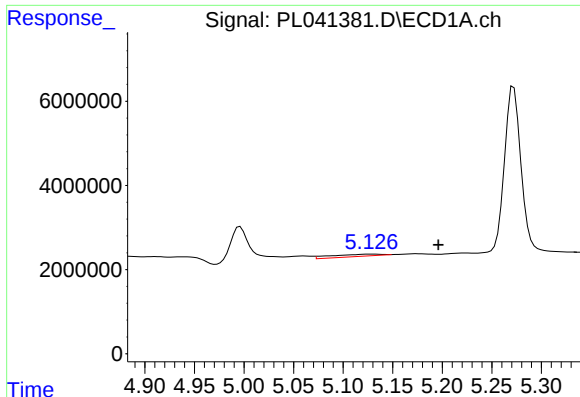

#8 Heptachlor epoxide


R.T.: 5.127 min
Delta R.T.: -0.069 min
Response: 1798776
Conc: 0.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

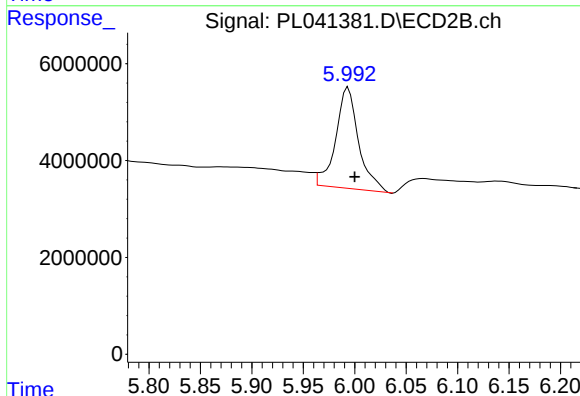


#8 Heptachlor epoxide

R.T.: 5.994 min
Delta R.T.: -0.006 min
Response: 32527383
Conc: 11.34 ng/ml

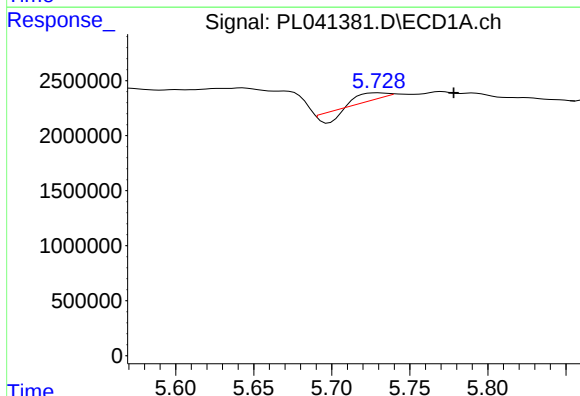


#13 Dieldrin

R.T.: 5.730 min
Delta R.T.: -0.049 min
Response: 397656
Conc: 0.06 ng/ml

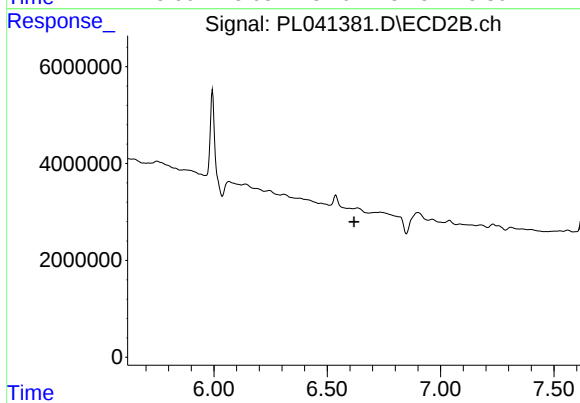

#13 Dieldrin


R.T.: 0.000 min
Exp R.T. : 6.618 min
Response: 0
Conc: N.D.

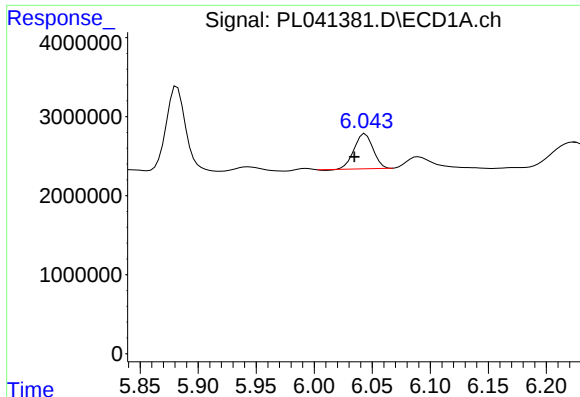

#14 Endrin


R.T.: 6.044 min
Delta R.T.: 0.009 min
Response: 5018090
Conc: 0.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

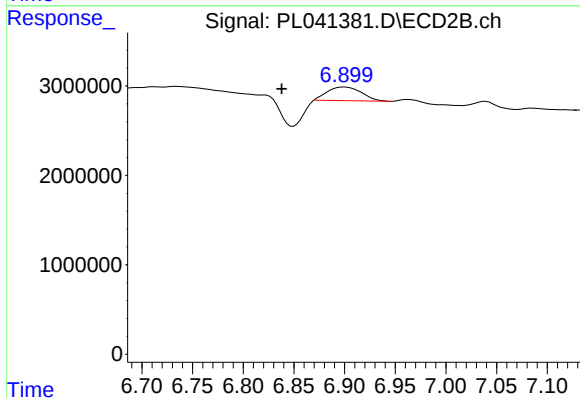


#14 Endrin

R.T.: 6.901 min
Delta R.T.: 0.062 min
Response: 3610397
Conc: 1.62 ng/ml

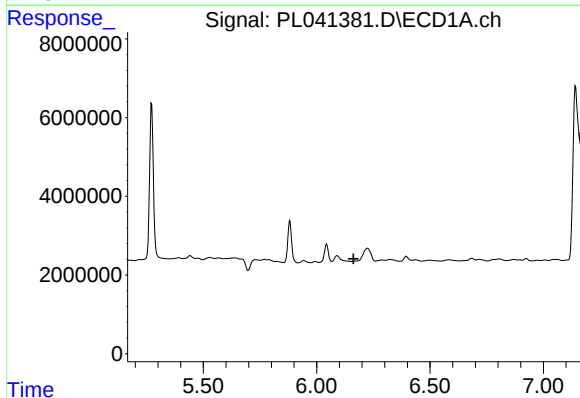


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.163 min
Response: 0
Conc: N.D.

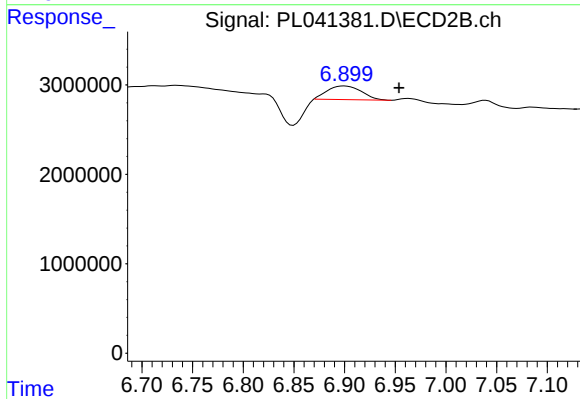

#16 4,4'-DDD


R.T.: 6.901 min
Delta R.T.: -0.053 min
Response: 3610397
Conc: 1.72 ng/ml

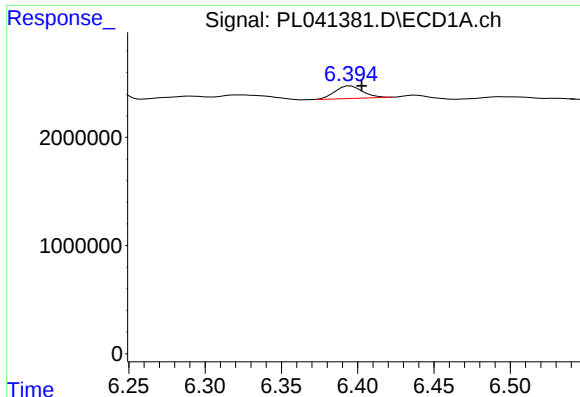

#17 4,4'-DDT


R.T.: 6.395 min
Delta R.T.: -0.007 min
Response: 1453022
Conc: 0.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

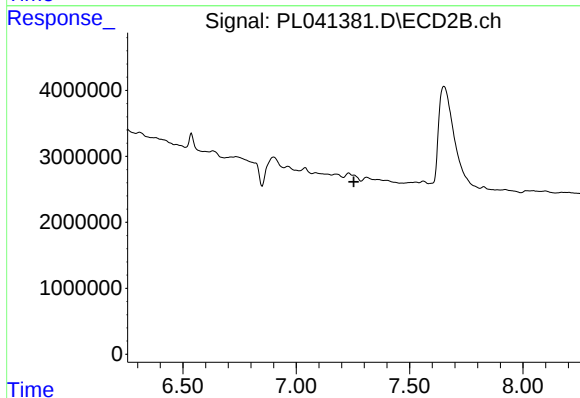


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

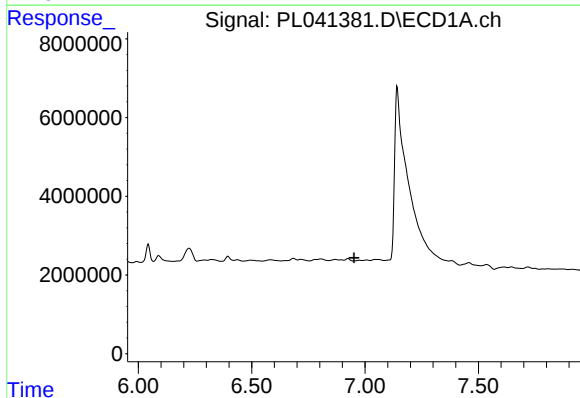


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.952 min
Response: 0
Conc: N.D.

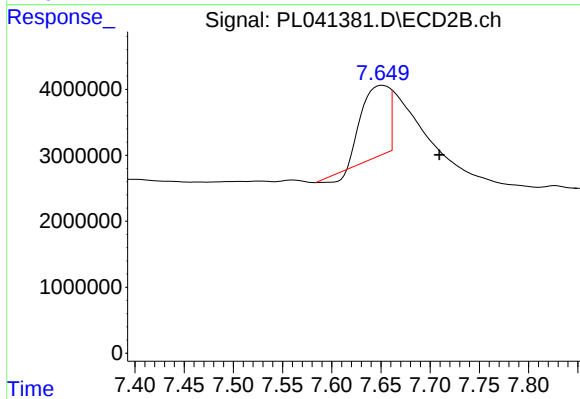

#20 Methoxychlor


R.T.: 7.652 min
Delta R.T.: -0.058 min
Response: 20659669
Conc: 17.55 ng/ml

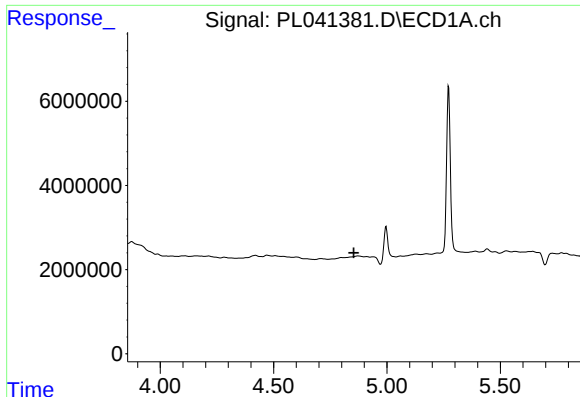

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 4.854 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

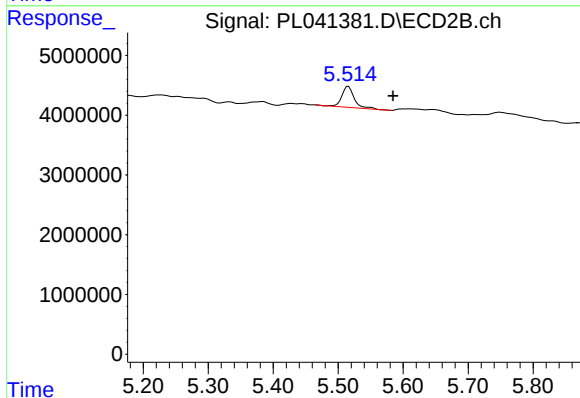


#24 Chlordane-2

R.T.: 5.516 min
Delta R.T.: -0.069 min
Response: 4651688
Conc: 37.61 ng/ml

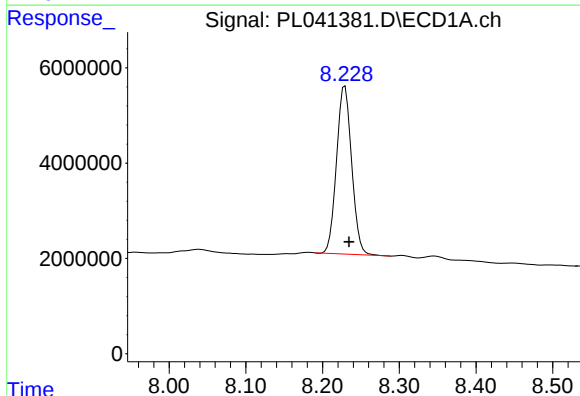

#28 Decachlorobiphenyl

R.T.: 8.229 min
Delta R.T.: -0.005 min
Response: 48210427
Conc: 9.27 ng/ml

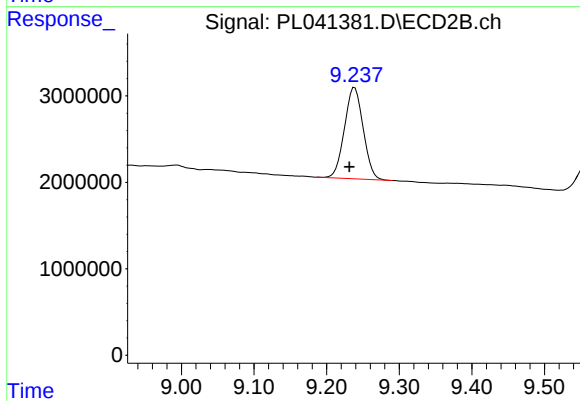

#28 Decachlorobiphenyl

R.T.: 9.239 min
Delta R.T.: 0.007 min
Response: 18901370
Conc: 7.31 ng/ml