

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
 Data File : PL041394.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2018 17:20
 Operator : AJ\SJ
 Sample : J5665-04
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 23:33:31 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.104	87732514	45810817	16.007	16.430
28)	SA Decachlor...	8.220	9.235	85860840	36539289	16.513	14.130
Target Compounds							
2)	A alpha-BHC	3.912	0.000	3976189	0	0.502	N.D. #
6)	B beta-BHC	0.000	4.997f	0	1706791	N.D.	1.065 #
16)	A 4,4'-DDD	6.230f	0.000	2392092	0	0.530	N.D. #
20)	A Methoxychlor	6.980	0.000	1403174	0	0.539	N.D. #
23)	Chlordane-1	4.354	0.000	2130150	0	8.346	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
Data File : PL041394.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 17:20
Operator : AJ\SJ
Sample : J5665-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 23:33:31 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

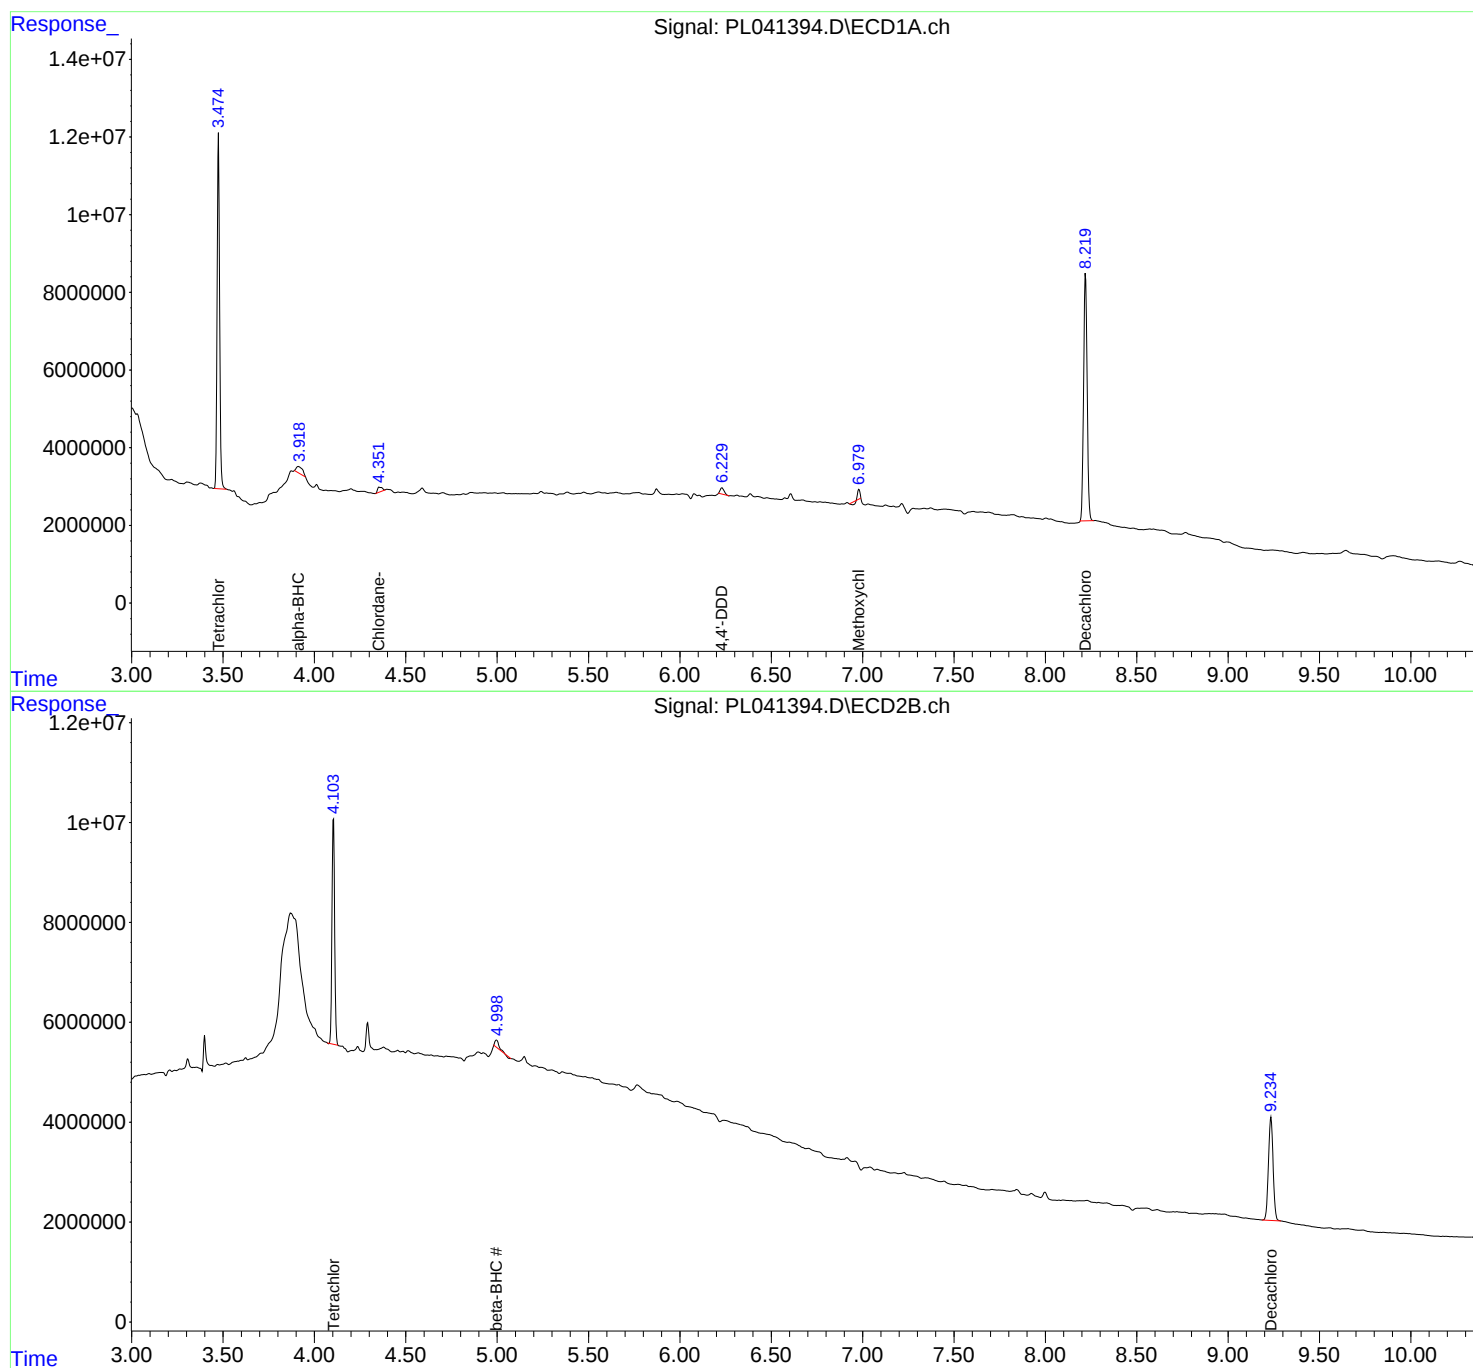


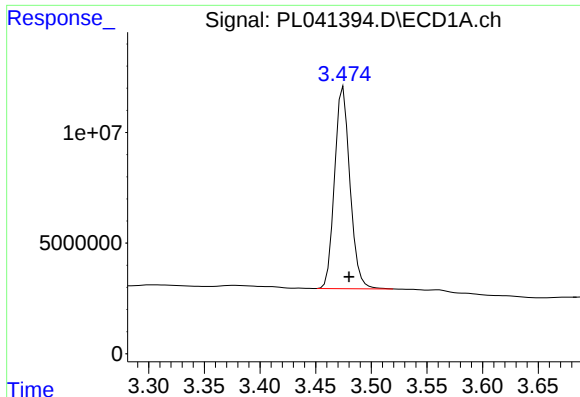

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 87732514
Conc: 16.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

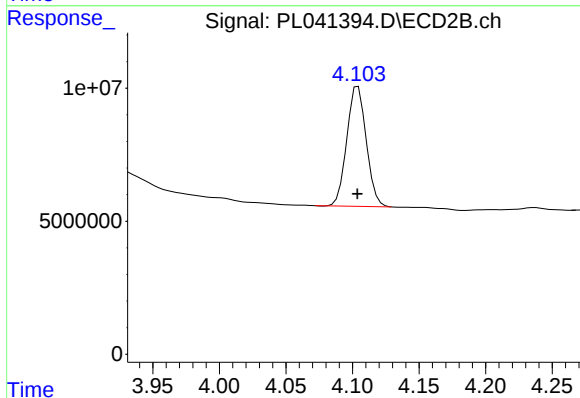


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 45810817
Conc: 16.43 ng/ml

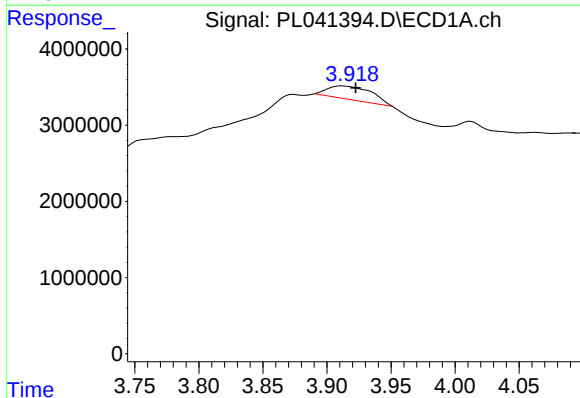


#2 alpha-BHC

R.T.: 3.912 min
Delta R.T.: -0.010 min
Response: 3976189
Conc: 0.50 ng/ml

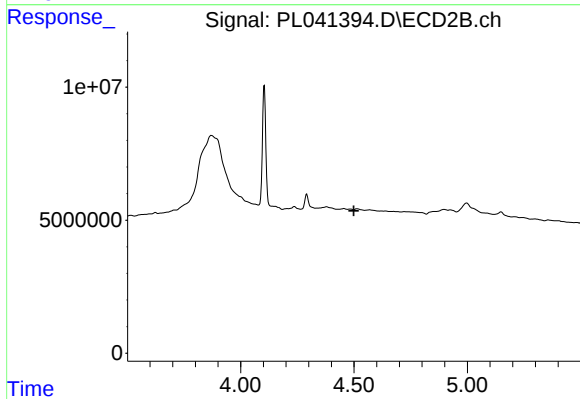

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.499 min
Response: 0
Conc: N.D.

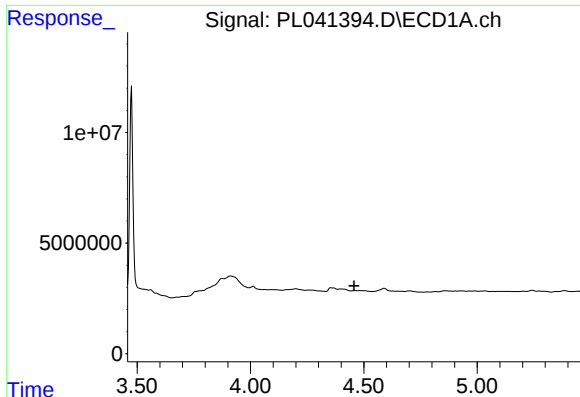

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

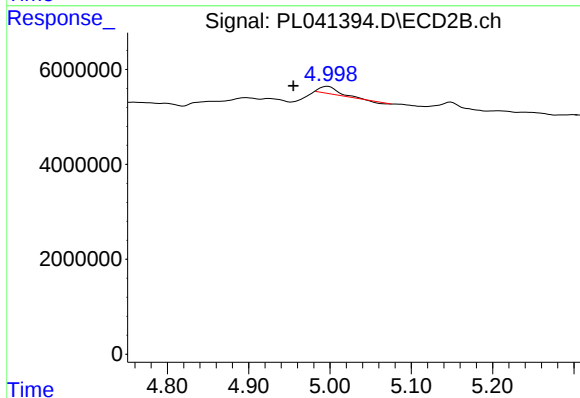


#6 beta-BHC

R.T.: 4.997 min
Delta R.T.: 0.042 min
Response: 1706791
Conc: 1.06 ng/ml

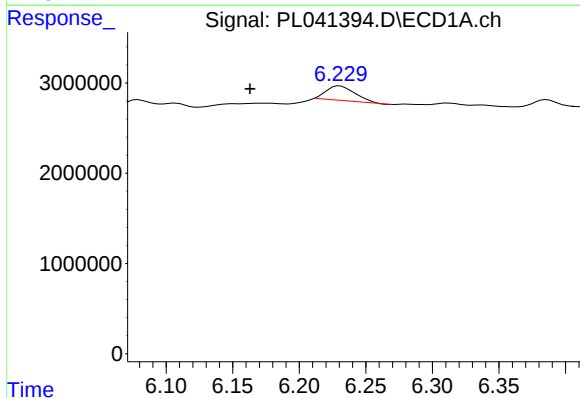


#16 4,4'-DDD

R.T.: 6.230 min
Delta R.T.: 0.067 min
Response: 2392092
Conc: 0.53 ng/ml

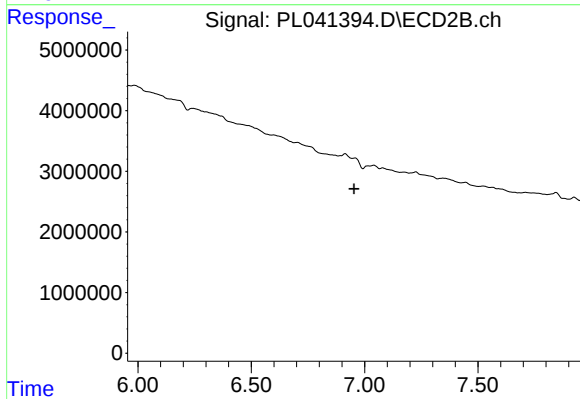

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.954 min
Response: 0
Conc: N.D.

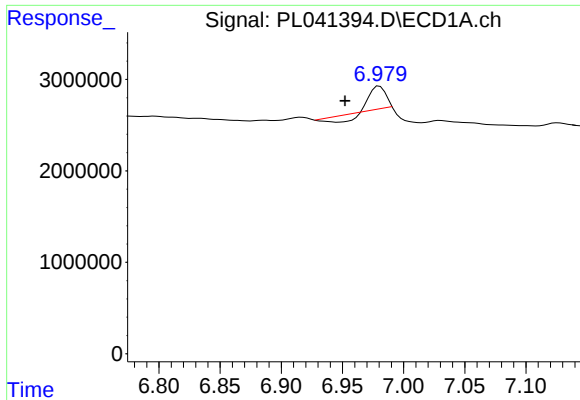

#20 Methoxychlor


R.T.: 6.980 min
Delta R.T.: 0.028 min
Response: 1403174
Conc: 0.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

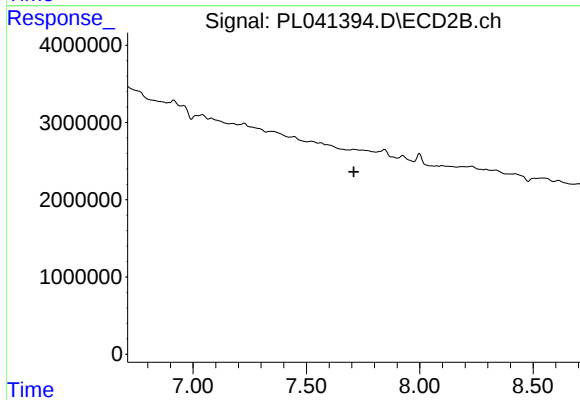


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

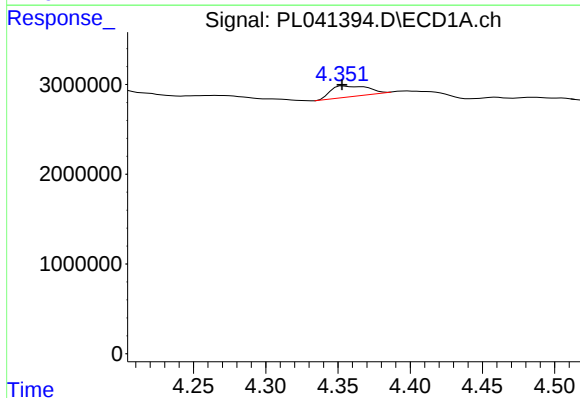


#23 Chlordane-1

R.T.: 4.354 min
Delta R.T.: 0.001 min
Response: 2130150
Conc: 8.35 ng/ml

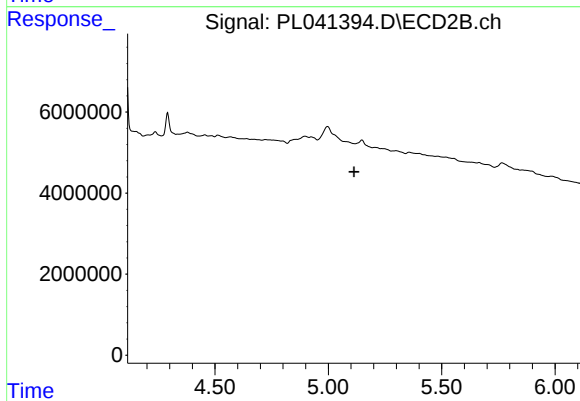

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

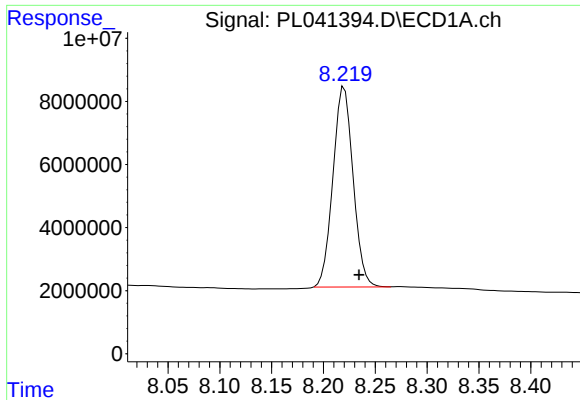

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 85860840
Conc: 16.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

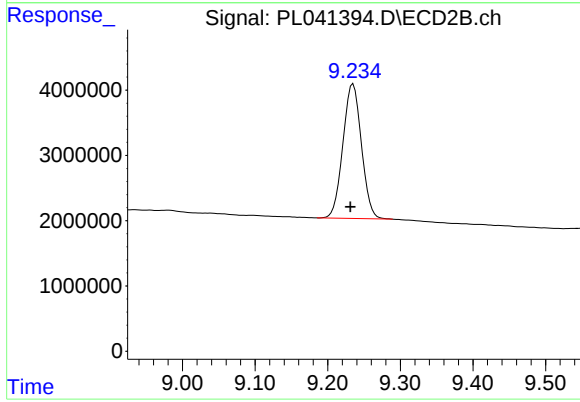

#28 Decachlorobiphenyl

R.T.: 9.235 min
Delta R.T.: 0.004 min
Response: 36539289
Conc: 14.13 ng/ml