

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
 Data File : PL041397.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2018 18:03
 Operator : AJ\SJ
 Sample : J5675-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 23:34:06 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.474	4.104	50509995	28236754	9.216	10.127
28)	SA Decachlor...	8.220	9.234	54464272	22739767	10.475	8.794
Target Compounds							
6)	B beta-BHC	4.411f	0.000	4844020	0	1.527	N.D. #
23)	Chlordane-1	4.411	0.000	4844020	0	18.980	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
Data File : PL041397.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 18:03
Operator : AJ\SJ
Sample : J5675-01
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 23:34:06 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

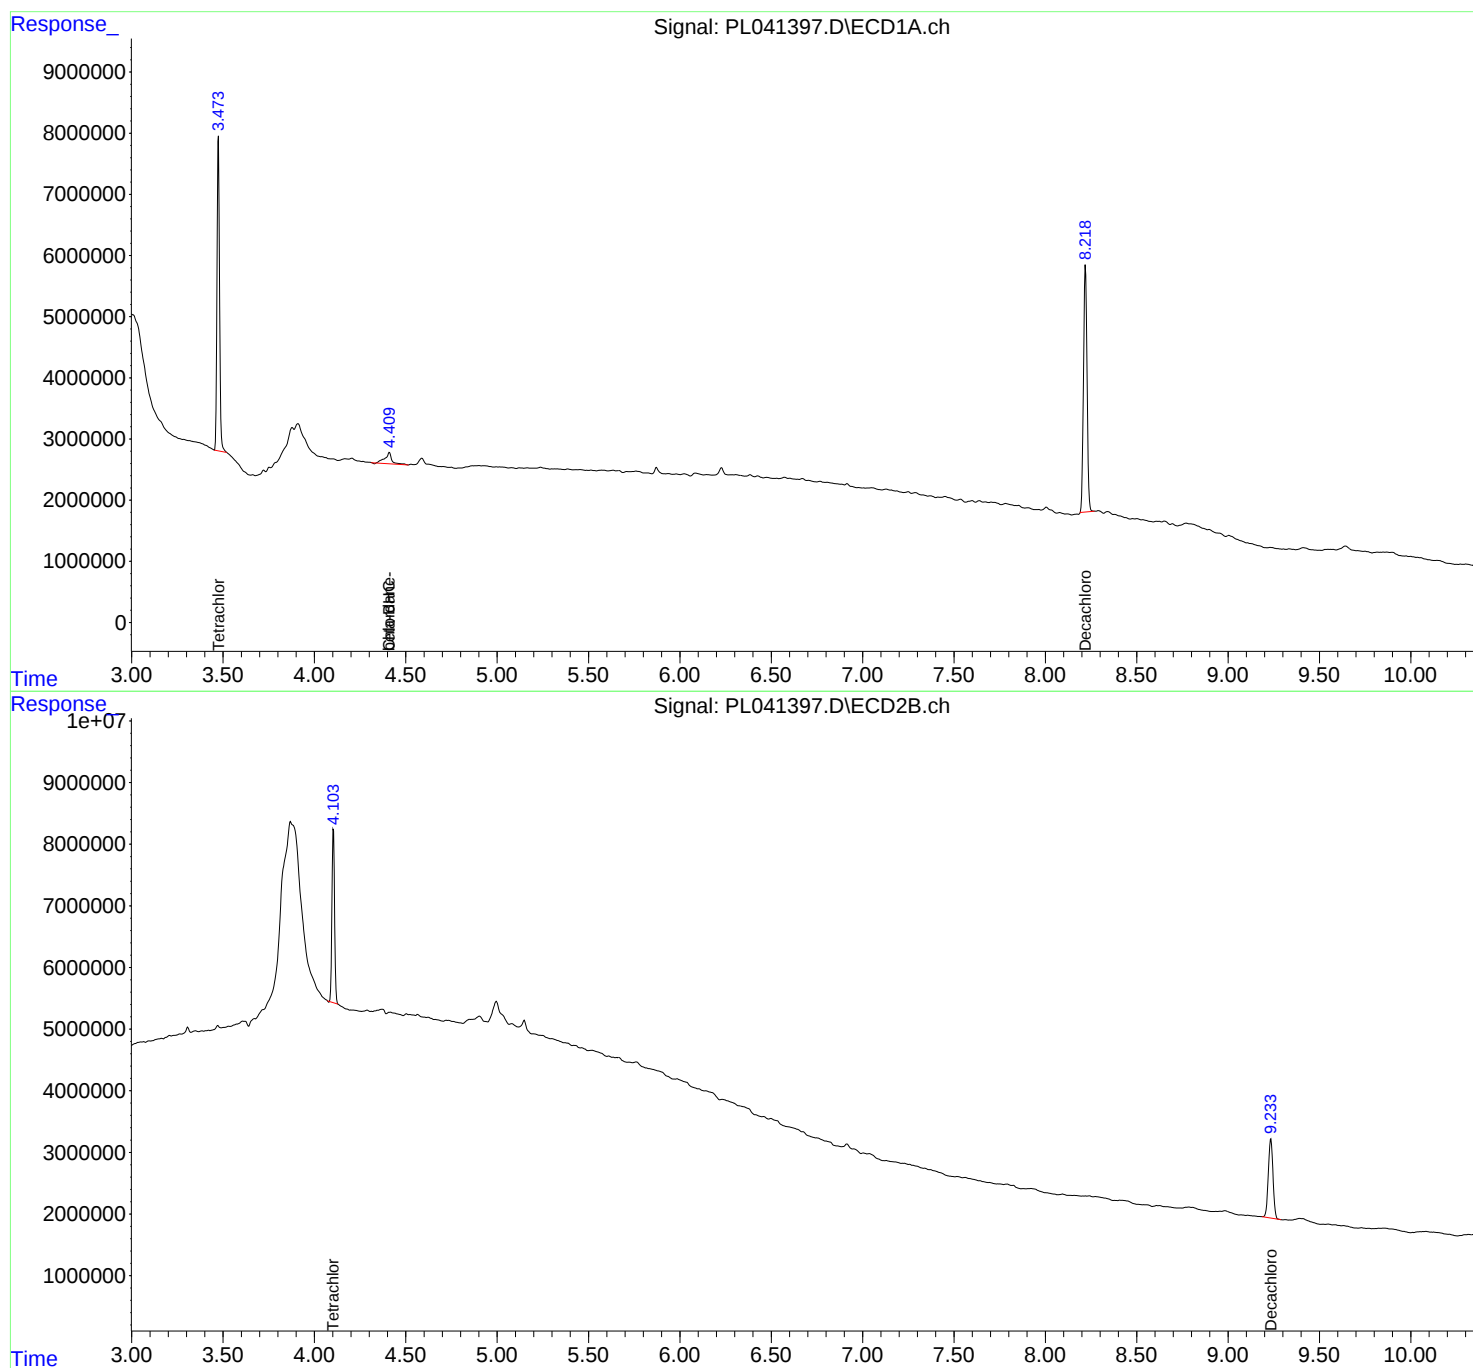


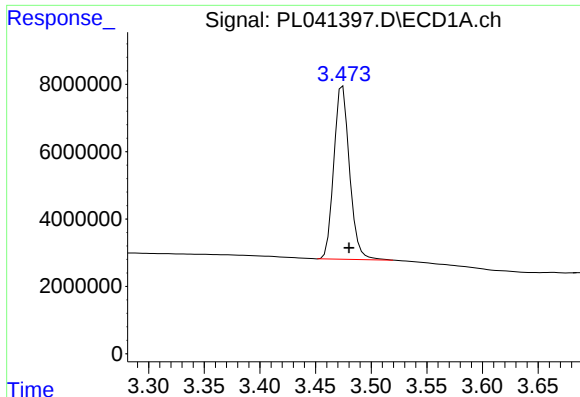

#1 Tetrachloro-m-xylene


R.T.: 3.474 min
Delta R.T.: -0.006 min
Response: 50509995
Conc: 9.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

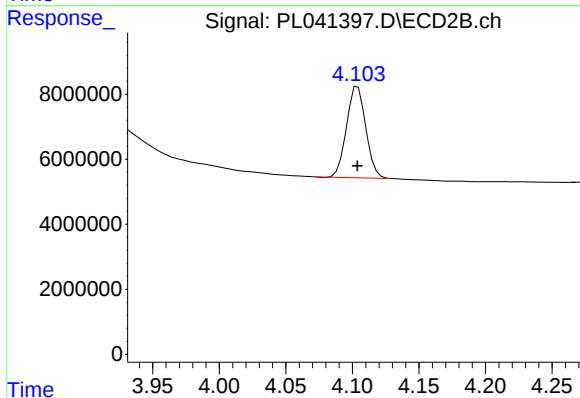


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 28236754
Conc: 10.13 ng/ml

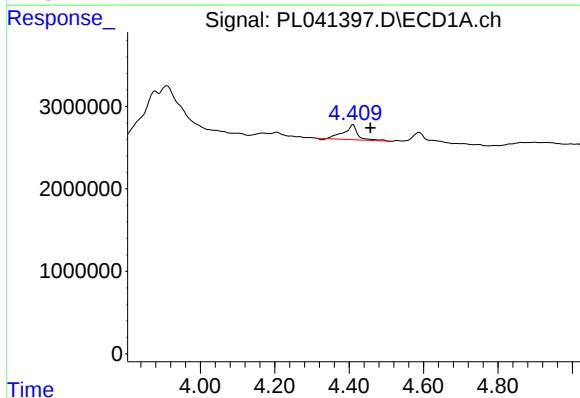


#6 beta-BHC

R.T.: 4.411 min
Delta R.T.: -0.047 min
Response: 4844020
Conc: 1.53 ng/ml

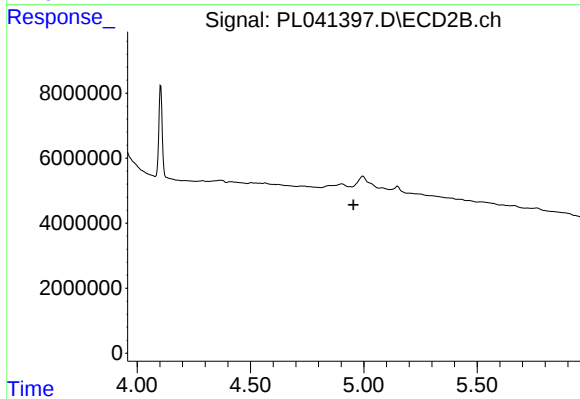

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.955 min
Response: 0
Conc: N.D.

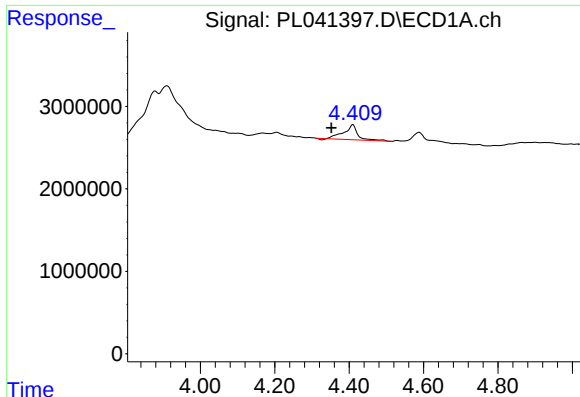

#23 Chlordane-1


R.T.: 4.411 min
Delta R.T.: 0.058 min
Response: 4844020
Conc: 18.98 ng/ml

Instrument :
ECD_L
ClientSampleId :

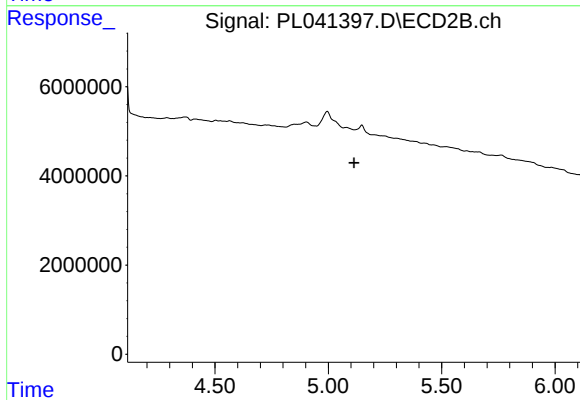


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

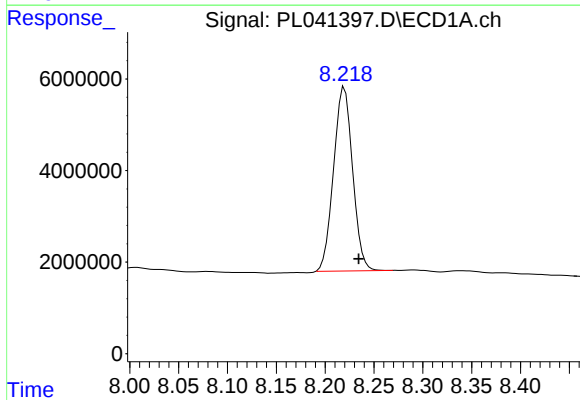

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 54464272
Conc: 10.47 ng/ml

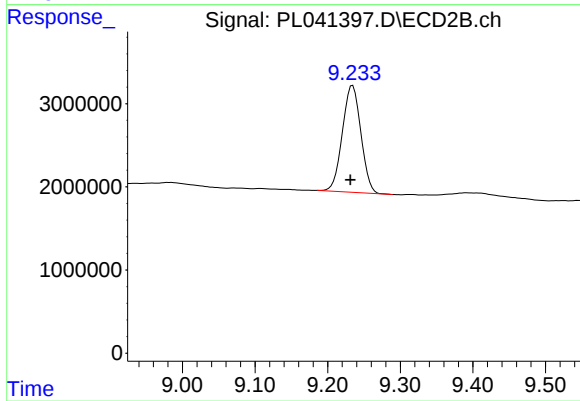

#28 Decachlorobiphenyl

R.T.: 9.234 min
Delta R.T.: 0.003 min
Response: 22739767
Conc: 8.79 ng/ml