

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL102618\  
 Data File : PL041398.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 26 Oct 2018 18:17  
 Operator : AJ\SJ  
 Sample : J5675-05  
 Misc :  
 ALS Vial : 23 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Oct 26 23:34:18 2018  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL101118.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Oct 11 03:28:36 2018  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

|                             | Compound        | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|--------|----------|----------|--------|---------|
| -----                       |                 |        |        |          |          |        |         |
| System Monitoring Compounds |                 |        |        |          |          |        |         |
| 1)                          | SA Tetrachlo... | 3.475  | 4.104  | 64300434 | 35155641 | 11.732 | 12.608  |
| 28)                         | SA Decachlor... | 8.219  | 9.235  | 76309113 | 31604950 | 14.676 | 12.222  |
| Target Compounds            |                 |        |        |          |          |        |         |
| 6)                          | B beta-BHC      | 4.410f | 4.996f | 4040230  | 3376082  | 1.273  | 2.106 # |
| 14)                         | MA Endrin       | 5.985f | 0.000  | 1045158  | 0        | 0.182  | N.D. #  |
| 17)                         | MA 4,4'-DDT     | 6.385  | 0.000  | 1838052  | 0        | 0.404  | N.D. #  |
| 20)                         | A Methoxychlor  | 6.916f | 0.000  | 1032629  | 0        | 0.397  | N.D. #  |
| 23)                         | Chlordane-1     | 4.410  | 0.000  | 4040230  | 0        | 15.831 | N.D. #  |
| 27)                         | Chlordane-5     | 6.385  | 0.000  | 1838052  | 0        | 8.481  | N.D. #  |
| -----                       |                 |        |        |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL102618\  
Data File : PL041398.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 26 Oct 2018 18:17  
Operator : AJ\SJ  
Sample : J5675-05  
Misc :  
ALS Vial : 23 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampled :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Oct 26 23:34:18 2018  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL101118.M  
Quant Title : GC Extractables  
QLast Update : Thu Oct 11 03:28:36 2018  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

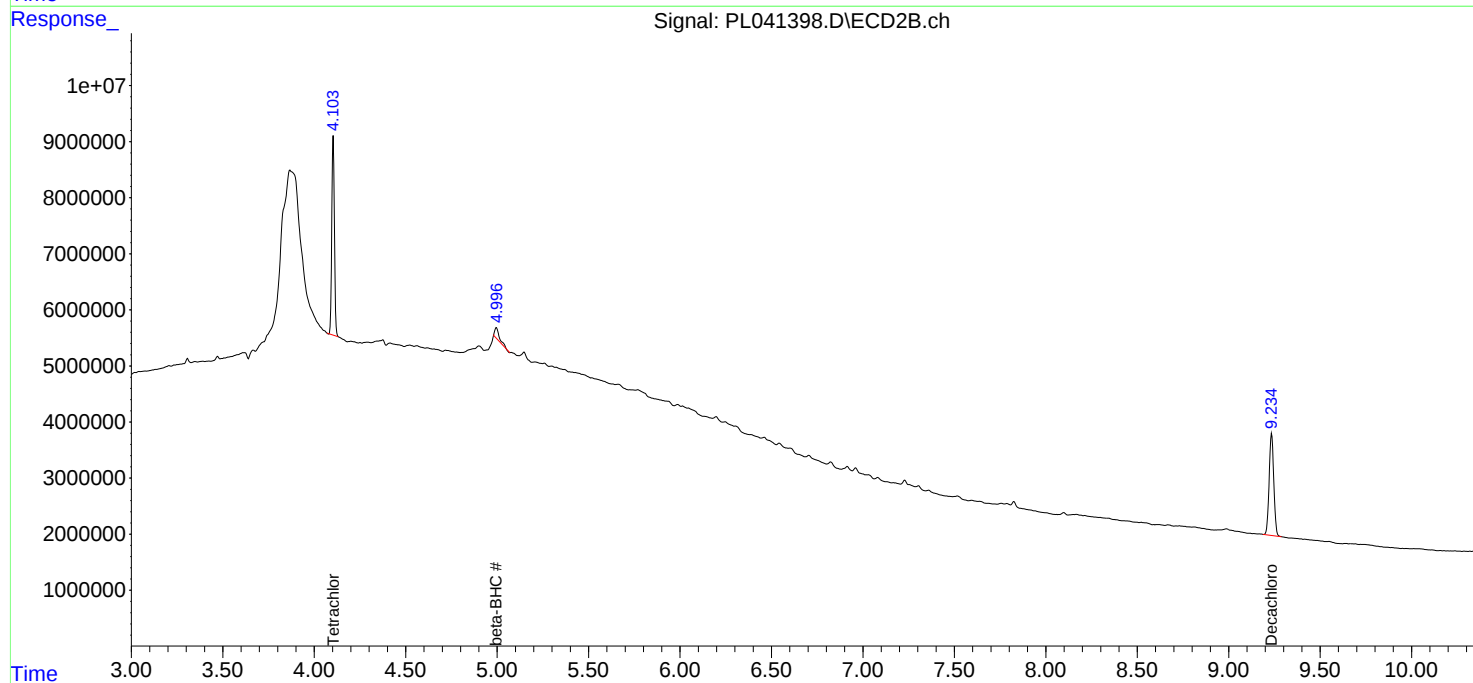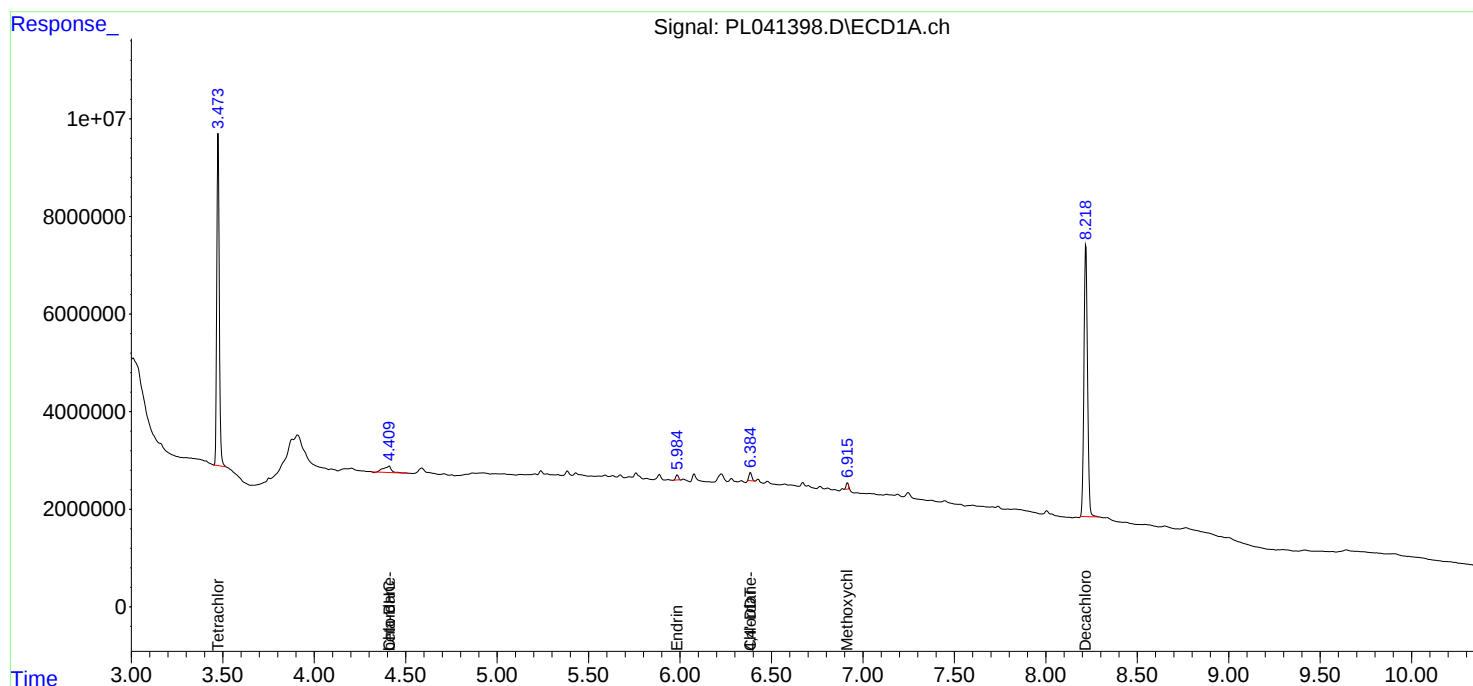


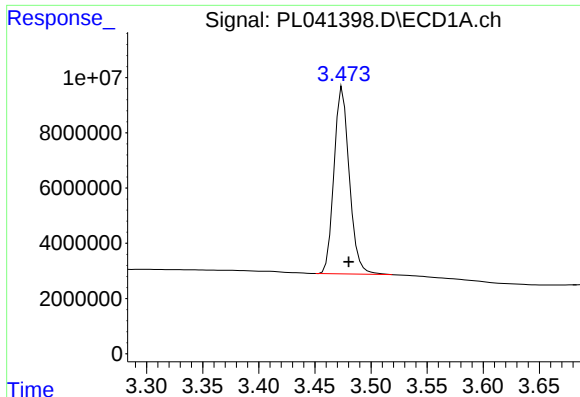

#1 Tetrachloro-m-xylene


R.T.: 3.475 min  
Delta R.T.: -0.005 min  
Response: 64300434  
Conc: 11.73 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

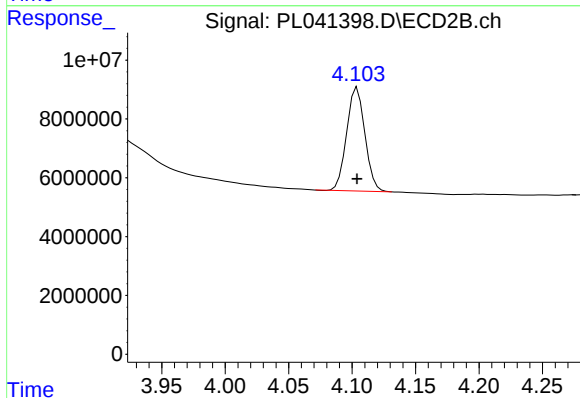


#1 Tetrachloro-m-xylene

R.T.: 4.104 min  
Delta R.T.: 0.000 min  
Response: 35155641  
Conc: 12.61 ng/ml

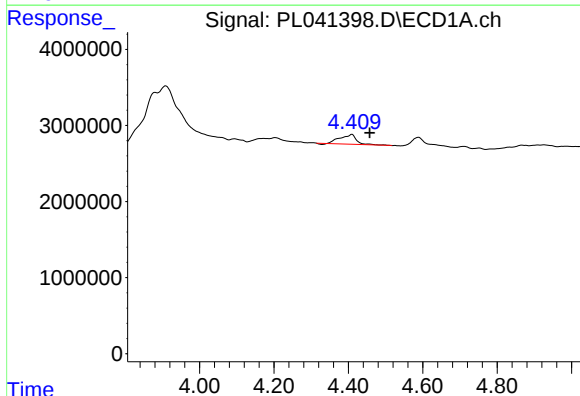


#6 beta-BHC

R.T.: 4.410 min  
Delta R.T.: -0.047 min  
Response: 4040230  
Conc: 1.27 ng/ml

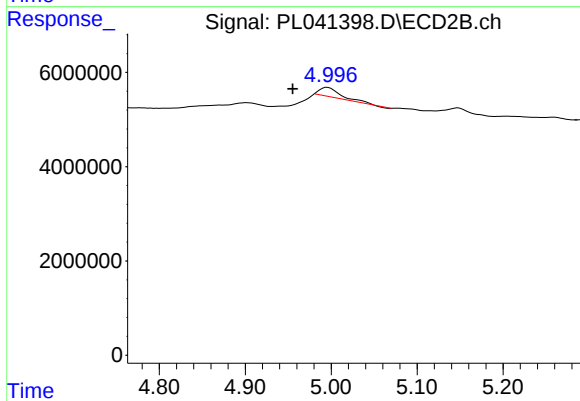

#6 beta-BHC


R.T.: 4.996 min  
Delta R.T.: 0.041 min  
Response: 3376082  
Conc: 2.11 ng/ml

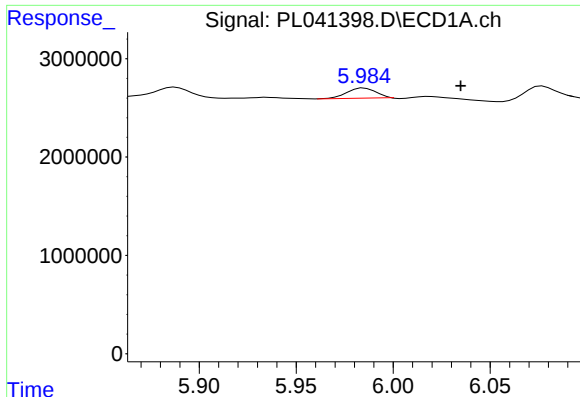

#14 Endrin


R.T.: 5.985 min  
Delta R.T.: -0.050 min  
Response: 1045158  
Conc: 0.18 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

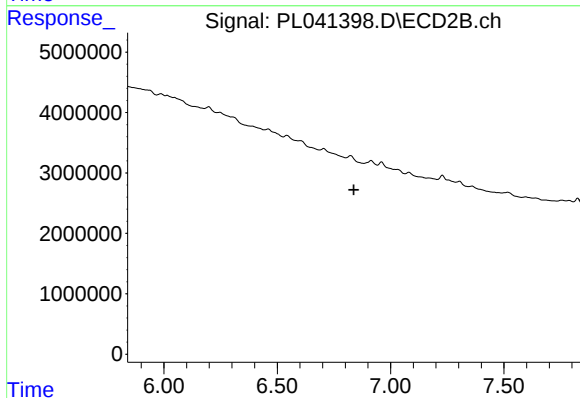


#14 Endrin

R.T.: 0.000 min  
Exp R.T. : 6.838 min  
Response: 0  
Conc: N.D.

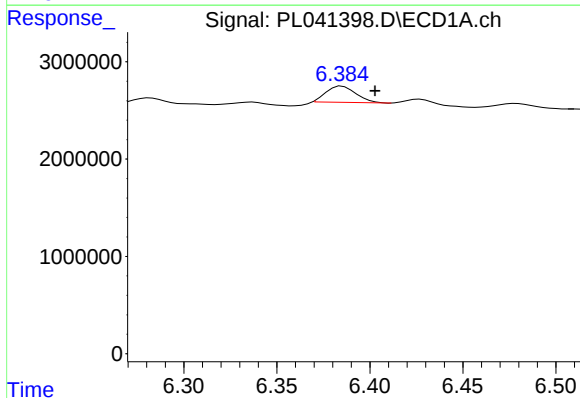


#17 4,4'-DDT

R.T.: 6.385 min  
Delta R.T.: -0.018 min  
Response: 1838052  
Conc: 0.40 ng/ml

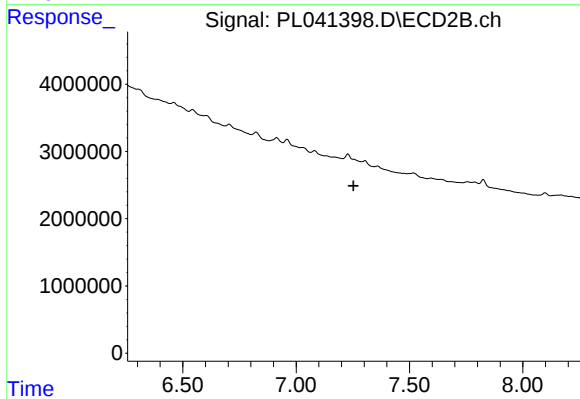

#17 4,4'-DDT


R.T.: 0.000 min  
Exp R.T. : 7.254 min  
Response: 0  
Conc: N.D.

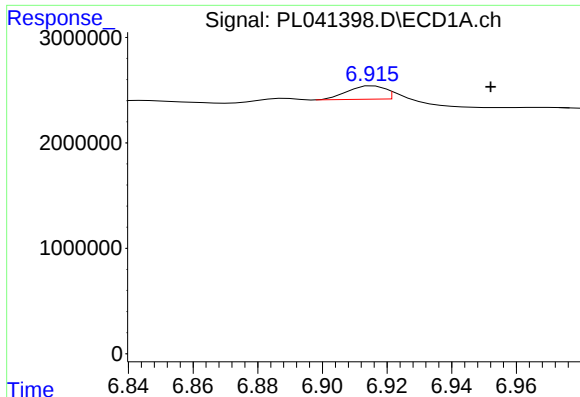

#20 Methoxychlor


R.T.: 6.916 min  
Delta R.T.: -0.036 min  
Response: 1032629  
Conc: 0.40 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

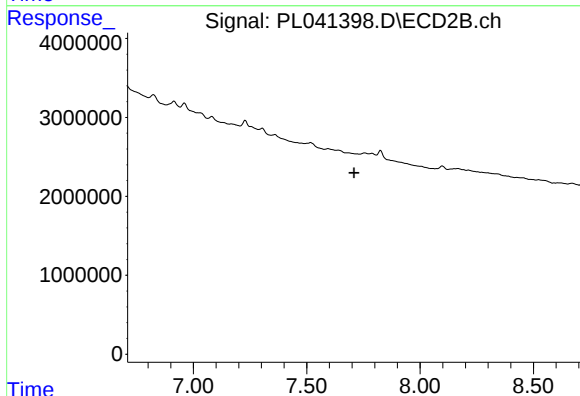


#20 Methoxychlor

R.T.: 0.000 min  
Exp R.T. : 7.709 min  
Response: 0  
Conc: N.D.

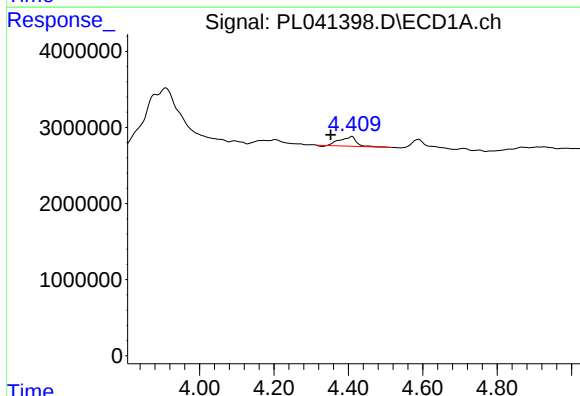


#23 Chlordane-1

R.T.: 4.410 min  
Delta R.T.: 0.057 min  
Response: 4040230  
Conc: 15.83 ng/ml

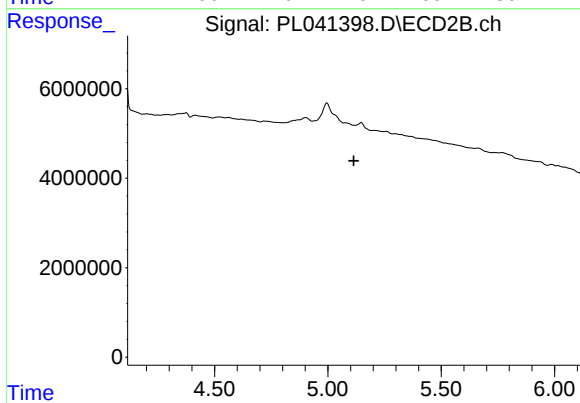

#23 Chlordane-1


R.T.: 0.000 min  
Exp R.T. : 5.114 min  
Response: 0  
Conc: N.D.

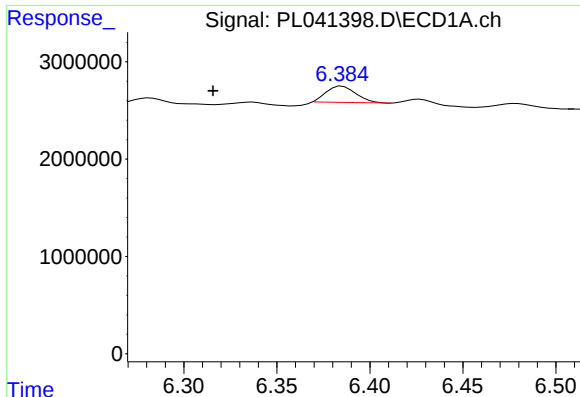

#27 Chlordane-5


R.T.: 6.385 min  
Delta R.T.: 0.069 min  
Response: 1838052  
Conc: 8.48 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

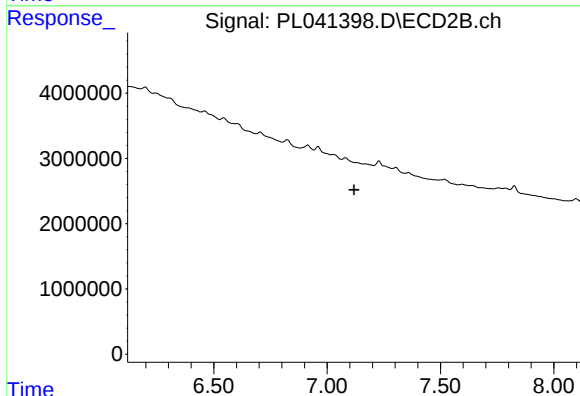


#27 Chlordane-5

R.T.: 0.000 min  
Exp R.T. : 7.120 min  
Response: 0  
Conc: N.D.

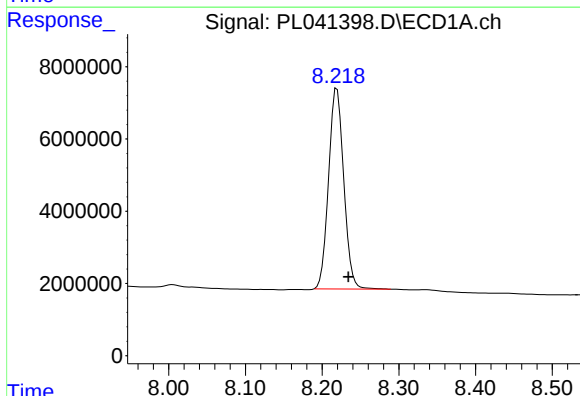

#28 Decachlorobiphenyl

R.T.: 8.219 min  
Delta R.T.: -0.015 min  
Response: 76309113  
Conc: 14.68 ng/ml

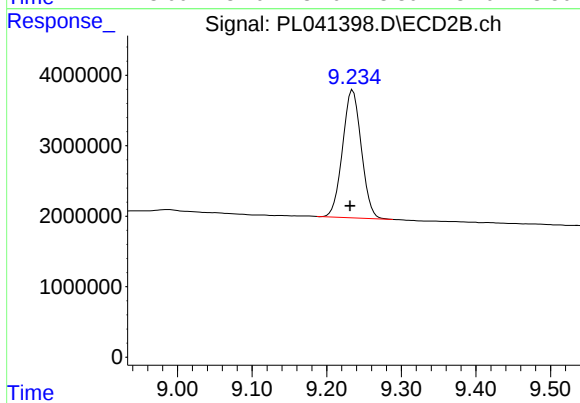

#28 Decachlorobiphenyl

R.T.: 9.235 min  
Delta R.T.: 0.004 min  
Response: 31604950  
Conc: 12.22 ng/ml