

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
 Data File : PL041399.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2018 18:31
 Operator : AJ\SJ
 Sample : J5683-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 26 23:34:27 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.104	132.9E6	69039505	24.251	24.761
28)	SA Decachlor...	8.219	9.235	129.8E6	52628568	24.967	20.353
Target Compounds							
4)	MA Heptachlor	0.000	5.356f	0	1995245	N.D.	0.589 #
6)	B beta-BHC	0.000	4.996f	0	3772810	N.D.	2.354 #
9)	A Endosulfan I	5.552	0.000	3426920	0	0.572	N.D. #
13)	MA Dieldrin	5.763	0.000	3908027	0	0.618	N.D. #
15)	B Endosulfa...	6.312	0.000	3024646	0	0.540	N.D. #
17)	MA 4,4'-DDT	6.386	0.000	2363001	0	0.519	N.D. #
20)	A Methoxychlor	6.979	0.000	645907	0	0.248	N.D. #
23)	Chlordane-1	4.354	0.000	1254012	0	4.914	N.D. #
27)	Chlordane-5	6.312	0.000	3024646	0	13.957	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
Data File : PL041399.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 18:31
Operator : AJ\SJ
Sample : J5683-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 23:34:27 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

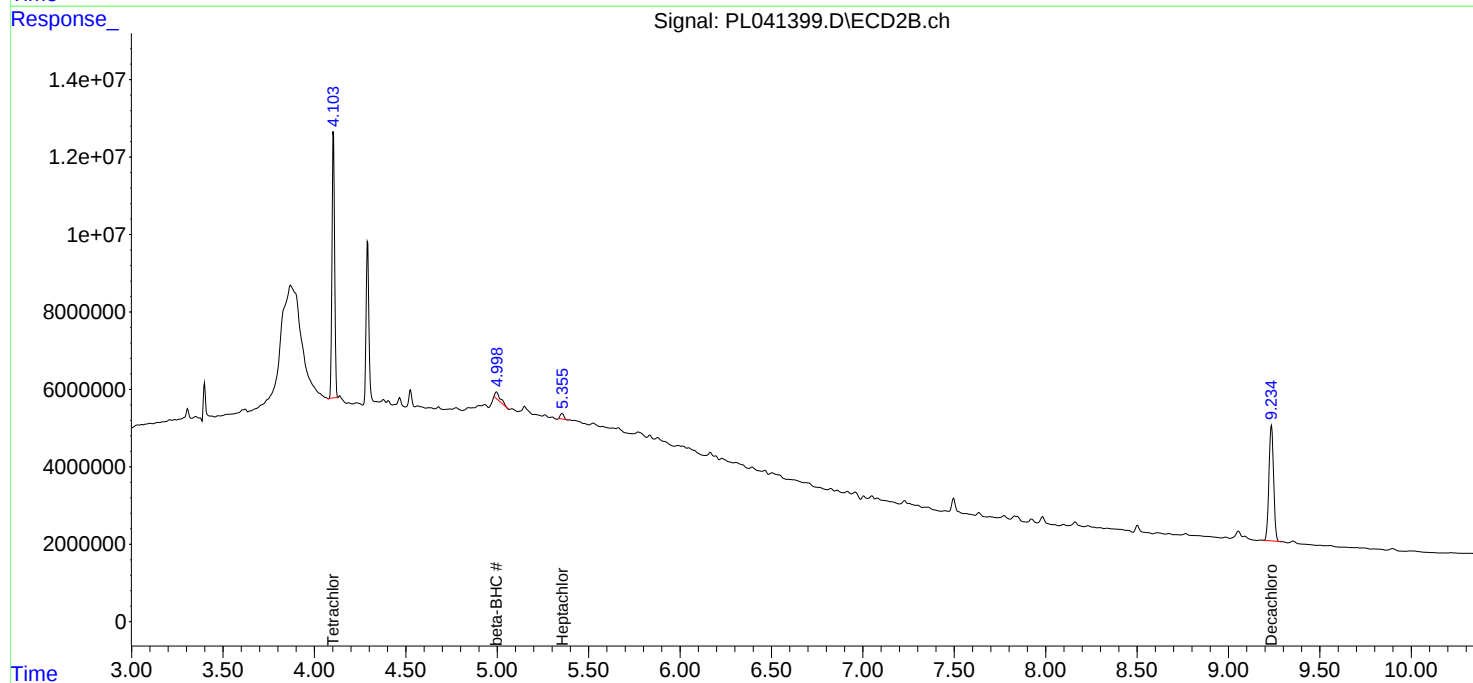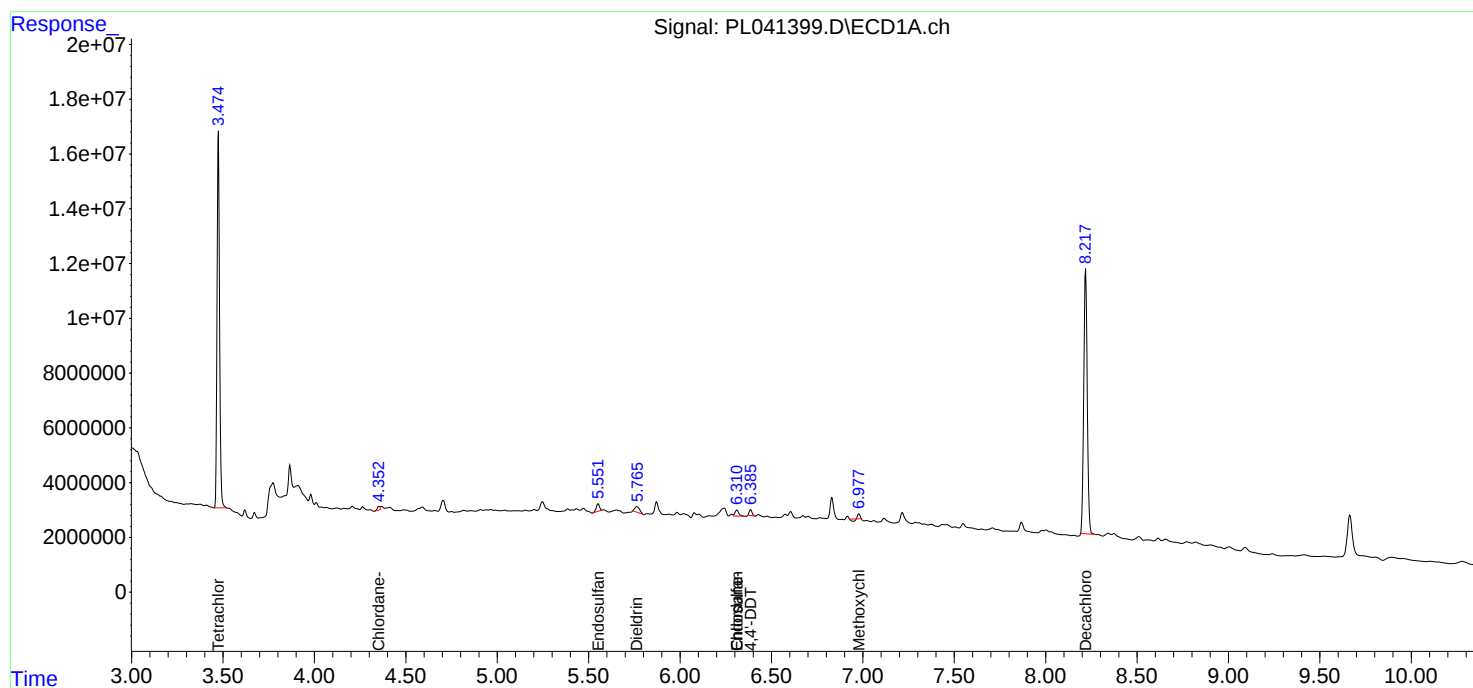


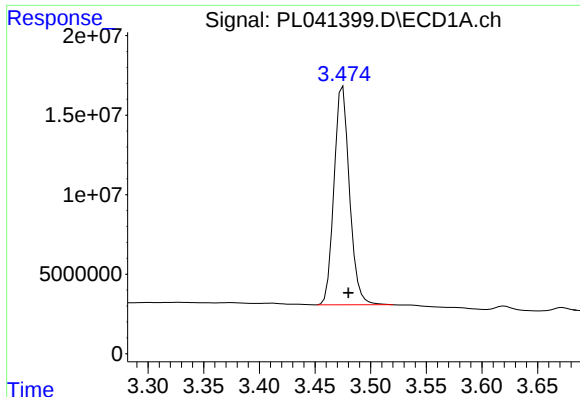

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 132913029
Conc: 24.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

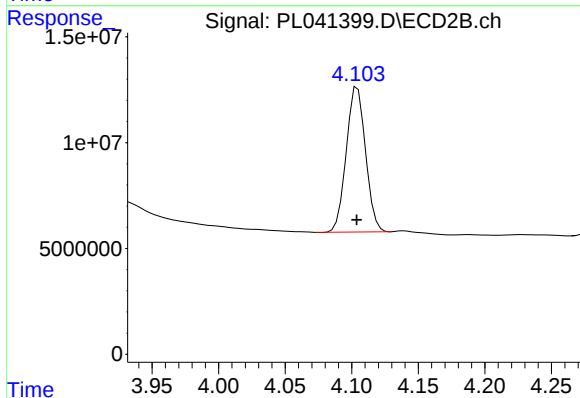


#1 Tetrachloro-m-xylene

R.T.: 4.104 min
Delta R.T.: 0.000 min
Response: 69039505
Conc: 24.76 ng/ml

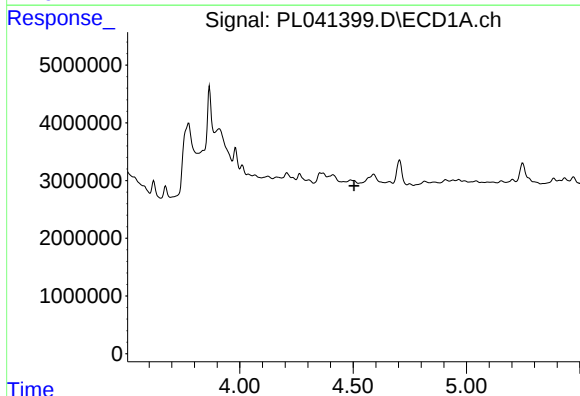


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.505 min
Response: 0
Conc: N.D.

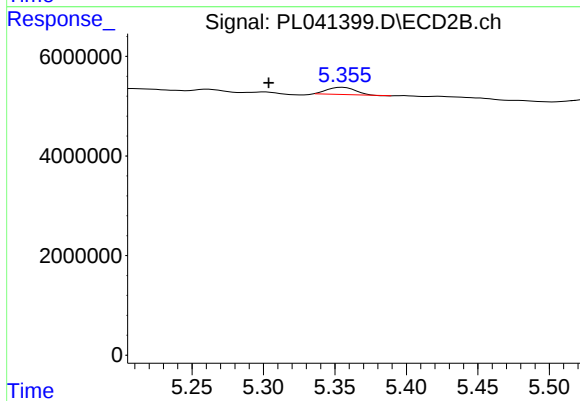

#4 Heptachlor


R.T.: 5.356 min
Delta R.T.: 0.052 min
Response: 1995245
Conc: 0.59 ng/ml

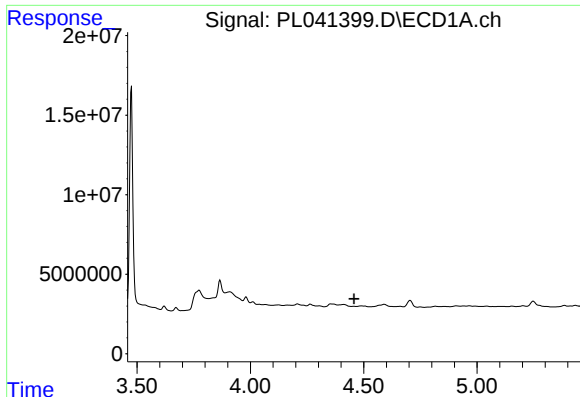

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.458 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

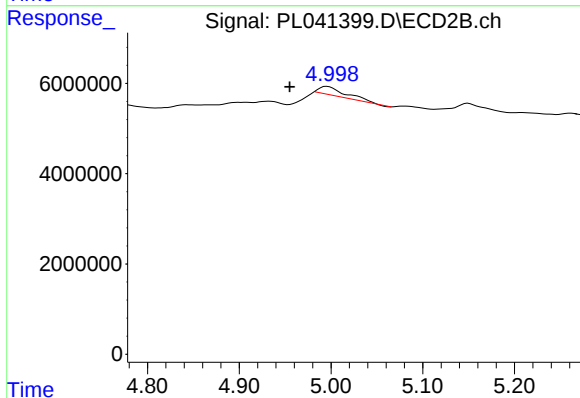


#6 beta-BHC

R.T.: 4.996 min
Delta R.T.: 0.041 min
Response: 3772810
Conc: 2.35 ng/ml

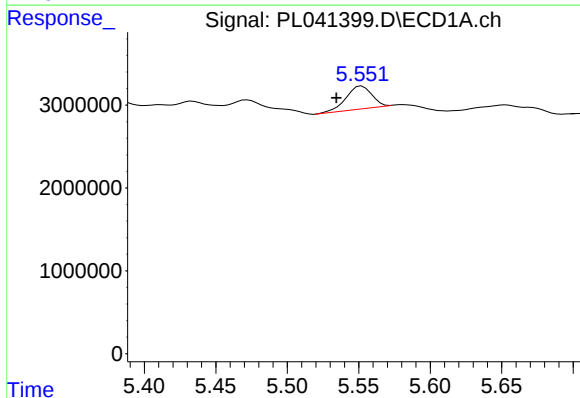


#9 Endosulfan I

R.T.: 5.552 min
Delta R.T.: 0.018 min
Response: 3426920
Conc: 0.57 ng/ml

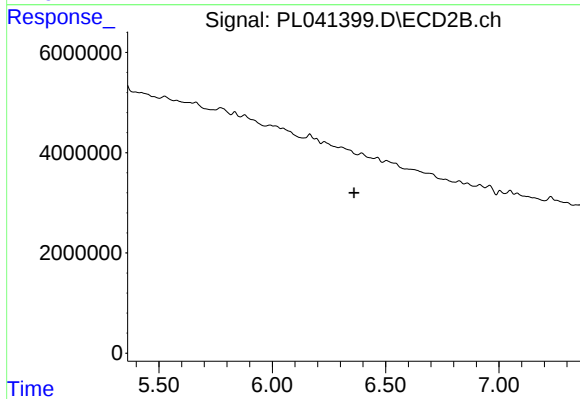

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.360 min
Response: 0
Conc: N.D.

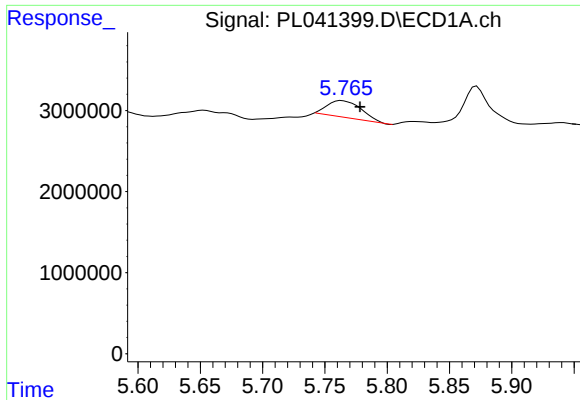

#13 Dieldrin


R.T.: 5.763 min
Delta R.T.: -0.015 min
Response: 3908027
Conc: 0.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

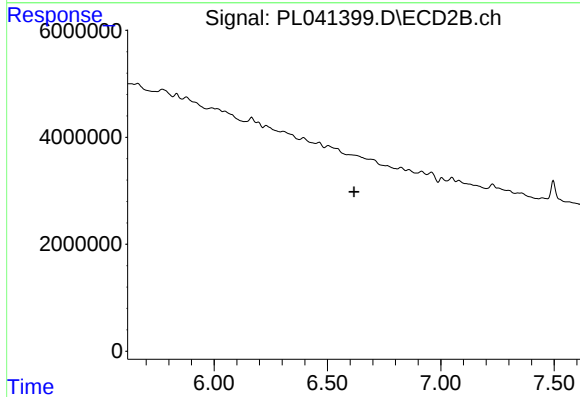


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.618 min
Response: 0
Conc: N.D.

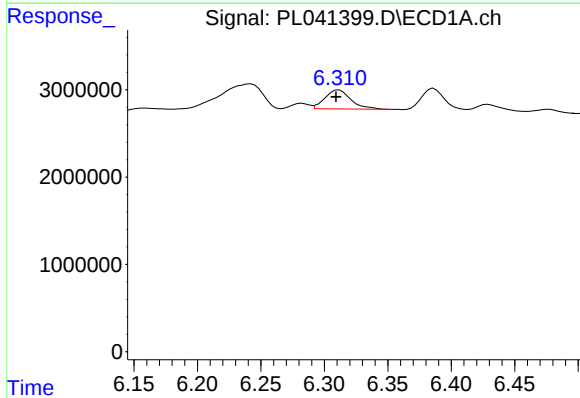


#15 Endosulfan II

R.T.: 6.312 min
Delta R.T.: 0.002 min
Response: 3024646
Conc: 0.54 ng/ml

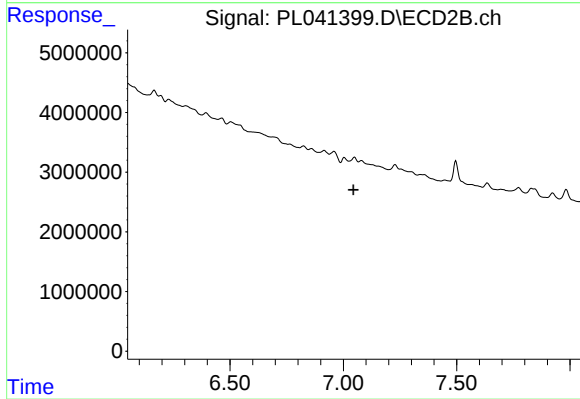

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.045 min
Response: 0
Conc: N.D.

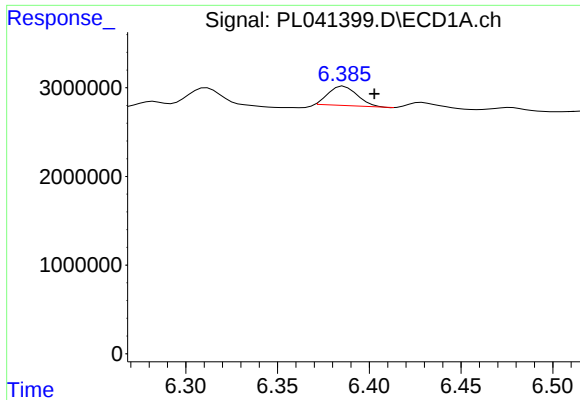

#17 4,4'-DDT


R.T.: 6.386 min
Delta R.T.: -0.017 min
Response: 2363001
Conc: 0.52 ng/ml

Instrument :
ECD_L
ClientSampleId :

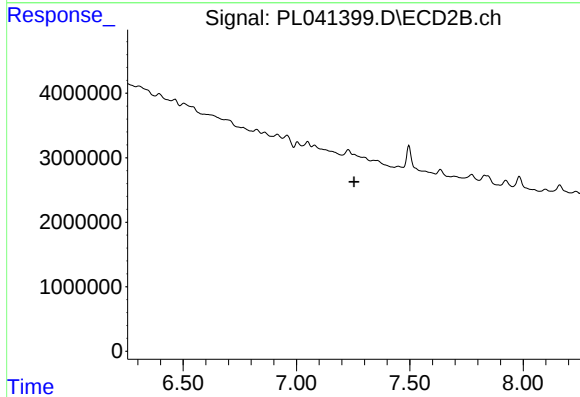


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.254 min
Response: 0
Conc: N.D.

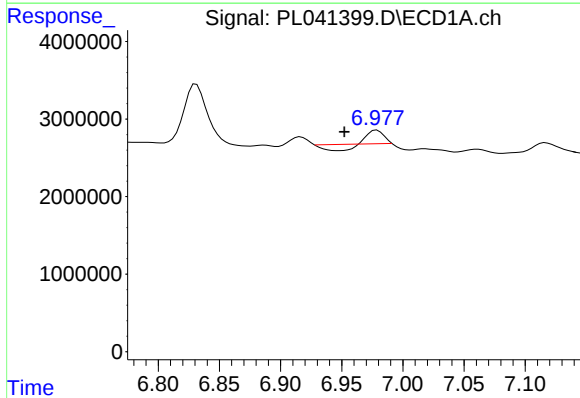


#20 Methoxychlor

R.T.: 6.979 min
Delta R.T.: 0.027 min
Response: 645907
Conc: 0.25 ng/ml

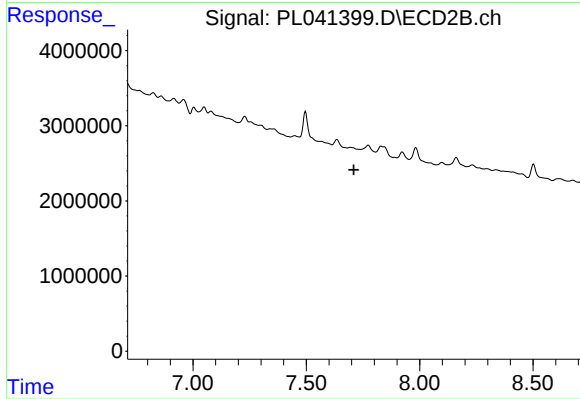

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.709 min
Response: 0
Conc: N.D.

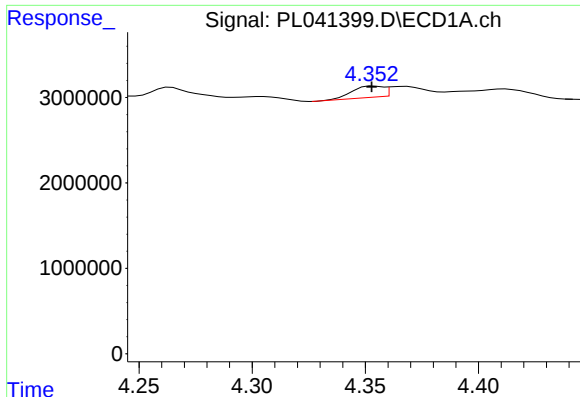

#23 Chlordane-1


R.T.: 4.354 min
Delta R.T.: 0.001 min
Response: 1254012
Conc: 4.91 ng/ml

Instrument :
ECD_L
ClientSampleId :

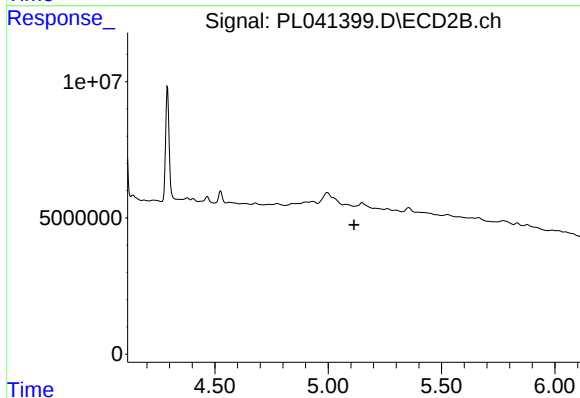


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

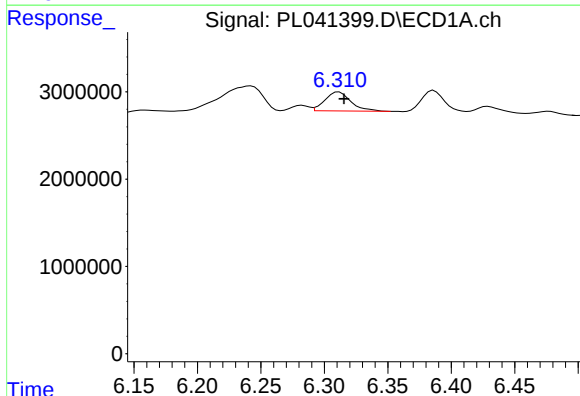


#27 Chlordane-5

R.T.: 6.312 min
Delta R.T.: -0.004 min
Response: 3024646
Conc: 13.96 ng/ml

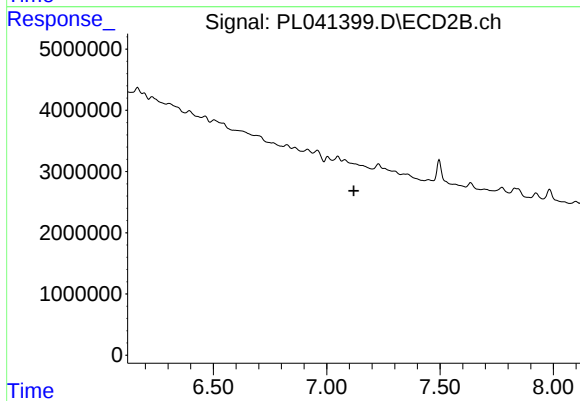

#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.120 min
Response: 0
Conc: N.D.

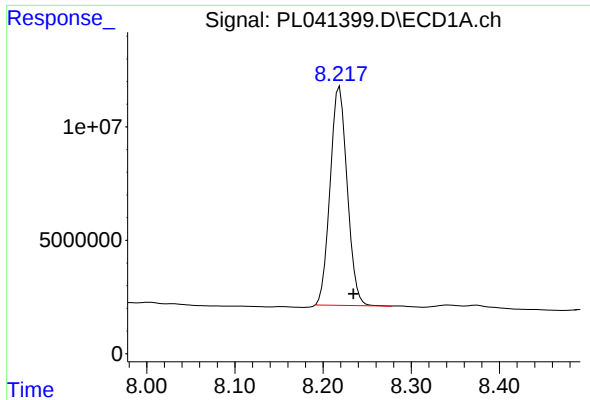

#28 Decachlorobiphenyl


R.T.: 8.219 min

Delta R.T.: -0.016 min

Response: 129817244

Conc: 24.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

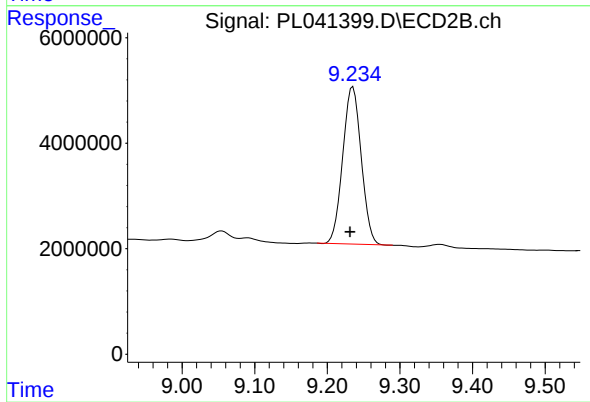

#28 Decachlorobiphenyl

R.T.: 9.235 min

Delta R.T.: 0.004 min

Response: 52628568

Conc: 20.35 ng/ml