

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
 Data File : PL041425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Oct 2018 00:38
 Operator : AJ\SJ
 Sample : J5204-12
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 01:03:59 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 11 03:28:36 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.106	120.2E6	61136020	21.923	21.926
28)	SA Decachlor...	8.220	9.238	117.9E6	49136720	22.682	19.002
Target Compounds							
2)	A alpha-BHC	0.000	4.450f	0	1083711	N.D.	0.280 #
3)	MA gamma-BHC...	4.208	4.769	4813882	1497775	0.659	0.421 #
6)	B beta-BHC	4.413f	0.000	8261611	0	2.604	N.D. #
7)	B delta-BHC	0.000	5.152	0	1571308	N.D.	0.479 #
9)	A Endosulfan I	5.552	0.000	2366557	0	0.395	N.D. #
10)	B gamma-Chl...	0.000	6.223	0	4390620	N.D.	1.565 #
16)	A 4,4'-DDD	6.109f	0.000	1889596	0	0.418	N.D. #
19)	B Endosulfa...	6.689	0.000	2112864	0	0.415	N.D. #
23)	Chlordane-1	4.353	5.152	1553022	1571308	6.085	12.722 #
25)	Chlordane-3	0.000	6.223	0	4390620	N.D.	10.891 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
Data File : PL041425.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Oct 2018 00:38
Operator : AJ\SJ
Sample : J5204-12
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 01:03:59 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

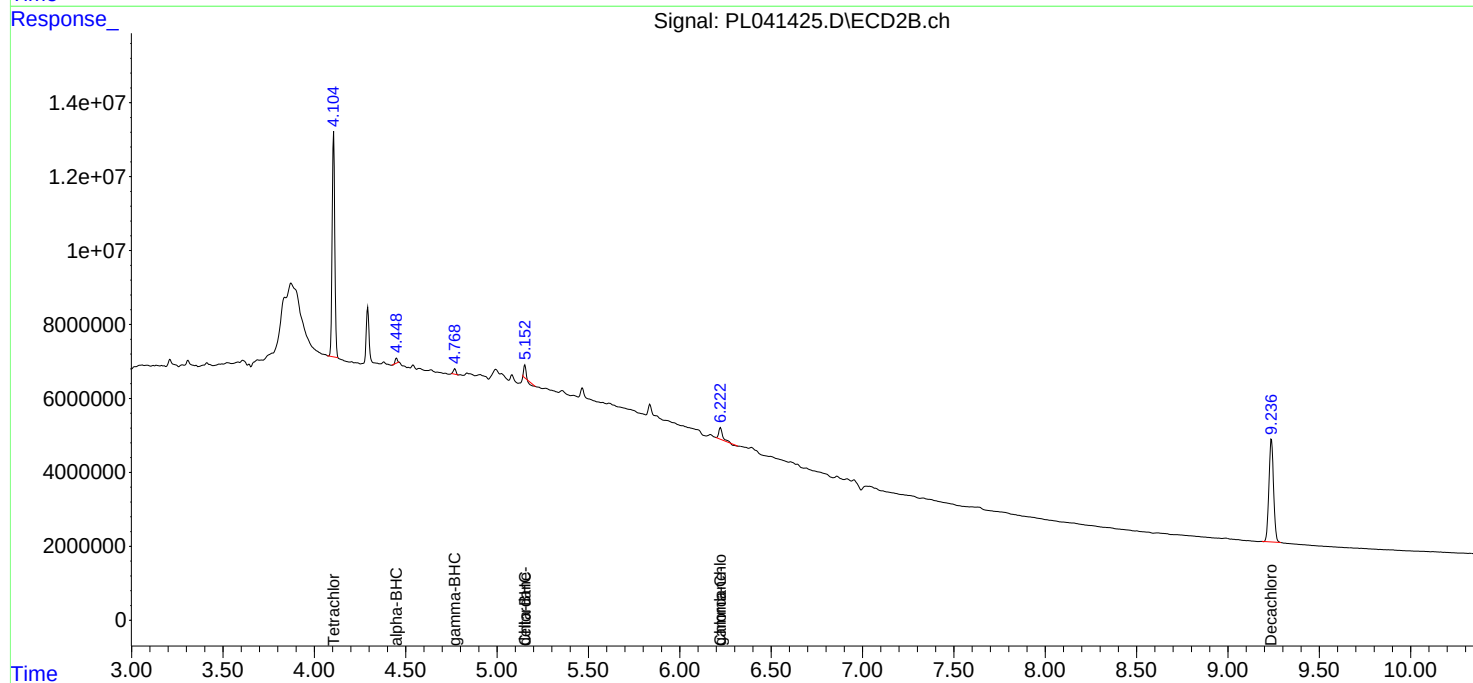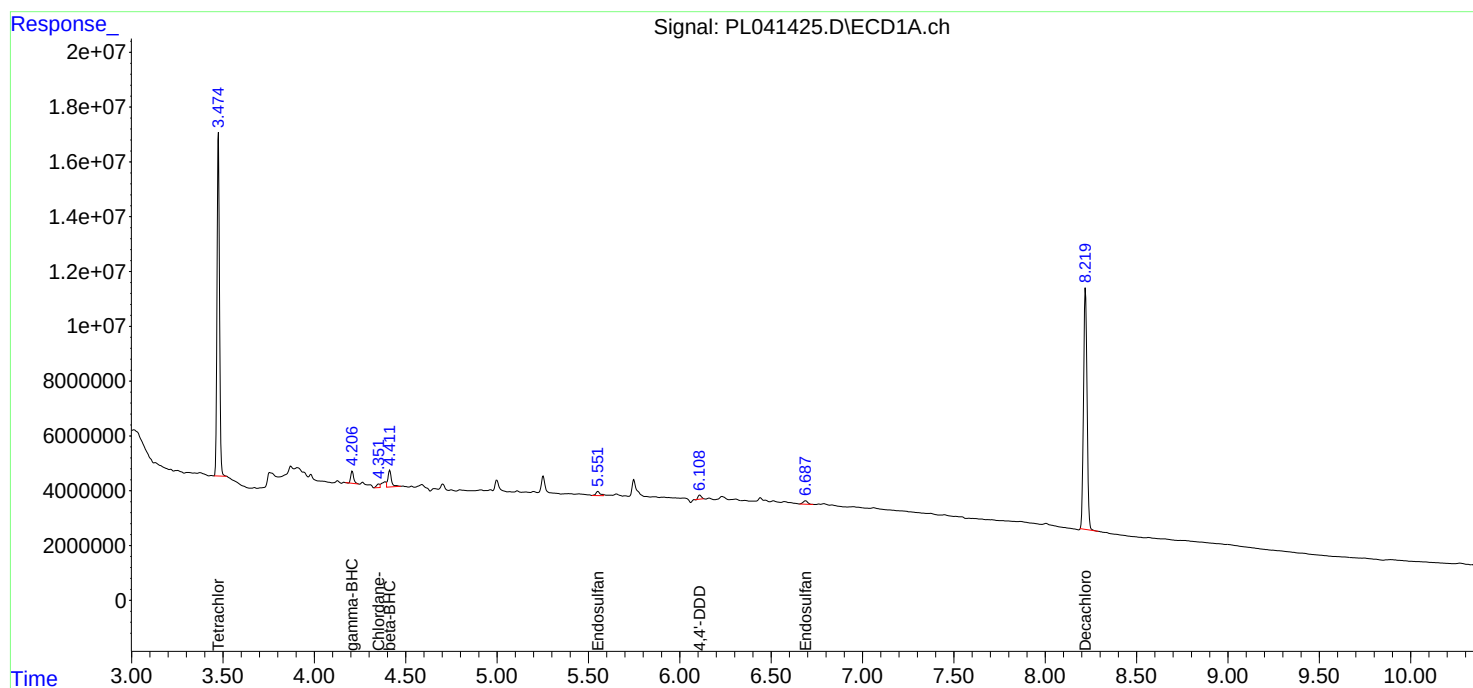


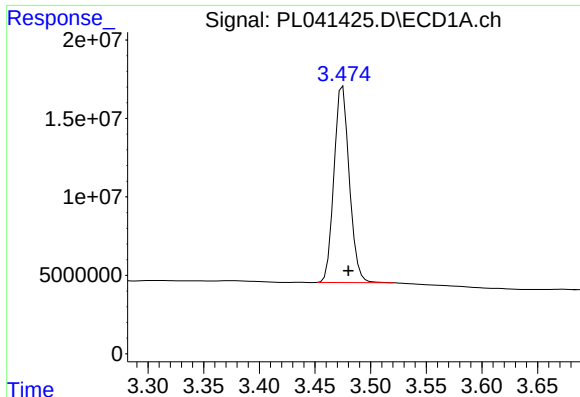

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 120155343
Conc: 21.92 ng/ml

Instrument :
ECD_L
ClientSampleId :

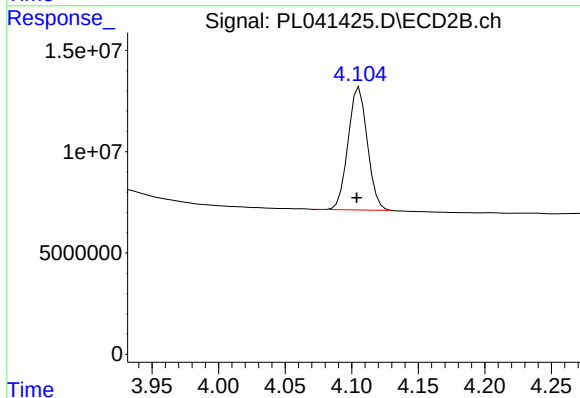


#1 Tetrachloro-m-xylene

R.T.: 4.106 min
Delta R.T.: 0.002 min
Response: 61136020
Conc: 21.93 ng/ml

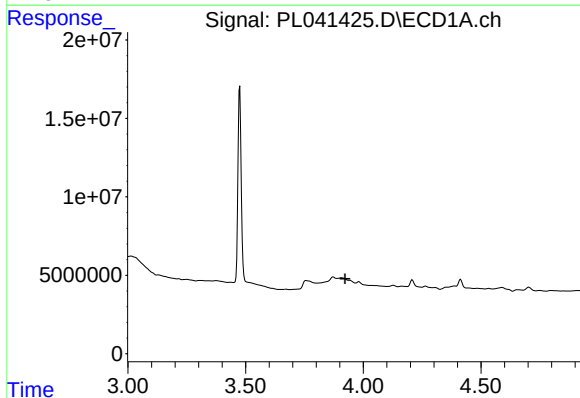


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.922 min
Response: 0
Conc: N.D.

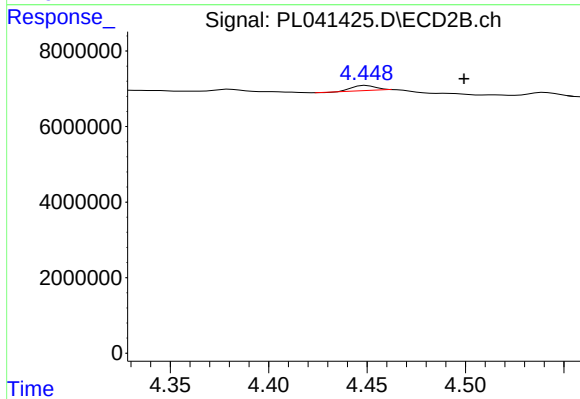

#2 alpha-BHC


R.T.: 4.450 min
Delta R.T.: -0.050 min
Response: 1083711
Conc: 0.28 ng/ml

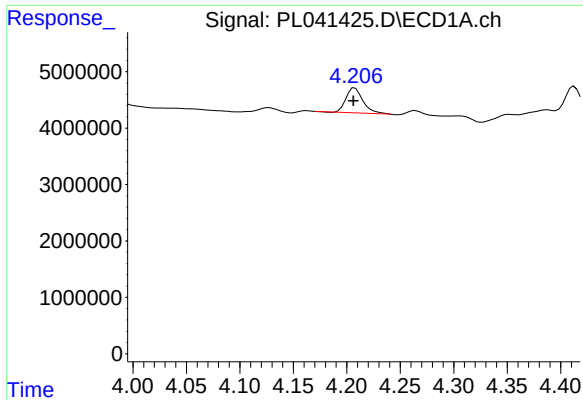

#3 gamma-BHC (Lindane)


R.T.: 4.208 min
Delta R.T.: 0.001 min
Response: 4813882
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :

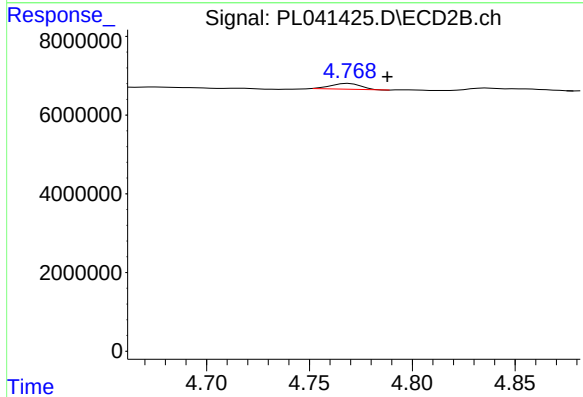


#3 gamma-BHC (Lindane)

R.T.: 4.769 min
Delta R.T.: -0.019 min
Response: 1497775
Conc: 0.42 ng/ml

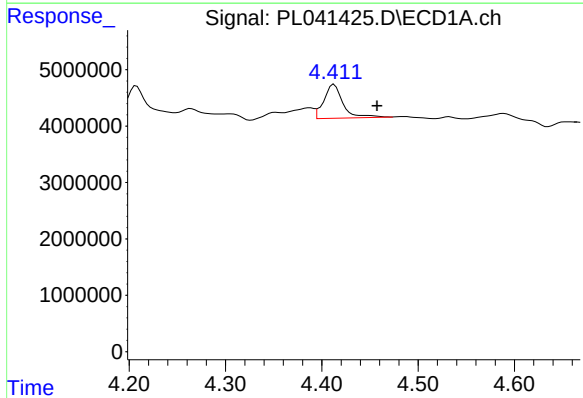


#6 beta-BHC

R.T.: 4.413 min
Delta R.T.: -0.045 min
Response: 8261611
Conc: 2.60 ng/ml

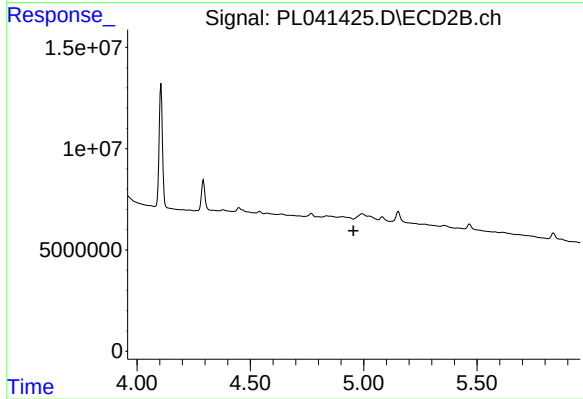

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.955 min
Response: 0
Conc: N.D.

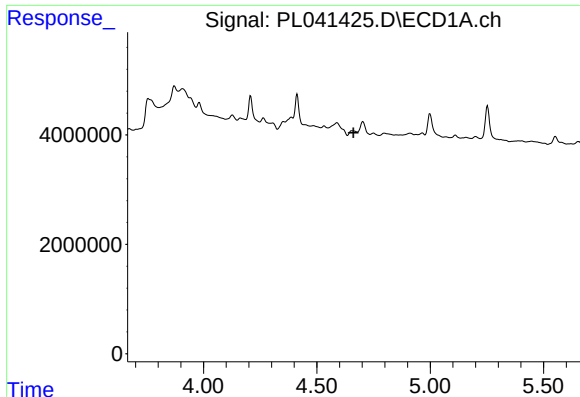

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.662 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

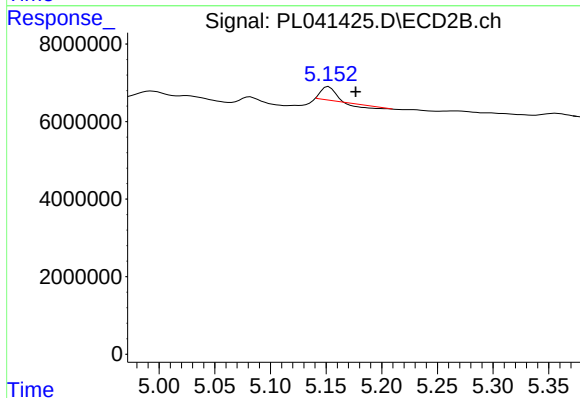


#7 delta-BHC

R.T.: 5.152 min
Delta R.T.: -0.024 min
Response: 1571308
Conc: 0.48 ng/ml

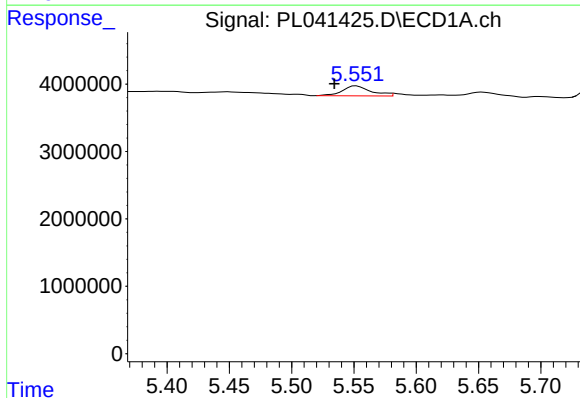


#9 Endosulfan I

R.T.: 5.552 min
Delta R.T.: 0.018 min
Response: 2366557
Conc: 0.40 ng/ml

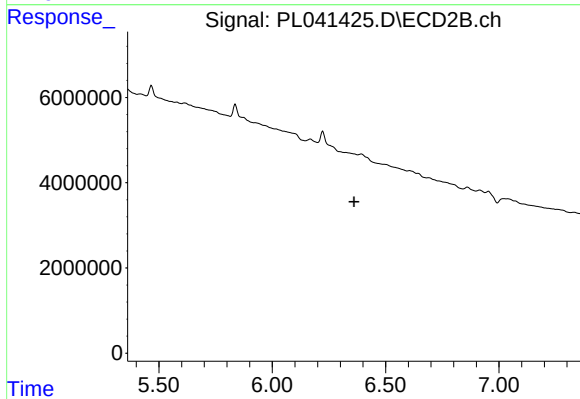

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 6.360 min
Response: 0
Conc: N.D.

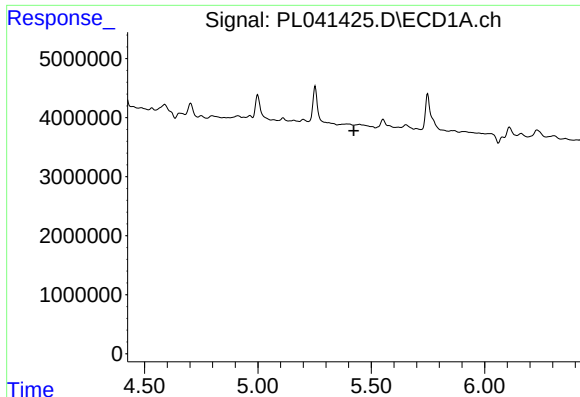

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

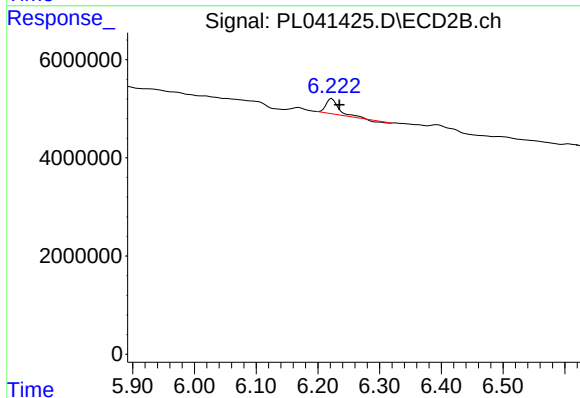


#10 gamma-Chlordane

R.T.: 6.223 min
Delta R.T.: -0.012 min
Response: 4390620
Conc: 1.57 ng/ml

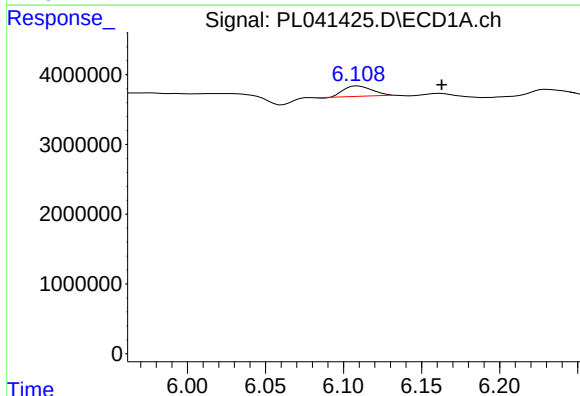


#16 4,4'-DDD

R.T.: 6.109 min
Delta R.T.: -0.054 min
Response: 1889596
Conc: 0.42 ng/ml

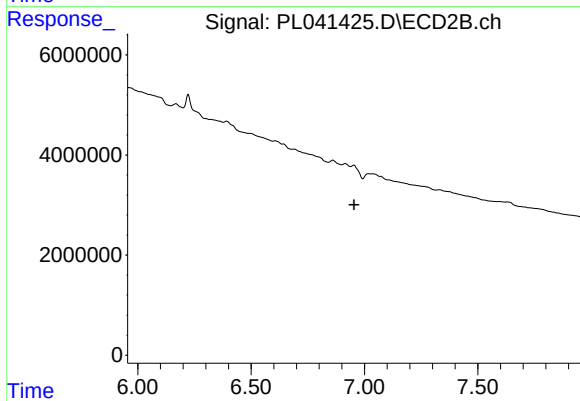

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 6.954 min
Response: 0
Conc: N.D.

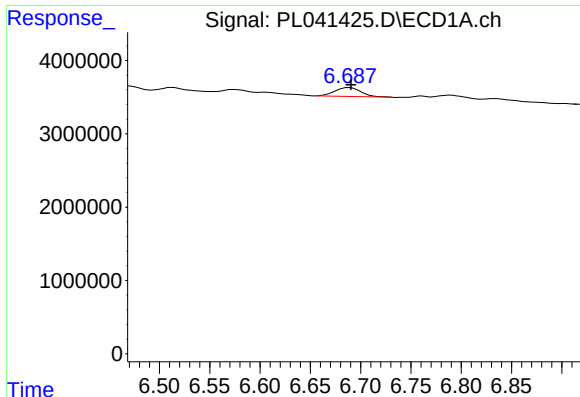

#19 Endosulfan Sulfate


R.T.: 6.689 min
Delta R.T.: -0.002 min
Response: 2112864
Conc: 0.42 ng/ml

Instrument :
ECD_L
ClientSampleId :

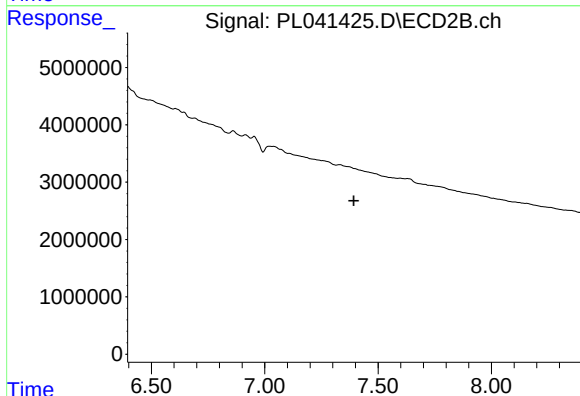


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.392 min
Response: 0
Conc: N.D.

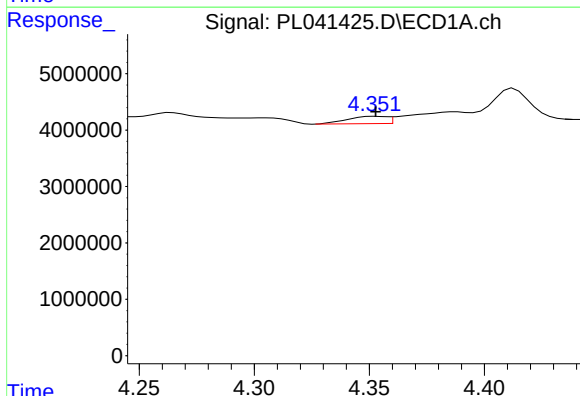


#23 Chlordane-1

R.T.: 4.353 min
Delta R.T.: 0.000 min
Response: 1553022
Conc: 6.09 ng/ml

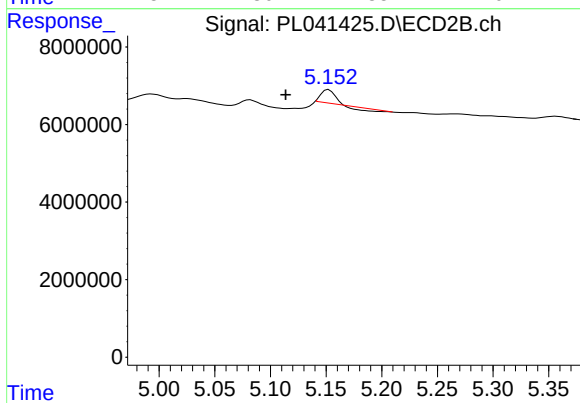

#23 Chlordane-1


R.T.: 5.152 min
Delta R.T.: 0.039 min
Response: 1571308
Conc: 12.72 ng/ml

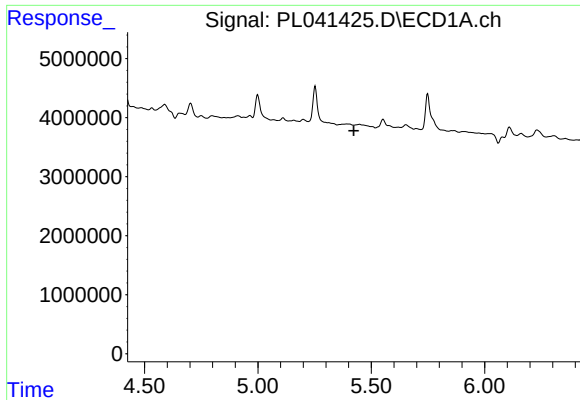

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.423 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

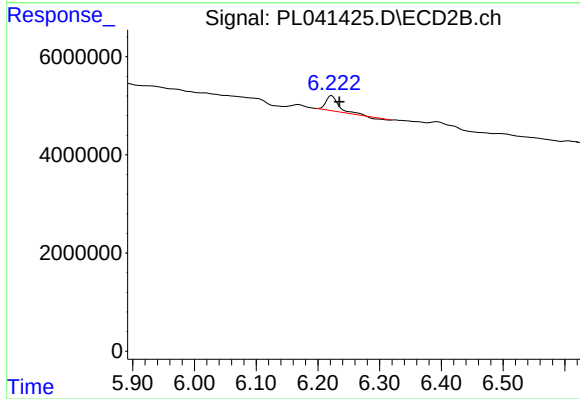


#25 Chlordane-3

R.T.: 6.223 min
Delta R.T.: -0.012 min
Response: 4390620
Conc: 10.89 ng/ml

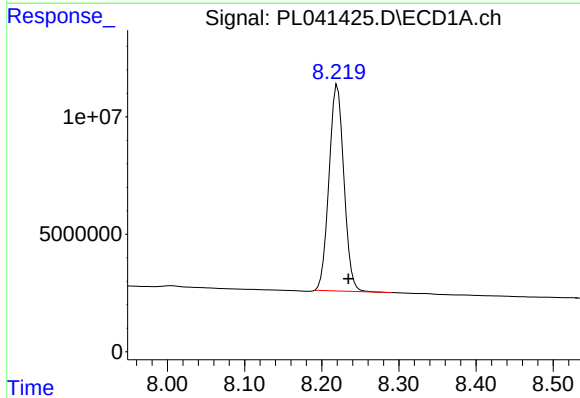

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.014 min
Response: 117936931
Conc: 22.68 ng/ml

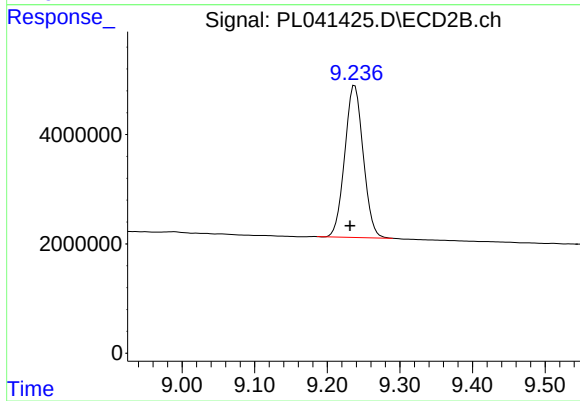

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.006 min
Response: 49136720
Conc: 19.00 ng/ml