

Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
Data File : PL041412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 21:35
Operator : AJ\SJ
Sample : J5676-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CB-1018-S-TCLP-GRID40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 23:40:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.475	4.105	108.7E6	54868530	19.837	19.678
28)	SA Decachlor...	8.220	9.238	114.9E6	47799839	22.105	18.485

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\Terastorage\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102618\
Data File : PL041412.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2018 21:35
Operator : AJ\SJ
Sample : J5676-01
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
CB-1018-S-TCLP-GRID40

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 26 23:40:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL101118.M
Quant Title : GC Extractables
QLast Update : Thu Oct 11 03:28:36 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

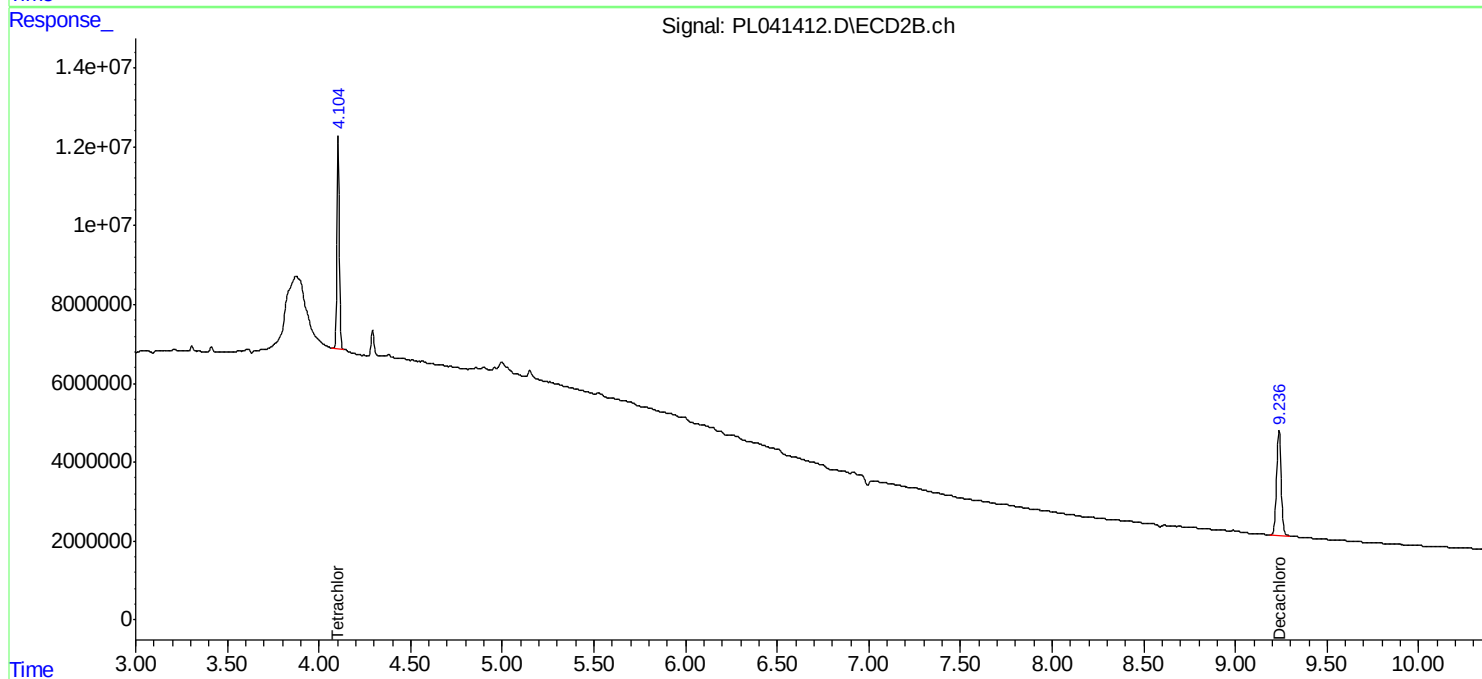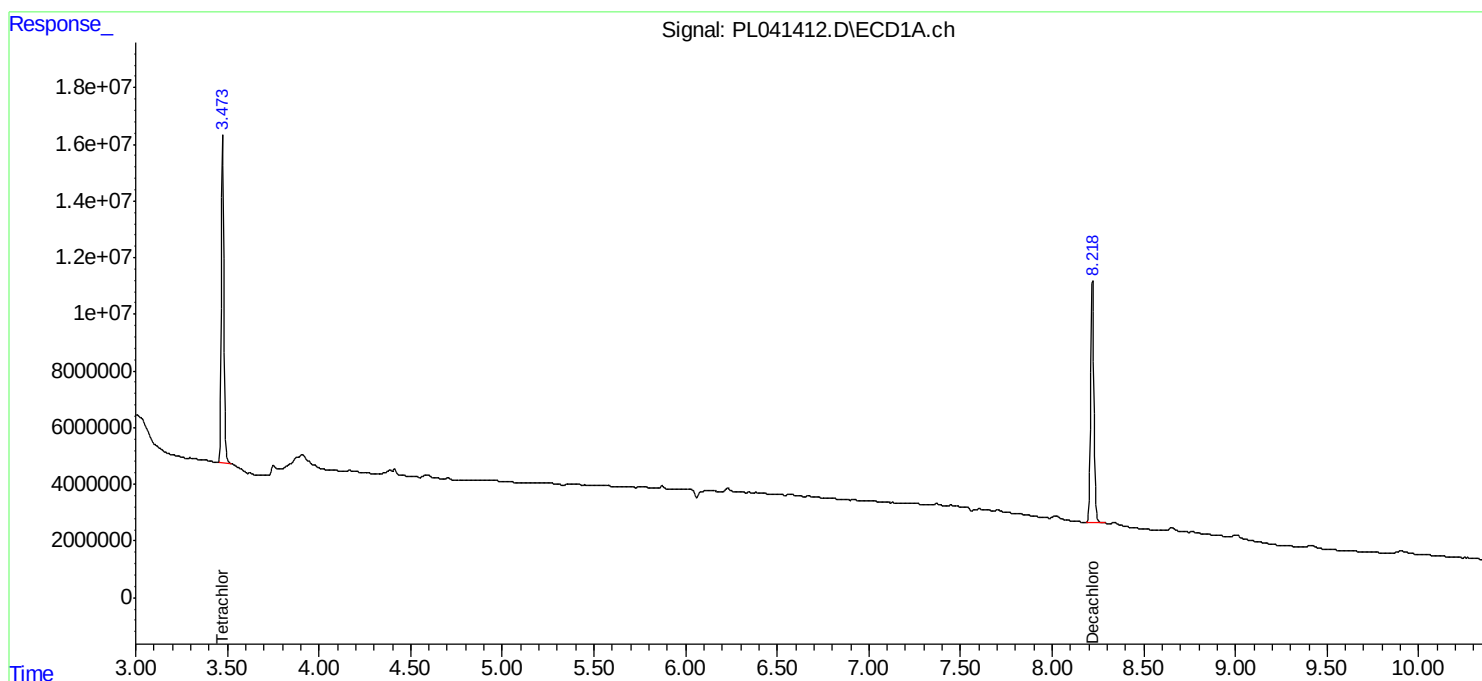


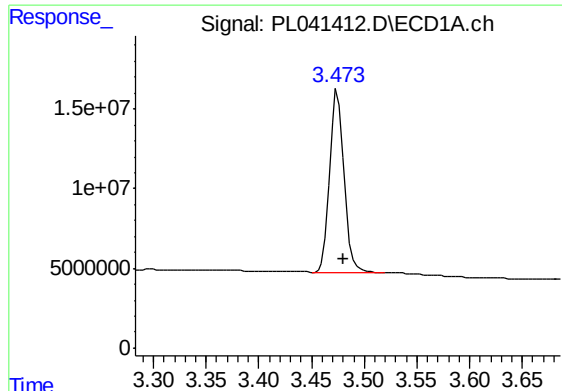

#1 Tetrachloro-m-xylene


R.T.: 3.475 min
Delta R.T.: -0.005 min
Response: 108719556
Conc: 19.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
CB-1018-S-TCLP-GRID40

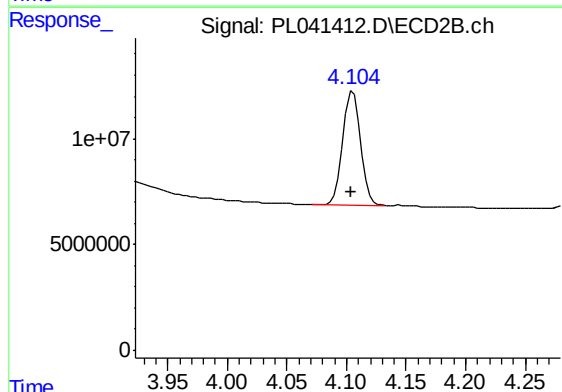


#1 Tetrachloro-m-xylene

R.T.: 4.105 min
Delta R.T.: 0.002 min
Response: 54868530
Conc: 19.68 ng/ml

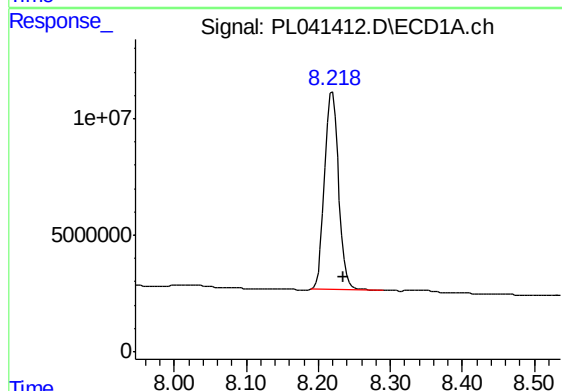

#28 Decachlorobiphenyl

R.T.: 8.220 min
Delta R.T.: -0.015 min
Response: 114936059
Conc: 22.11 ng/ml

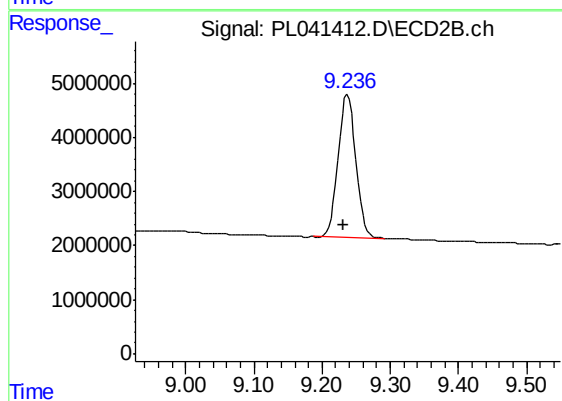

#28 Decachlorobiphenyl

R.T.: 9.238 min
Delta R.T.: 0.006 min
Response: 47799839
Conc: 18.49 ng/ml