

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
 Data File : PL062575.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 08:50
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:00:35 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

4) MA	Heptachlor	4.438f	0.000	105449	0	0.049	N.D.	#
5) MB	Aldrin	4.667	0.000	252480	0	0.132	N.D.	#
8) B	Heptachlo...	5.102	0.000	989051	0	0.542	N.D.	#
16) A	4,4'-DDD	6.053	0.000	1387271	0	0.981	N.D.	#
17) MA	4,4'-DDT	6.288	0.000	545364	0	0.409	N.D.	#
20) A	Methoxychlor	6.864f	0.000	10750178	0	12.481	N.D.	#
21) B	Endrin ke...	7.060	0.000	4273574	0	2.370	N.D.	#
23)	Chlordane-1	4.261	0.000	1833950	0	35.576	N.D.	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
Data File : PL062575.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 08:50
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:00:35 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

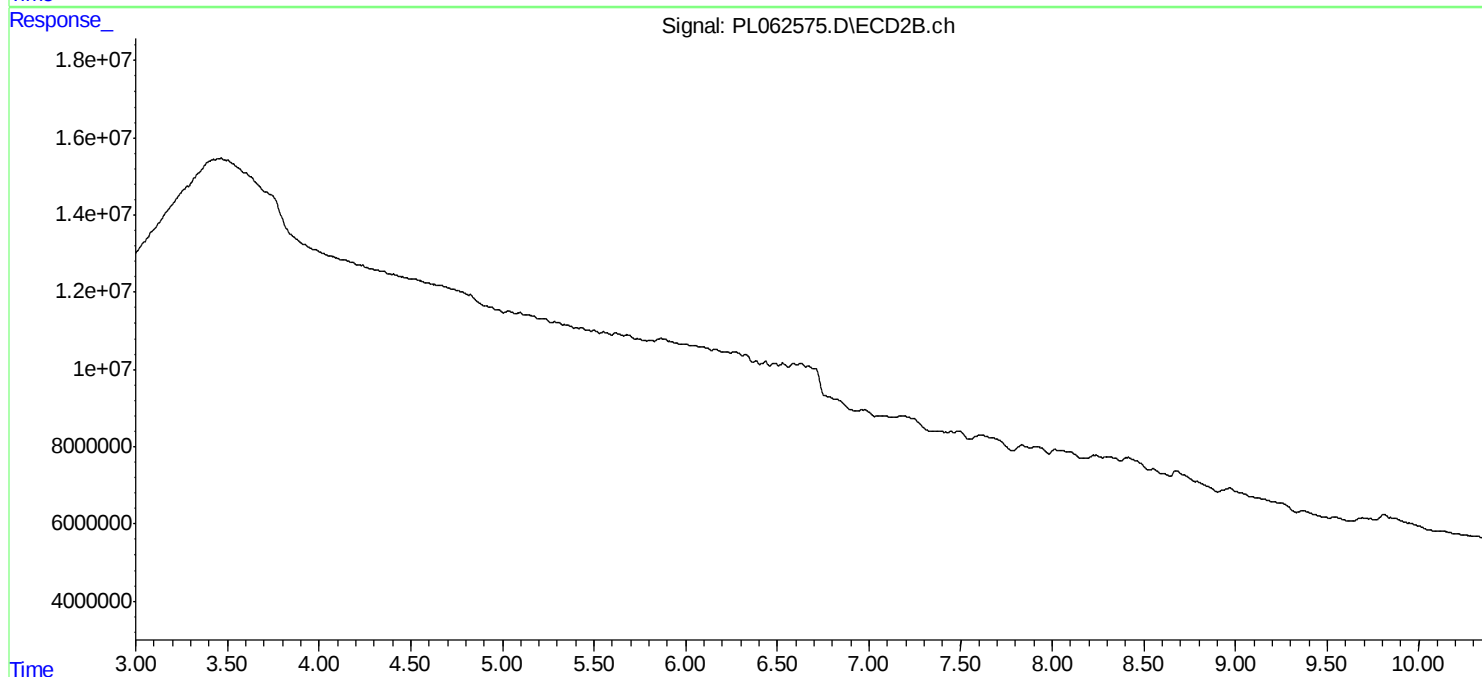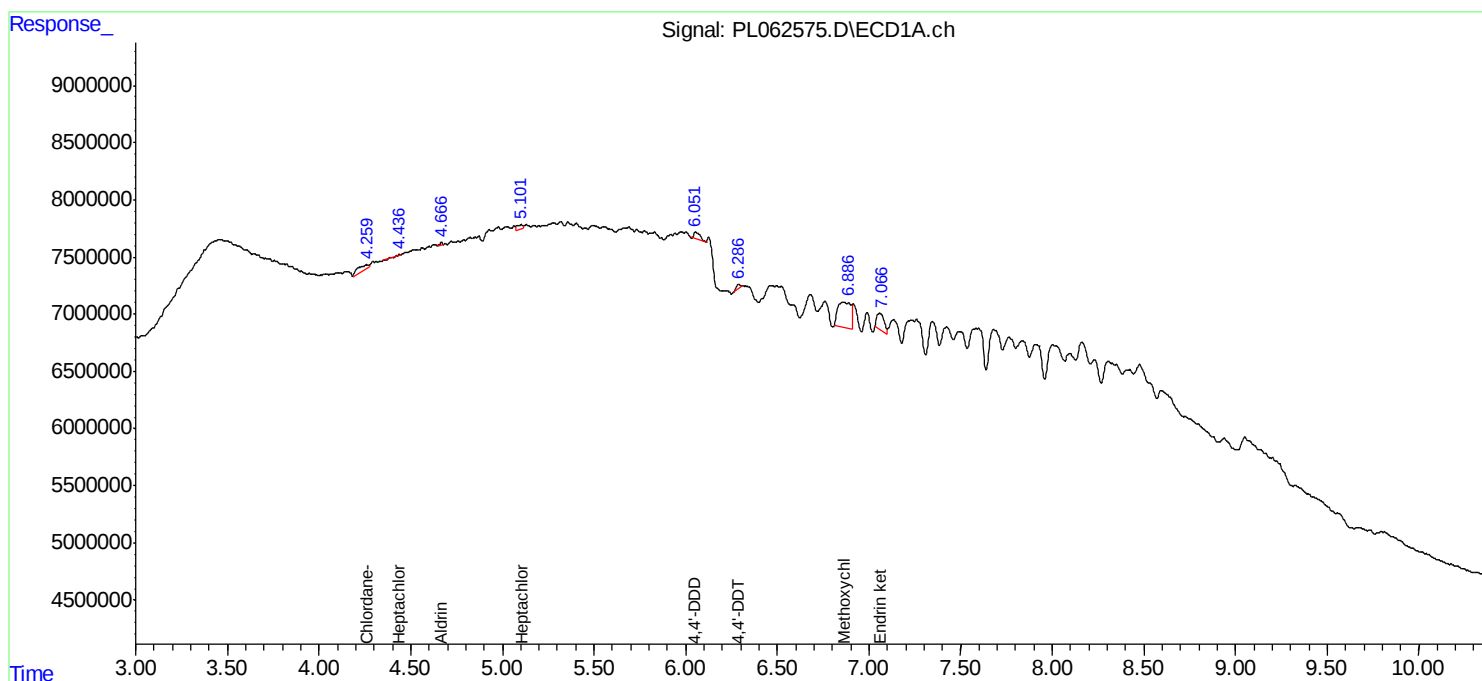


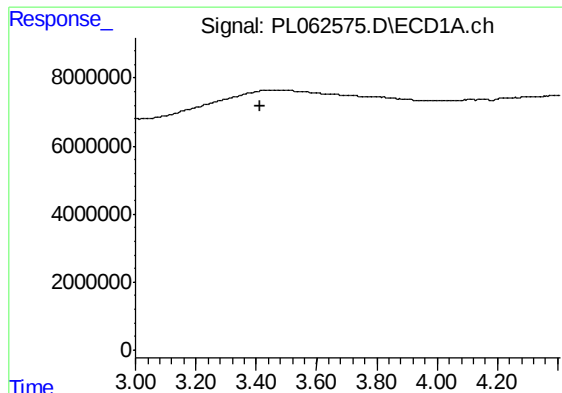

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 3.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
HEXANE

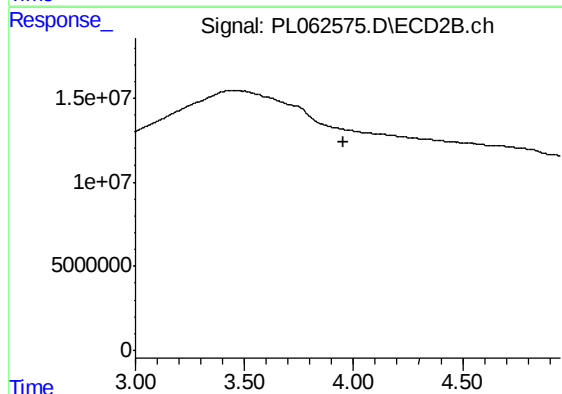


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.952 min
Response: 0
Conc: N.D.

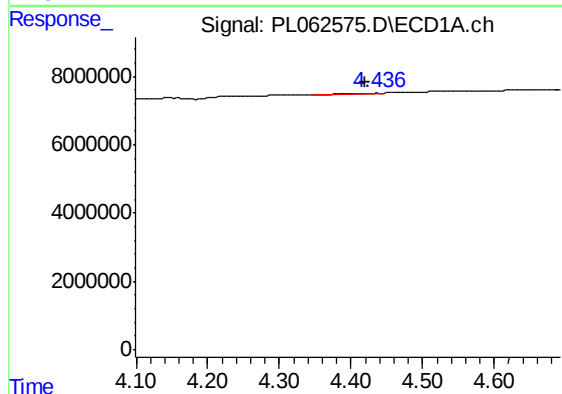


#4 Heptachlor

R.T.: 4.438 min
Delta R.T.: 0.017 min
Response: 105449
Conc: 0.05 ng/ml

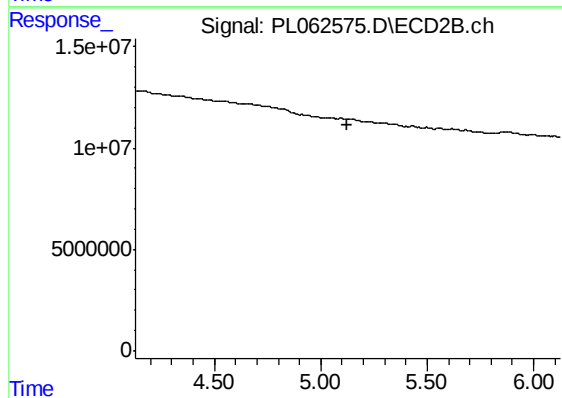

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 5.126 min
Response: 0
Conc: N.D.

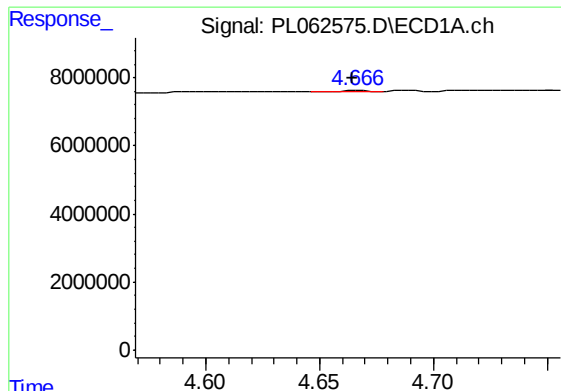

#5 Aldrin


R.T.: 4.667 min
Delta R.T.: 0.003 min
Response: 252480
Conc: 0.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

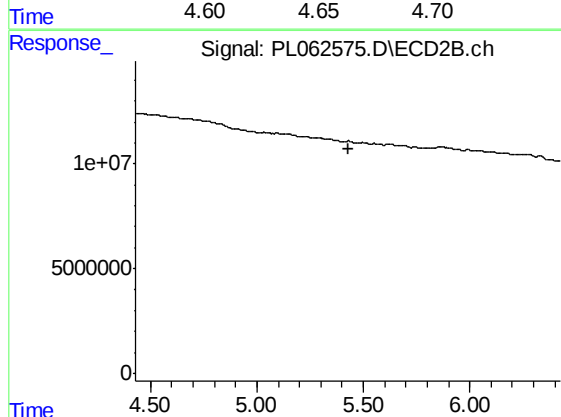


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 5.429 min
Response: 0
Conc: N.D.

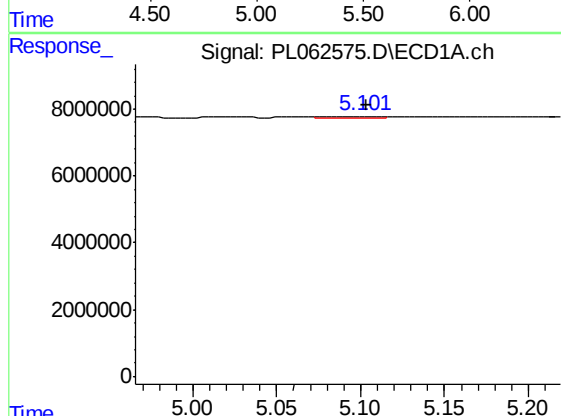


#8 Heptachlor epoxide

R.T.: 5.102 min
Delta R.T.: -0.001 min
Response: 989051
Conc: 0.54 ng/ml

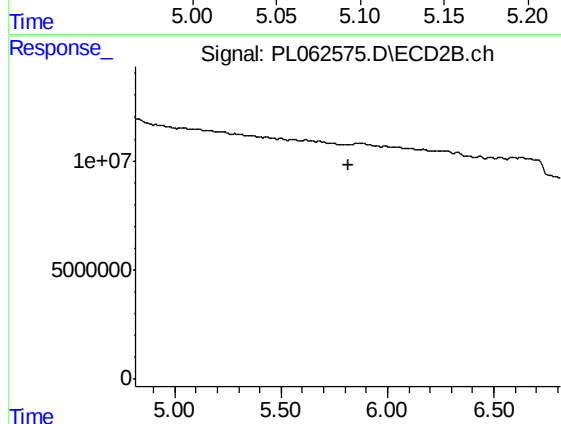

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.815 min
Response: 0
Conc: N.D.

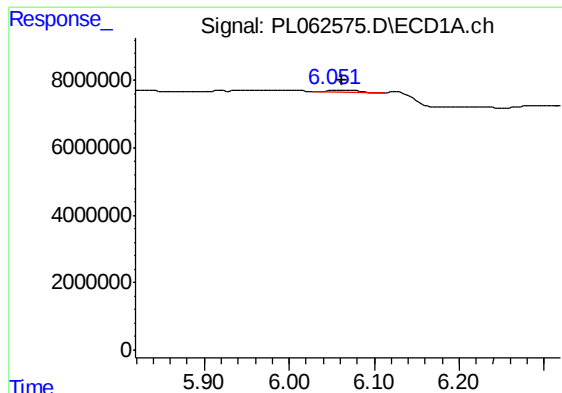

#16 4,4'-DDD


R.T.: 6.053 min
Delta R.T.: -0.009 min
Response: 1387271
Conc: 0.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

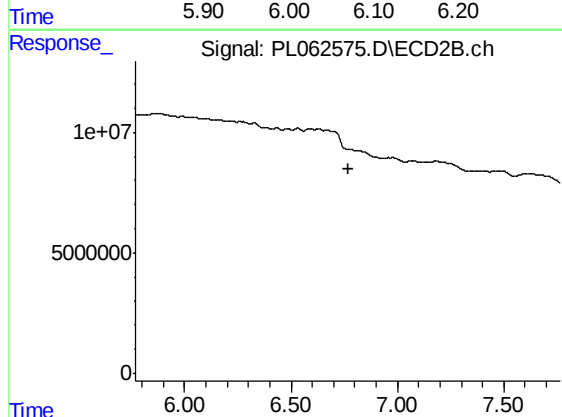


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.768 min
Response: 0
Conc: N.D.

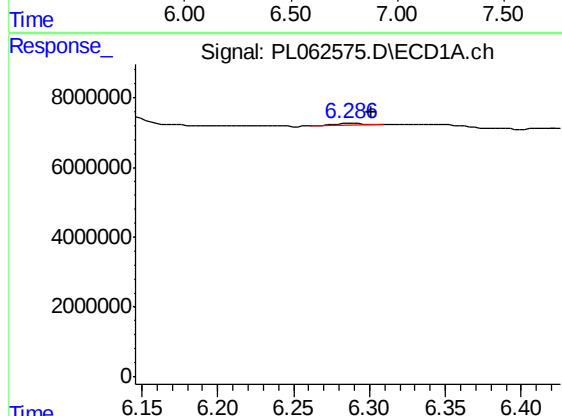


#17 4,4'-DDT

R.T.: 6.288 min
Delta R.T.: -0.013 min
Response: 545364
Conc: 0.41 ng/ml

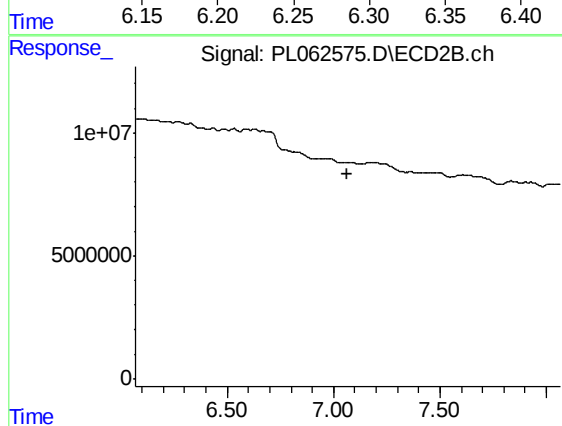

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T. : 7.066 min
Response: 0
Conc: N.D.

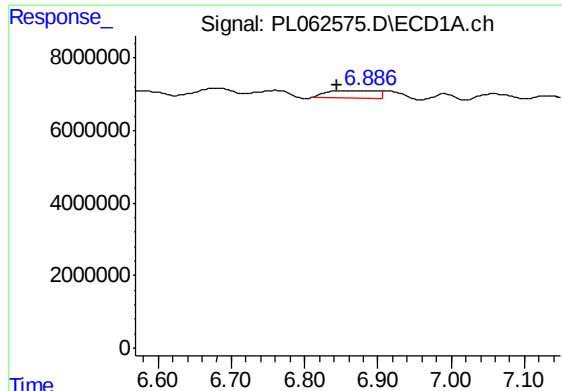

#20 Methoxychlor


R.T.: 6.864 min
Delta R.T.: 0.019 min
Response: 10750178
Conc: 12.48 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

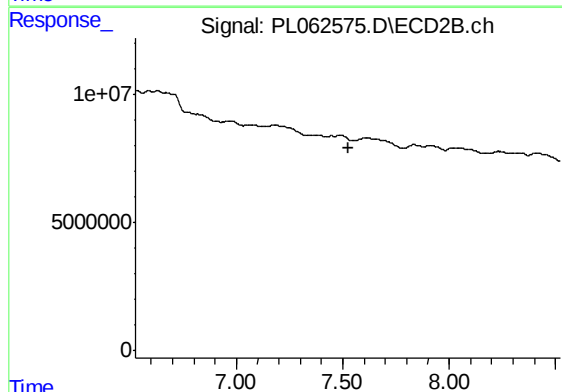


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.526 min
Response: 0
Conc: N.D.

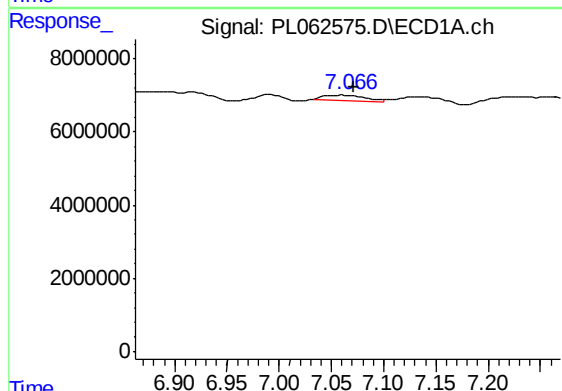


#21 Endrin ketone

R.T.: 7.060 min
Delta R.T.: -0.011 min
Response: 4273574
Conc: 2.37 ng/ml

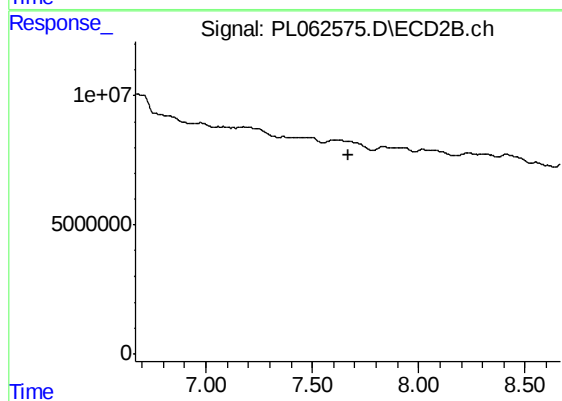

#21 Endrin ketone


R.T.: 0.000 min
Exp R.T. : 7.668 min
Response: 0
Conc: N.D.

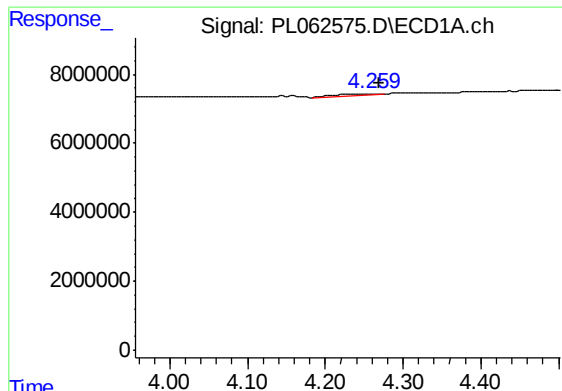

#23 Chlordane-1


R.T.: 4.261 min
Delta R.T.: -0.009 min
Response: 1833950
Conc: 35.58 ng/ml

Instrument :
ECD_L
ClientSampleId :
HEXANE

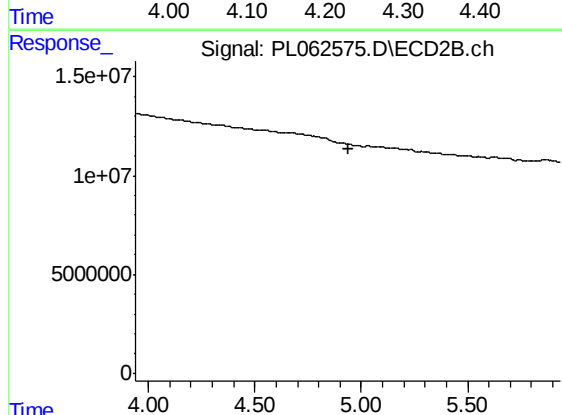


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

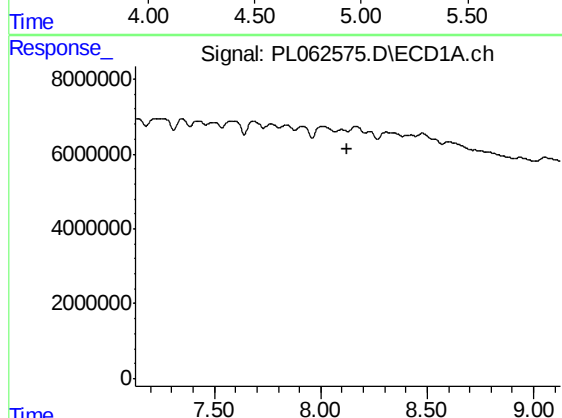

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.126 min
Response: 0
Conc: N.D.

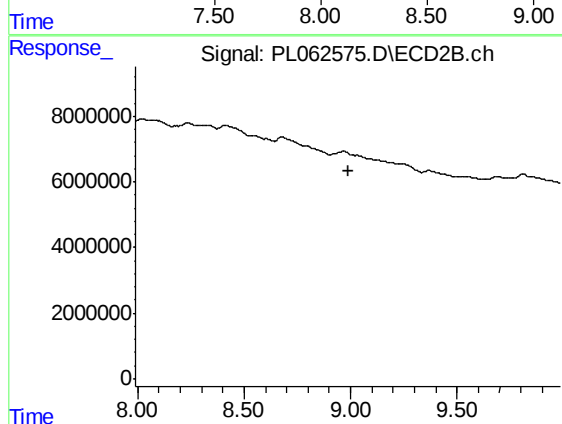

#28 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.989 min
Response: 0
Conc: N.D.