

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
 Data File : PL062580.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 10:59
 Operator : DD\AJ
 Sample : L4491-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:02:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.413	3.951	40281722	68346337	23.418	23.257
28)	SA Decachlor...	8.128	8.990	34959397	46780596	21.791	22.351
Target Compounds							
2)	A alpha-BHC	3.846	0.000	2423476	0	0.950	N.D. #
6)	B beta-BHC	0.000	4.781	0	1127300	N.D.	0.599 #
7)	B delta-BHC	0.000	5.003	0	2511853	N.D.	0.718 #
10)	B gamma-Chl...	0.000	6.068f	0	3042946	N.D.	0.904 #
15)	B Endosulfa...	0.000	6.868f	0	5823199	N.D.	2.037 #
19)	B Endosulfa...	0.000	7.197	0	2685328	N.D.	1.119 #
21)	B Endrin ke...	0.000	7.672	0	2862674	N.D.	1.208 #
25)	Chlordane-3	0.000	6.068f	0	3042946	N.D.	7.533 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
Data File : PL062580.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 10:59
Operator : DD\AJ
Sample : L4491-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:02:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

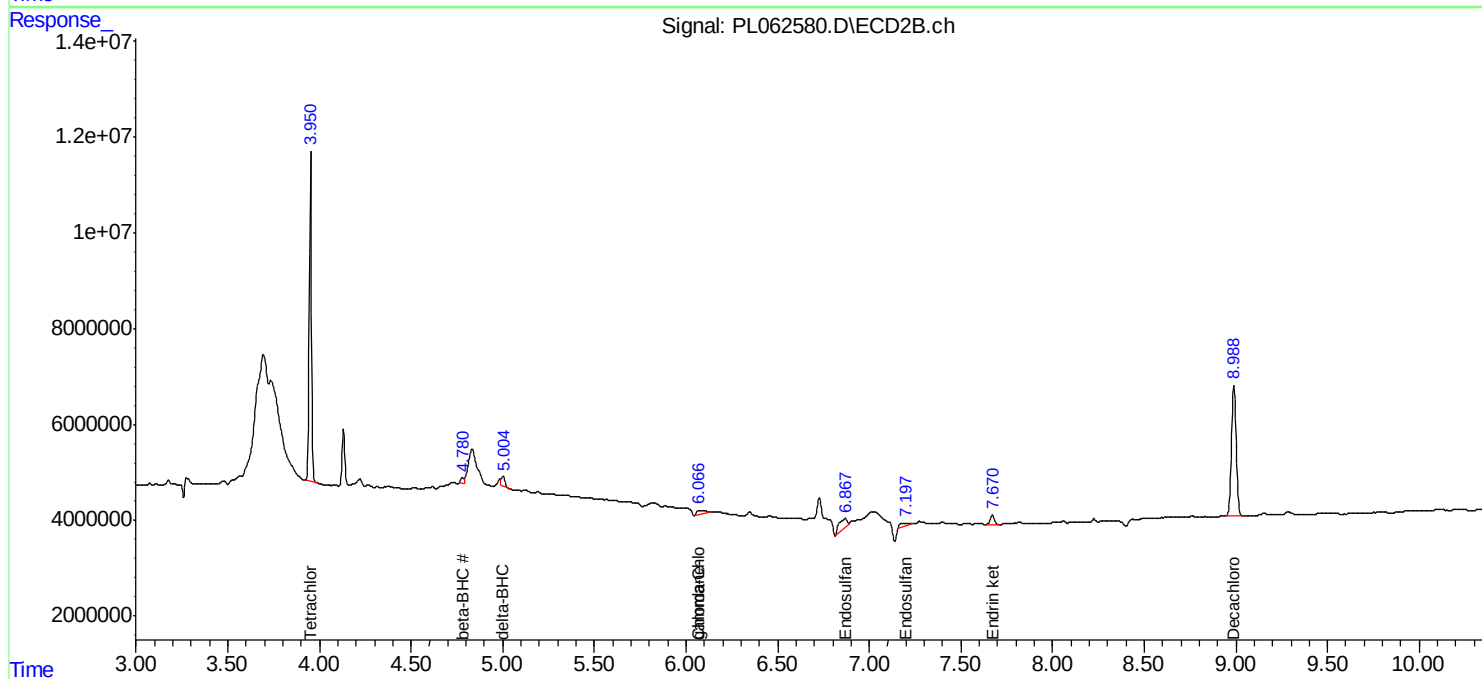


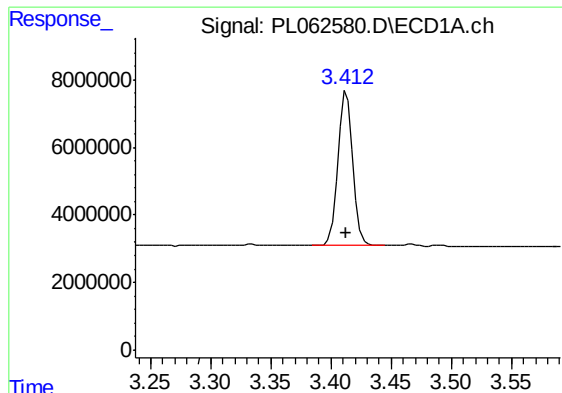

#1 Tetrachloro-m-xylene


R.T.: 3.413 min
Delta R.T.: 0.000 min
Response: 40281722
Conc: 23.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-2

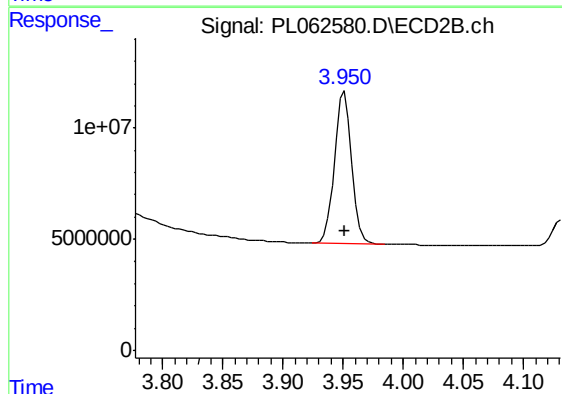


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 68346337
Conc: 23.26 ng/ml

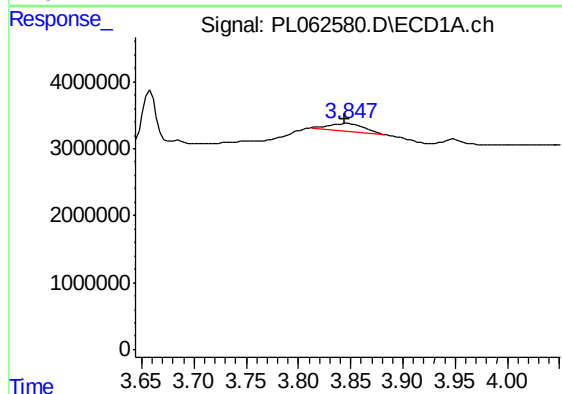


#2 alpha-BHC

R.T.: 3.846 min
Delta R.T.: 0.001 min
Response: 2423476
Conc: 0.95 ng/ml

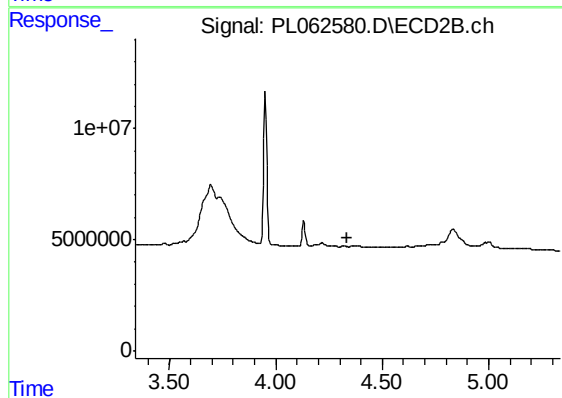

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.338 min
Response: 0
Conc: N.D.

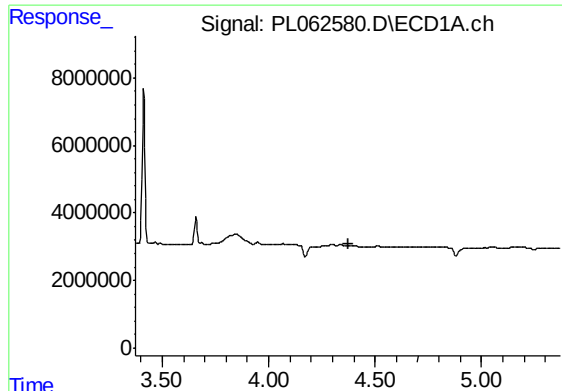

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.372 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-2

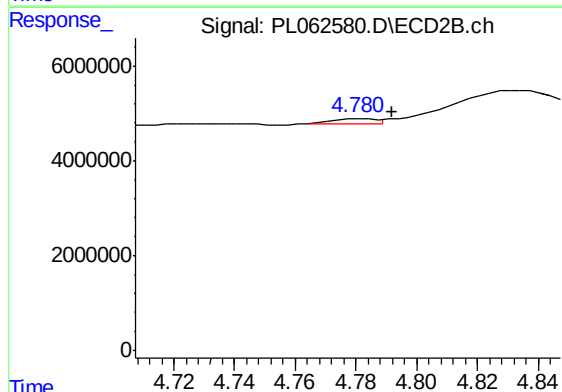


#6 beta-BHC

R.T.: 4.781 min
Delta R.T.: -0.011 min
Response: 1127300
Conc: 0.60 ng/ml

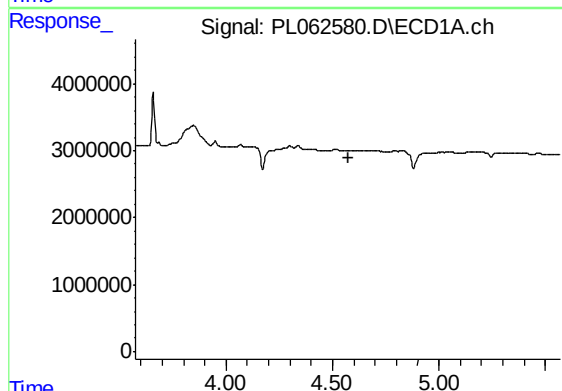


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.573 min
Response: 0
Conc: N.D.

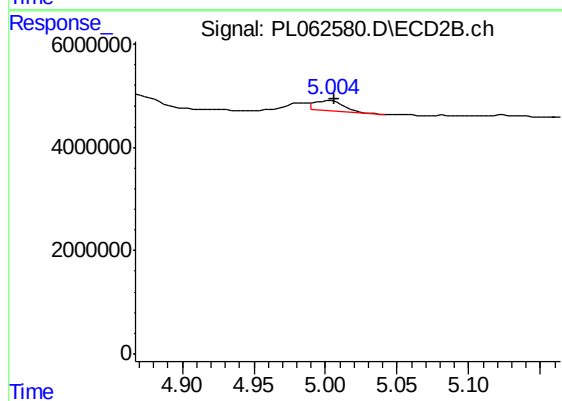

#7 delta-BHC


R.T.: 5.003 min
Delta R.T.: -0.003 min
Response: 2511853
Conc: 0.72 ng/ml

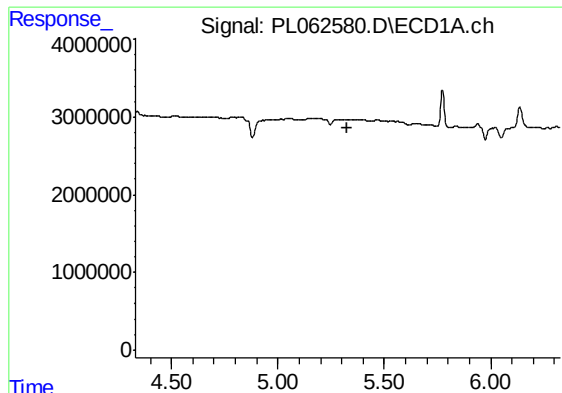

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-2

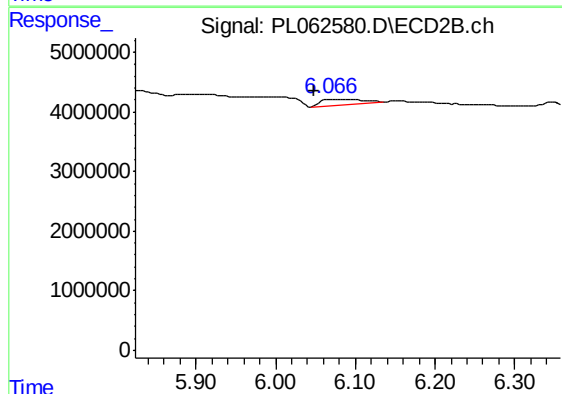


#10 gamma-Chlordane

R.T.: 6.068 min
Delta R.T.: 0.020 min
Response: 3042946
Conc: 0.90 ng/ml

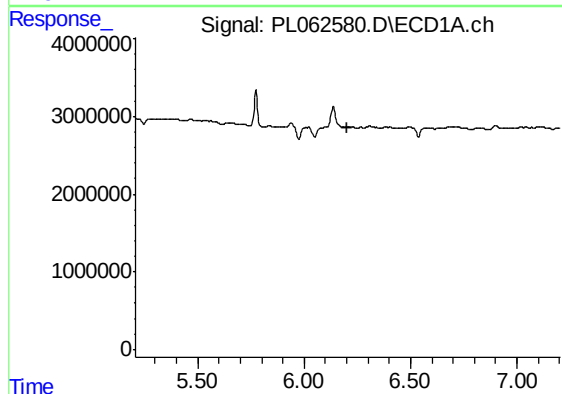


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

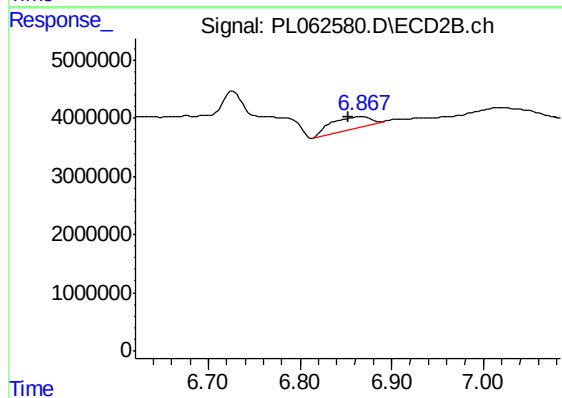

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.015 min
Response: 5823199
Conc: 2.04 ng/ml

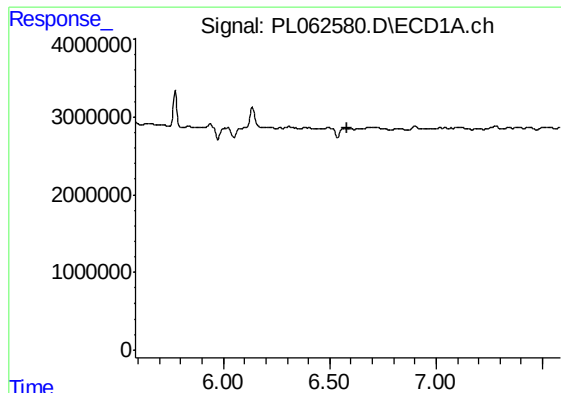

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 6.585 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-2

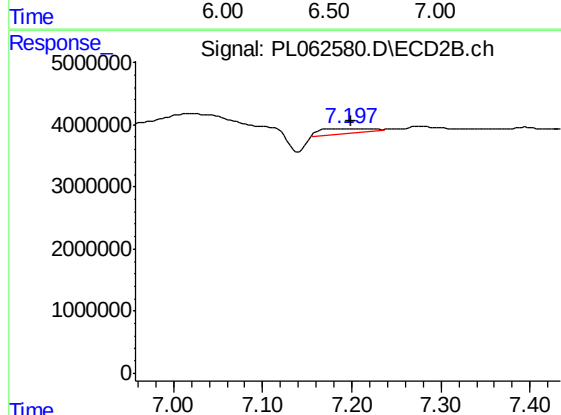


#19 Endosulfan Sulfate

R.T.: 7.197 min
Delta R.T.: -0.002 min
Response: 2685328
Conc: 1.12 ng/ml

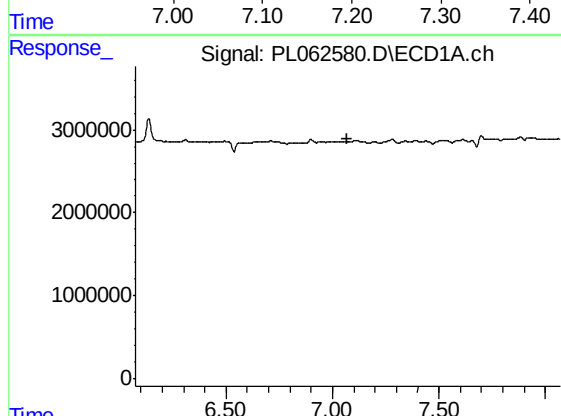


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.071 min
Response: 0
Conc: N.D.

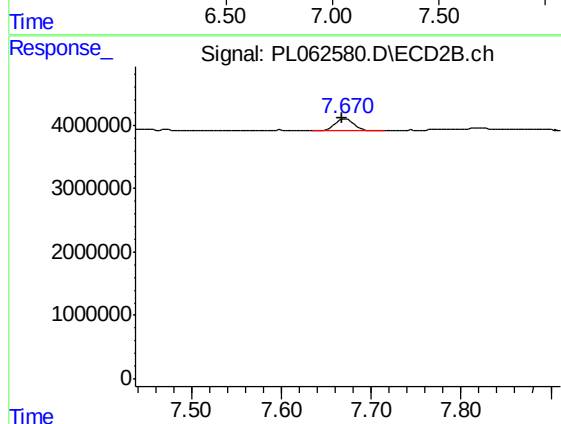

#21 Endrin ketone


R.T.: 7.672 min
Delta R.T.: 0.004 min
Response: 2862674
Conc: 1.21 ng/ml

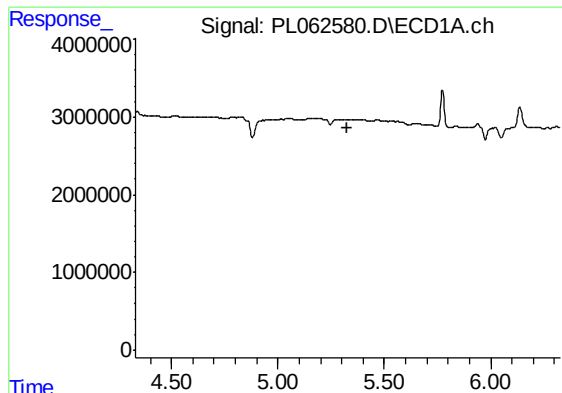

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.328 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-2

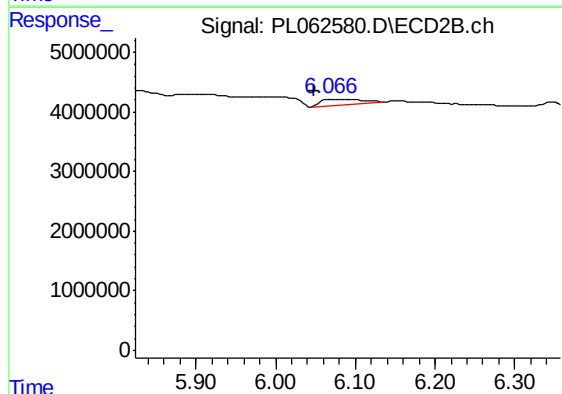


#25 Chlordane-3

R.T.: 6.068 min
Delta R.T.: 0.020 min
Response: 3042946
Conc: 7.53 ng/ml

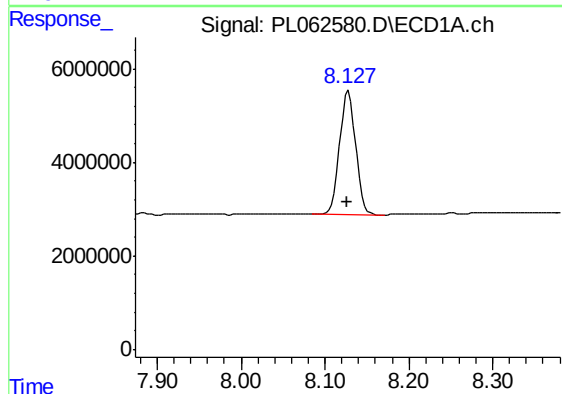

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.002 min
Response: 34959397
Conc: 21.79 ng/ml

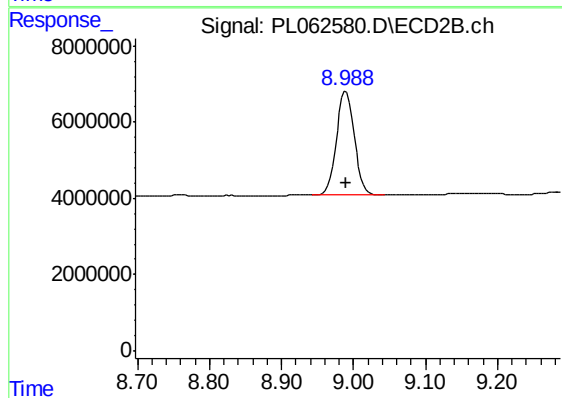

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 46780596
Conc: 22.35 ng/ml