

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
 Data File : PL062582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 11:28
 Operator : DD\AJ
 Sample : PB132576BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB132576BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:02:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.412	3.952	33128371	58290794	19.260	19.835
28) SA Decachlor...	8.128	8.990	30682939	41564741	19.126	19.859
Target Compounds						
15) B Endosulfa...	0.000	6.868f	0	2007114	N.D.	0.702 #
23) Chlordane-1	4.299f	0.000	268466	0	5.208	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
Data File : PL062582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 11:28
Operator : DD\AJ
Sample : PB132576BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB132576BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:02:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

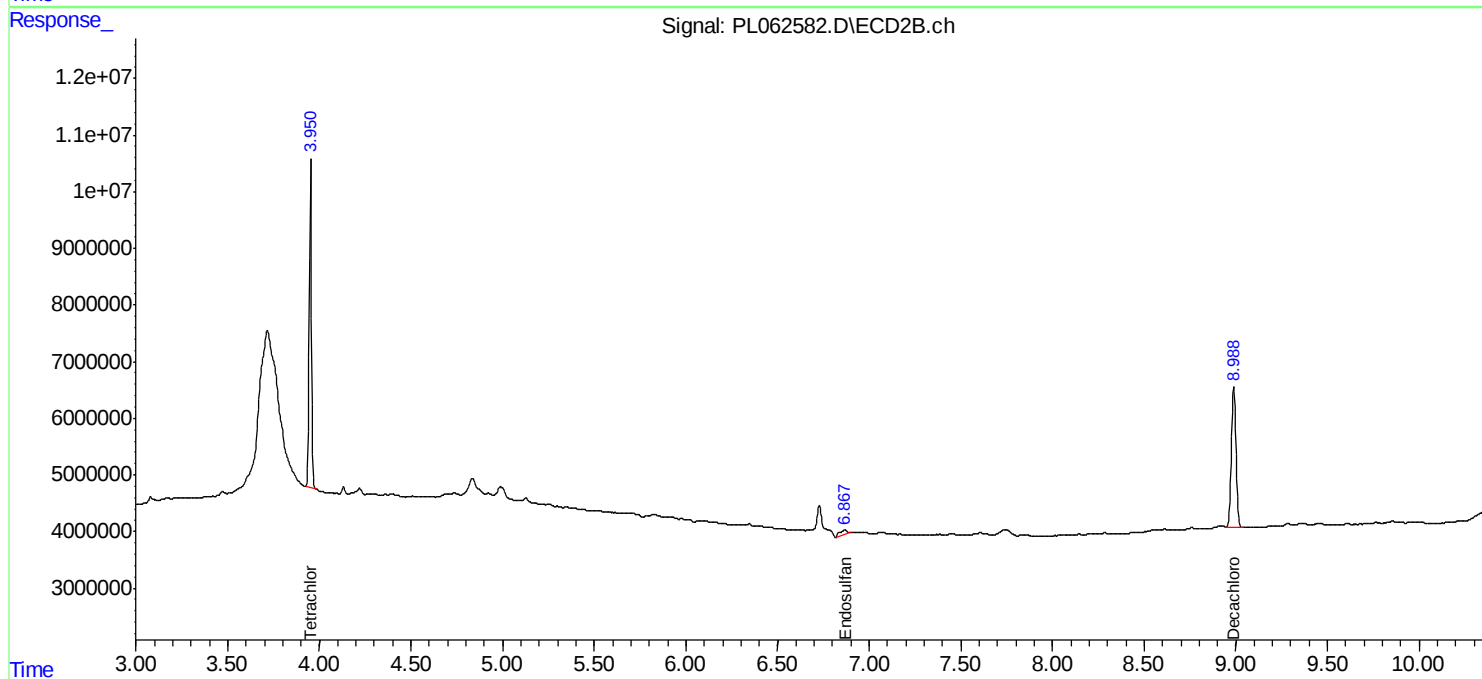


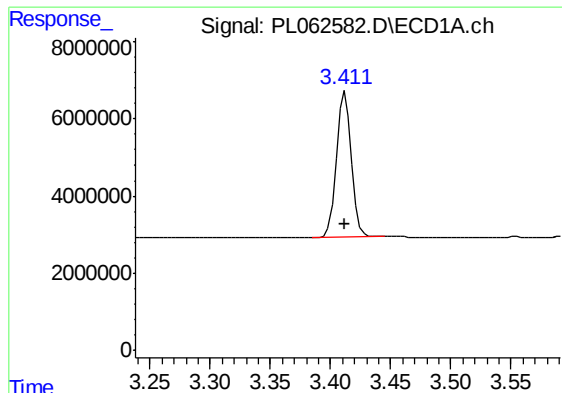

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 33128371
Conc: 19.26 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132576BL

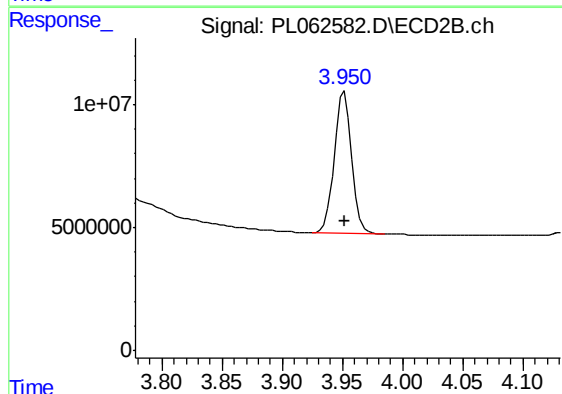


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 58290794
Conc: 19.84 ng/ml

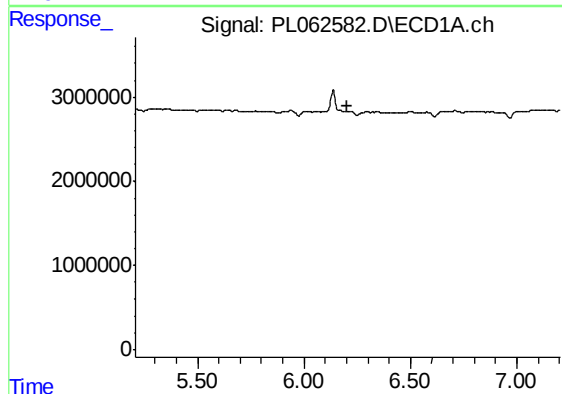


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

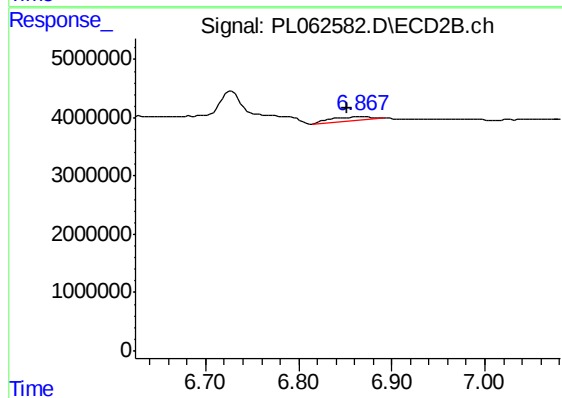

#15 Endosulfan II


R.T.: 6.868 min
Delta R.T.: 0.015 min
Response: 2007114
Conc: 0.70 ng/ml

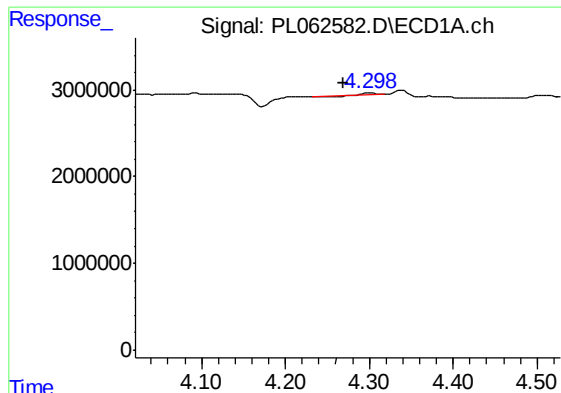

#23 Chlordane-1


R.T.: 4.299 min
Delta R.T.: 0.030 min
Response: 268466
Conc: 5.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB132576BL

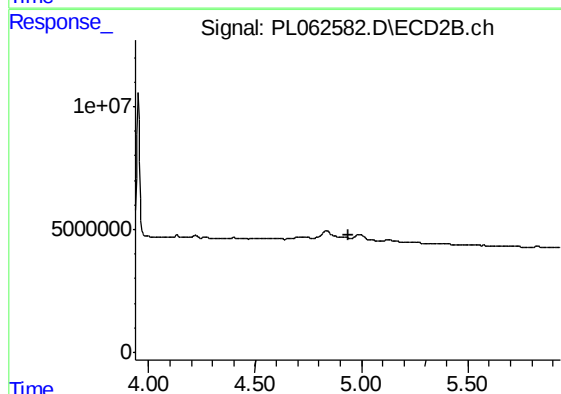


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

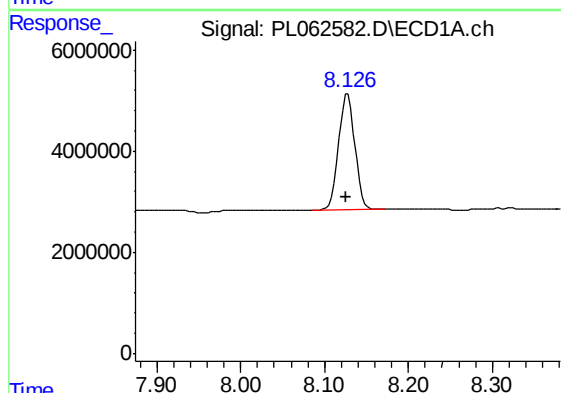

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 30682939
Conc: 19.13 ng/ml

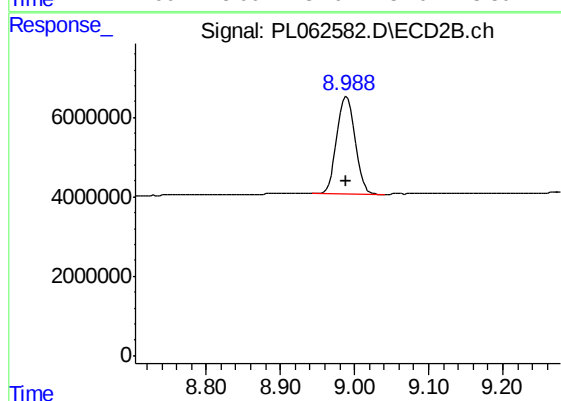

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 41564741
Conc: 19.86 ng/ml