

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
 Data File : PL062590.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 13:26
 Operator : DD\AJ
 Sample : L4501-001
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:05:36 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	38348988	65656326	22.295	22.342
28)	SA Decachlor...	8.128	8.989	31645449	43104247	19.726	20.595
Target Compounds							
2)	A alpha-BHC	0.000	4.345	0	1793165	N.D.	0.404 #
15)	B Endosulfa...	0.000	6.866	0	3716468	N.D.	1.300 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
Data File : PL062590.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 13:26
Operator : DD\AJ
Sample : L4501-001
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
COMP-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:05:36 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

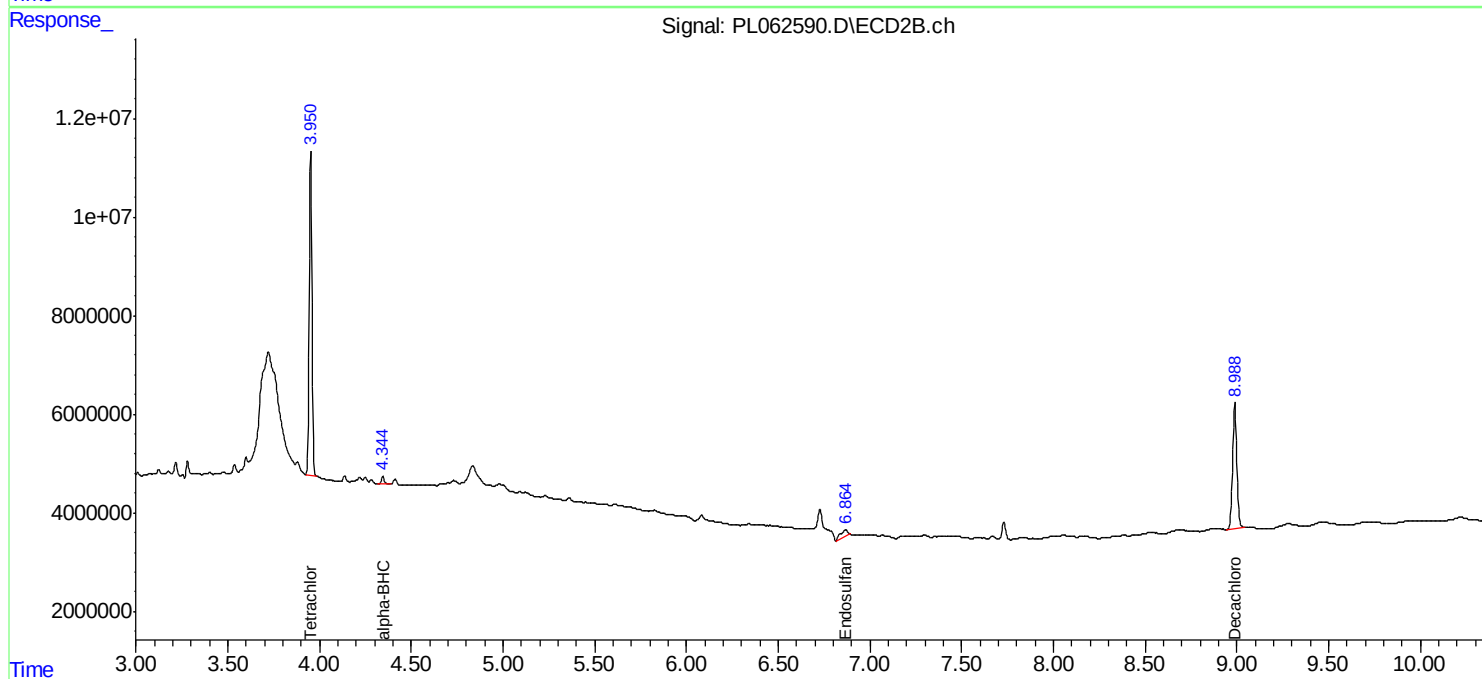


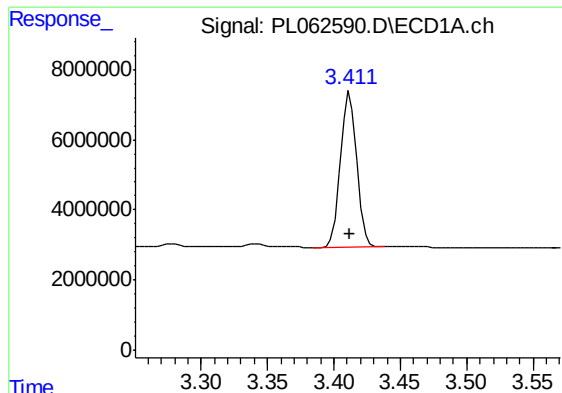

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 38348988
Conc: 22.29 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

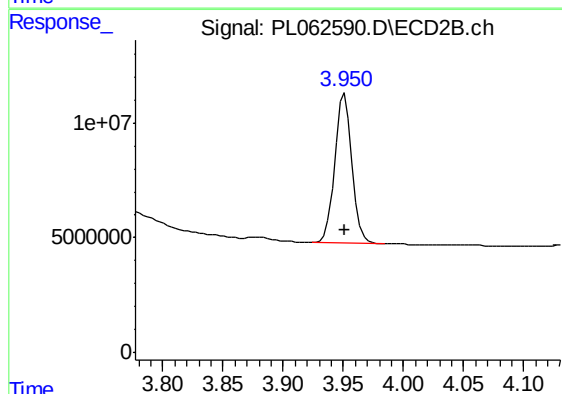


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 65656326
Conc: 22.34 ng/ml

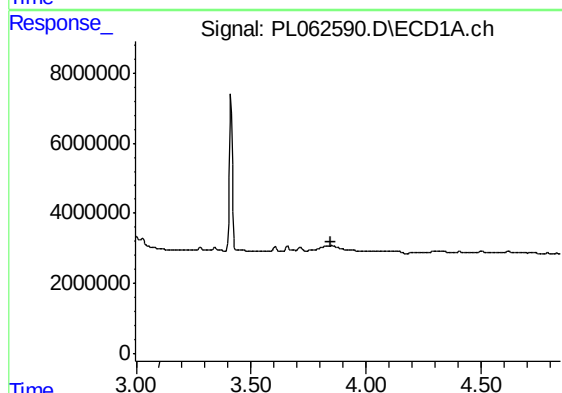


#2 alpha-BHC

R.T.: 0.000 min
Exp R.T. : 3.844 min
Response: 0
Conc: N.D.

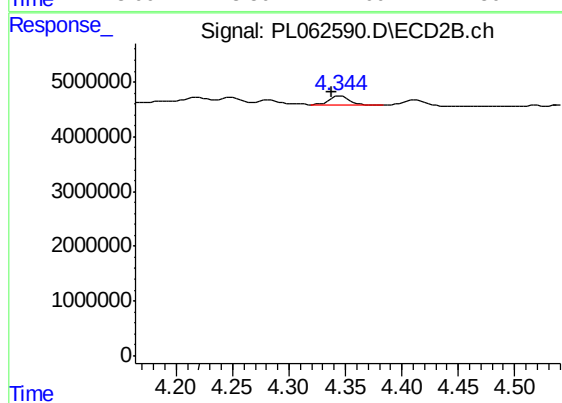

#2 alpha-BHC


R.T.: 4.345 min
Delta R.T.: 0.007 min
Response: 1793165
Conc: 0.40 ng/ml

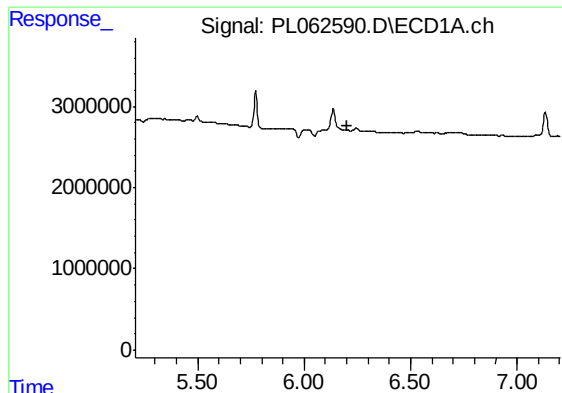

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.205 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
COMP-1

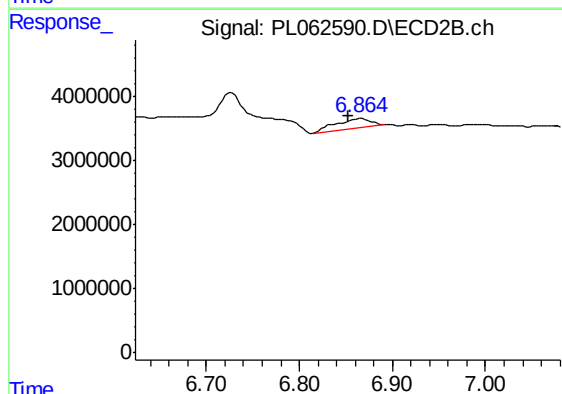


#15 Endosulfan II

R.T.: 6.866 min
Delta R.T.: 0.014 min
Response: 3716468
Conc: 1.30 ng/ml

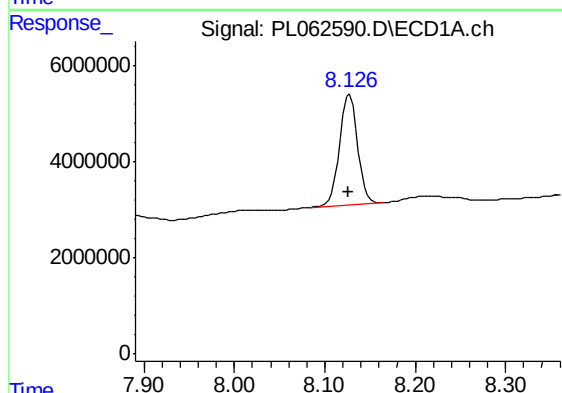

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 31645449
Conc: 19.73 ng/ml

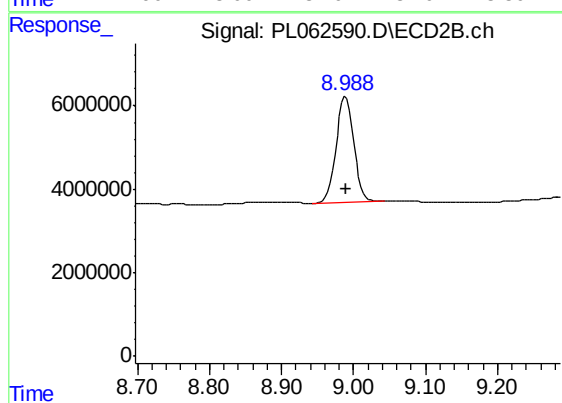

#28 Decachlorobiphenyl

R.T.: 8.989 min
Delta R.T.: 0.000 min
Response: 43104247
Conc: 20.59 ng/ml