

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
 Data File : PL062600.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 15:56
 Operator : DD\AJ
 Sample : L4510-18
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:09:30 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	24636458	42162501	14.323	14.347
28)	SA Decachlor...	8.128	8.991	20646811	29535093	12.870	14.112
Target Compounds							
9)	A Endosulfan I	5.452	0.000	1068125	0	0.639	N.D. #
12)	B 4,4'-DDE	5.552	6.274	520360	2437078	0.315	0.756 #
15)	B Endosulfa...	0.000	6.866	0	2964245	N.D.	1.037 #
17)	MA 4,4'-DDT	6.299	7.040f	763355	1050242	0.572	0.468
20)	A Methoxychlor	6.830f	0.000	656893	0	0.763	N.D. #
23)	Chlordane-1	4.275	0.000	759333	0	14.730	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
Data File : PL062600.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 15:56
Operator : DD\AJ
Sample : L4510-18
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
COMP-3

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:09:30 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

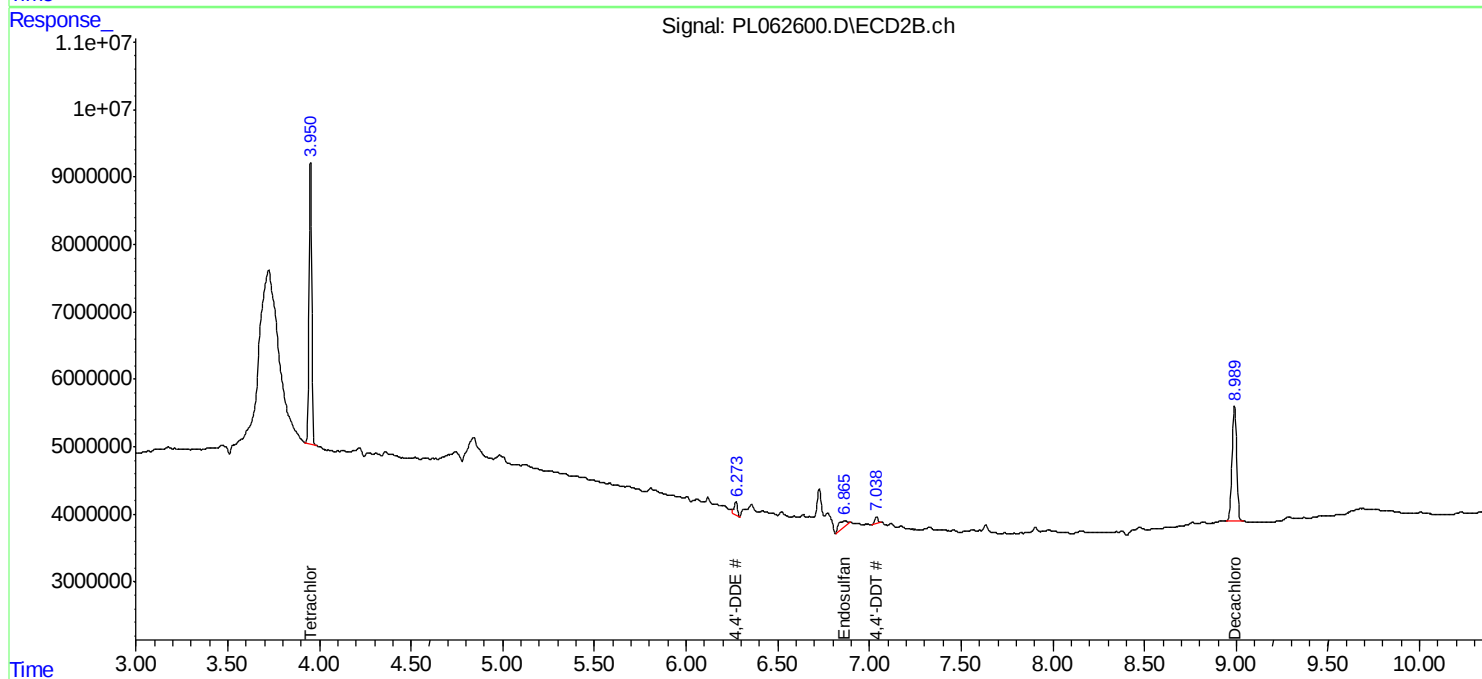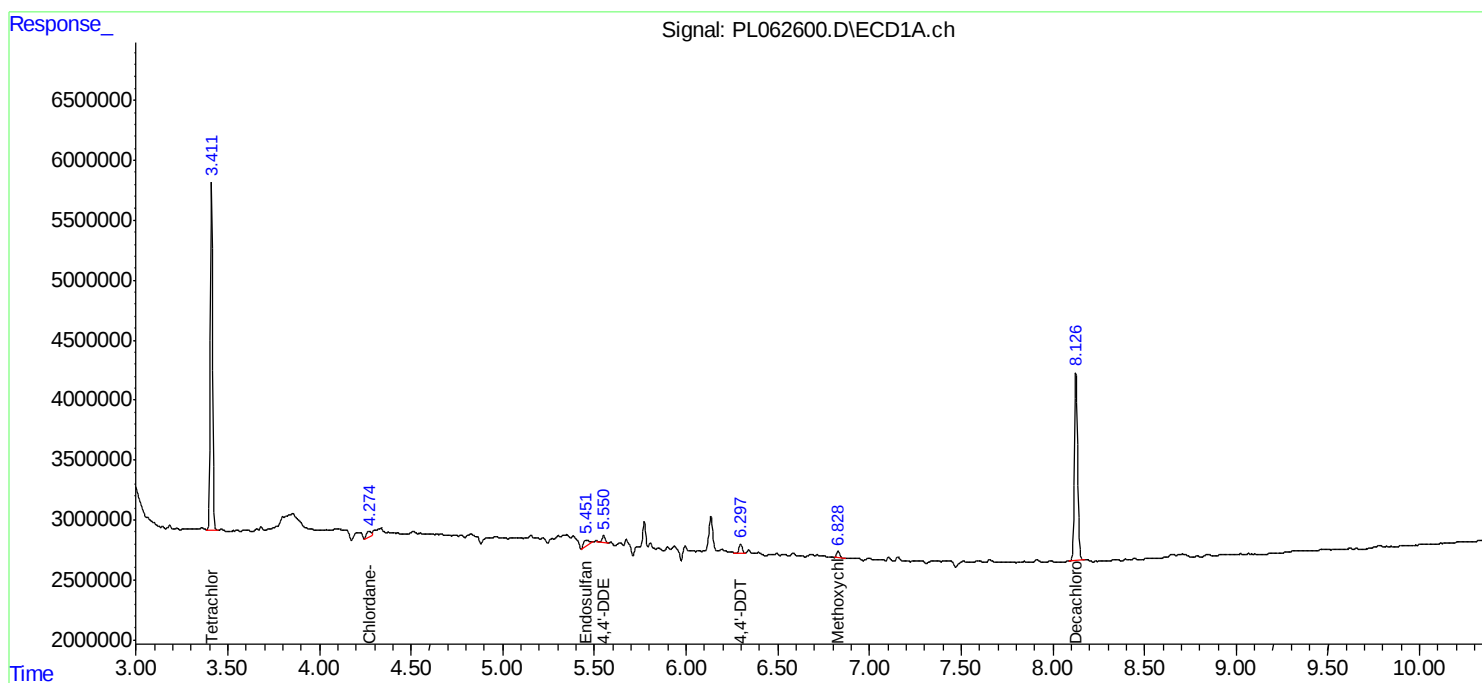


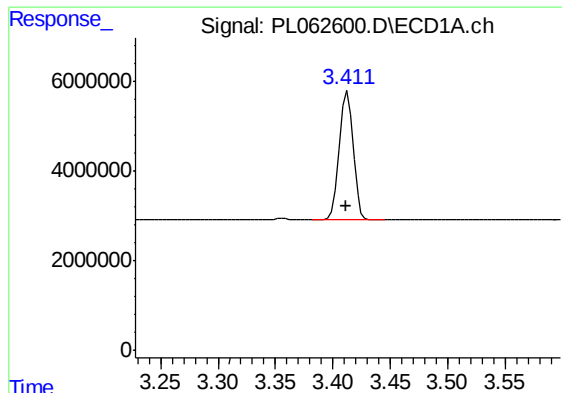

#1 Tetrachloro-m-xylene


R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 24636458
Conc: 14.32 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

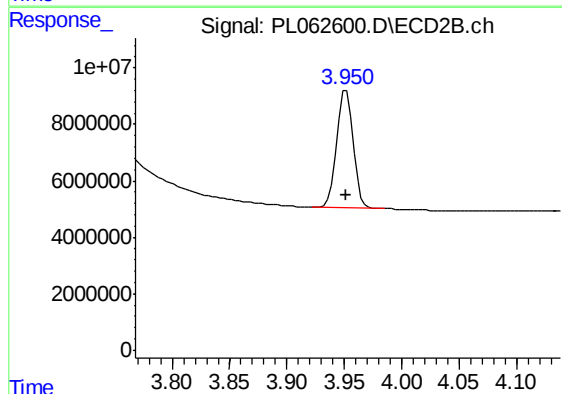


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 42162501
Conc: 14.35 ng/ml

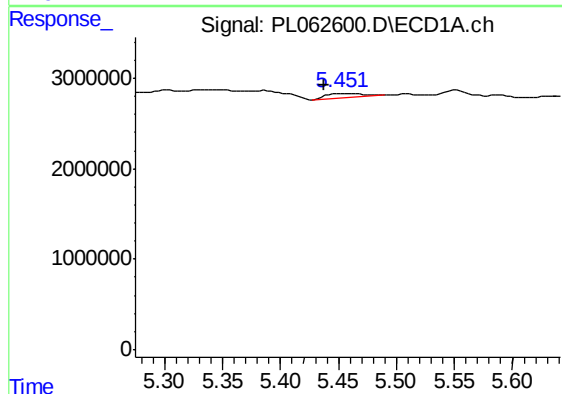


#9 Endosulfan I

R.T.: 5.452 min
Delta R.T.: 0.014 min
Response: 1068125
Conc: 0.64 ng/ml

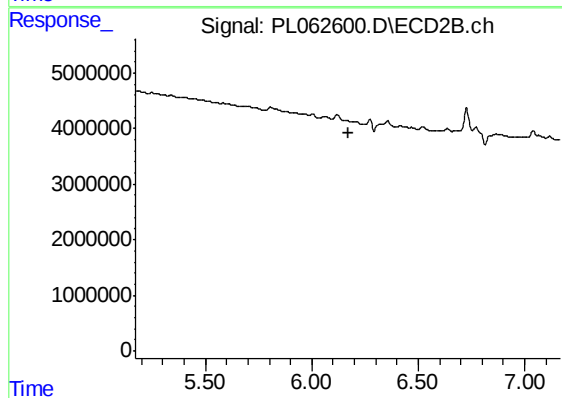

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.170 min
Response: 0
Conc: N.D.

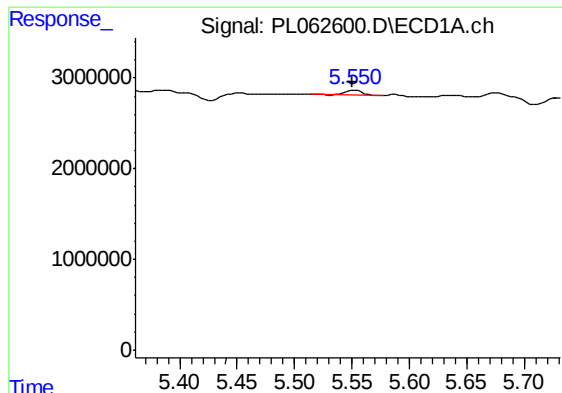

#12 4,4'-DDE


R.T.: 5.552 min
Delta R.T.: 0.001 min
Response: 520360
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

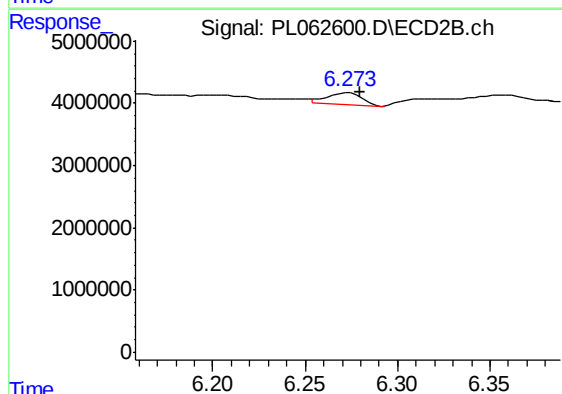


#12 4,4'-DDE

R.T.: 6.274 min
Delta R.T.: -0.005 min
Response: 2437078
Conc: 0.76 ng/ml

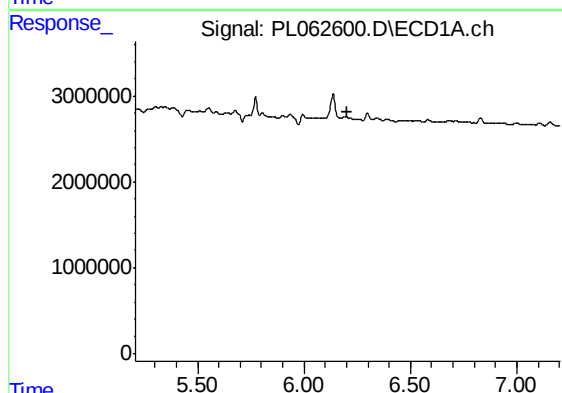


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.205 min
Response: 0
Conc: N.D.

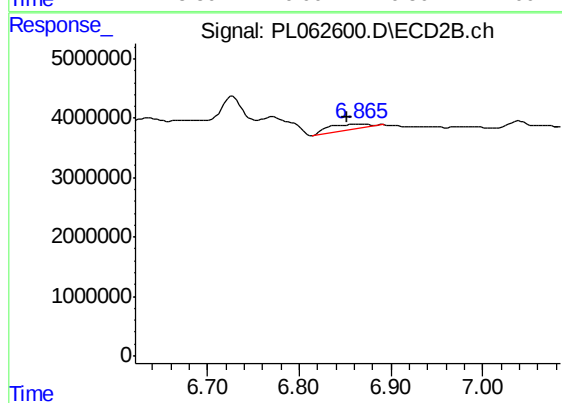

#15 Endosulfan II


R.T.: 6.866 min
Delta R.T.: 0.013 min
Response: 2964245
Conc: 1.04 ng/ml

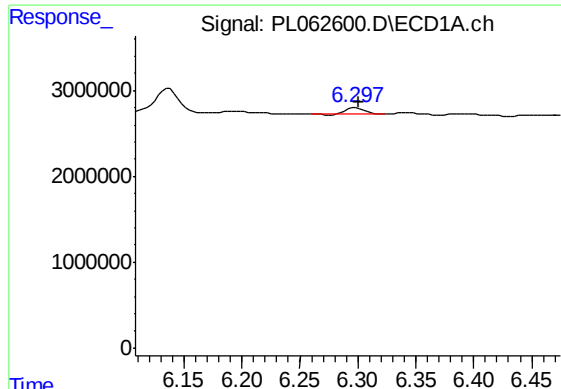

#17 4,4'-DDT


R.T.: 6.299 min
Delta R.T.: -0.003 min
Response: 763355
Conc: 0.57 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

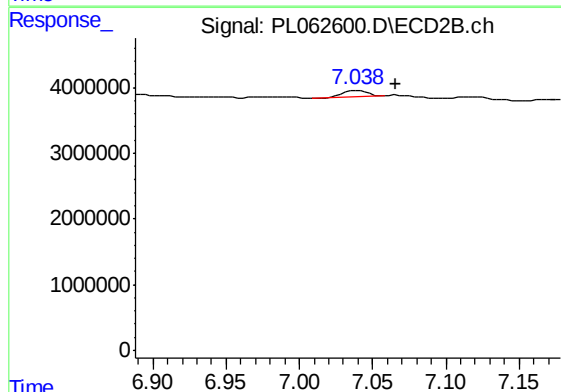


#17 4,4'-DDT

R.T.: 7.040 min
Delta R.T.: -0.026 min
Response: 1050242
Conc: 0.47 ng/ml

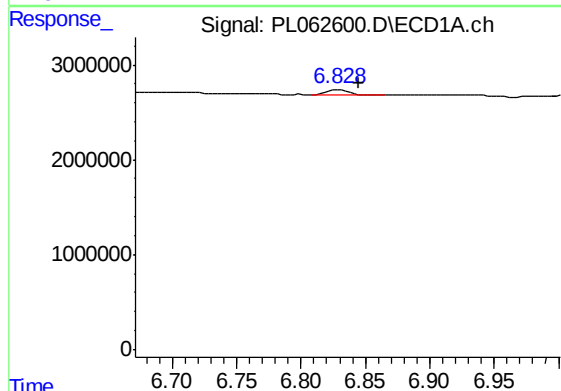


#20 Methoxychlor

R.T.: 6.830 min
Delta R.T.: -0.015 min
Response: 656893
Conc: 0.76 ng/ml

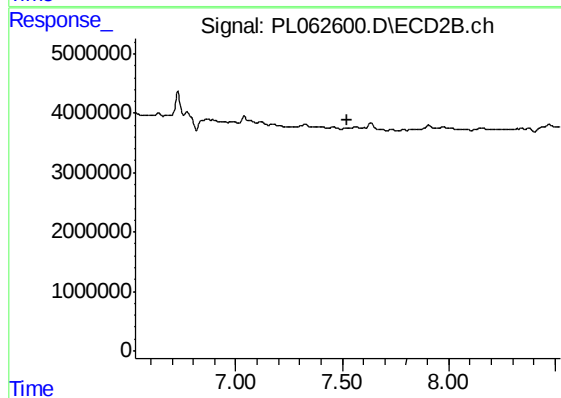

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.526 min
Response: 0
Conc: N.D.

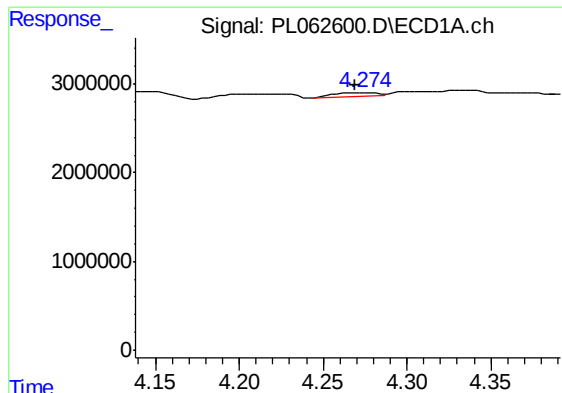

#23 Chlordane-1


R.T.: 4.275 min
Delta R.T.: 0.005 min
Response: 759333
Conc: 14.73 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

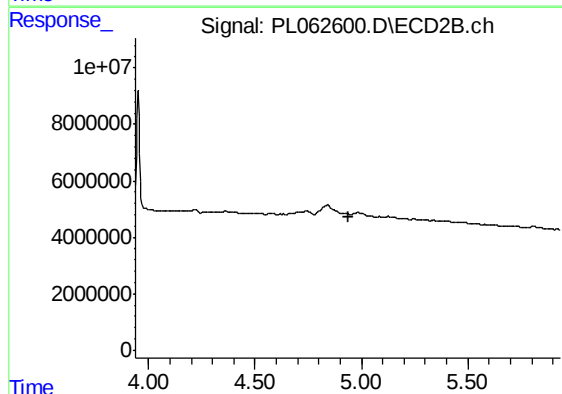


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.938 min
Response: 0
Conc: N.D.

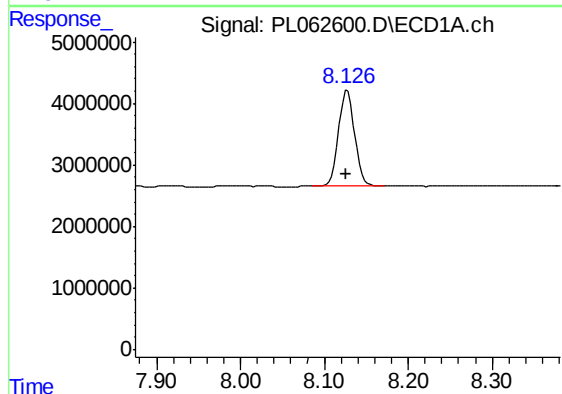

#28 Decachlorobiphenyl

R.T.: 8.128 min
Delta R.T.: 0.001 min
Response: 20646811
Conc: 12.87 ng/ml

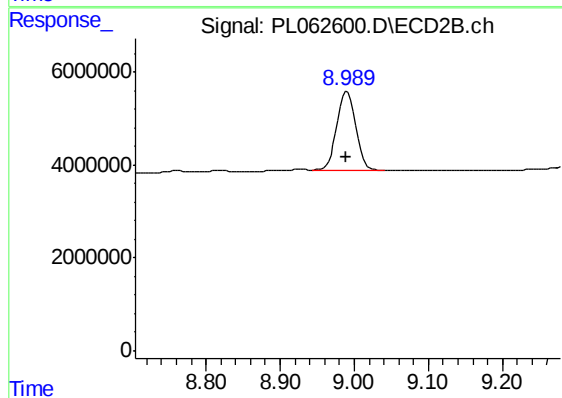

#28 Decachlorobiphenyl

R.T.: 8.991 min
Delta R.T.: 0.002 min
Response: 29535093
Conc: 14.11 ng/ml