

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
 Data File : PL062594.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 14:23
 Operator : DD\AJ
 Sample : L4501-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-3

Manual Integrations
 APPROVED

Ankita
 10/27/2020 10:05:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:07:09 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.952	20469132	35374271	11.900	12.037
28)	SA Decachlor...	8.127	8.990	17630981	22030136	10.990	10.526
Target Compounds							
12)	B 4,4'-DDE	5.549	6.271	854518	2139901	0.516m	0.664m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
Data File : PL062594.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 14:23
Operator : DD\AJ
Sample : L4501-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:07:09 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

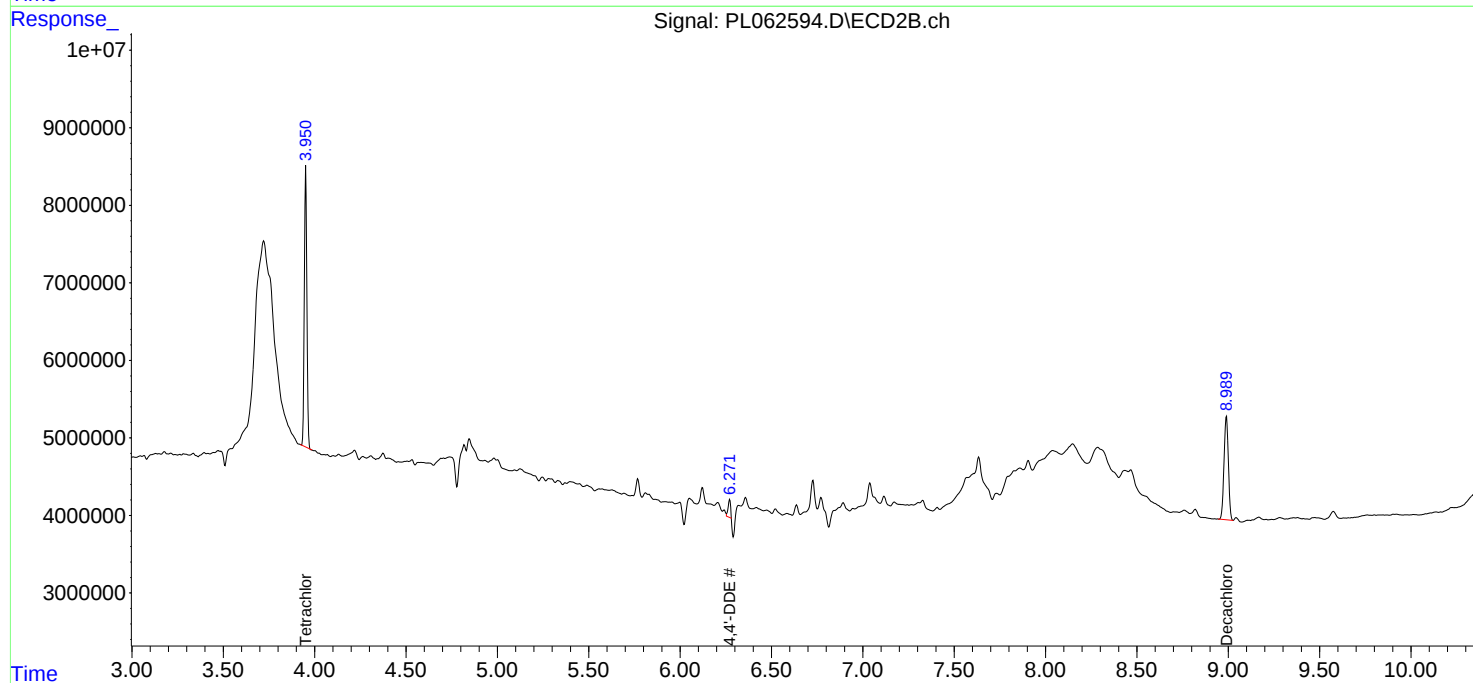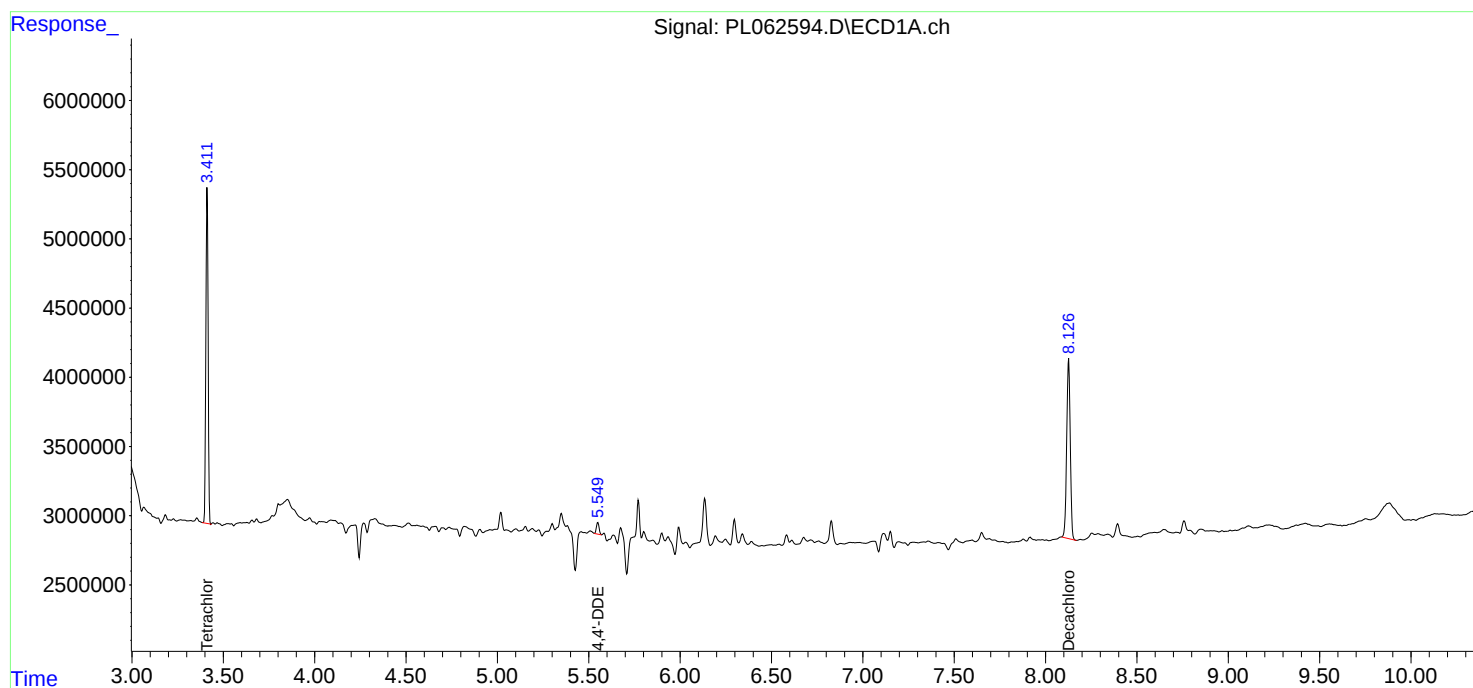

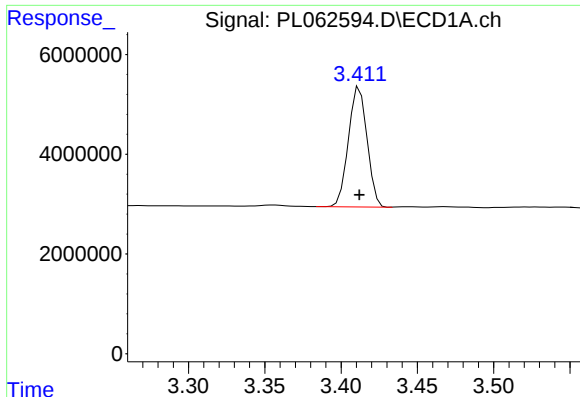


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 20469132
Conc: 11.90 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:18 AM

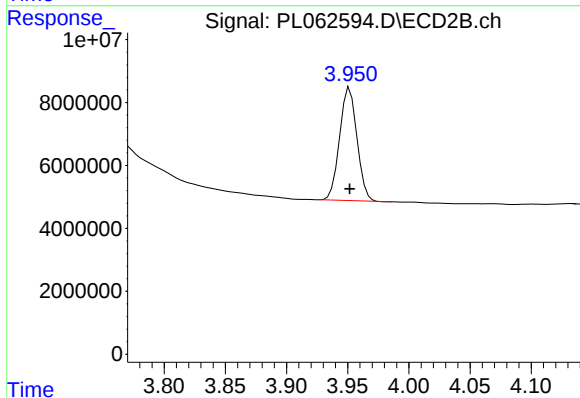


#1 Tetrachloro-m-xylene

R.T.: 3.952 min
Delta R.T.: 0.000 min
Response: 35374271
Conc: 12.04 ng/ml

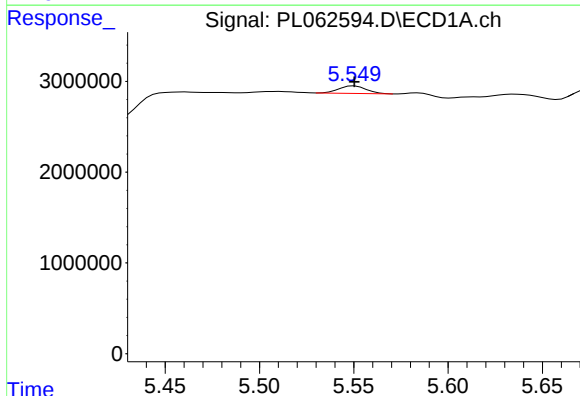


#12 4,4'-DDE

R.T.: 5.549 min
Delta R.T.: -0.001 min
Response: 854518
Conc: 0.52 ng/ml m

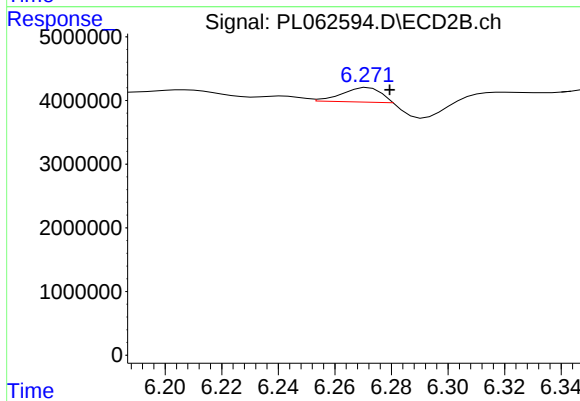

#12 4,4'-DDE

R.T.: 6.271 min
Delta R.T.: -0.009 min
Response: 2139901
Conc: 0.66 ng/ml m

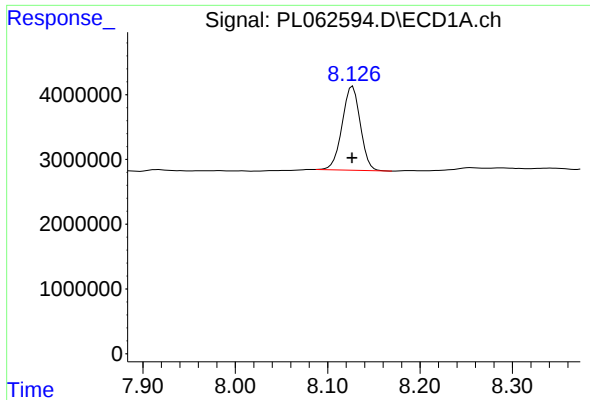


#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 17630981
Conc: 10.99 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-3

Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:18 AM

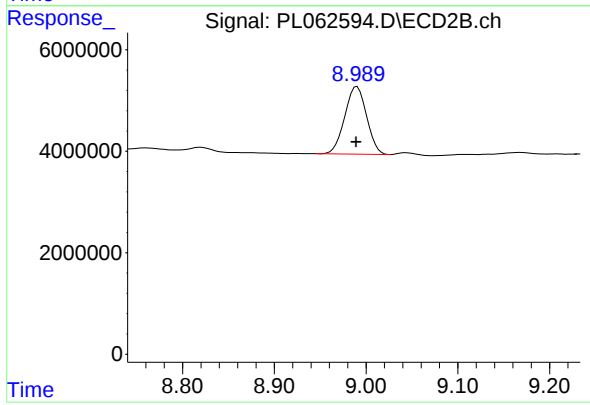

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.001 min
Response: 22030136
Conc: 10.53 ng/ml