

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
 Data File : PL062595.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Oct 2020 14:37
 Operator : DD\AJ
 Sample : L4510-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 COMP-1

Manual Integrations
 APPROVED

Ankita
 10/27/2020 10:05:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Oct 27 04:07:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
 Quant Title : GC Extractables
 QLast Update : Thu Oct 22 04:25:31 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.412	3.951	25667100	41305924	14.922	14.056
28)	SA Decachlor...	8.127	8.990	22682263	30490941	14.139	14.568
Target Compounds							
11)	B alpha-Chl...	5.384	6.120	943835	3056221	0.522m	0.907m#
12)	B 4,4'-DDE	5.550	6.270	923494	1641425	0.558	0.509m
17)	MA 4,4'-DDT	6.297	7.064	772866	1122762	0.579m	0.500m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL102620\
Data File : PL062595.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Oct 2020 14:37
Operator : DD\AJ
Sample : L4510-16
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
COMP-1


Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Oct 27 04:07:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL102120.M
Quant Title : GC Extractables
QLast Update : Thu Oct 22 04:25:31 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

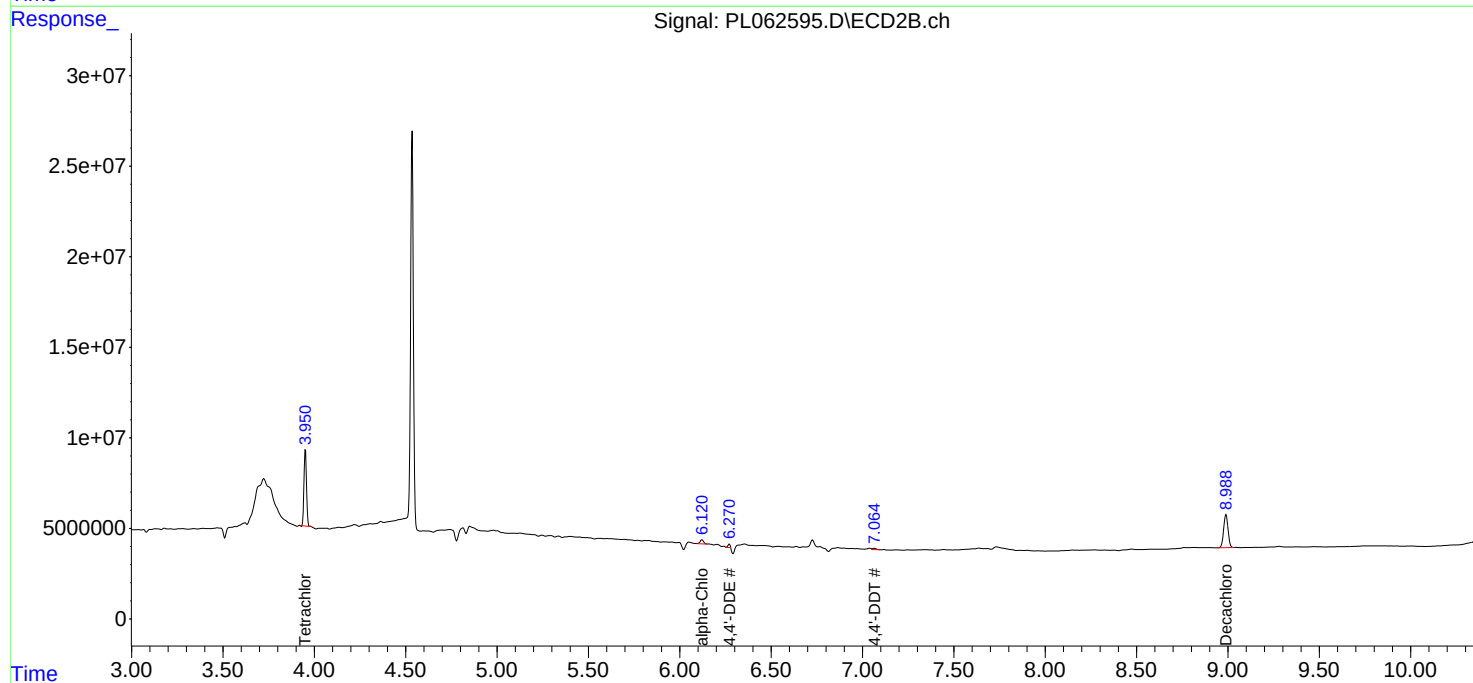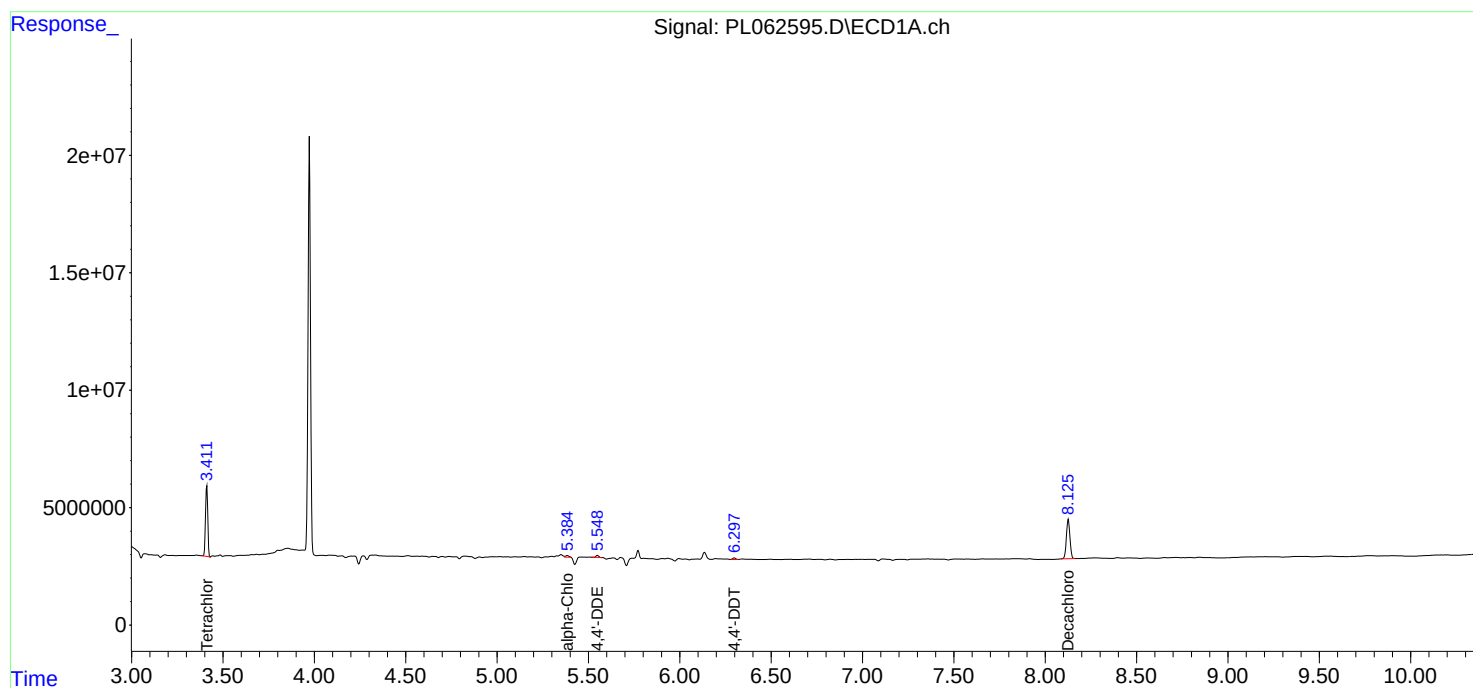

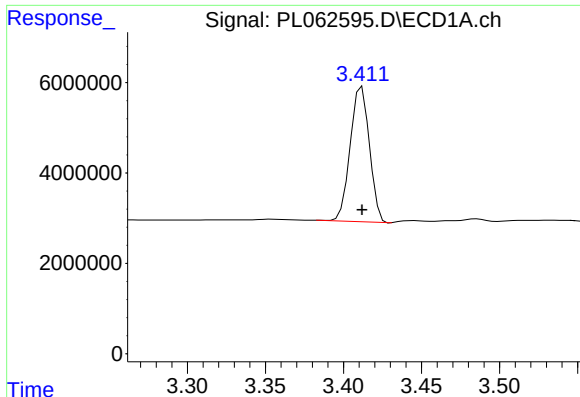


#1 Tetrachloro-m-xylene

R.T.: 3.412 min
Delta R.T.: 0.000 min
Response: 25667100
Conc: 14.92 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:21 AM

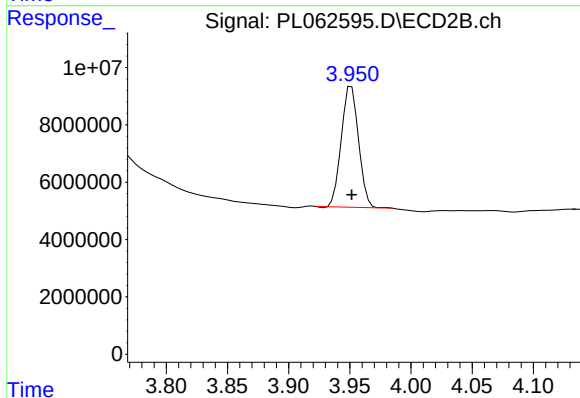


#1 Tetrachloro-m-xylene

R.T.: 3.951 min
Delta R.T.: 0.000 min
Response: 41305924
Conc: 14.06 ng/ml

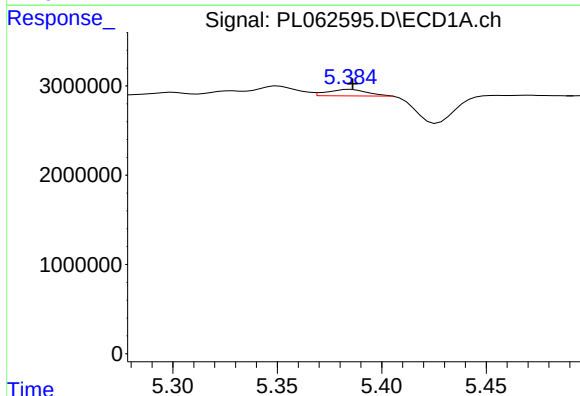


#11 alpha-Chlordane

R.T.: 5.384 min
Delta R.T.: -0.002 min
Response: 943835
Conc: 0.52 ng/ml m

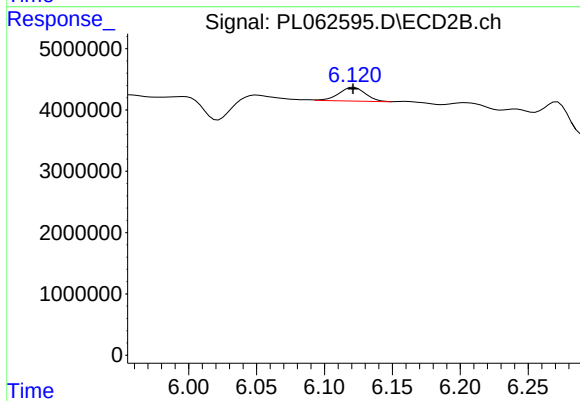

#11 alpha-Chlordane

R.T.: 6.120 min
Delta R.T.: 0.000 min
Response: 3056221
Conc: 0.91 ng/ml m

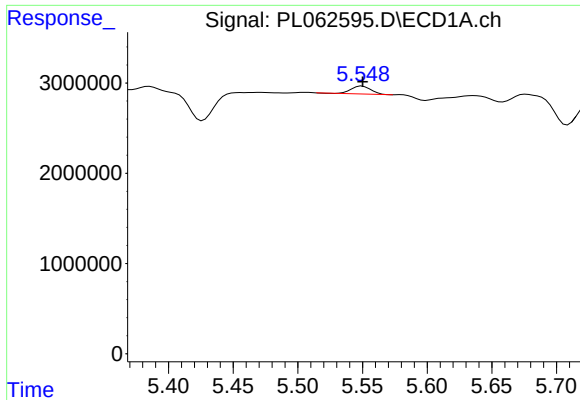


#12 4,4'-DDE

R.T.: 5.550 min
Delta R.T.: 0.000 min
Response: 923494
Conc: 0.56 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:21 AM

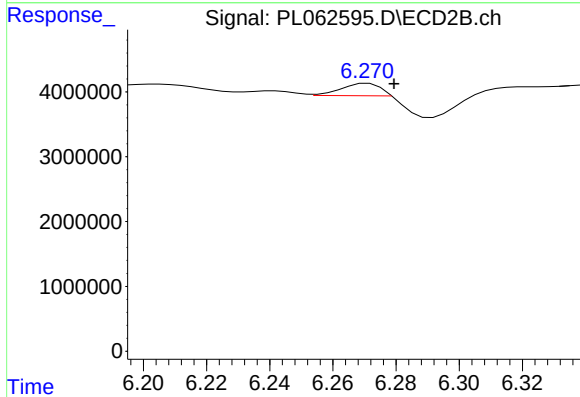


#12 4,4'-DDE

R.T.: 6.270 min
Delta R.T.: -0.009 min
Response: 1641425
Conc: 0.51 ng/ml m

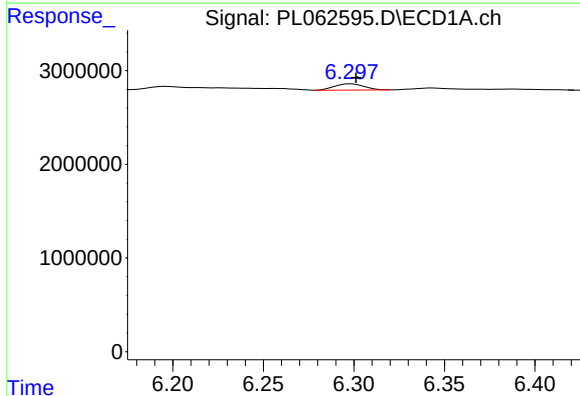


#17 4,4'-DDT

R.T.: 6.297 min
Delta R.T.: -0.004 min
Response: 772866
Conc: 0.58 ng/ml m

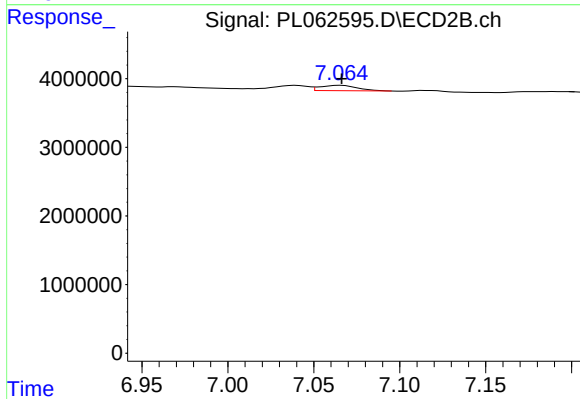

#17 4,4'-DDT

R.T.: 7.064 min
Delta R.T.: -0.002 min
Response: 1122762
Conc: 0.50 ng/ml m

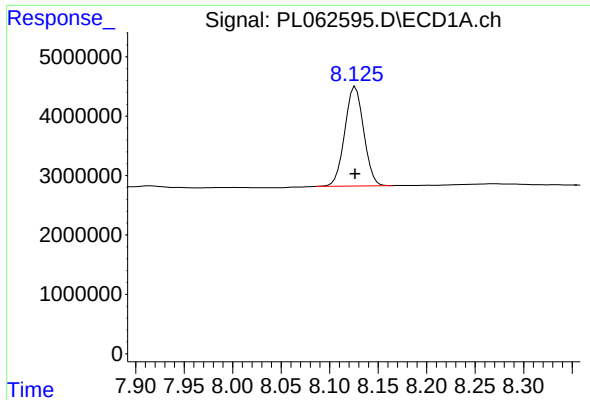


#28 Decachlorobiphenyl

R.T.: 8.127 min
Delta R.T.: 0.000 min
Response: 22682263
Conc: 14.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
COMP-1

Manual Integrations
APPROVED

Ankita
10/27/2020 10:05:21 AM

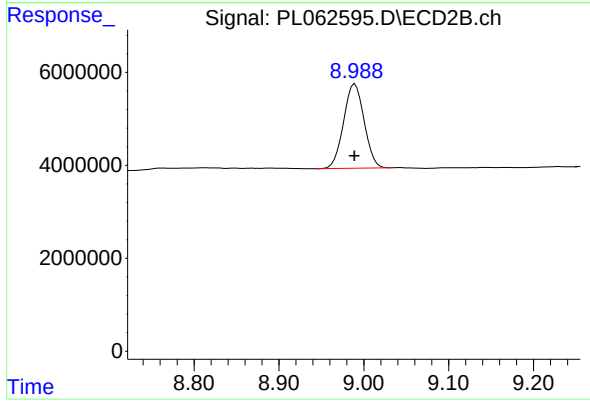

#28 Decachlorobiphenyl

R.T.: 8.990 min
Delta R.T.: 0.000 min
Response: 30490941
Conc: 14.57 ng/ml